

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016053.D
 Acq On : 07 Jul 2023 03:10
 Operator : MA/JU
 Sample : 03237-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBW77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	40	rVB	67047	104173	1.02%	0.125%
2	3.811	103	106	127	rBV	223967	495128	4.85%	0.593%
3	4.011	137	140	145	rVB2	21813	35140	0.34%	0.042%
4	4.123	156	159	165	rVB	16344	25403	0.25%	0.030%
5	7.252	682	691	703	rBV	147153	454233	4.45%	0.544%
6	7.358	703	709	731	rVB	661080	1595048	15.63%	1.912%
7	7.575	738	746	766	rBV	601275	1614056	15.82%	1.934%
8	8.034	816	824	841	rBV	616796	1655184	16.22%	1.984%
9	8.781	942	951	981	rBV	450964	1527442	14.97%	1.831%
10	9.228	1019	1027	1057	rVV	858647	2074994	20.34%	2.487%
11	9.546	1076	1081	1088	rVB9	9370	17805	0.17%	0.021%
12	9.958	1143	1151	1169	rBV	553195	1699493	16.66%	2.037%
13	10.540	1240	1250	1292	rBV	519755	2489683	24.40%	2.984%
14	10.858	1296	1304	1323	rVB	1116543	2511820	24.62%	3.010%
15	11.046	1327	1336	1371	rBV	565058	2325334	22.79%	2.787%
16	12.281	1537	1546	1553	rBV9	19561	64973	0.64%	0.078%
17	12.510	1579	1585	1592	rBV4	13218	28302	0.28%	0.034%
18	12.987	1660	1666	1668	rBV6	9333	17390	0.17%	0.021%
19	13.281	1711	1716	1723	rBV7	13345	24786	0.24%	0.030%
20	13.563	1758	1764	1771	rBV5	17932	42997	0.42%	0.052%
21	14.093	1847	1854	1875	rBV	2351769	4758473	46.63%	5.703%
22	14.375	1895	1902	1927	rBV2	3221568	5413478	53.05%	6.488%
23	14.675	1945	1953	1979	rVB	2250180	3873157	37.96%	4.642%
24	15.081	2015	2022	2025	rBV5	45199	129771	1.27%	0.156%
25	15.357	2066	2069	2075	rVB2	17702	31782	0.31%	0.038%
26	15.440	2079	2083	2089	rVV8	5528	13923	0.14%	0.017%
27	15.498	2089	2093	2099	rVV7	16793	31090	0.30%	0.037%
28	15.563	2099	2104	2111	rVB8	9872	22864	0.22%	0.027%
29	15.681	2117	2124	2143	rBV	3276201	6951547	68.13%	8.331%
30	15.863	2149	2155	2203	rVB	647016	2140898	20.98%	2.566%
31	16.187	2208	2210	2214	rVB4	9893	12413	0.12%	0.015%
32	16.375	2237	2242	2246	rBV7	12350	20259	0.20%	0.024%
33	16.475	2255	2259	2263	rBV7	6232	12010	0.12%	0.014%
34	17.010	2347	2350	2359	rVB3	24441	37136	0.36%	0.045%
35	17.110	2364	2367	2372	rVB7	8627	12894	0.13%	0.015%
36	17.192	2378	2381	2385	rBV6	10046	16725	0.16%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016053.D
 Acq On : 07 Jul 2023 03:10
 Operator : MA/JU
 Sample : 03237-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBW77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	17.440	2417	2423	2435	rBV	2850209	4369749	42.82%	5.237%
38	17.545	2435	2441	2466	rVV2	3743324	8127080	79.65%	9.740%
39	18.075	2527	2531	2538	rBV2	141570	182609	1.79%	0.219%
40	18.298	2565	2569	2576	rBV3	59322	120673	1.18%	0.145%
41	19.351	2745	2748	2753	rVB	72030	92283	0.90%	0.111%
42	19.428	2758	2761	2767	rVB	59996	85465	0.84%	0.102%
43	19.775	2814	2820	2837	rBV	5412929	10204048	100.00%	12.229%
44	19.957	2847	2851	2858	rVB	167072	253752	2.49%	0.304%
45	20.651	2965	2969	2974	rBV	428622	597763	5.86%	0.716%
46	21.545	3116	3121	3138	rBV2	2142488	4811878	47.16%	5.767%
47	23.904	3515	3522	3540	rVB2	3200874	8004032	78.44%	9.593%
48	24.080	3545	3552	3576	rVB	1359902	4308029	42.22%	5.163%




Sum of corrected areas: 83439165

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016053.D
Acq On : 07 Jul 2023 03:10
Operator : MA/JU
Sample : 03237-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

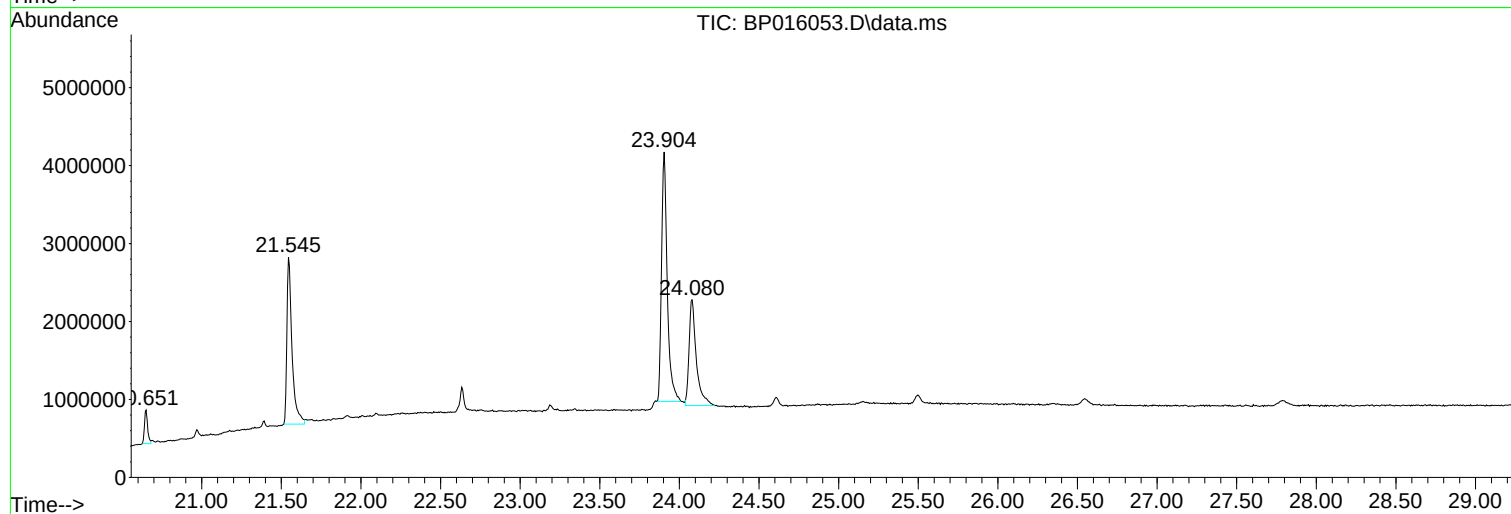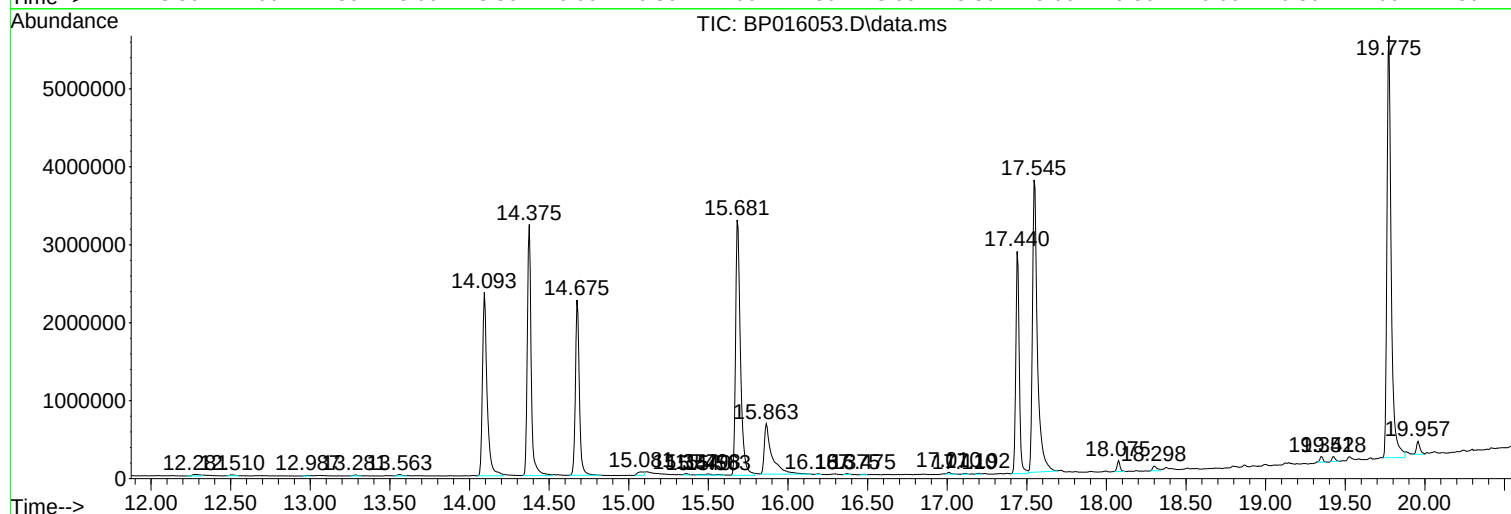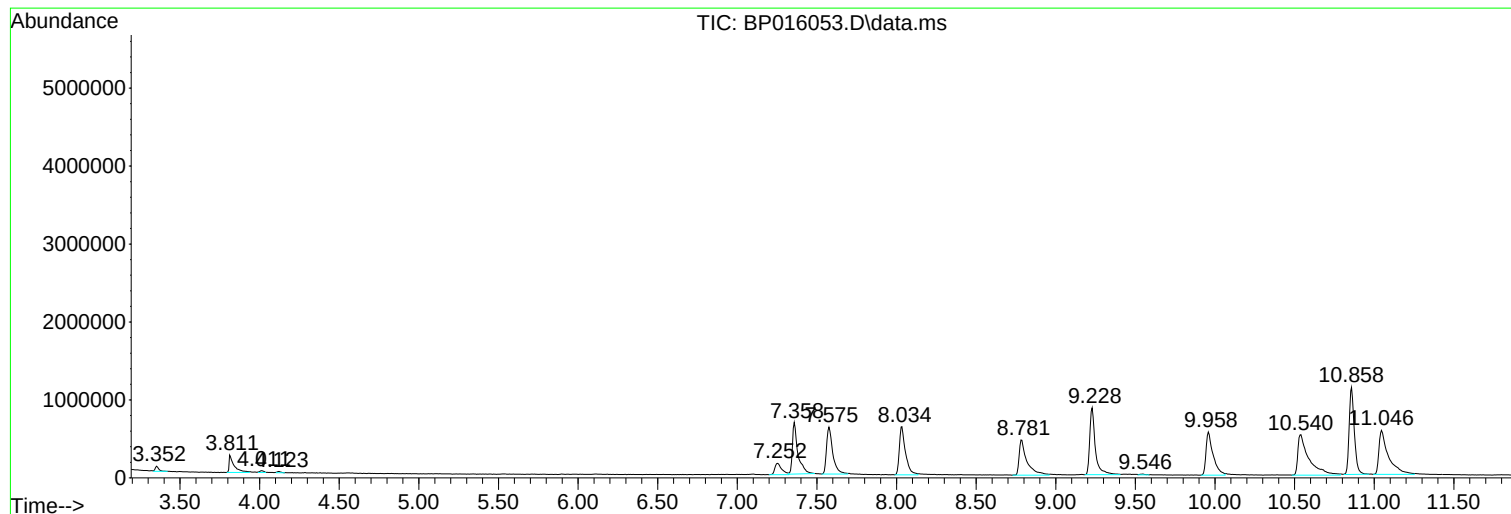

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016053.D
Acq On : 07 Jul 2023 03:10
Operator : MA/JU
Sample : 03237-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW77










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzyl butyl phthalate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.651	2.48 ng/ul	597763	Chrysene-d12	21.545

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzyl butyl phthalate	312	C19H20O4	000085-68-7	94
2			Benzyl butyl phthalate	312	C19H20O4	000085-68-7	91
3			Benzyl butyl phthalate	312	C19H20O4	000085-68-7	87
4			Phthalic acid, benzyl isobutyl e...	312	C19H20O4	1000309-04-3	86
5			Phthalic acid, butyl 2-methoxybe...	342	C20H22O5	1000382-49-3	86

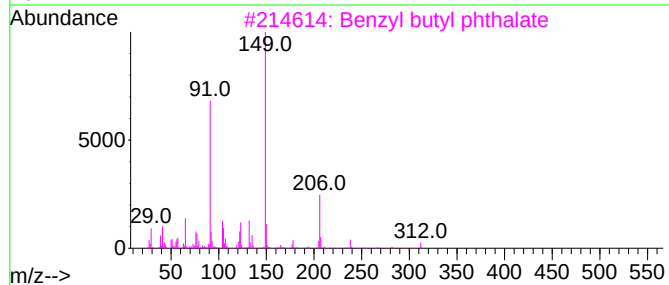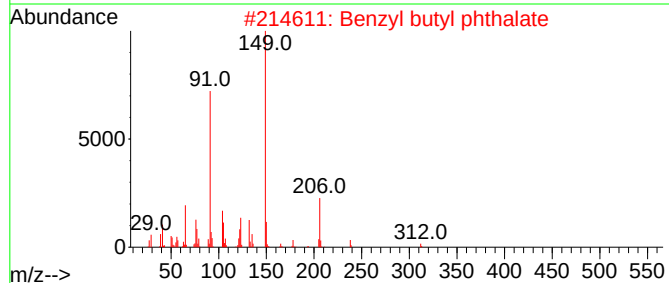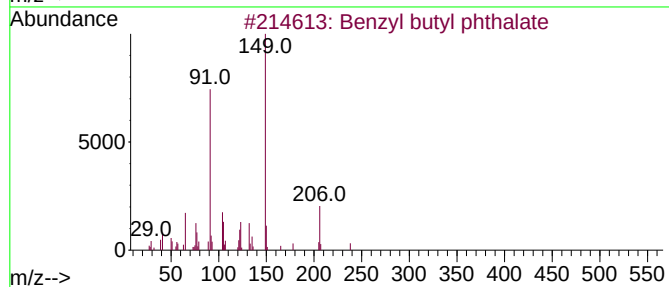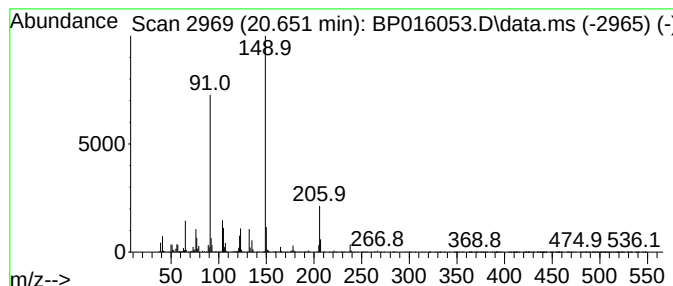

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016053.D
Acq On : 07 Jul 2023 03:10
Operator : MA/JU
Sample : 03237-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzy1 butyl ph...	20.651	2.5	ng/u1	597763	5	21.545	4811880	20.0