

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016057.D
 Acq On : 07 Jul 2023 05:59
 Operator : MA/JU
 Sample : PB153600BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK600

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	37	rVB	70262	102666	1.55%	0.168%
2	3.799	101	104	127	rBV	636832	1297705	19.59%	2.118%
3	4.552	228	232	234	rBV5	7169	9335	0.14%	0.015%
4	7.222	678	686	703	rBV	480749	1540898	23.26%	2.515%
5	7.358	703	709	734	rVV	563443	1396361	21.08%	2.280%
6	7.563	737	744	773	rVB	697198	1666319	25.16%	2.720%
7	8.028	816	823	846	rBV	418936	1160106	17.51%	1.894%
8	8.781	943	951	982	rBV	622074	2093752	31.61%	3.418%
9	9.228	1019	1027	1053	rBV	630648	1697198	25.62%	2.771%
10	9.963	1144	1152	1177	rBV2	400412	1421045	21.45%	2.320%
11	10.546	1242	1251	1273	rBV	369263	1713408	25.87%	2.797%
12	10.857	1297	1304	1321	rVB	702930	1710975	25.83%	2.793%
13	11.051	1329	1337	1368	rBV	453970	1975431	29.82%	3.225%
14	12.522	1581	1587	1593	rBV8	10739	29859	0.45%	0.049%
15	13.569	1760	1765	1767	rBV5	4919	7007	0.11%	0.011%
16	14.098	1846	1855	1889	rBV	1507139	3583281	54.10%	5.850%
17	14.375	1895	1902	1929	rBV2	2244215	4066387	61.39%	6.638%
18	14.681	1947	1954	1972	rBV	1456729	2439324	36.83%	3.982%
19	15.016	2003	2011	2047	rBV4	185307	1227083	18.53%	2.003%
20	15.687	2118	2125	2146	rBV2	2111035	4988253	75.31%	8.143%
21	15.875	2150	2157	2196	rVV	325954	1406270	21.23%	2.296%
22	16.492	2256	2262	2265	rBV8	4431	7432	0.11%	0.012%
23	17.116	2363	2368	2373	rBV9	7101	15153	0.23%	0.025%
24	17.445	2416	2424	2436	rBV	1847808	2970054	44.84%	4.849%
25	17.551	2436	2442	2480	rVB	2135832	5548585	83.77%	9.058%
26	19.357	2746	2749	2754	rBV3	43119	56454	0.85%	0.092%
27	19.433	2759	2762	2767	rBV3	28040	47650	0.72%	0.078%
28	19.780	2815	2821	2848	rBV	2891784	6623707	100.00%	10.813%
29	21.557	3118	3123	3137	rBV2	1236046	3013171	45.49%	4.919%
30	23.915	3517	3524	3543	rVB2	1773399	4908965	74.11%	8.014%
31	24.092	3548	3554	3577	rVB	710505	2532827	38.24%	4.135%




Sum of corrected areas: 61256661

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016057.D
Acq On : 07 Jul 2023 05:59
Operator : MA/JU
Sample : PB153600BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK600

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

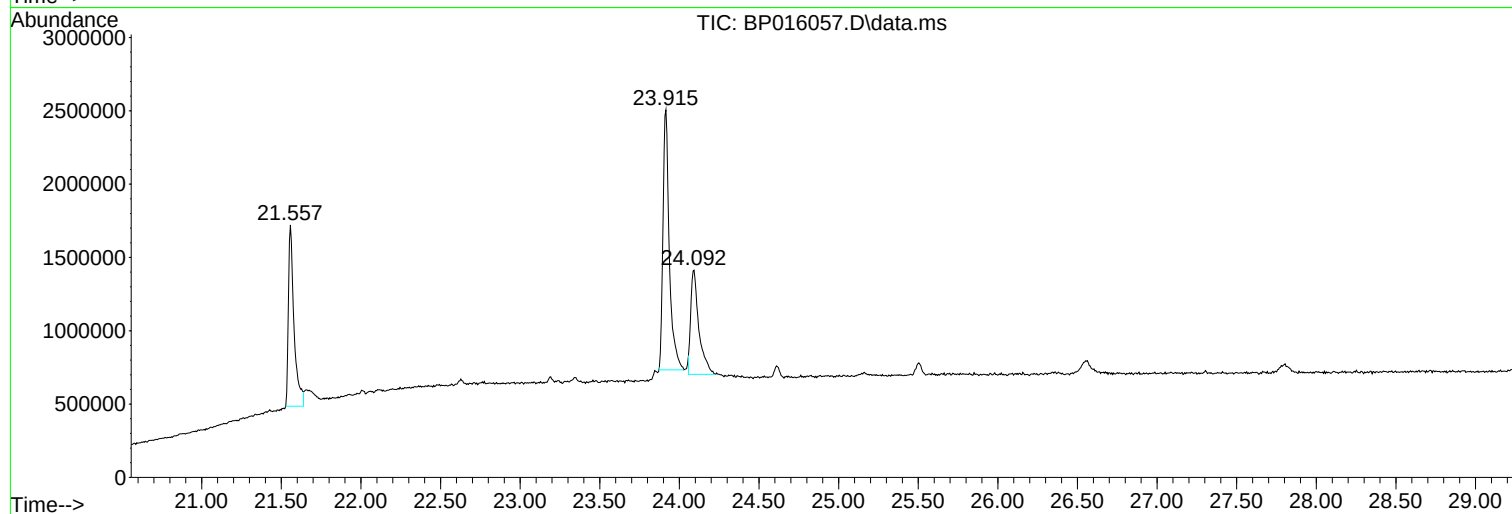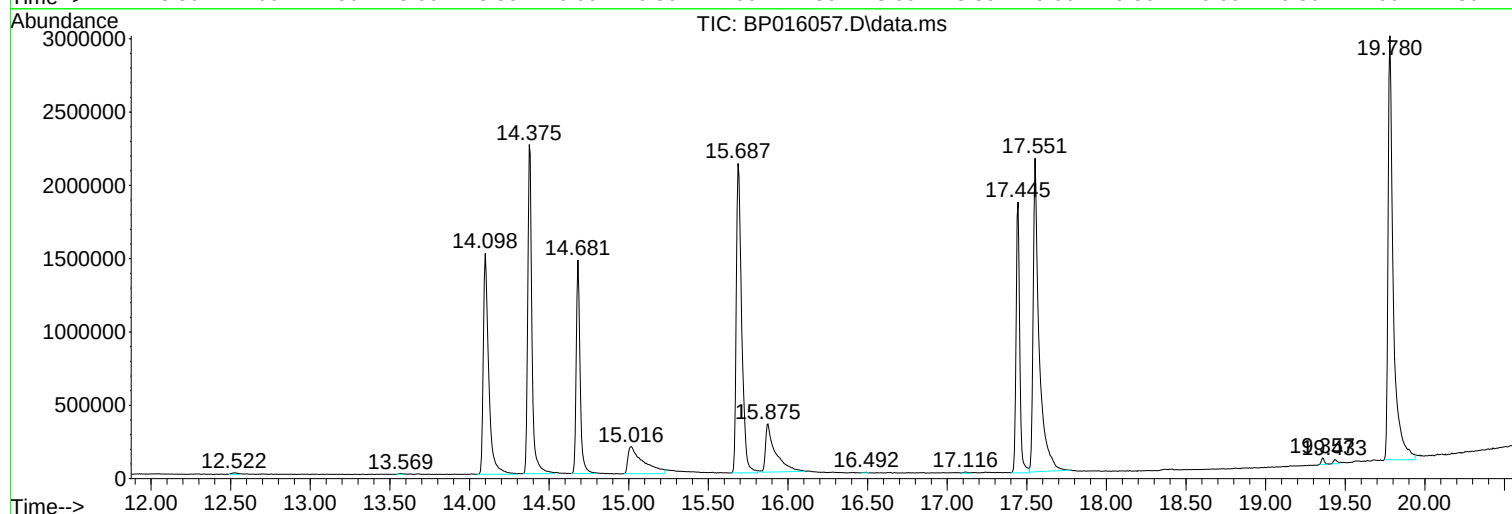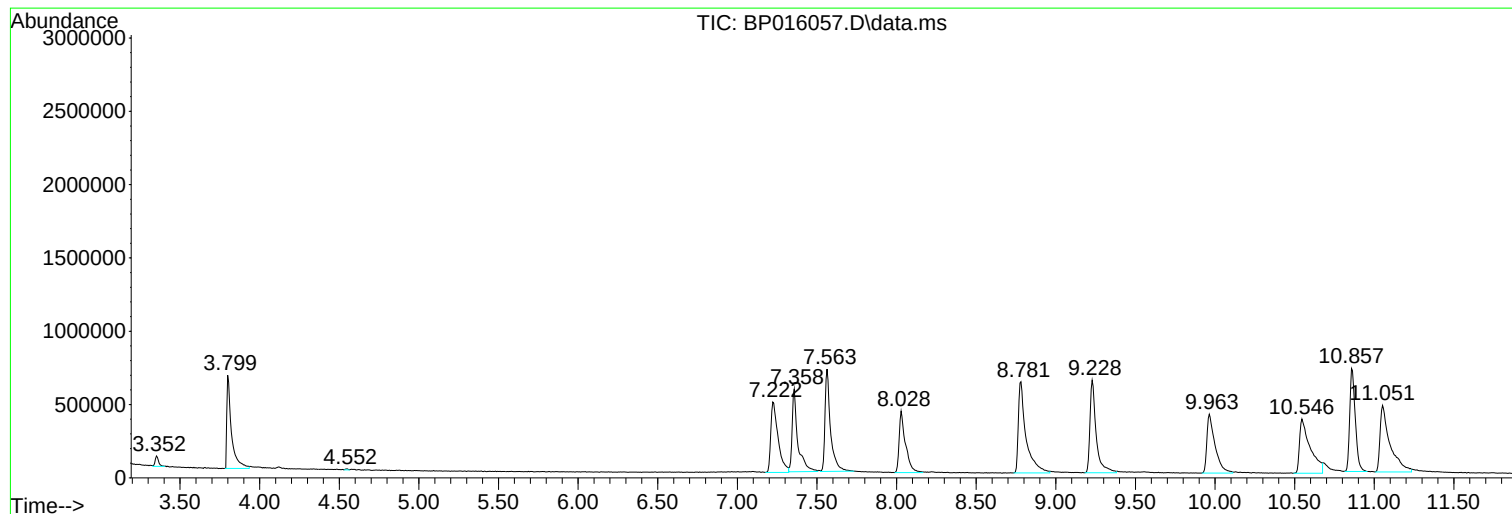

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016057.D
Acq On : 07 Jul 2023 05:59
Operator : MA/JU
Sample : PB153600BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK600

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016057.D
Acq On : 07 Jul 2023 05:59
Operator : MA/JU
Sample : PB153600BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK600

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------