

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016058.D
 Acq On : 07 Jul 2023 06:33
 Operator : MA/JU
 Sample : PB153602BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK602

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	40	rVB	74293	116688	1.69%	0.180%
2	3.799	101	104	126	rBV	696331	1383468	19.99%	2.133%
3	7.222	679	686	703	rBV2	514908	1640401	23.70%	2.529%
4	7.358	703	709	737	rVV	600836	1495080	21.60%	2.305%
5	7.563	737	744	772	rVB	757732	1768374	25.55%	2.726%
6	8.028	816	823	844	rBV	452694	1225910	17.71%	1.890%
7	8.216	852	855	862	rVB9	5417	9036	0.13%	0.014%
8	8.775	943	950	980	rBV	697957	2221482	32.09%	3.424%
9	9.228	1020	1027	1060	rBV	687896	1832231	26.47%	2.824%
10	9.963	1144	1152	1183	rBV	441039	1527235	22.06%	2.354%
11	10.540	1242	1250	1271	rBV	401914	1797257	25.96%	2.770%
12	10.857	1297	1304	1321	rVB	780874	1858311	26.85%	2.865%
13	11.051	1329	1337	1367	rBV	481301	2118117	30.60%	3.265%
14	12.522	1576	1587	1594	rBV6	12367	35660	0.52%	0.055%
15	13.569	1759	1765	1768	rBV7	8195	13119	0.19%	0.020%
16	14.098	1847	1855	1883	rBV	1606390	3723022	53.78%	5.739%
17	14.375	1895	1902	1925	rBV2	2397235	4254688	61.47%	6.559%
18	14.681	1947	1954	1976	rBV	1526480	2621736	37.87%	4.041%
19	15.004	2002	2009	2027	rBV	195829	976896	14.11%	1.506%
20	15.687	2118	2125	2147	rBV	2301094	5203589	75.17%	8.021%
21	15.869	2150	2156	2195	rVV	357530	1449874	20.95%	2.235%
22	17.445	2417	2424	2435	rBV	1955995	3178064	45.91%	4.899%
23	17.551	2435	2442	2482	rVB2	2236486	5825621	84.16%	8.980%
24	19.357	2745	2749	2755	rBV2	47189	74709	1.08%	0.115%
25	19.433	2759	2762	2771	rVV	29699	57906	0.84%	0.089%
26	19.780	2815	2821	2851	rBV	2967751	6922078	100.00%	10.670%
27	21.557	3117	3123	3137	rBV	1355375	3347378	48.36%	5.160%
28	23.910	3516	3523	3542	rBV2	1906100	5391690	77.89%	8.311%
29	24.086	3547	3553	3575	rVB	831716	2802747	40.49%	4.320%




Sum of corrected areas: 64872367

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016058.D
Acq On : 07 Jul 2023 06:33
Operator : MA/JU
Sample : PB153602BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK602

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

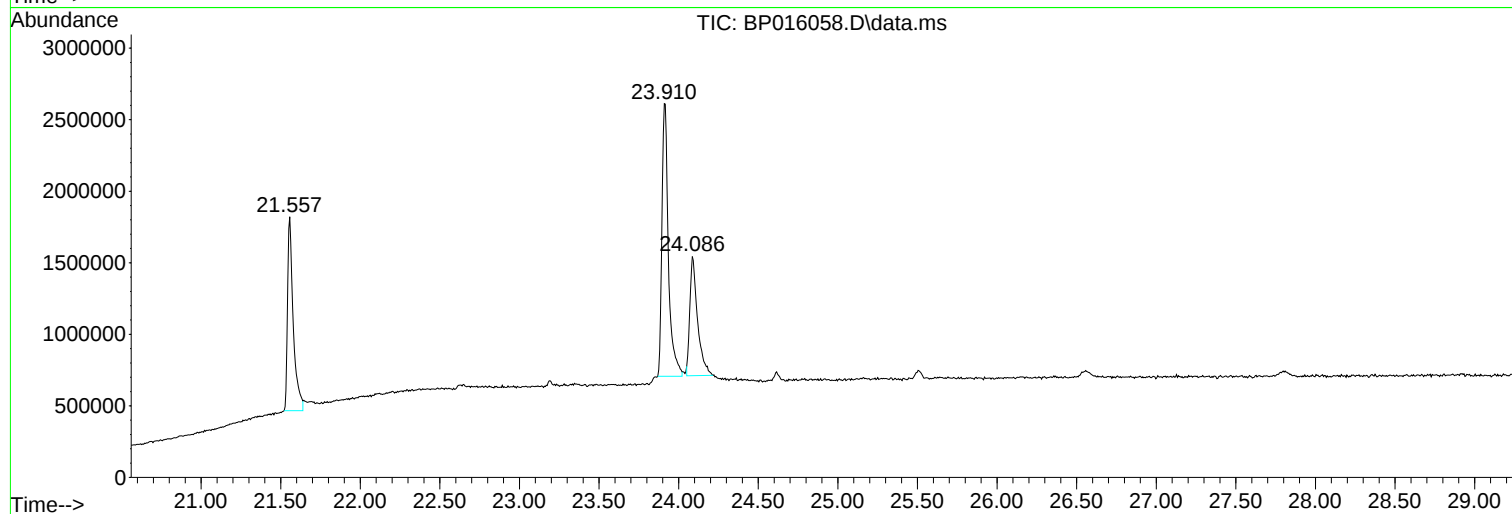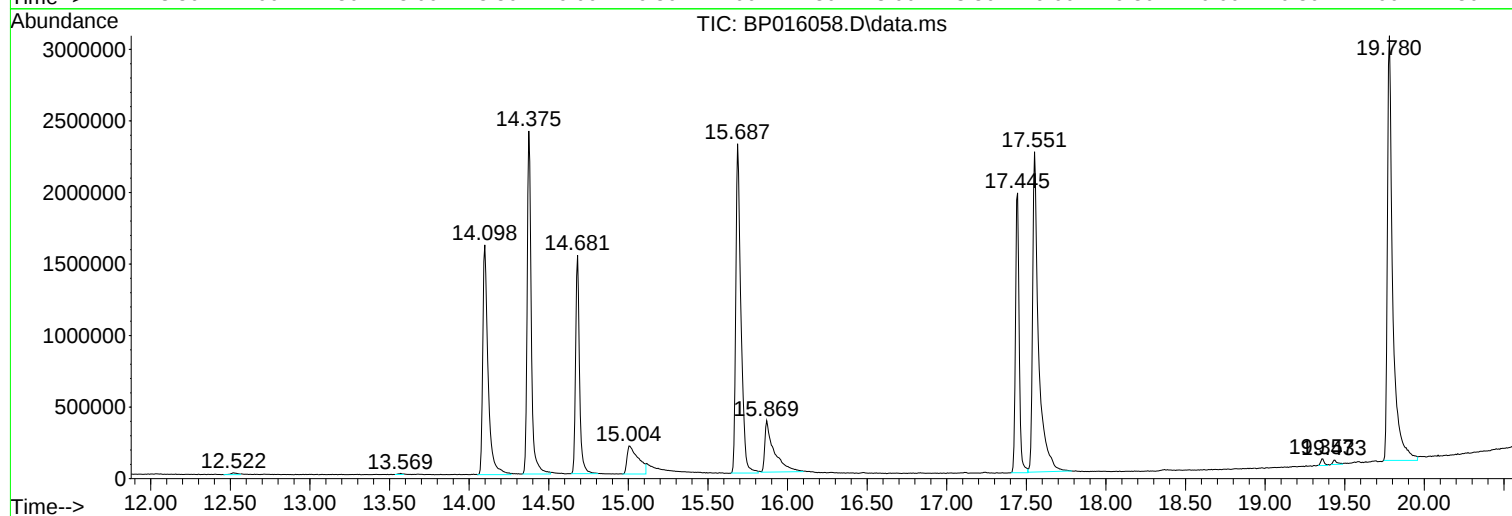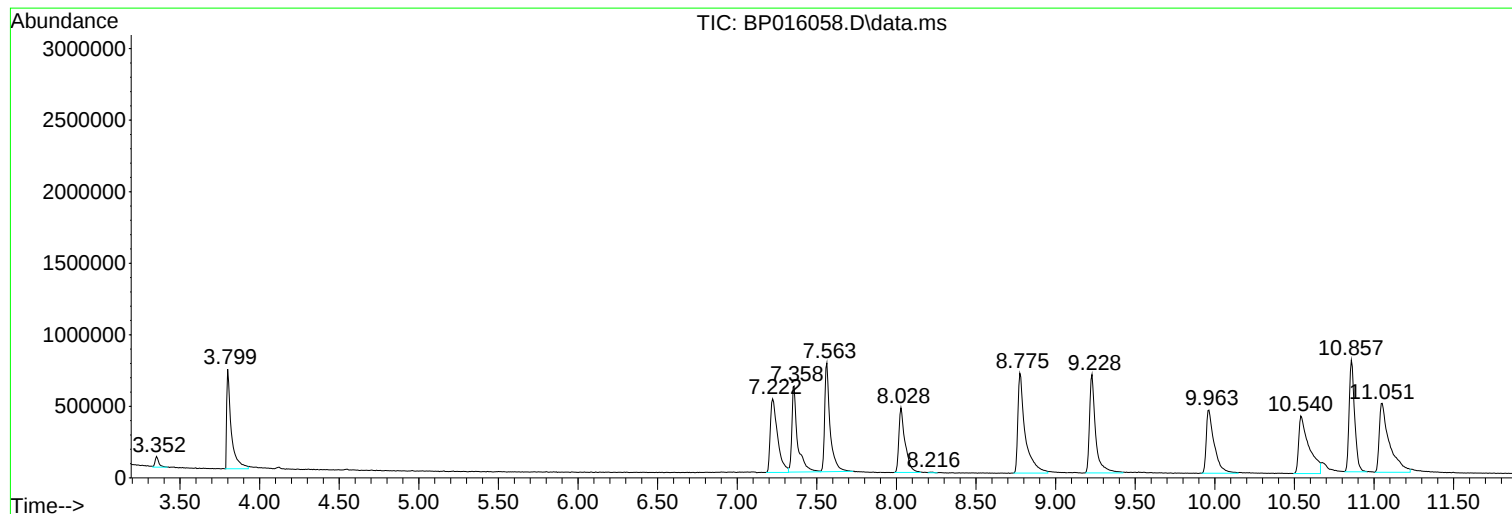

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016058.D
Acq On : 07 Jul 2023 06:33
Operator : MA/JU
Sample : PB153602BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK602

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016058.D
Acq On : 07 Jul 2023 06:33
Operator : MA/JU
Sample : PB153602BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK602

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------