

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016061.D
 Acq On : 07 Jul 2023 09:00
 Operator : MA/JU
 Sample : PB153592BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK592

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	40	rVB	77335	126255	1.98%	0.213%
2	3.811	104	106	119	rBV	253146	534933	8.41%	0.903%
3	4.117	155	158	162	rBV3	11790	17508	0.28%	0.030%
4	7.222	679	686	703	rBV	488141	1564518	24.60%	2.642%
5	7.358	703	709	733	rVB	585410	1378776	21.68%	2.328%
6	7.563	738	744	768	rVB	733654	1679163	26.40%	2.835%
7	8.028	816	823	849	rBV	469302	1336783	21.02%	2.257%
8	8.222	853	856	862	rVB8	6991	12623	0.20%	0.021%
9	8.781	944	951	993	rBV	603495	2164506	34.03%	3.655%
10	9.234	1020	1028	1048	rBV	610461	1717340	27.00%	2.900%
11	9.969	1144	1153	1178	rBV2	340028	1450579	22.80%	2.450%
12	10.575	1247	1256	1273	rBV	365398	1649533	25.93%	2.785%
13	10.863	1297	1305	1325	rBV	705244	1938012	30.47%	3.273%
14	11.110	1339	1347	1377	rBV2	90965	469872	7.39%	0.793%
15	12.528	1580	1588	1600	rBV9	10911	40184	0.63%	0.068%
16	14.010	1836	1840	1845	rBV8	4864	7348	0.12%	0.012%
17	14.104	1849	1856	1882	rBV	1510659	3572023	56.15%	6.032%
18	14.381	1896	1903	1937	rBV	2344016	4136120	65.02%	6.984%
19	14.687	1948	1955	1971	rBV	1573361	2771743	43.57%	4.680%
20	15.022	2004	2012	2039	rBV2	176733	1089159	17.12%	1.839%
21	15.581	2105	2107	2111	rVB5	5378	6777	0.11%	0.011%
22	15.692	2118	2126	2146	rBV	2176278	5089072	80.00%	8.594%
23	15.875	2151	2157	2190	rVV2	333004	1394702	21.93%	2.355%
24	17.122	2365	2369	2374	rBV8	5563	10087	0.16%	0.017%
25	17.245	2386	2390	2396	rBV7	5343	9698	0.15%	0.016%
26	17.451	2418	2425	2437	rBV	2001801	3342724	52.55%	5.645%
27	17.557	2437	2443	2475	rVB	1955613	5395719	84.82%	9.111%
28	19.363	2747	2750	2757	rBV2	43187	67827	1.07%	0.115%
29	19.445	2760	2764	2769	rBV	26216	55053	0.87%	0.093%
30	19.786	2816	2822	2851	rBV	2558545	6361014	100.00%	10.741%
31	21.563	3119	3124	3144	rBV	1236712	3251244	51.11%	5.490%
32	23.927	3519	3526	3547	rBV2	1383859	4155445	65.33%	7.017%
33	24.104	3550	3556	3579	rVB	651540	2423031	38.09%	4.092%




Sum of corrected areas: 59219371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016061.D
Acq On : 07 Jul 2023 09:00
Operator : MA/JU
Sample : PB153592BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

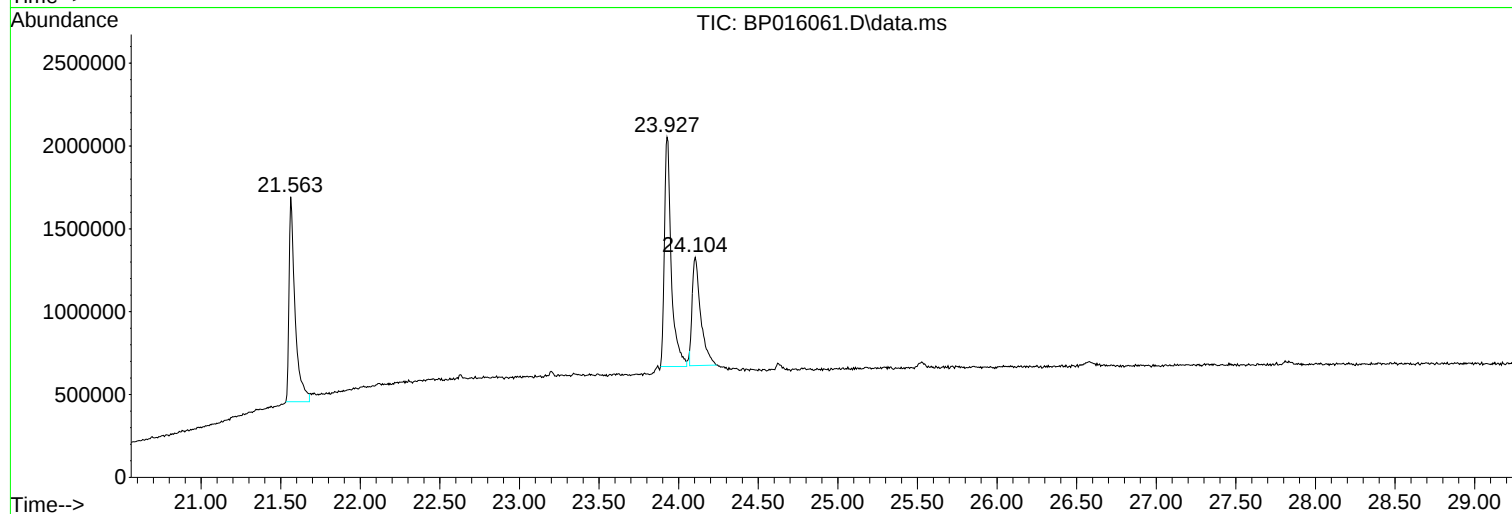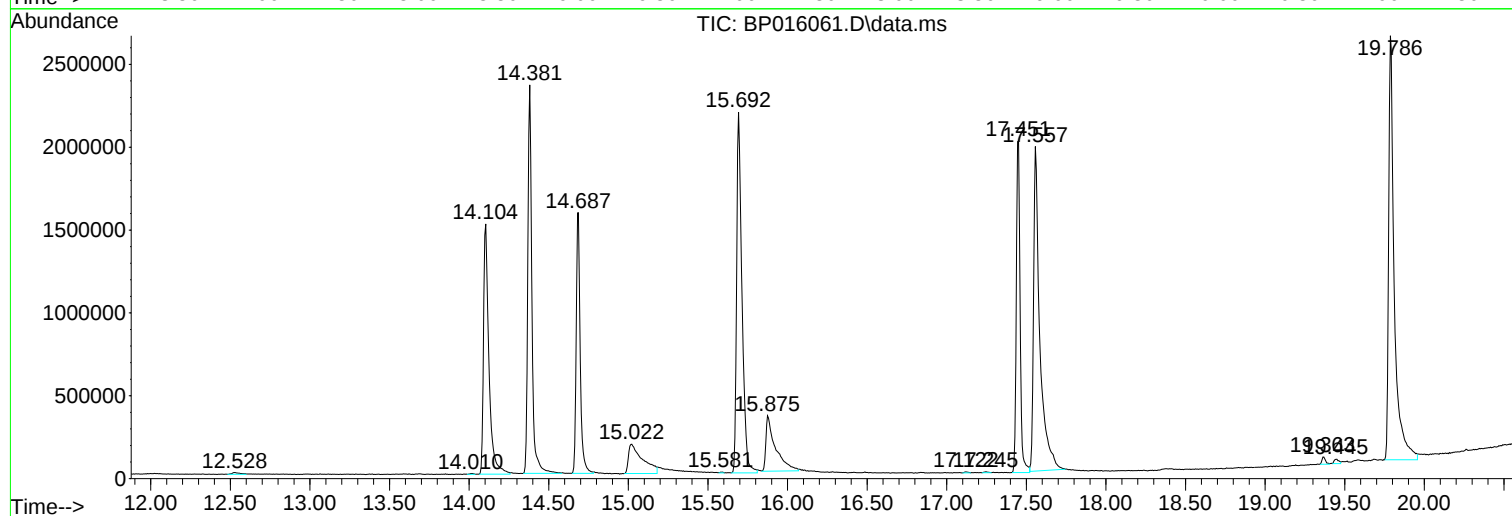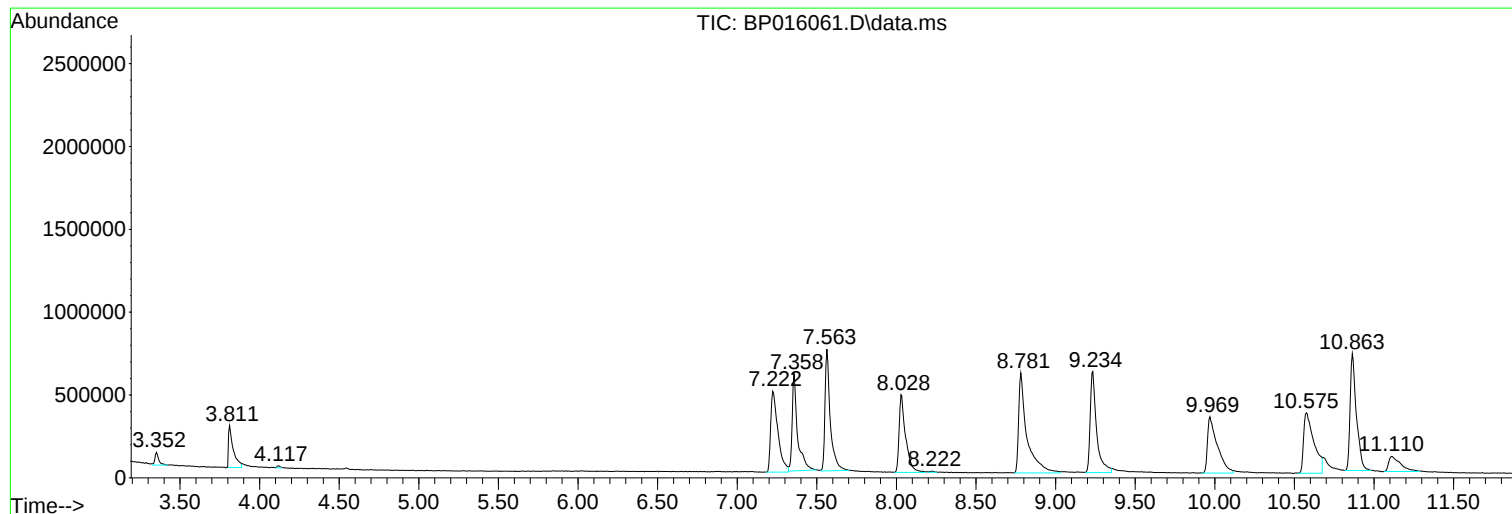

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016061.D
Acq On : 07 Jul 2023 09:00
Operator : MA/JU
Sample : PB153592BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016061.D
Acq On : 07 Jul 2023 09:00
Operator : MA/JU
Sample : PB153592BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK592

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------