

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016062.D
 Acq On : 07 Jul 2023 09:34
 Operator : MA/JU
 Sample : PB153518BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK518

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	38	rVB	76736	108414	1.75%	0.187%
2	3.811	103	106	126	rBV	259680	596568	9.61%	1.026%
3	7.222	679	686	703	rBV	469032	1527459	24.60%	2.628%
4	7.358	703	709	733	rVV	555418	1403031	22.59%	2.414%
5	7.564	737	744	770	rVB	699791	1647708	26.53%	2.835%
6	8.028	816	823	844	rBV	444877	1263142	20.34%	2.173%
7	8.781	944	951	987	rBV	571110	2092889	33.70%	3.601%
8	9.228	1019	1027	1059	rBV	560774	1698312	27.35%	2.922%
9	9.969	1145	1153	1180	rBV2	318251	1405963	22.64%	2.419%
10	10.575	1247	1256	1297	rBV	341349	1920257	30.92%	3.304%
11	10.863	1297	1305	1329	rVB	655547	1937871	31.21%	3.334%
12	11.122	1341	1349	1372	rBV4	68715	368597	5.94%	0.634%
13	12.528	1583	1588	1590	rBV6	9605	16135	0.26%	0.028%
14	14.004	1833	1839	1841	rBV7	4158	7399	0.12%	0.013%
15	14.098	1848	1855	1889	rBV	1480722	3560785	57.34%	6.126%
16	14.375	1895	1902	1923	rBV2	2181377	4019444	64.72%	6.915%
17	14.681	1947	1954	1970	rBV	1593212	2722427	43.84%	4.684%
18	15.016	2002	2011	2032	rBV3	172104	954259	15.37%	1.642%
19	15.687	2118	2125	2146	rBV	2104885	4996657	80.46%	8.597%
20	15.875	2151	2157	2190	rVV	315357	1343170	21.63%	2.311%
21	17.122	2364	2369	2372	rBV7	7568	13882	0.22%	0.024%
22	17.234	2386	2388	2394	rVB6	4626	6709	0.11%	0.012%
23	17.445	2417	2424	2436	rBV	2088744	3247850	52.30%	5.588%
24	17.551	2436	2442	2479	rVB2	1856751	5351115	86.17%	9.206%
25	18.381	2580	2583	2586	rBV4	5874	10026	0.16%	0.017%
26	19.363	2746	2750	2755	rBV3	40411	63227	1.02%	0.109%
27	19.786	2815	2822	2852	rBV	2457871	6210116	100.00%	10.684%
28	21.563	3118	3124	3144	rBV	1176841	3227217	51.97%	5.552%
29	23.921	3518	3525	3547	rBV2	1340335	4067069	65.49%	6.997%
30	24.098	3549	3555	3578	rVB	641541	2335890	37.61%	4.019%




Sum of corrected areas: 58123588

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016062.D
Acq On : 07 Jul 2023 09:34
Operator : MA/JU
Sample : PB153518BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK518

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

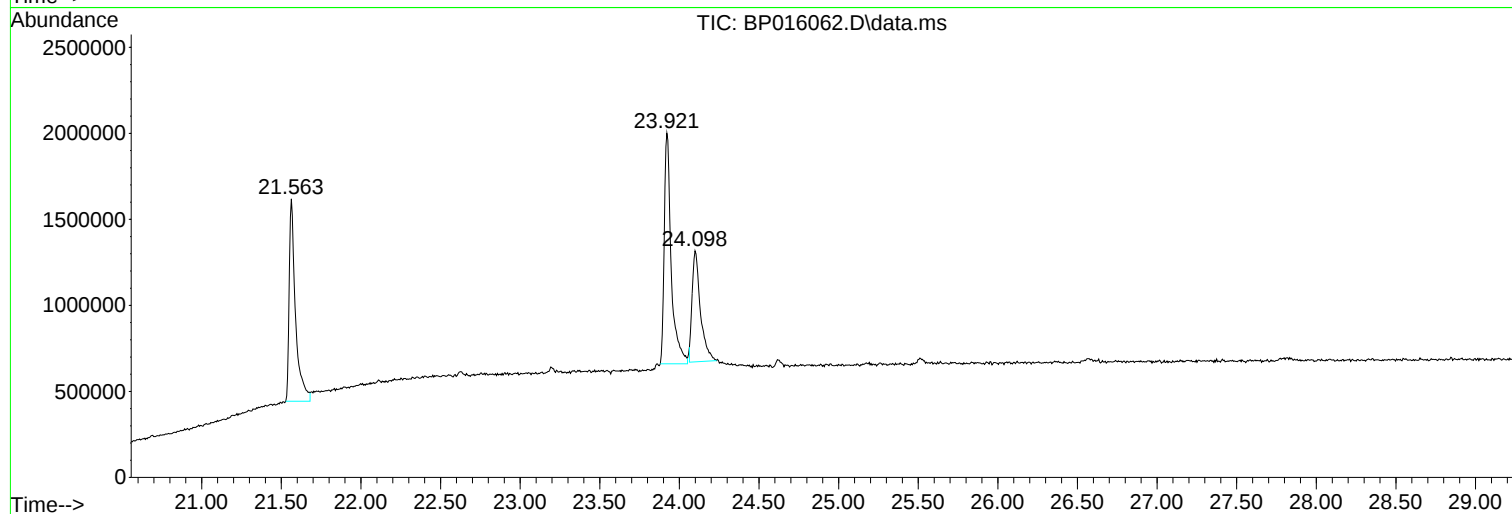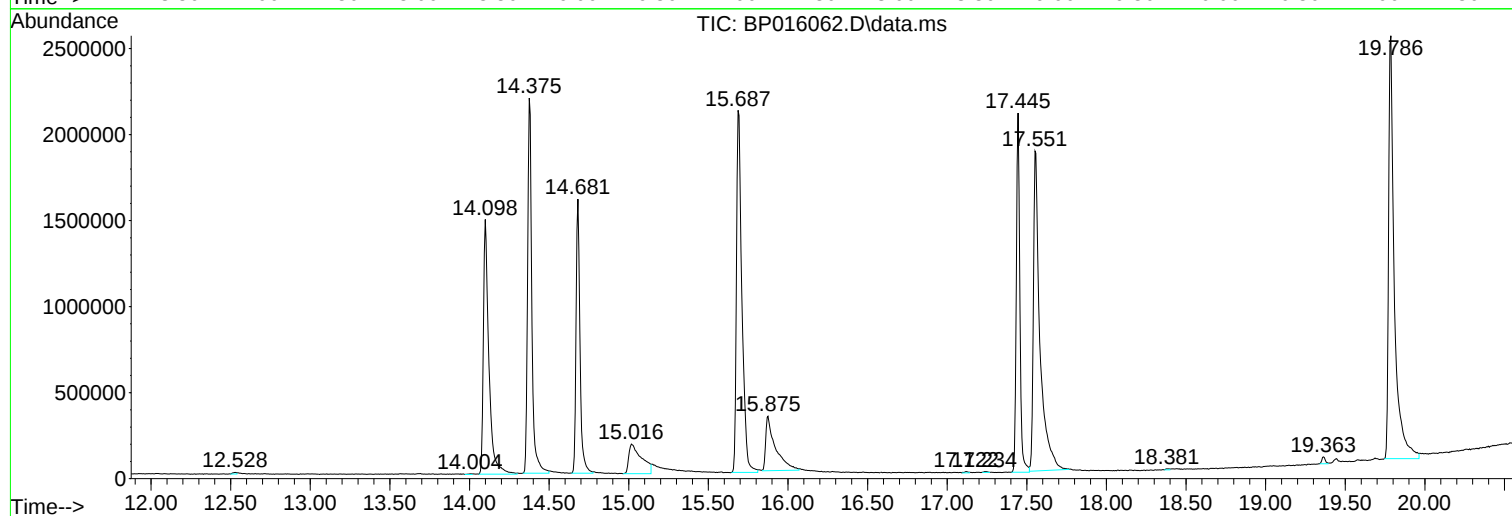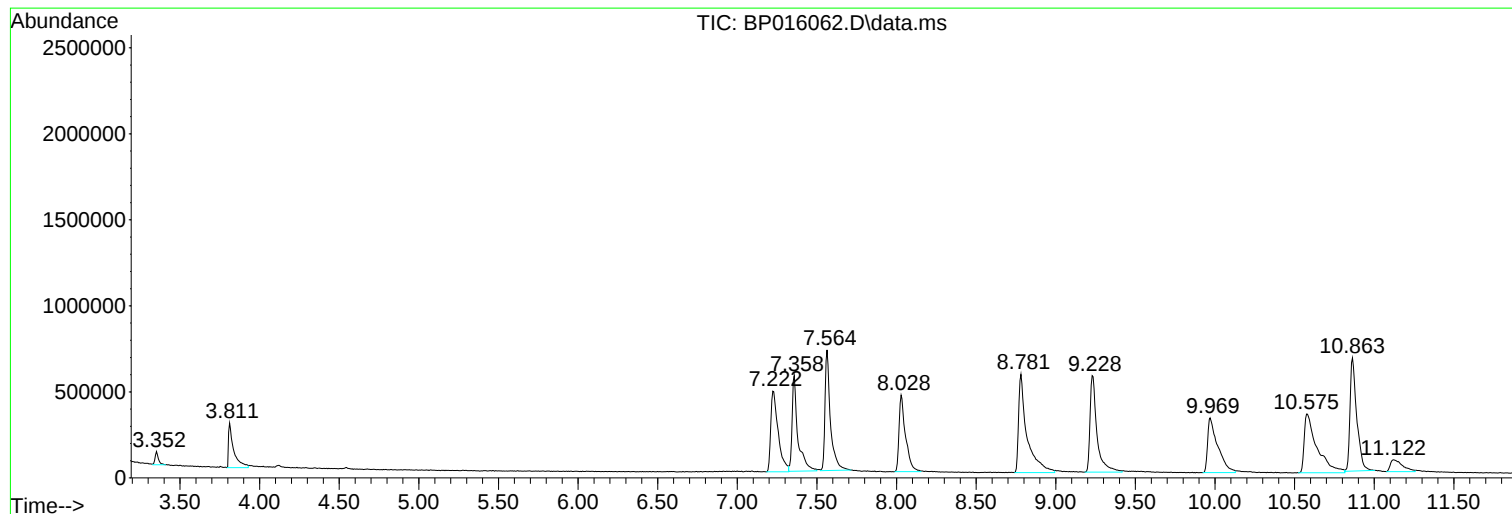

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016062.D
Acq On : 07 Jul 2023 09:34
Operator : MA/JU
Sample : PB153518BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK518

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016062.D
Acq On : 07 Jul 2023 09:34
Operator : MA/JU
Sample : PB153518BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK518

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc