

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016067.D
 Acq On : 07 Jul 2023 13:01
 Operator : MA/JU
 Sample : PB153590BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK590

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	38	rVB	82811	123890	1.49%	0.169%
2	3.799	102	104	133	rBV	717950	1463880	17.57%	2.001%
3	4.116	155	158	164	rVB3	13311	18229	0.22%	0.025%
4	7.222	679	686	703	rBV	528463	1714666	20.58%	2.344%
5	7.352	703	708	731	rVB	602747	1463043	17.56%	2.000%
6	7.563	737	744	773	rVB	790364	1887563	22.65%	2.580%
7	8.028	816	823	850	rBV	488888	1347883	16.18%	1.842%
8	8.781	941	951	988	rBV	702949	2403117	28.84%	3.285%
9	9.228	1019	1027	1054	rBV	690322	1901420	22.82%	2.599%
10	9.963	1144	1152	1185	rBV2	446870	1613198	19.36%	2.205%
11	10.546	1242	1251	1272	rBV	418749	1917620	23.01%	2.621%
12	10.857	1297	1304	1323	rVB	802032	1993219	23.92%	2.724%
13	11.051	1330	1337	1374	rBV	493569	2198776	26.39%	3.005%
14	12.522	1583	1587	1597	rBV6	9395	24281	0.29%	0.033%
15	14.028	1837	1843	1846	rBV8	4460	9481	0.11%	0.013%
16	14.098	1848	1855	1885	rVV	1682067	3989406	47.88%	5.453%
17	14.375	1895	1902	1931	rBV	2555357	4622060	55.47%	6.317%
18	14.681	1947	1954	1971	rBV	1654497	2844139	34.13%	3.887%
19	15.016	2004	2011	2037	rBV3	194186	1197064	14.37%	1.636%
20	15.686	2118	2125	2151	rBV	2422374	5795125	69.54%	7.921%
21	15.875	2151	2157	2195	rVV2	367821	1582764	18.99%	2.163%
22	17.239	2387	2389	2395	rVB7	7195	8570	0.10%	0.012%
23	17.445	2417	2424	2435	rBV	2298065	3586966	43.05%	4.903%
24	17.551	2435	2442	2476	rVB2	2408718	6478817	77.75%	8.855%
25	19.363	2746	2750	2754	rBV3	53751	76373	0.92%	0.104%
26	19.439	2760	2763	2770	rBV2	29807	47758	0.57%	0.065%
27	19.780	2815	2821	2856	rBV	3494023	8332942	100.00%	11.389%
28	21.557	3118	3123	3142	rBV2	1597220	4173607	50.09%	5.704%
29	23.915	3517	3524	3545	rBV2	2407291	6682113	80.19%	9.133%
30	24.092	3548	3554	3577	rVB	981826	3666520	44.00%	5.011%




Sum of corrected areas: 73164490

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016067.D
Acq On : 07 Jul 2023 13:01
Operator : MA/JU
Sample : PB153590BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

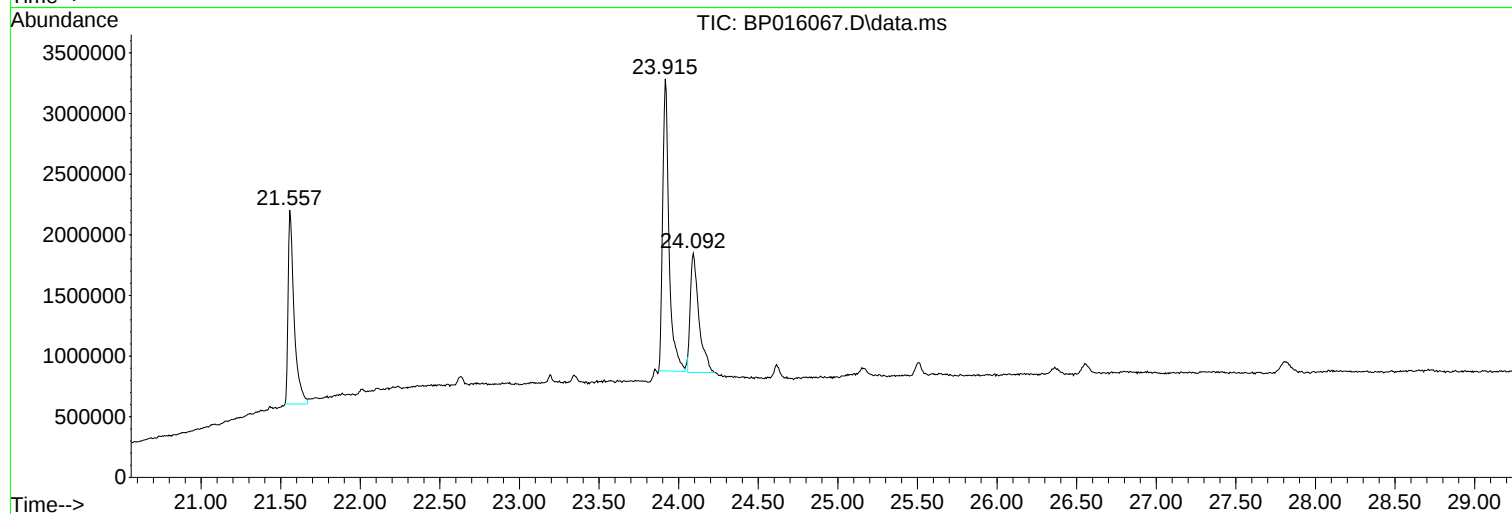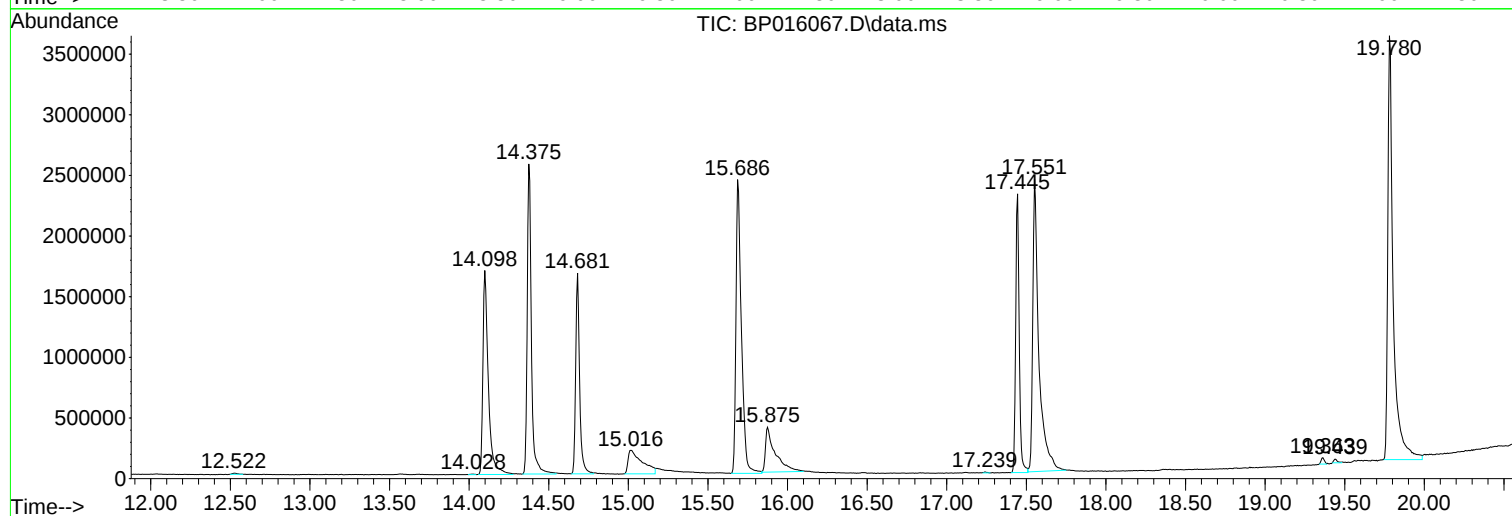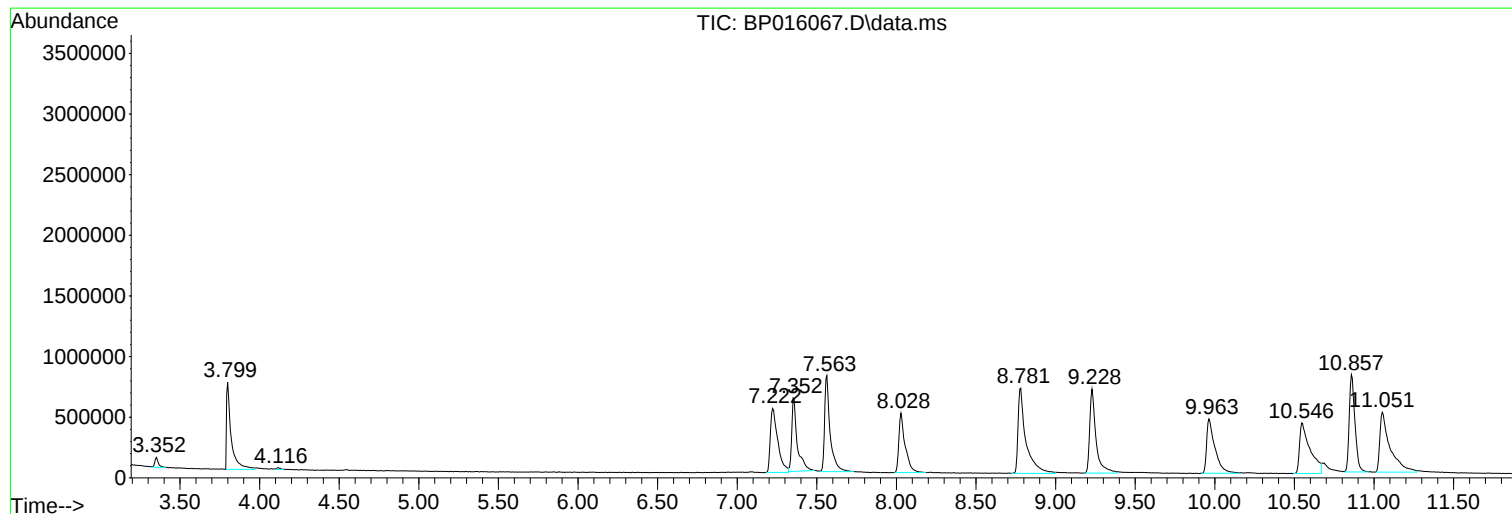

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016067.D
Acq On : 07 Jul 2023 13:01
Operator : MA/JU
Sample : PB153590BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016067.D
Acq On : 07 Jul 2023 13:01
Operator : MA/JU
Sample : PB153590BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK590

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------