

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016070.D
 Acq On : 07 Jul 2023 14:44
 Operator : MA/JU
 Sample : 03237-08
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBW78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	38	rVB	37350	59047	0.69%	0.088%
2	3.822	106	108	128	rBV	108917	302241	3.53%	0.450%
3	4.017	137	141	146	rVB4	15807	28817	0.34%	0.043%
4	4.117	154	158	166	rVB	60031	92859	1.08%	0.138%
5	6.111	492	497	506	rBV	10035	32761	0.38%	0.049%
6	7.246	682	690	703	rBV	196893	661041	7.71%	0.984%
7	7.358	703	709	736	rVV	606131	1592553	18.58%	2.371%
8	7.569	738	745	769	rVV	644379	1711014	19.96%	2.547%
9	8.028	817	823	843	rBV	442980	1259276	14.69%	1.875%
10	8.787	943	952	986	rBV2	447618	1587213	18.52%	2.363%
11	9.228	1020	1027	1051	rBV	707458	1985240	23.16%	2.955%
12	9.981	1147	1155	1181	rBV	321191	1150024	13.42%	1.712%
13	10.534	1241	1249	1284	rBV	510481	2445901	28.54%	3.641%
14	10.857	1296	1304	1322	rBV	907860	1941662	22.65%	2.890%
15	11.046	1327	1336	1368	rBV	495829	2187367	25.52%	3.256%
16	12.275	1539	1545	1550	rBV6	15084	39877	0.47%	0.059%
17	12.516	1577	1586	1591	rBV8	8888	24121	0.28%	0.036%
18	12.987	1661	1666	1668	rBV6	7321	9370	0.11%	0.014%
19	13.287	1710	1717	1724	rVB5	11691	21078	0.25%	0.031%
20	13.557	1758	1763	1768	rBV8	8537	15031	0.18%	0.022%
21	14.093	1844	1854	1885	rBV	2059842	4365507	50.93%	6.499%
22	14.375	1895	1902	1929	rBV	2870960	4874347	56.87%	7.256%
23	14.675	1945	1953	1974	rVB	1674440	2950298	34.42%	4.392%
24	15.245	2042	2050	2054	rBV	6905	18705	0.22%	0.028%
25	15.687	2117	2125	2155	rBV	2499979	6316140	73.69%	9.402%
26	15.945	2165	2169	2176	rVB10	9294	20938	0.24%	0.031%
27	16.192	2207	2211	2218	rBV8	5548	10371	0.12%	0.015%
28	16.322	2228	2233	2237	rBV8	4784	9168	0.11%	0.014%
29	17.016	2348	2351	2358	rBV7	9008	14445	0.17%	0.022%
30	17.128	2366	2370	2374	rBV7	7273	11611	0.14%	0.017%
31	17.445	2418	2424	2436	rBV	2054630	3229939	37.69%	4.808%
32	17.557	2436	2443	2470	rVB2	2611103	7093724	82.77%	10.560%
33	18.081	2528	2532	2540	rBV3	67651	96916	1.13%	0.144%
34	18.339	2573	2576	2578	rBV4	12729	15295	0.18%	0.023%
35	18.875	2664	2667	2674	rVB8	12250	18485	0.22%	0.028%
36	19.151	2711	2714	2720	rVB2	37218	47824	0.56%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016070.D
Acq On : 07 Jul 2023 14:44
Operator : MA/JU
Sample : 03237-08
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW78

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	19.357	2745	2749	2756	rBV3	60605	87984	1.03%	0.131%
38	19.433	2759	2762	2766	rBV	29573	43141	0.50%	0.064%
39	19.780	2814	2821	2853	rBV	3831422	8570804	100.00%	12.759%
40	21.557	3118	3123	3138	rBV2	1342214	3272476	38.18%	4.871%
41	23.916	3516	3524	3544	rBV2	2219660	6218733	72.56%	9.257%
42	24.086	3547	3553	3574	rVB	769251	2743229	32.01%	4.084%




Sum of corrected areas: 67176573

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016070.D
Acq On : 07 Jul 2023 14:44
Operator : MA/JU
Sample : 03237-08
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

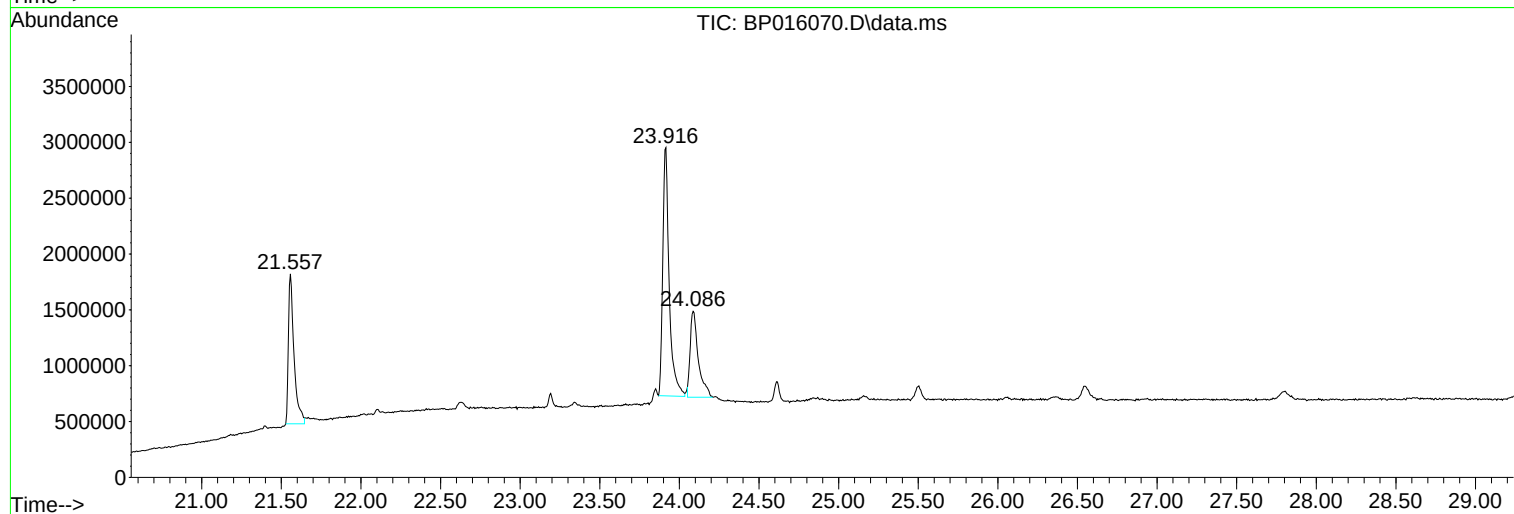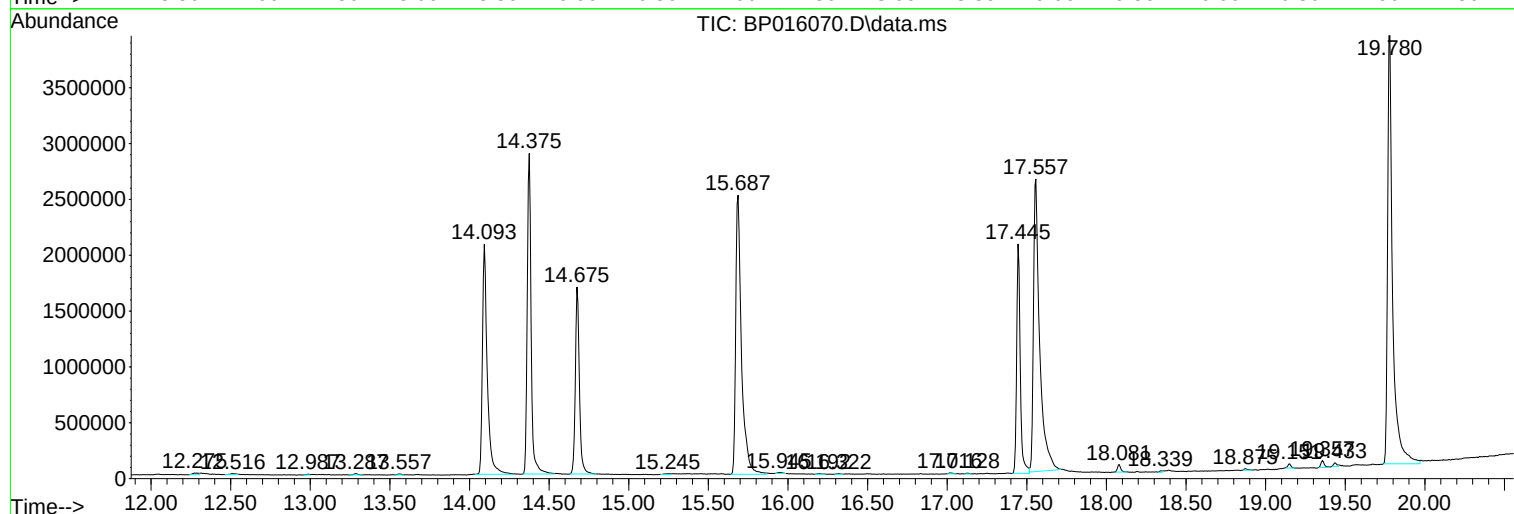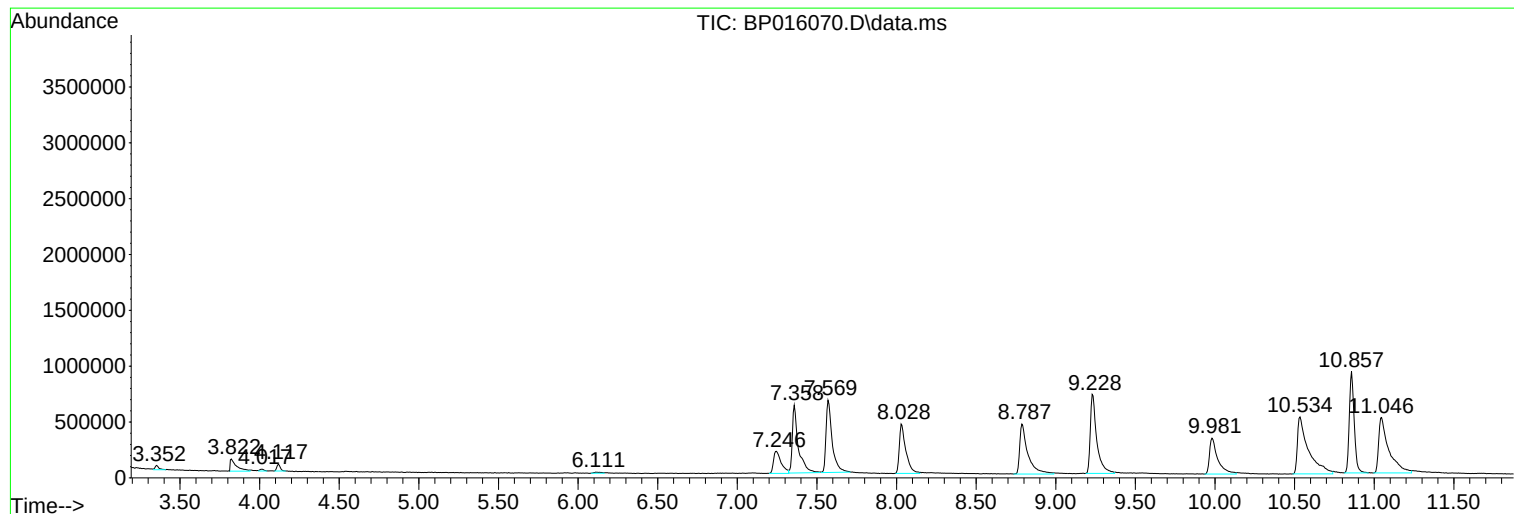

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016070.D
Acq On : 07 Jul 2023 14:44
Operator : MA/JU
Sample : 03237-08
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016070.D
Acq On : 07 Jul 2023 14:44
Operator : MA/JU
Sample : 03237-08
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
