

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016072.D
 Acq On : 07 Jul 2023 15:52
 Operator : MA/JU
 Sample : 03283-11
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	34	rVB	55908	77544	1.11%	0.132%
2	3.817	106	107	126	rBV	115158	284150	4.05%	0.483%
3	4.011	138	140	144	rVB3	16723	18797	0.27%	0.032%
4	4.117	155	158	165	rVB2	16186	22350	0.32%	0.038%
5	4.658	245	250	259	rVB	57761	100633	1.44%	0.171%
6	7.269	686	694	704	rBV	80953	254063	3.62%	0.432%
7	7.363	704	710	732	rVB	399546	1172829	16.73%	1.993%
8	7.587	741	748	772	rVB	389371	1136081	16.20%	1.931%
9	8.034	817	824	848	rBV	443658	1331343	18.99%	2.263%
10	8.799	947	954	987	rBV	231327	991522	14.14%	1.685%
11	9.234	1020	1028	1057	rBV	578036	1606182	22.91%	2.730%
12	9.969	1145	1153	1179	rBV	333856	1310671	18.69%	2.227%
13	10.557	1243	1253	1271	rBV	315168	1406655	20.06%	2.391%
14	10.857	1296	1304	1328	rVB	829542	2081368	29.69%	3.537%
15	11.057	1330	1338	1374	rBV	365656	1705618	24.33%	2.899%
16	12.516	1578	1586	1594	rBV7	10754	29737	0.42%	0.051%
17	13.345	1722	1727	1730	rBV5	6402	9669	0.14%	0.016%
18	13.563	1759	1764	1773	rBV6	11361	26272	0.37%	0.045%
19	14.098	1847	1855	1884	rBV	1546873	3622978	51.67%	6.157%
20	14.375	1895	1902	1924	rBV	2321340	3987086	56.87%	6.776%
21	14.681	1947	1954	1971	rBV	1710320	2949642	42.07%	5.013%
22	15.140	2027	2032	2033	rBV5	16686	23275	0.33%	0.040%
23	15.451	2081	2085	2093	rVB3	13177	28367	0.40%	0.048%
24	15.687	2118	2125	2144	rBV	2137552	5171246	73.76%	8.789%
25	15.881	2151	2158	2185	rBV2	361503	1505201	21.47%	2.558%
26	16.075	2187	2191	2198	rVB	44034	86783	1.24%	0.147%
27	17.116	2366	2368	2375	rVB8	7178	11730	0.17%	0.020%
28	17.445	2417	2424	2435	rBV	2211623	3518839	50.19%	5.980%
29	17.551	2436	2442	2470	rVB2	2238371	5827488	83.12%	9.904%
30	18.310	2566	2571	2581	rBV4	85082	217507	3.10%	0.370%
31	19.357	2745	2749	2753	rBV2	48962	65126	0.93%	0.111%
32	19.433	2759	2762	2770	rBV	35622	61531	0.88%	0.105%
33	19.533	2776	2779	2786	rBV4	48171	98627	1.41%	0.168%
34	19.780	2815	2821	2850	rBV	3137546	7011155	100.00%	11.915%
35	21.557	3117	3123	3143	rBV	1454797	3743340	53.39%	6.362%
36	23.916	3517	3524	3542	rBV2	1709462	4622751	65.93%	7.856%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016072.D
Acq On : 07 Jul 2023 15:52
Operator : MA/JU
Sample : 03283-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	24.092	3548	3554	3575	rVB	791906	2722806	38.84%	4.627%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 58840962

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016072.D
Acq On : 07 Jul 2023 15:52
Operator : MA/JU
Sample : 03283-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

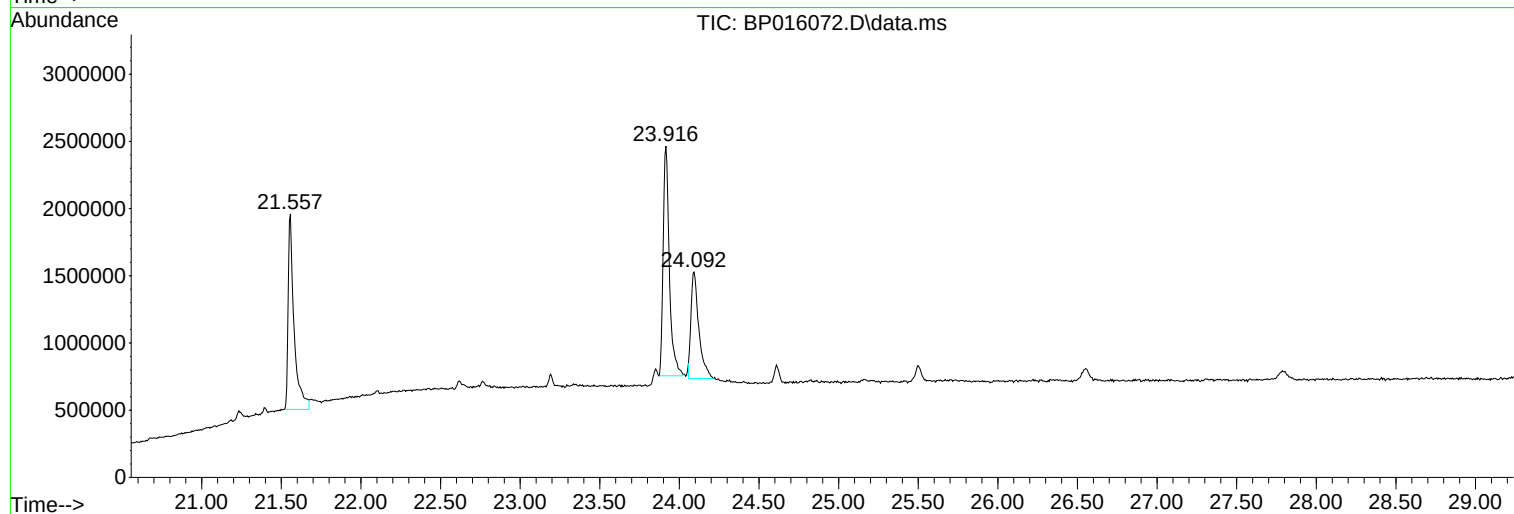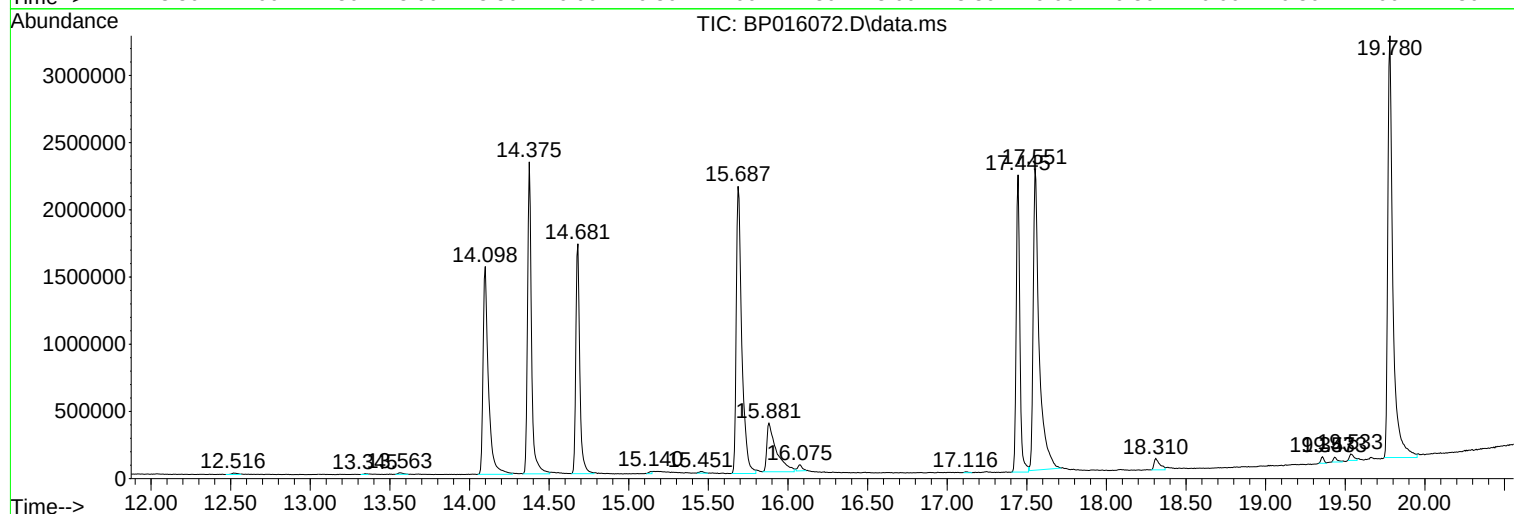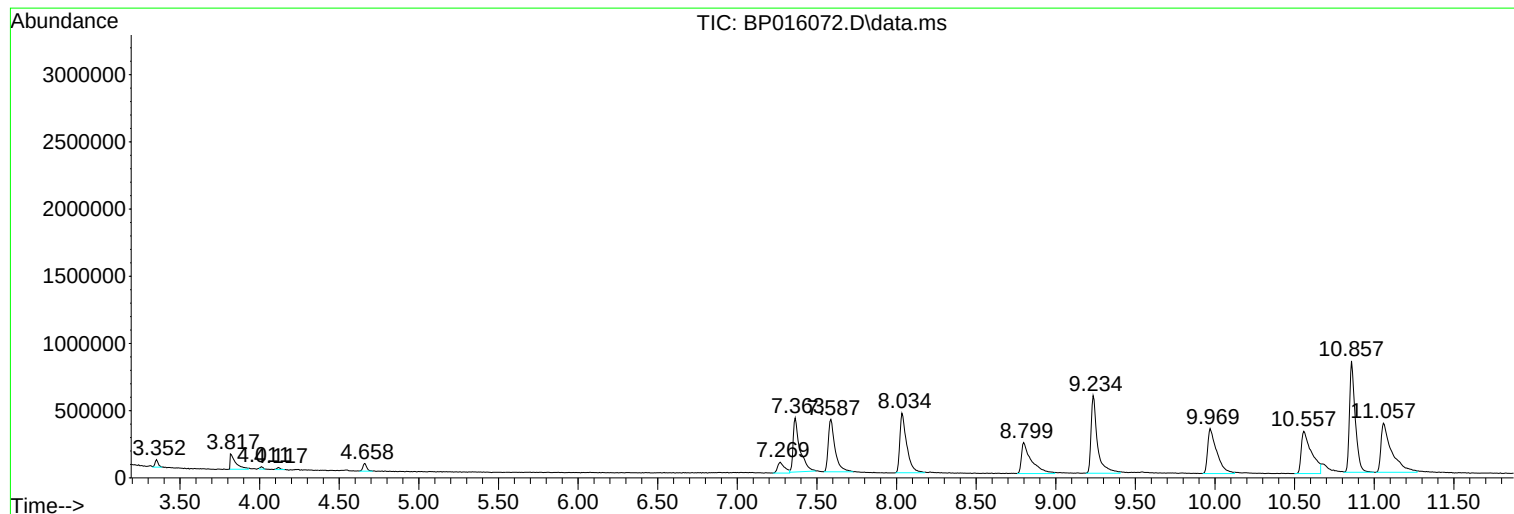

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016072.D
Acq On : 07 Jul 2023 15:52
Operator : MA/JU
Sample : 03283-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016072.D
Acq On : 07 Jul 2023 15:52
Operator : MA/JU
Sample : 03283-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------