

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016073.D
 Acq On : 07 Jul 2023 16:26
 Operator : MA/JU
 Sample : 03283-10
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	39	rVB	49753	83398	1.36%	0.164%
2	3.817	105	107	127	rBV	133715	327248	5.33%	0.642%
3	4.117	155	158	167	rVB5	13969	27145	0.44%	0.053%
4	4.540	229	230	236	rVB5	9954	10269	0.17%	0.020%
5	4.658	247	250	259	rVB6	18671	35417	0.58%	0.070%
6	7.281	688	696	705	rBV2	60164	194375	3.16%	0.382%
7	7.369	705	711	742	rVB	292728	1021343	16.62%	2.005%
8	7.593	742	749	770	rBV	293580	929963	15.14%	1.825%
9	8.040	815	825	848	rBV	326622	1118697	18.21%	2.196%
10	8.811	948	956	984	rBV2	161921	792681	12.90%	1.556%
11	9.246	1023	1030	1054	rBV	432413	1263442	20.57%	2.480%
12	9.981	1147	1155	1181	rBV2	236055	1052473	17.13%	2.066%
13	10.575	1248	1256	1274	rBV	231579	1108532	18.04%	2.176%
14	10.863	1297	1305	1326	rVB	596457	1641909	26.73%	3.223%
15	11.063	1331	1339	1379	rBV	291383	1468223	23.90%	2.882%
16	12.534	1585	1589	1595	rBV8	6511	16248	0.26%	0.032%
17	12.957	1656	1661	1665	rBV8	3276	6548	0.11%	0.013%
18	13.363	1722	1730	1732	rBV9	5047	8647	0.14%	0.017%
19	13.569	1760	1765	1770	rBV7	5088	11904	0.19%	0.023%
20	14.104	1848	1856	1883	rBV	1099181	2849931	46.39%	5.594%
21	14.381	1896	1903	1924	rBV2	1668182	3198687	52.07%	6.279%
22	14.681	1947	1954	1977	rBV	1259563	2280981	37.13%	4.477%
23	15.163	2031	2036	2037	rBV5	11470	15427	0.25%	0.030%
24	15.463	2082	2087	2096	rVB5	17187	37360	0.61%	0.073%
25	15.693	2118	2126	2154	rBV	1662254	4211867	68.56%	8.268%
26	15.892	2154	2160	2187	rVV2	247517	1121165	18.25%	2.201%
27	16.075	2187	2191	2199	rVB	94580	166622	2.71%	0.327%
28	16.292	2224	2228	2231	rVB6	4237	6426	0.10%	0.013%
29	16.834	2314	2320	2323	rBV8	5159	8933	0.15%	0.018%
30	17.445	2418	2424	2436	rBV	1709802	2806088	45.68%	5.508%
31	17.557	2436	2443	2472	rVB2	1702978	4753869	77.38%	9.332%
32	18.086	2529	2533	2543	rBV2	9860	24863	0.40%	0.049%
33	18.316	2568	2572	2581	rBV6	40152	109356	1.78%	0.215%
34	19.357	2746	2749	2757	rVB2	37076	47949	0.78%	0.094%
35	19.439	2759	2763	2766	rBV2	27620	43176	0.70%	0.085%
36	19.539	2777	2780	2787	rBV9	24126	51374	0.84%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016073.D
Acq On : 07 Jul 2023 16:26
Operator : MA/JU
Sample : 03283-10
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	19.781	2815	2821	2848	rBV	2650581	6143478	100.00%	12.059%
38	21.551	3117	3122	3141	rBV2	1327058	3469381	56.47%	6.810%
39	23.910	3516	3523	3544	rBV2	2014725	5333114	86.81%	10.469%
40	24.086	3547	3553	3579	rVB2	893235	3145115	51.19%	6.174%




Sum of corrected areas: 50943624

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016073.D
Acq On : 07 Jul 2023 16:26
Operator : MA/JU
Sample : 03283-10
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

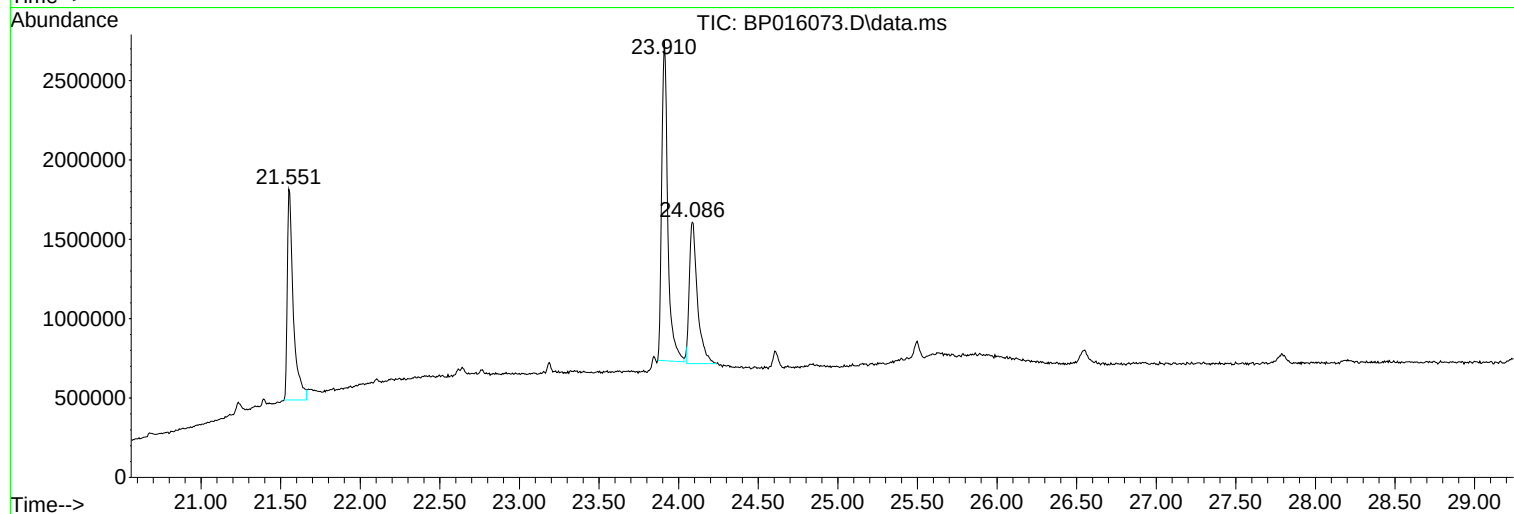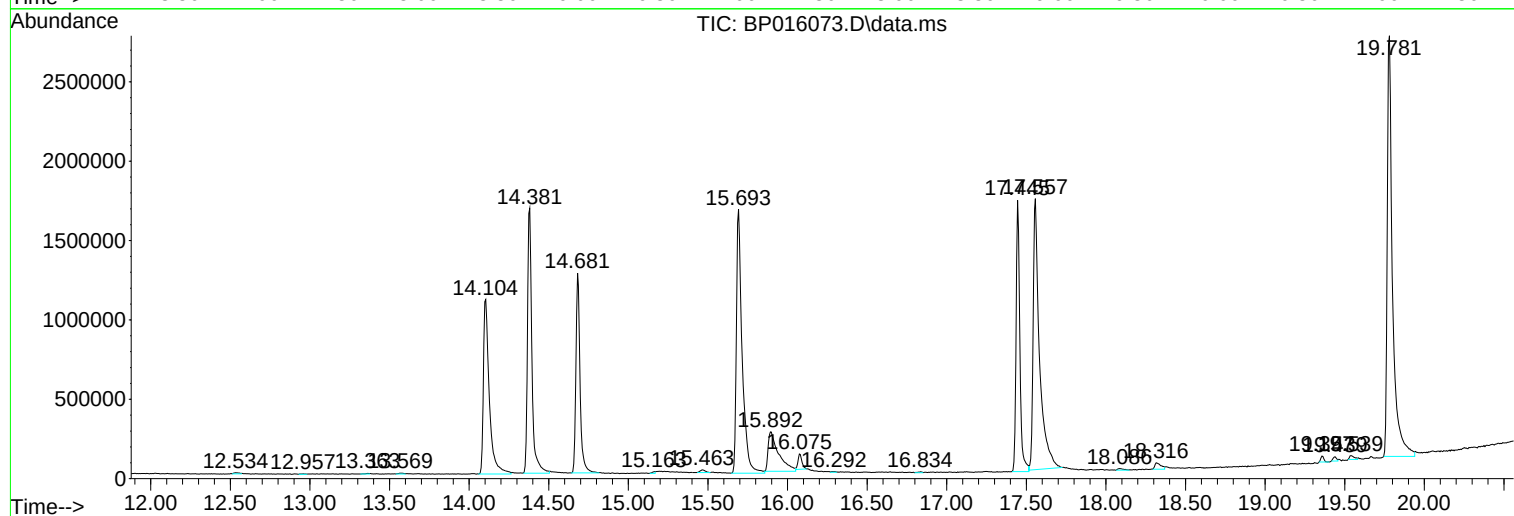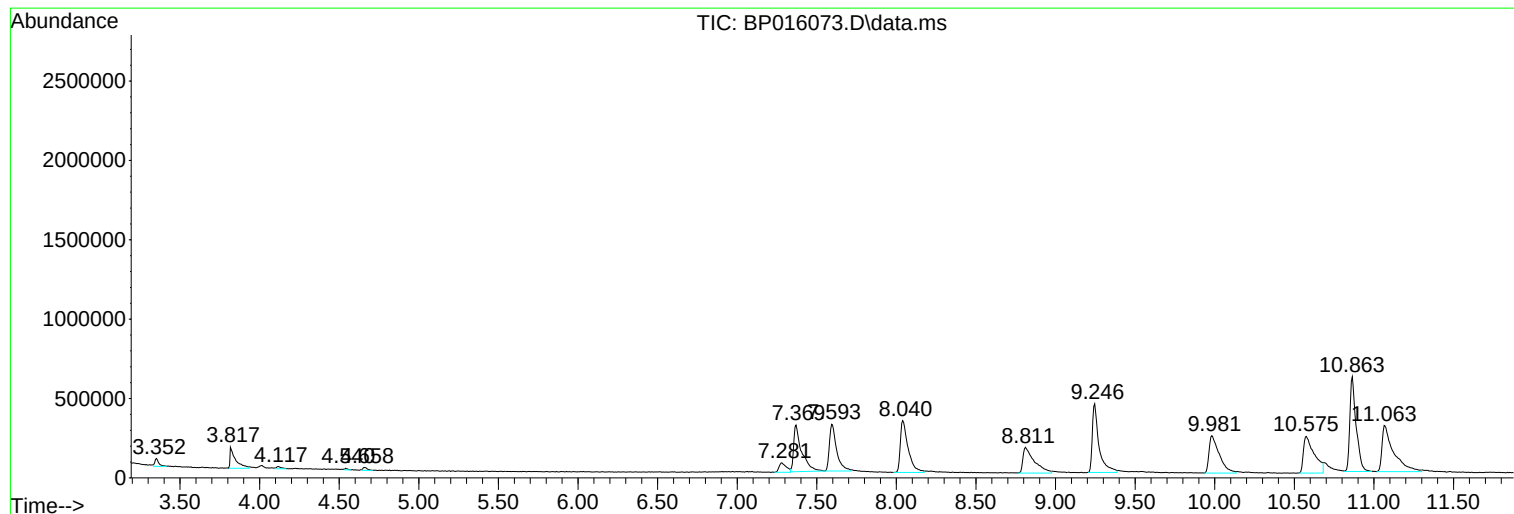

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016073.D
Acq On : 07 Jul 2023 16:26
Operator : MA/JU
Sample : 03283-10
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016073.D
Acq On : 07 Jul 2023 16:26
Operator : MA/JU
Sample : 03283-10
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc