

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016076.D
 Acq On : 07 Jul 2023 18:09
 Operator : MA/JU
 Sample : 03283-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	45	rVB2	35693	78410	1.20%	0.147%
2	3.816	105	107	125	rBV	128916	311139	4.76%	0.583%
3	4.011	136	140	147	rVB	29289	52180	0.80%	0.098%
4	4.116	155	158	164	rVB2	12131	18996	0.29%	0.036%
5	5.116	325	328	332	rBV4	8362	13202	0.20%	0.025%
6	7.281	688	696	704	rBV3	58180	183845	2.81%	0.344%
7	7.363	704	710	740	rVB	393842	1220475	18.66%	2.285%
8	7.593	742	749	764	rBV	315133	949414	14.52%	1.778%
9	8.040	817	825	851	rBV	392661	1268177	19.39%	2.374%
10	8.810	949	956	972	rBV2	166939	719847	11.01%	1.348%
11	8.928	973	976	997	rVB4	51336	156027	2.39%	0.292%
12	9.175	1011	1018	1023	rBV5	13995	33325	0.51%	0.062%
13	9.240	1023	1029	1060	rVV	510170	1539334	23.53%	2.882%
14	9.998	1148	1158	1177	rBV	140785	576307	8.81%	1.079%
15	10.116	1177	1178	1184	rVB6	6596	8405	0.13%	0.016%
16	10.569	1247	1255	1272	rBV	253833	1140661	17.44%	2.136%
17	10.857	1297	1304	1320	rBV	737336	1899461	29.04%	3.556%
18	11.063	1331	1339	1368	rBV	307762	1383711	21.16%	2.591%
19	11.663	1435	1441	1442	rBV4	7641	10763	0.16%	0.020%
20	12.516	1580	1586	1594	rBV6	10146	24766	0.38%	0.046%
21	12.704	1611	1618	1625	rBV	16111	38742	0.59%	0.073%
22	13.281	1710	1716	1722	rBV7	11102	23630	0.36%	0.044%
23	13.345	1722	1727	1733	rVB10	5340	13092	0.20%	0.025%
24	13.557	1756	1763	1776	rBV4	26538	77413	1.18%	0.145%
25	13.922	1818	1825	1827	rBV8	4853	9094	0.14%	0.017%
26	14.098	1845	1855	1880	rBV	1488581	3507567	53.63%	6.567%
27	14.375	1895	1902	1928	rBV	2243161	3960811	60.56%	7.416%
28	14.681	1947	1954	1964	rBV	1594982	2798656	42.79%	5.240%
29	15.451	2080	2085	2094	rVB	21706	39086	0.60%	0.073%
30	15.533	2095	2099	2103	rVB4	9194	13605	0.21%	0.025%
31	15.686	2118	2125	2155	rBV	1898629	5100543	77.98%	9.550%
32	15.957	2166	2171	2179	rVB10	12385	23793	0.36%	0.045%
33	16.098	2193	2195	2201	rVB7	6626	11659	0.18%	0.022%
34	17.022	2349	2352	2356	rBV5	6695	9300	0.14%	0.017%
35	17.257	2388	2392	2396	rVB5	6276	9286	0.14%	0.017%
36	17.380	2409	2413	2417	rBV5	9133	14455	0.22%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
 Data File : BP016076.D
 Acq On : 07 Jul 2023 18:09
 Operator : MA/JU
 Sample : 03283-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXYY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	17.451	2418	2425	2437	rBV	1882636	3267736	49.96%	6.118%
38	17.557	2437	2443	2468	rVB2	1865919	5240688	80.12%	9.812%
39	18.074	2526	2531	2543	rBV	633456	821752	12.56%	1.539%
40	18.327	2570	2574	2578	rBV6	18814	34042	0.52%	0.064%
41	18.386	2581	2584	2591	rVB	22663	38493	0.59%	0.072%
42	19.357	2745	2749	2757	rBV2	49743	75073	1.15%	0.141%
43	19.433	2760	2762	2769	rVV2	25970	43149	0.66%	0.081%
44	19.780	2815	2821	2848	rBV2	2990908	6540652	100.00%	12.246%
45	21.557	3117	3123	3133	rBV	1369101	3246964	49.64%	6.079%
46	23.909	3517	3523	3540	rBV2	1640037	4389912	67.12%	8.219%
47	24.086	3547	3553	3570	rVB	762677	2473211	37.81%	4.631%

Sum of corrected areas: 53410849

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016076.D
Acq On : 07 Jul 2023 18:09
Operator : MA/JU
Sample : 03283-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 7,9-Di-tert-butyl-1-oxaspiro... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.075	5.03 ng/ul	821752	Phenanthrene-d10	17.451

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	98		
2	7,9-Di-tert-butyl-1-oxaspiro(4,5...	276	C17H24O3	082304-66-3	93		
3	Ethanone, 1-(5,6,7,8-tetrahydro-...	220	C14H20O2	071596-88-8	50		
4	1-(3-Amino-4,6-dimethylthieno[2,...	220	C11H12N2OS	052505-42-7	45		
5	(1R,3aR,5aR,9aS)-1,4,4,7-Tetrame...	220	C15H24O	104188-25-2	43		

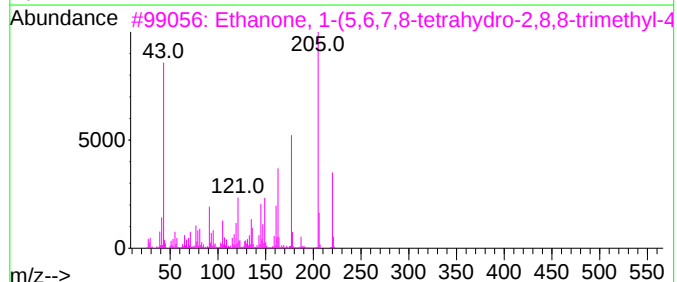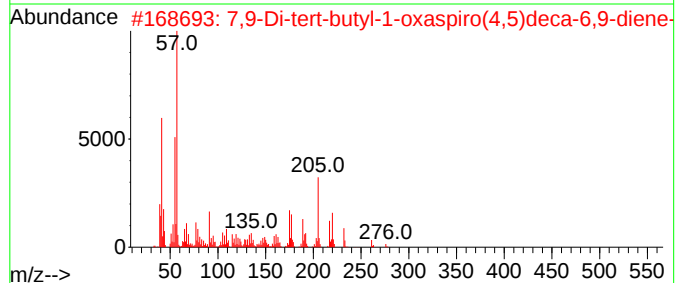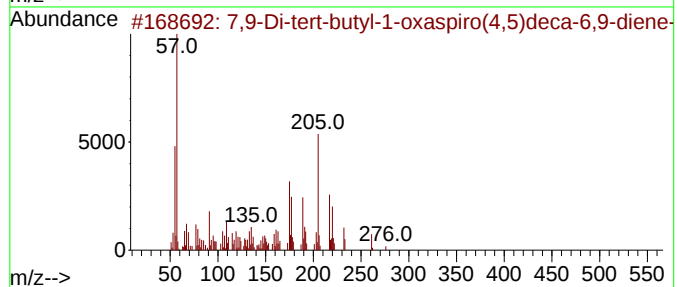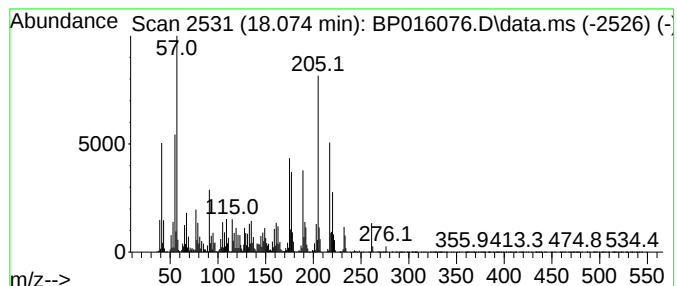

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070623\
Data File : BP016076.D
Acq On : 07 Jul 2023 18:09
Operator : MA/JU
Sample : 03283-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXYY8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
7,9-Di-tert-but...	18.075	5.0	ng/u1	821752	4	17.451	3267740	20.0