

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070820\
Data File : BP002682.D
Acq On : 08 Jul 2020 19:09
Operator : CG/JU
Sample : L3203-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-16

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	386	394	404	rBV	26087	58051	2.85%	1.372%
2	6.781	655	662	673	rBV	29141	72249	3.55%	1.708%
3	7.887	842	850	858	rBV	27141	52321	2.57%	1.237%
4	8.722	983	992	1000	rBV	13682	33147	1.63%	0.784%
5	10.346	1262	1268	1274	rBV	13881	27065	1.33%	0.640%
6	12.834	1685	1691	1705	rBV	47305	94549	4.64%	2.235%
7	14.216	1920	1926	1935	rBV	31093	53423	2.62%	1.263%
8	15.722	2176	2182	2199	rBV	101861	203789	10.00%	4.817%
9	16.981	2391	2396	2402	rBV	63315	101926	5.00%	2.409%
10	17.116	2414	2419	2427	rBV	16184	29125	1.43%	0.688%
11	19.004	2736	2740	2748	rBV	27524	41695	2.05%	0.986%
12	19.357	2797	2800	2804	rBV	23031	26024	1.28%	0.615%
13	19.563	2830	2835	2846	rBV	484657	586202	28.78%	13.857%
14	21.086	3088	3094	3098	rBV	575936	813787	39.95%	19.237%
15	23.280	3461	3467	3481	rVB2	1092219	2037056	100.00%	48.153%


Sum of corrected areas: 4230409

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP070820\
Data File : BP002682.D
Acq On : 08 Jul 2020 19:09
Operator : CG/JU
Sample : L3203-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

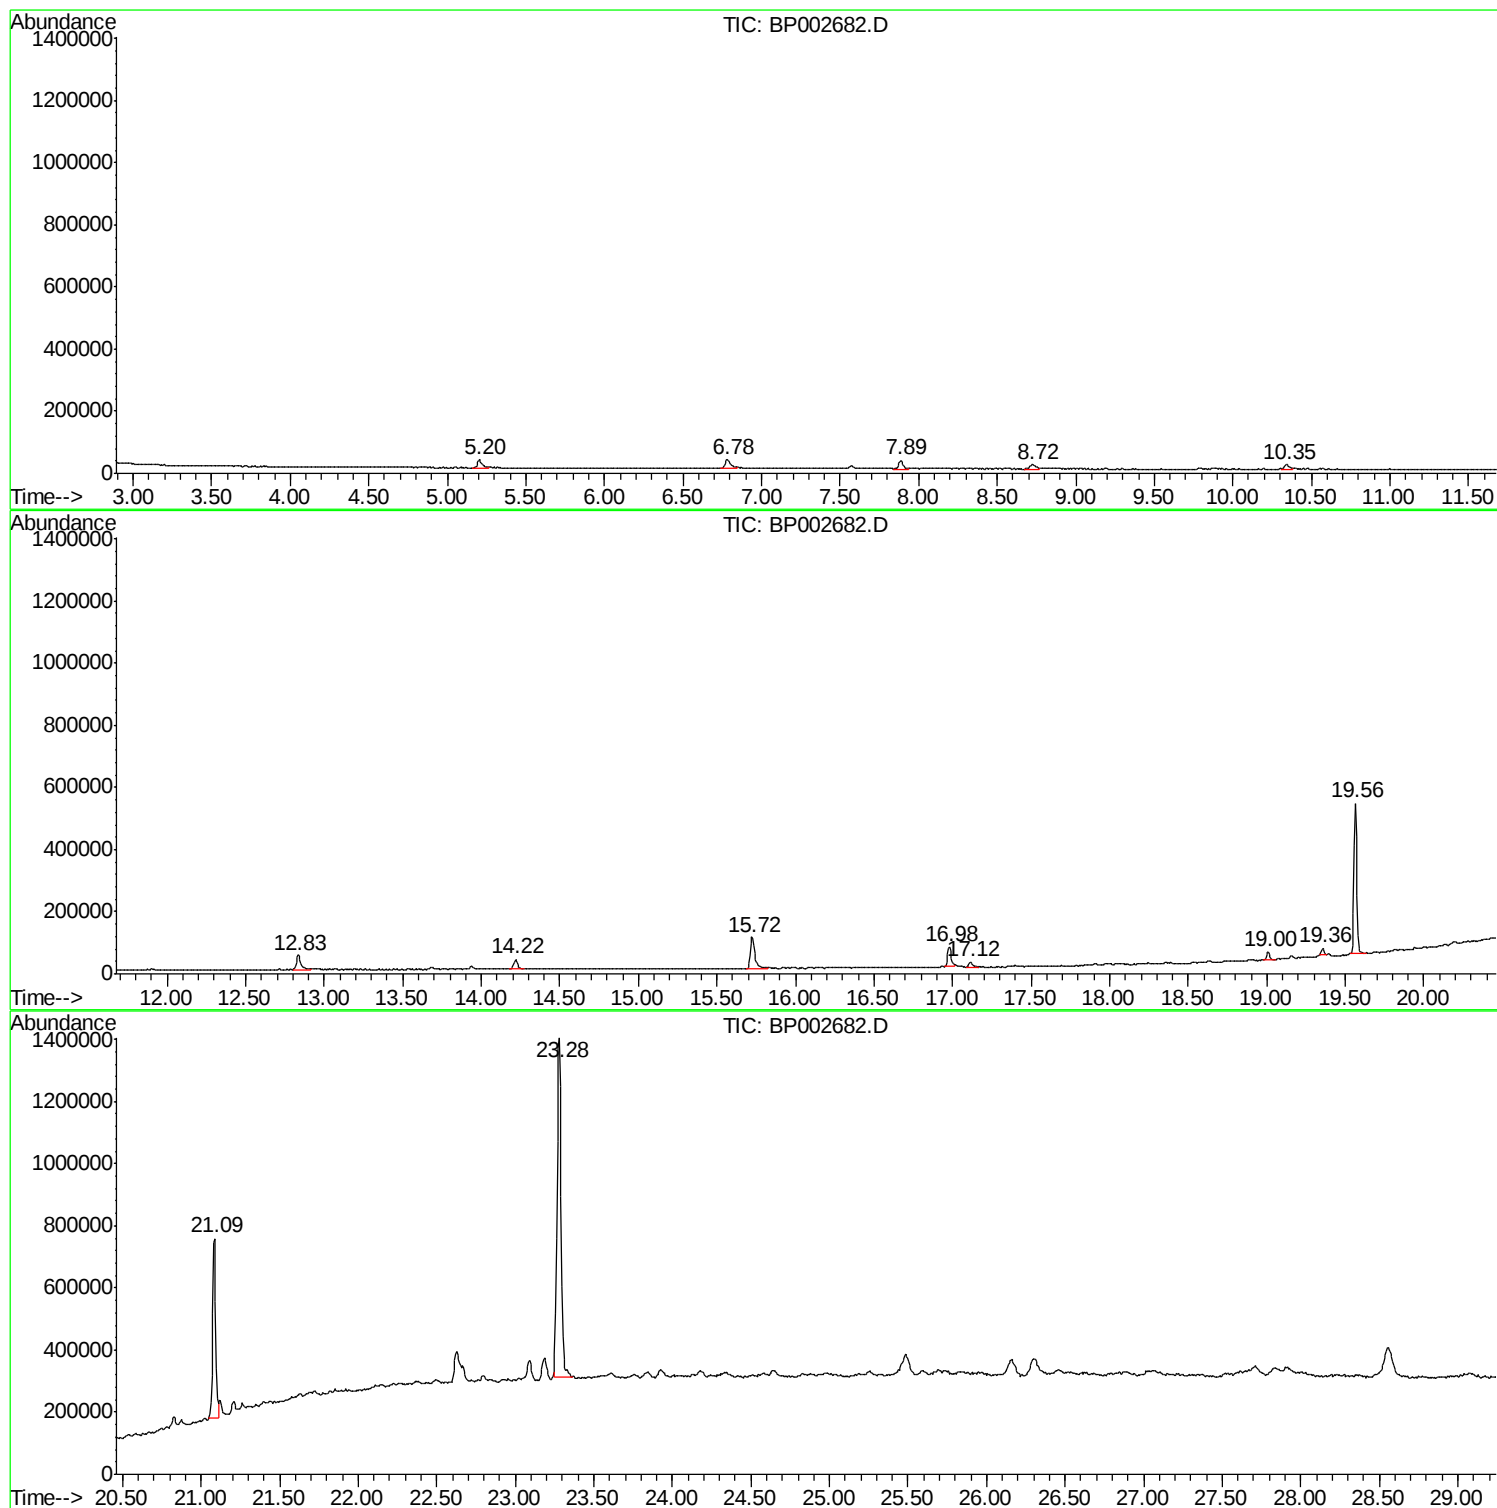

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070820\
Data File : BP002682.D
Acq On : 08 Jul 2020 19:09
Operator : CG/JU
Sample : L3203-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070820\
Data File : BP002682.D
Acq On : 08 Jul 2020 19:09
Operator : CG/JU
Sample : L3203-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RO-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc