


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP070820\
 Data File : BP002667.D
 Acq On : 08 Jul 2020 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP062920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 16:51:57 2020

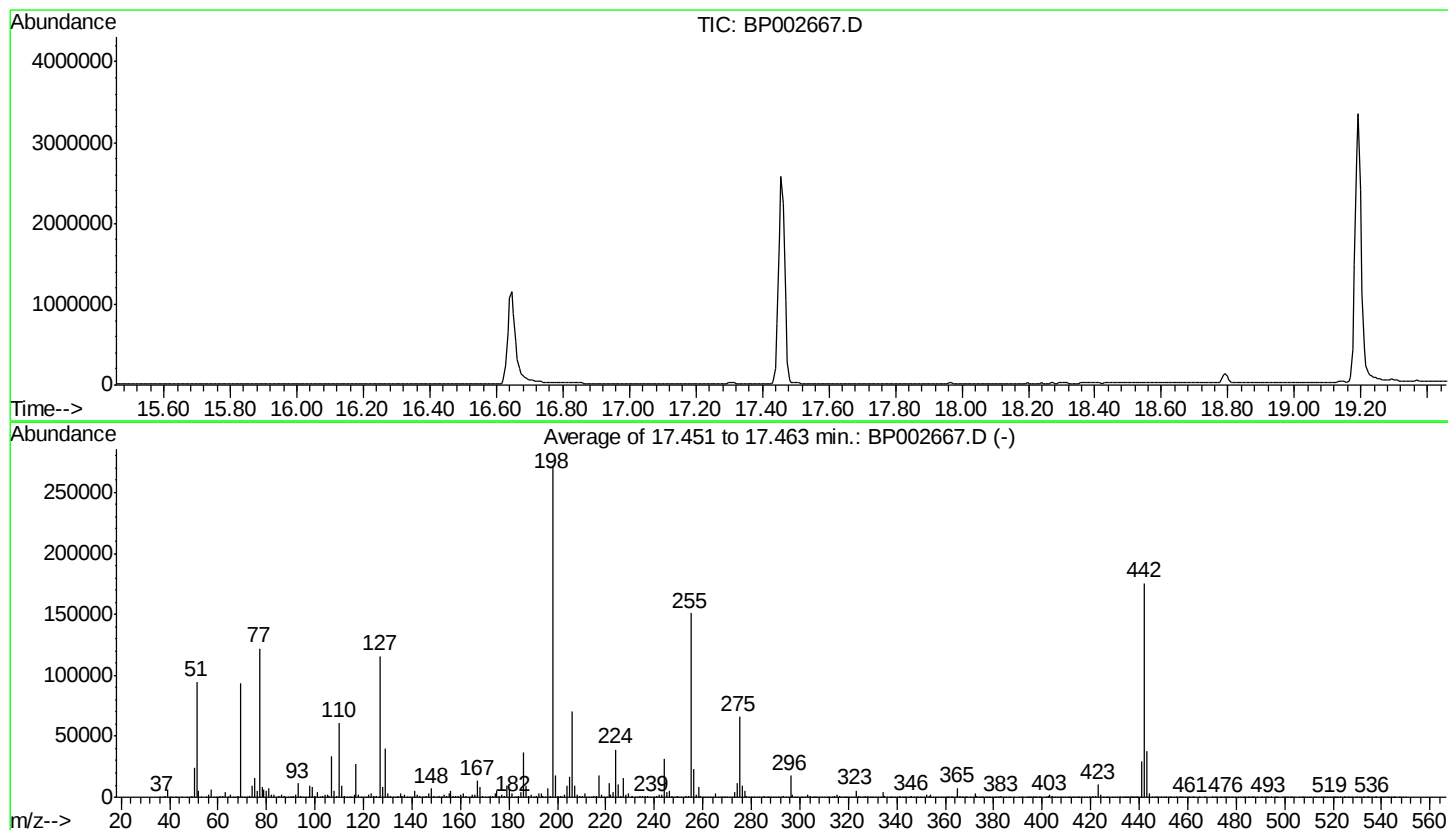

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	95017	PASS
68	69	0.00	2	1.6	1508	PASS
69	198	0.00	100	34.2	93067	PASS
70	69	0.00	2	0.5	487	PASS
127	198	10	80	42.7	116008	PASS
197	198	0.00	2	0.3	756	PASS
198	198	100	100	100.0	271995	PASS
199	198	5	9	6.8	18381	PASS
275	198	10	60	24.2	65932	PASS
365	198	1	100	2.8	7658	PASS
441	198	0.01	100	10.8	29304	PASS
442	198	50	100	64.6	175600	PASS
443	442	15	24	21.5	37730	PASS