




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 22:16:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

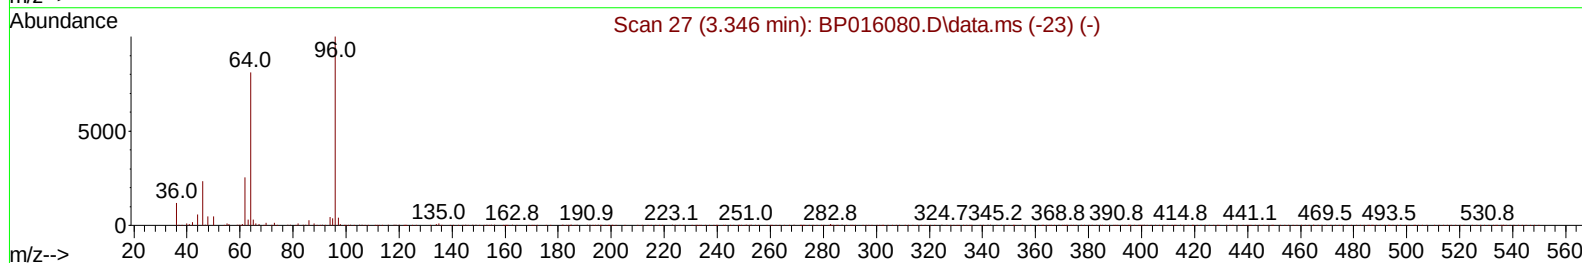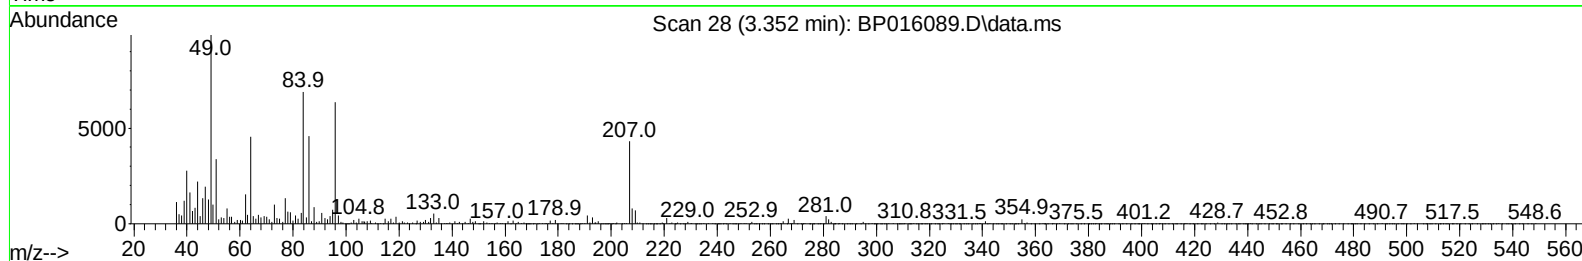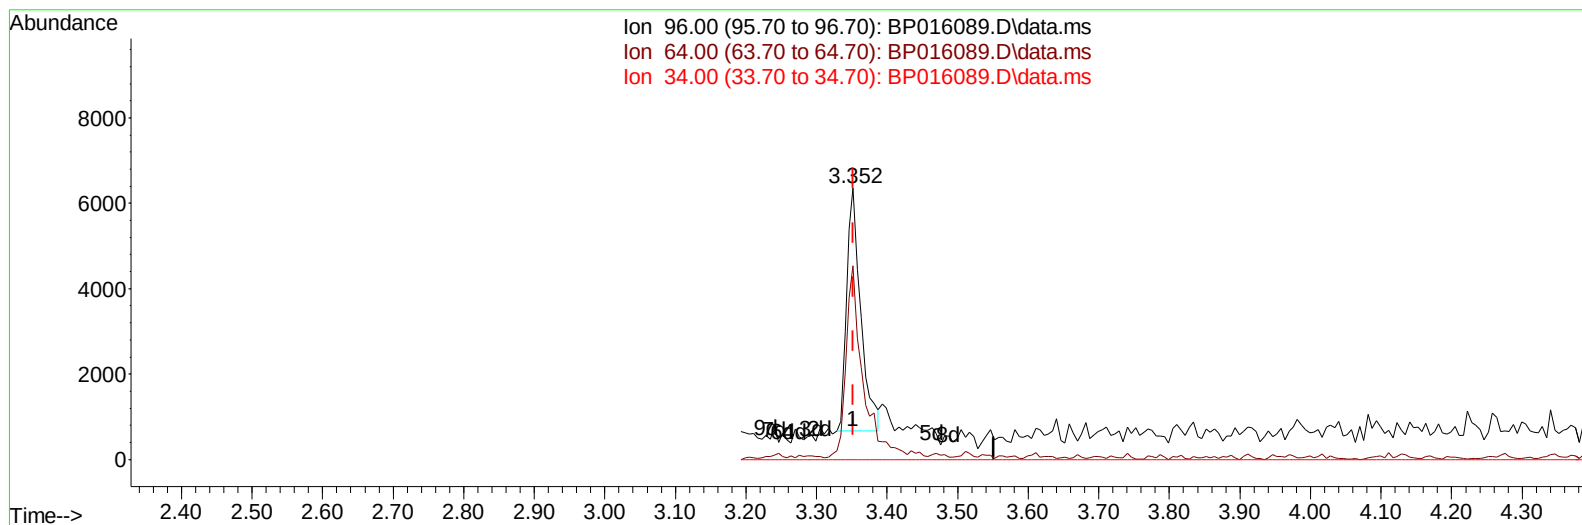

TIC: BP016089.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (+ 0.000) 2.58 ng/uL

response 7968

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.90	71.34
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 22:16:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

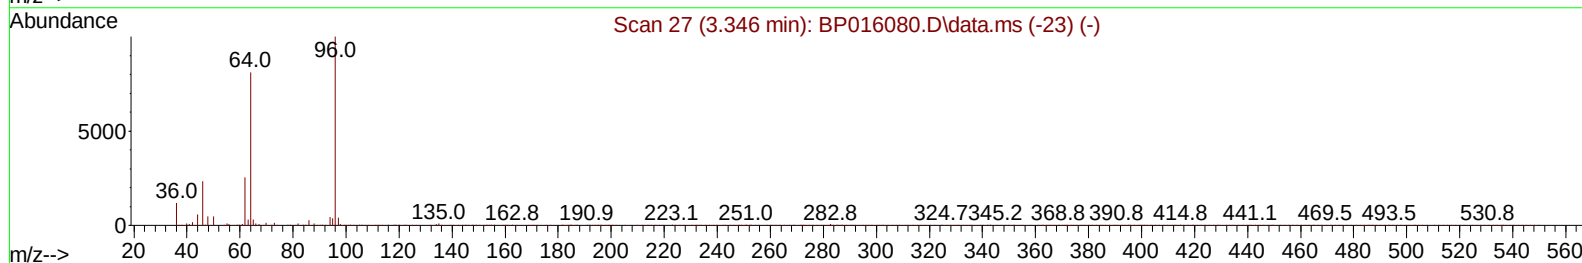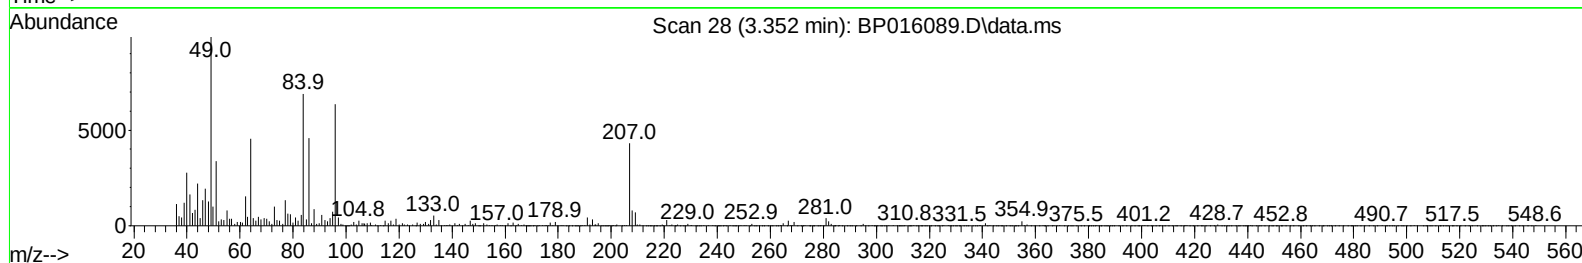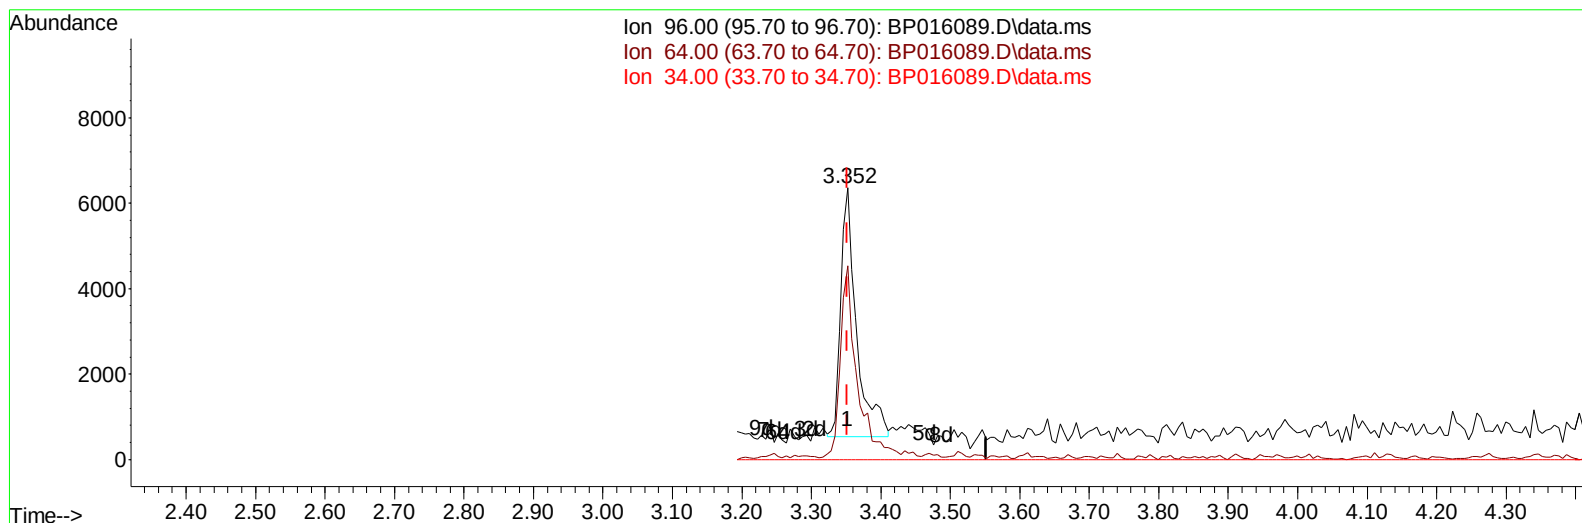

TIC: BP016089.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (+ 0.000) 2.97 ng/uL m

response 9177

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	71.90	71.34
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:17:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

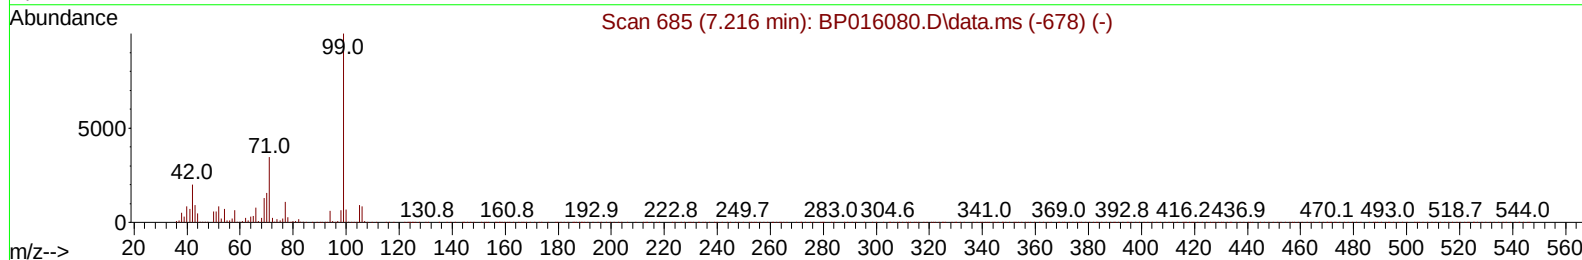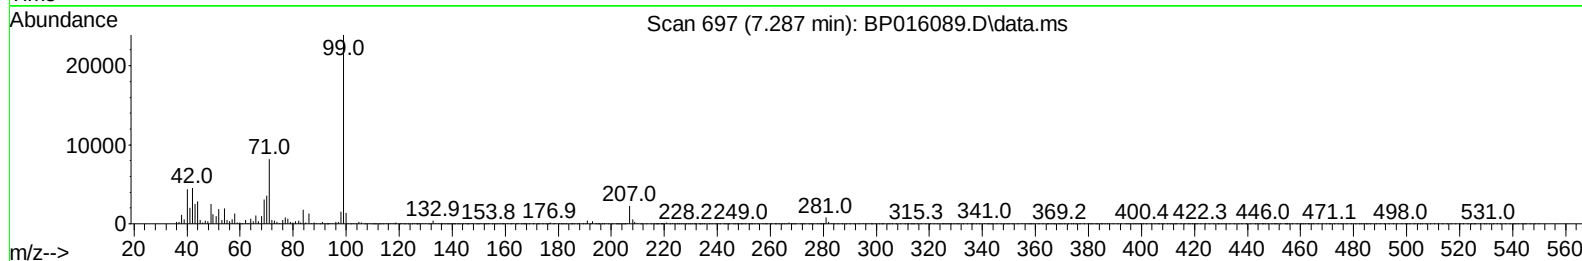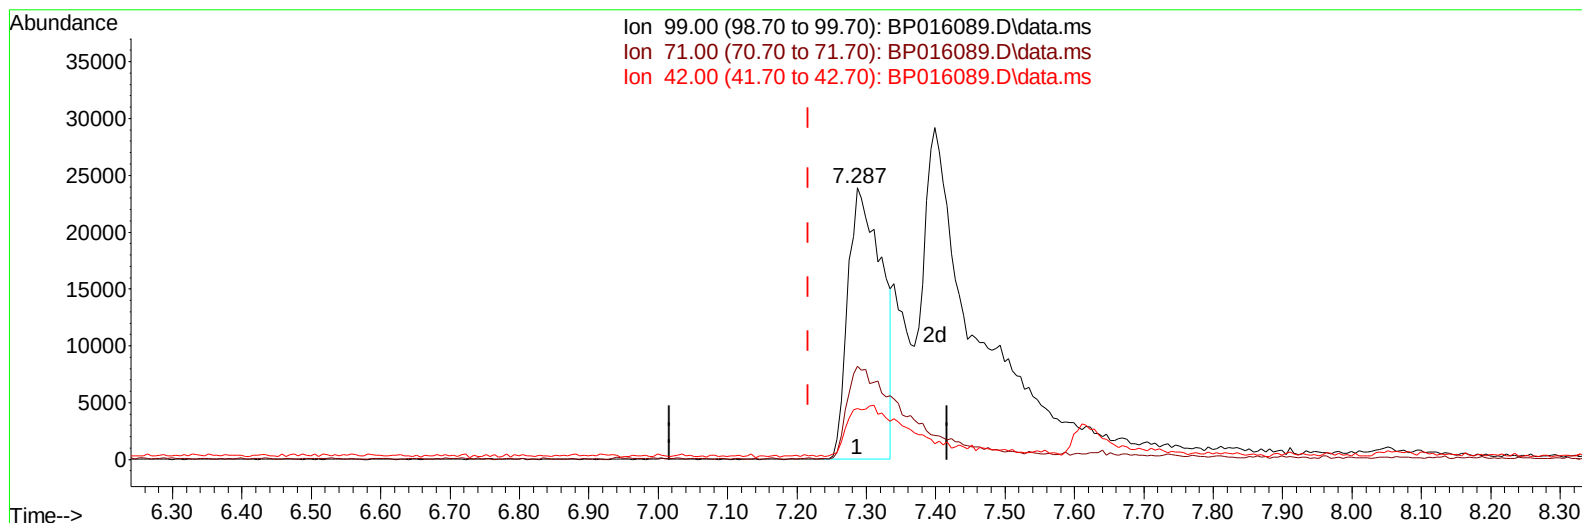

TIC: BP016089.D\data.ms

(7) Phenol-d5 (S)

7.287min (+ 0.071) 8.50 ng/ul

response 80911

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	34.36
42.00	21.90	18.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:17:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

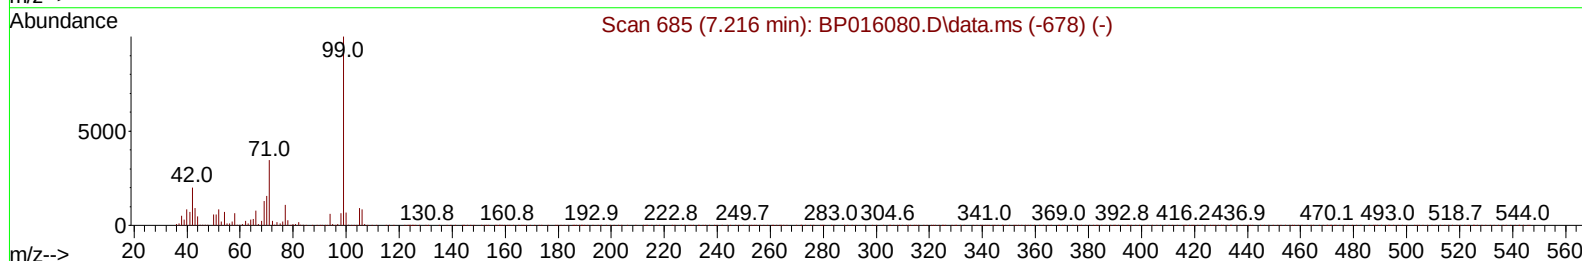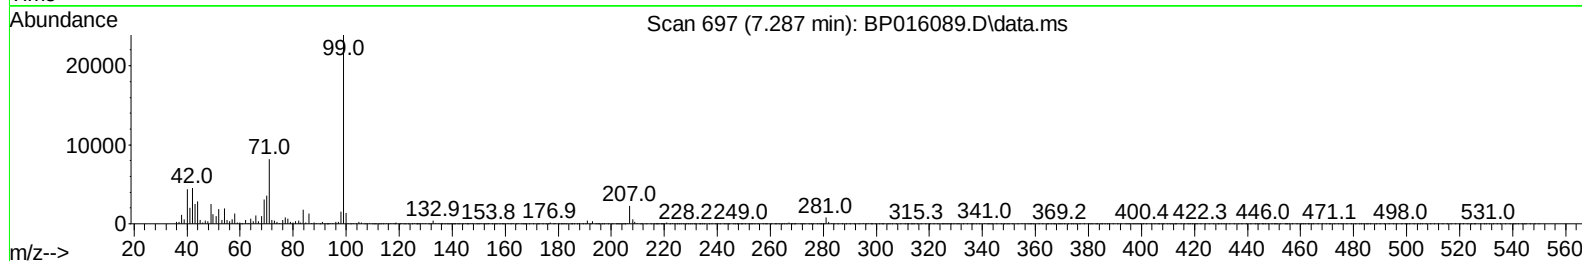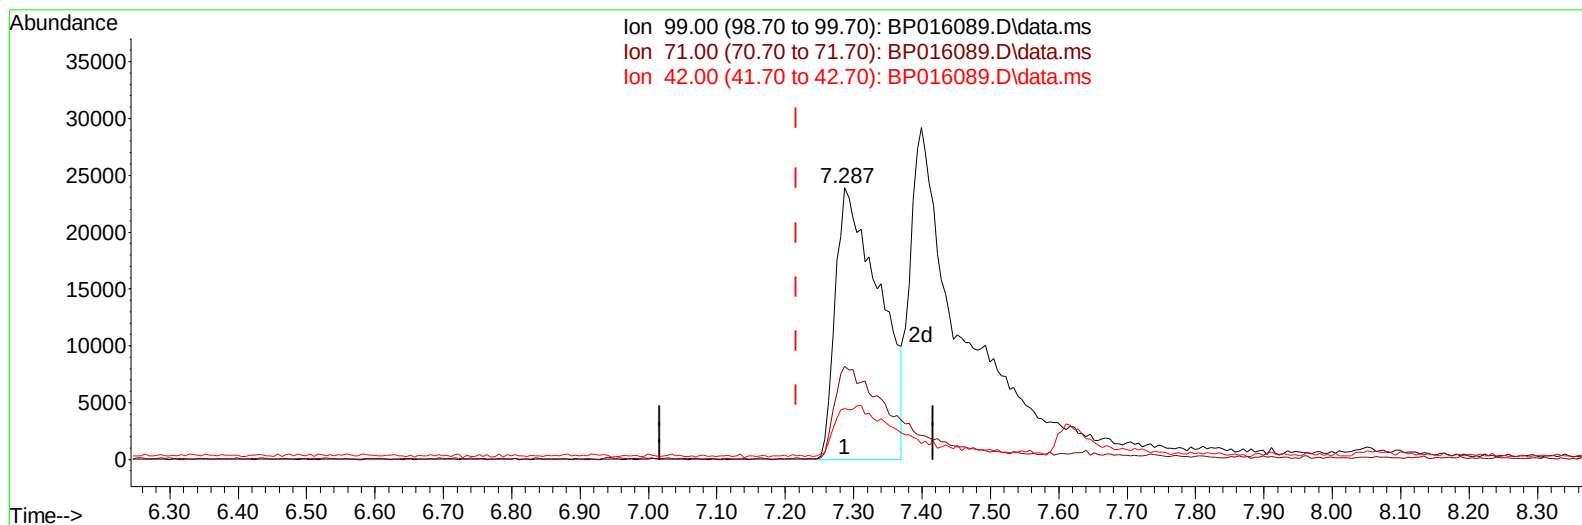

TIC: BP016089.D\data.ms

(7) Phenol-d5 (S)

7.287min (+ 0.071) 11.24 ng/ul m

response 106945

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	34.36
42.00	21.90	18.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:17:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

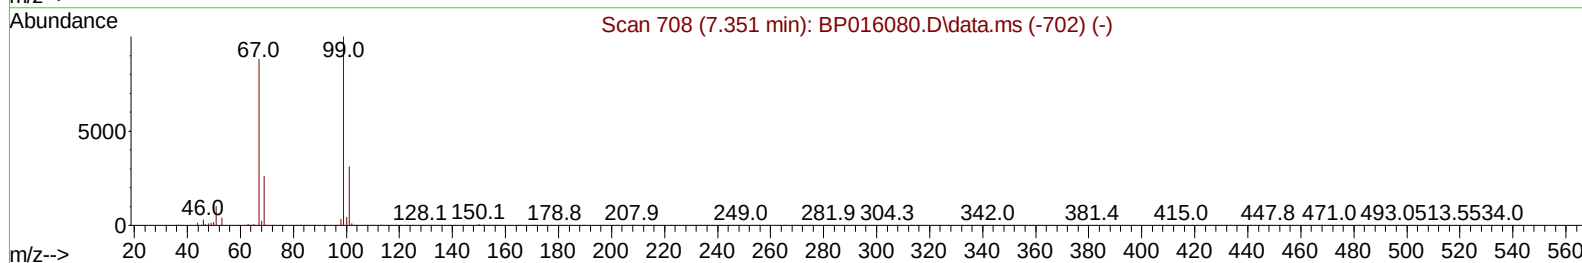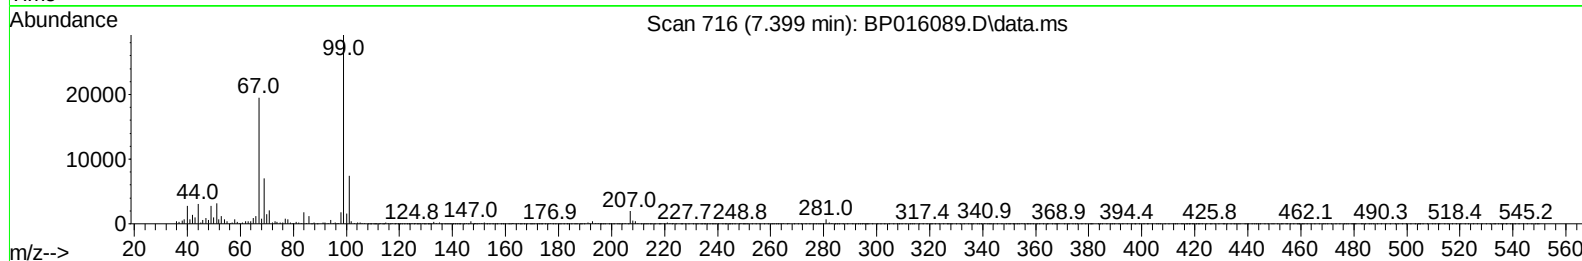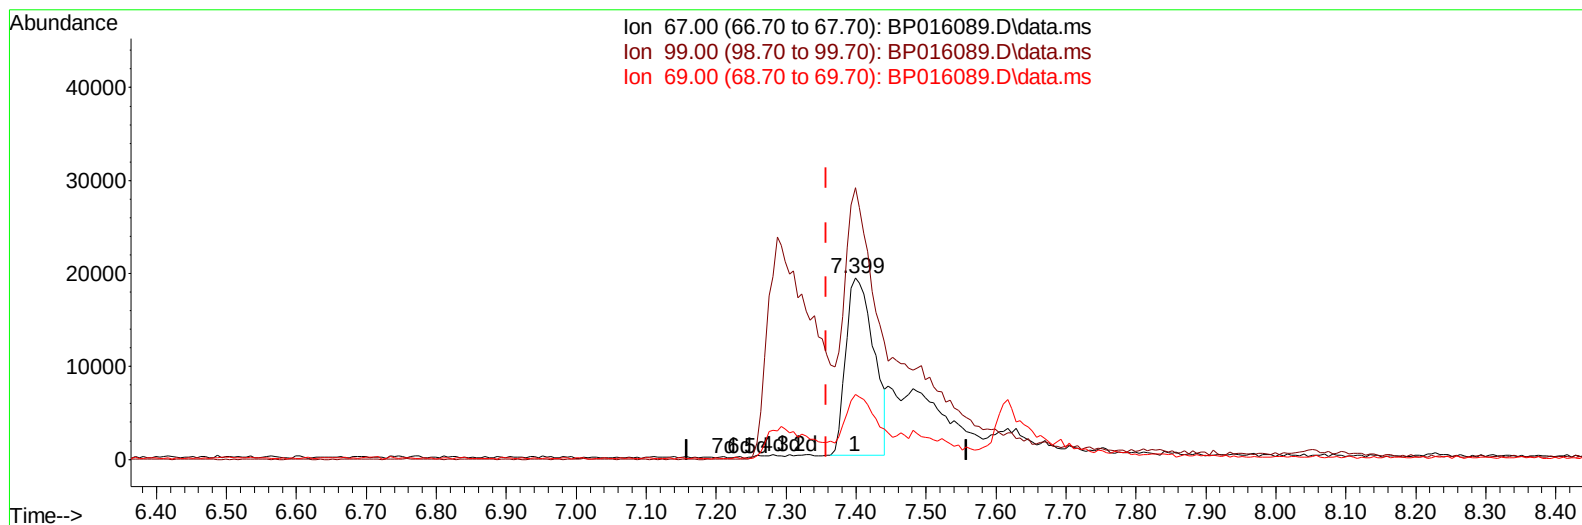

TIC: BP016089.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.399min (+ 0.041) 8.98 ng/uL

response 52877

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	149.47#
69.00	32.10	35.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:17:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

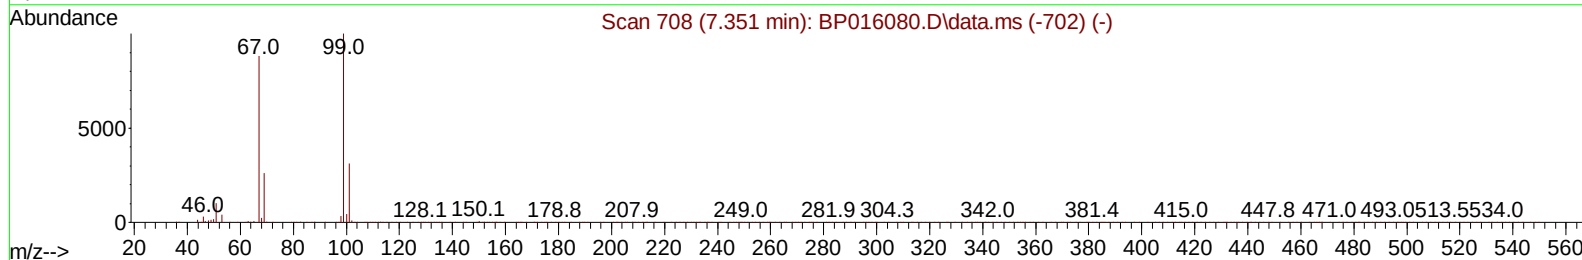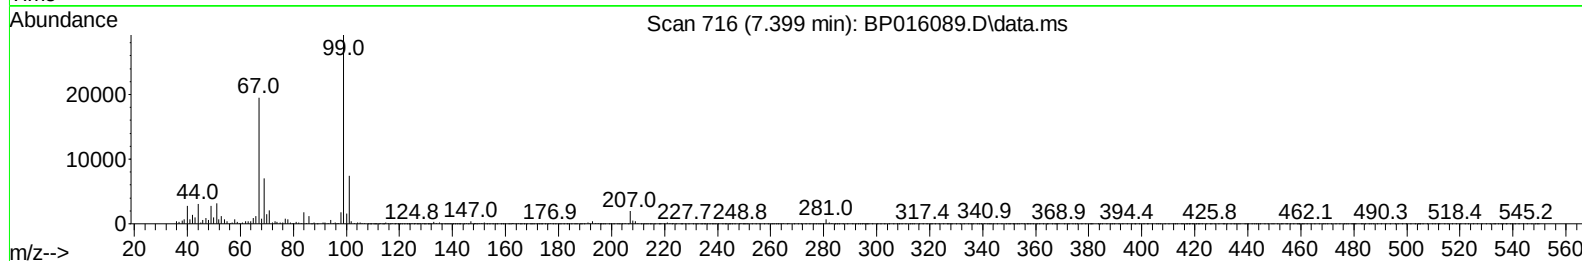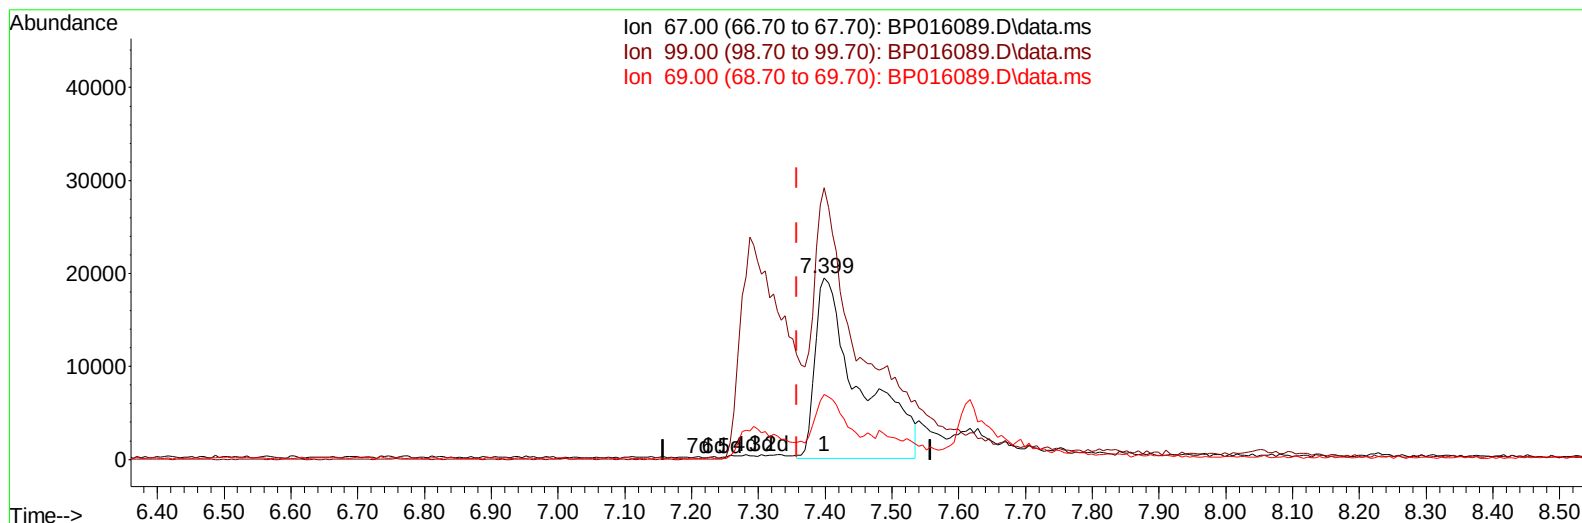

TIC: BP016089.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.399min (+ 0.041) 15.28 ng/ul m

response 89932

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	149.47#
69.00	32.10	35.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:17:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

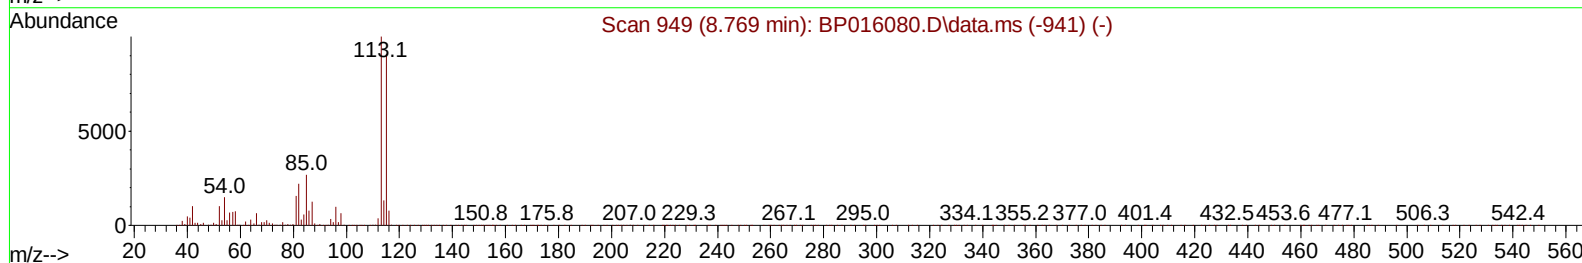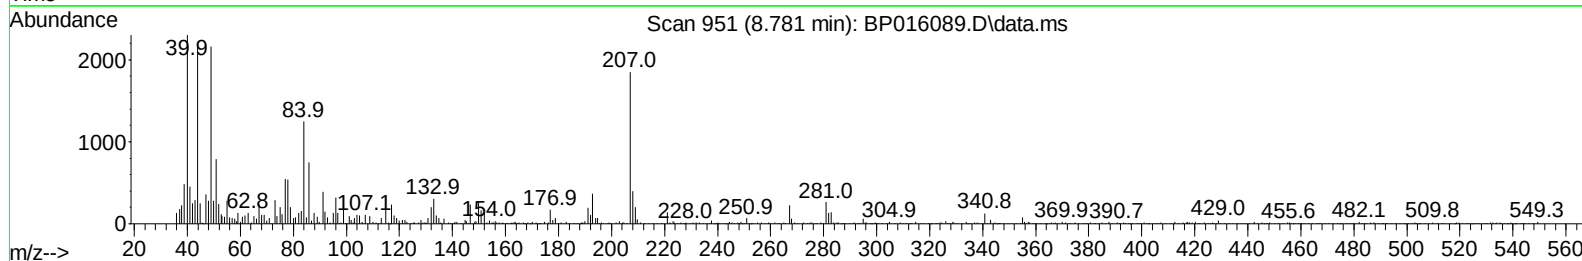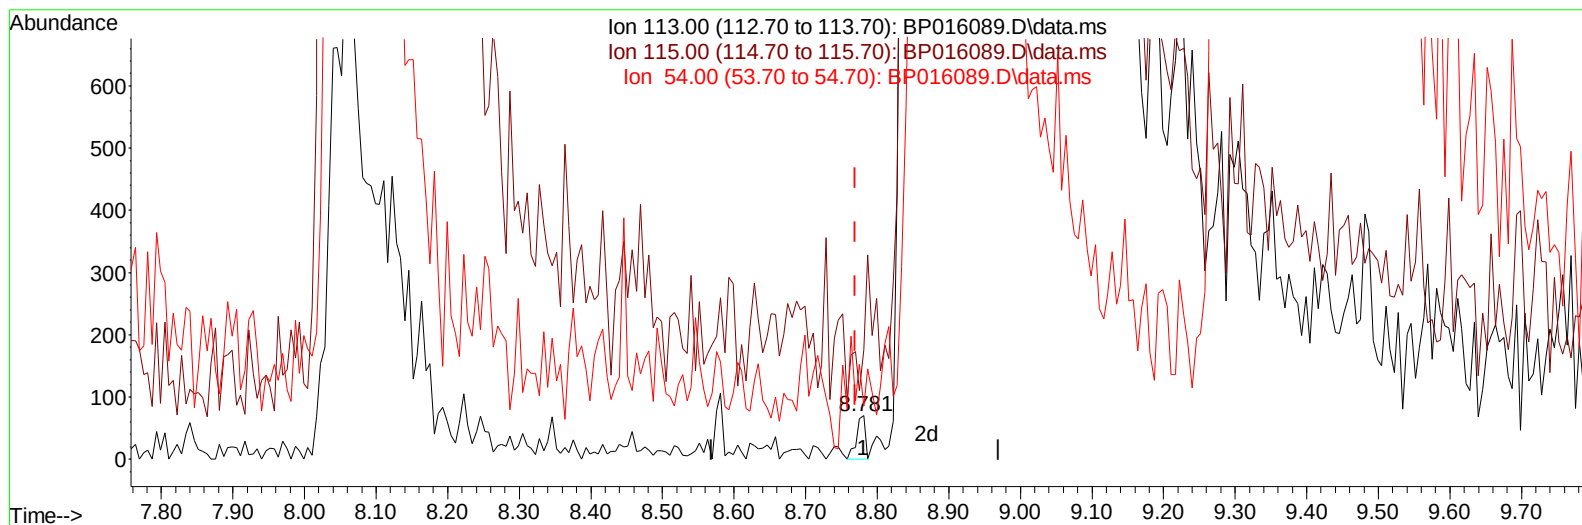

TIC: BP016089.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.781min (+ 0.012) 0.01 ng/uL

response 60

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	271.43#
54.00	16.10	122.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:17:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

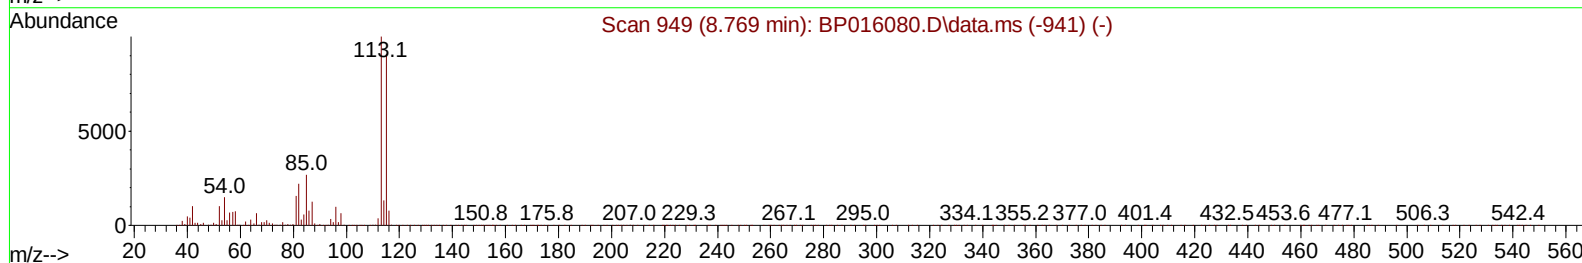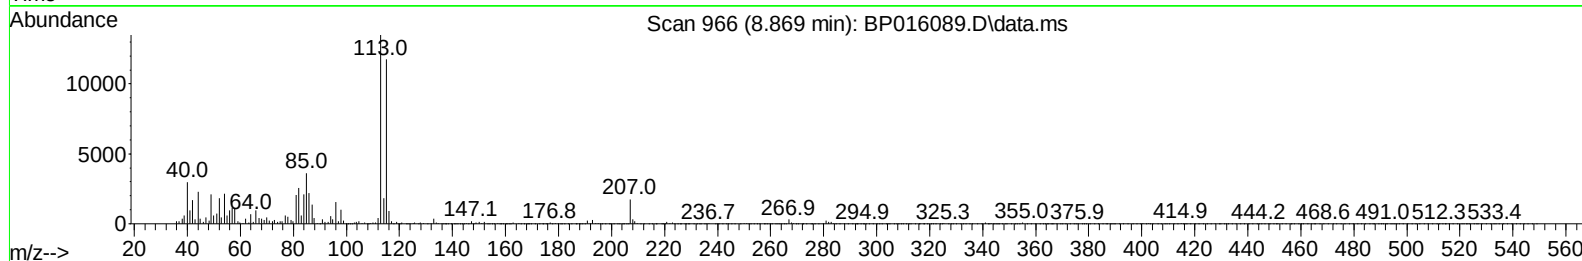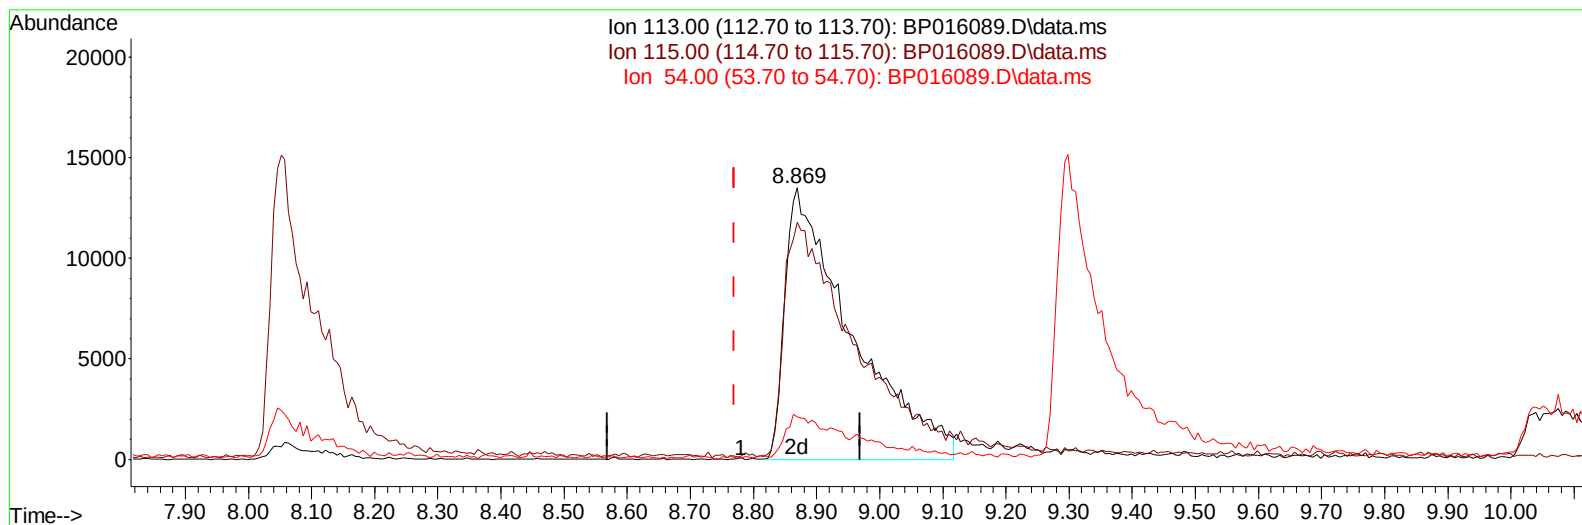

TIC: BP016089.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.869min (+ 0.100) 13.12 ng/ul m

response 98585

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	87.29
54.00	16.10	15.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:18:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

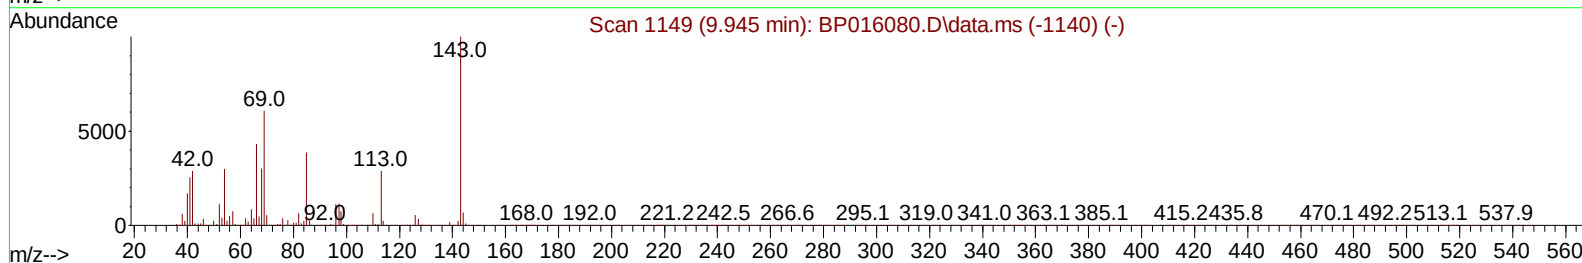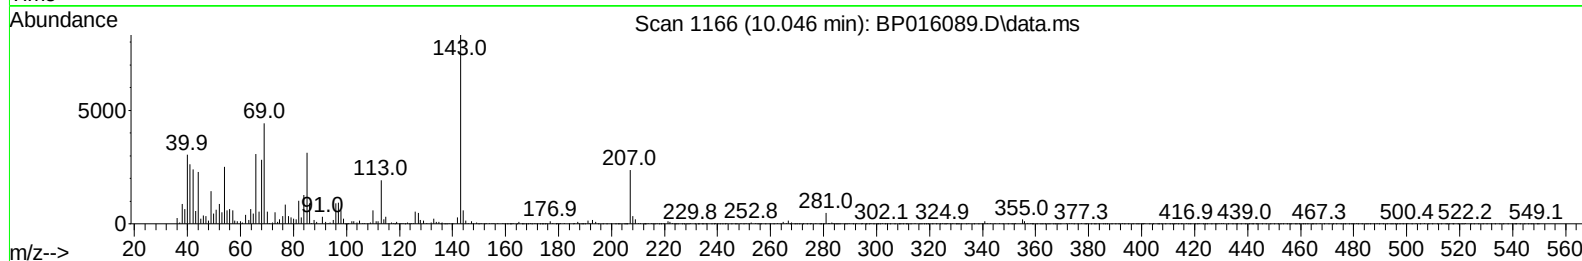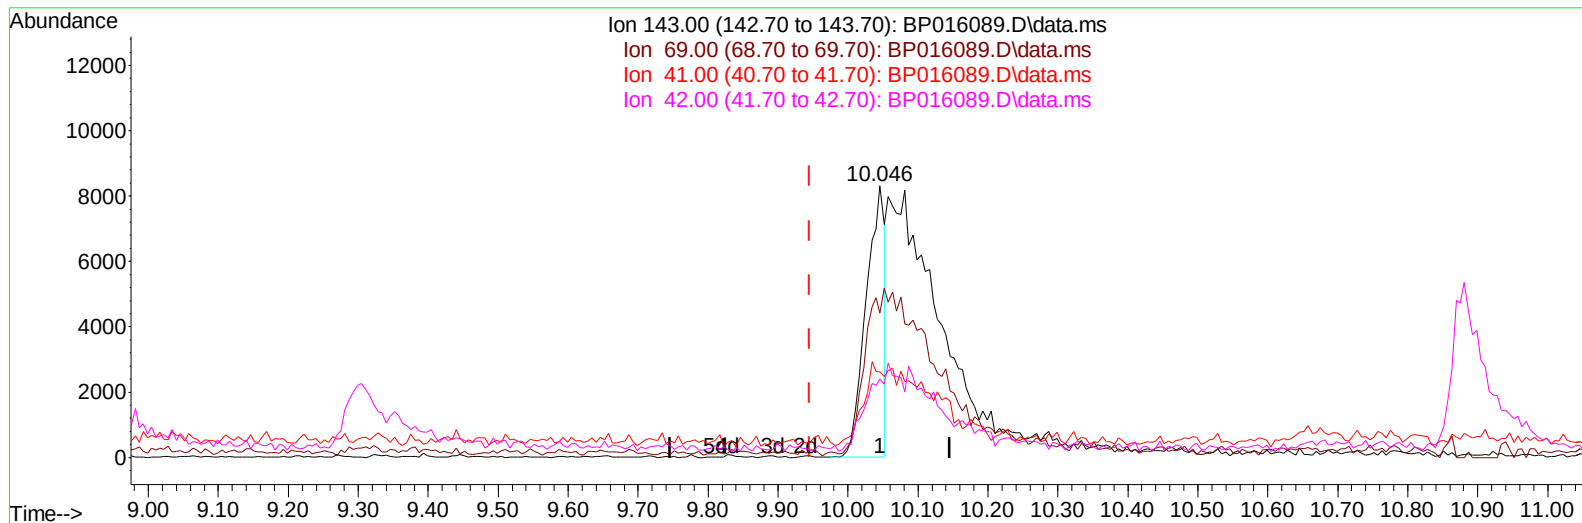

TIC: BP016089.D\data.ms

(24) 2-Nitrophenol-d4 (S)

10.046min (+ 0.100) 2.91 ng/ul

response 15305

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	53.25
41.00	26.80	31.55
42.00	30.50	28.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:18:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

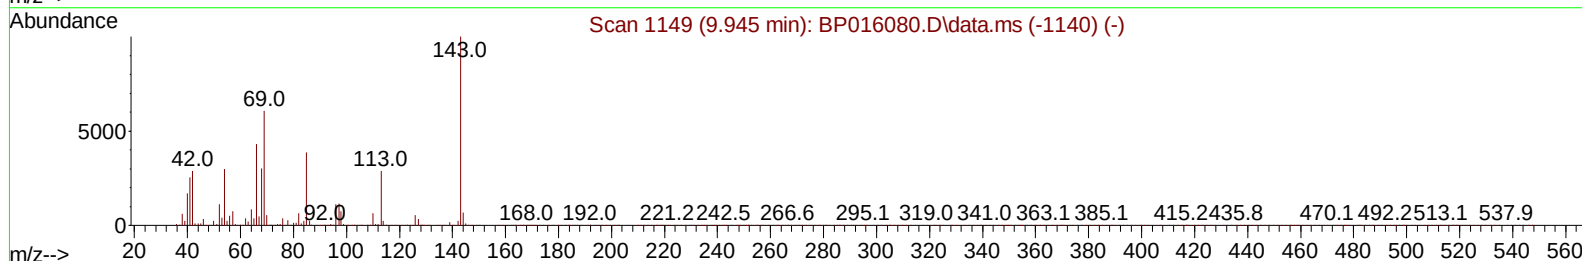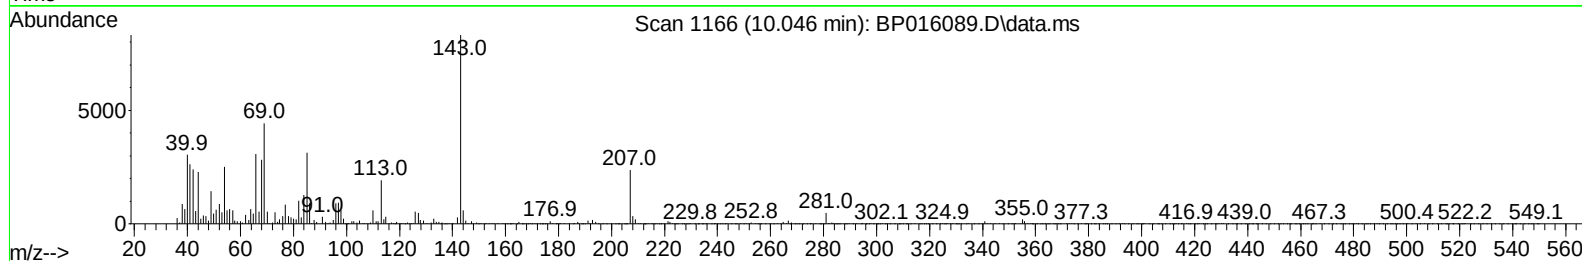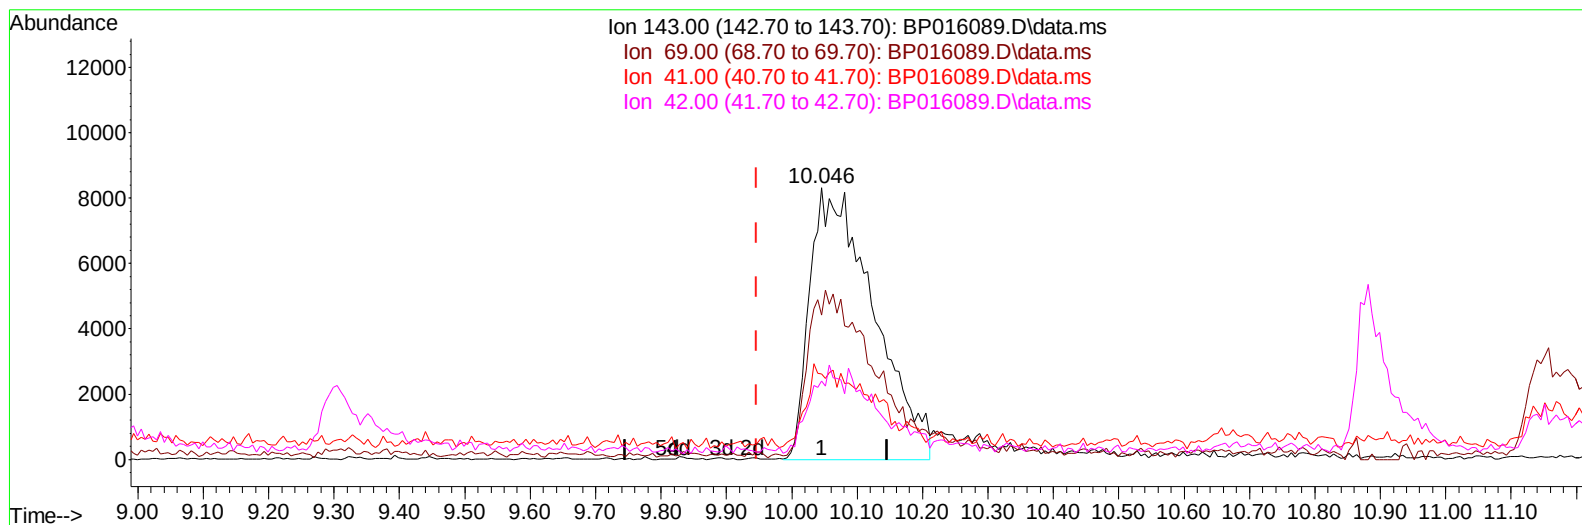

TIC: BP016089.D\data.ms

(24) 2-Nitrophenol-d4 (S)

10.046min (+ 0.100) 10.64 ng/ul m

response 56043

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	53.25
41.00	26.80	31.55
42.00	30.50	28.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:18:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

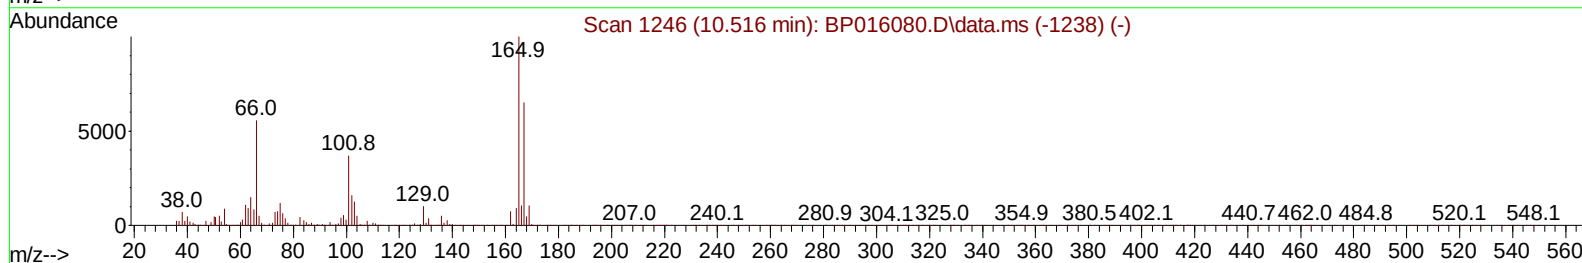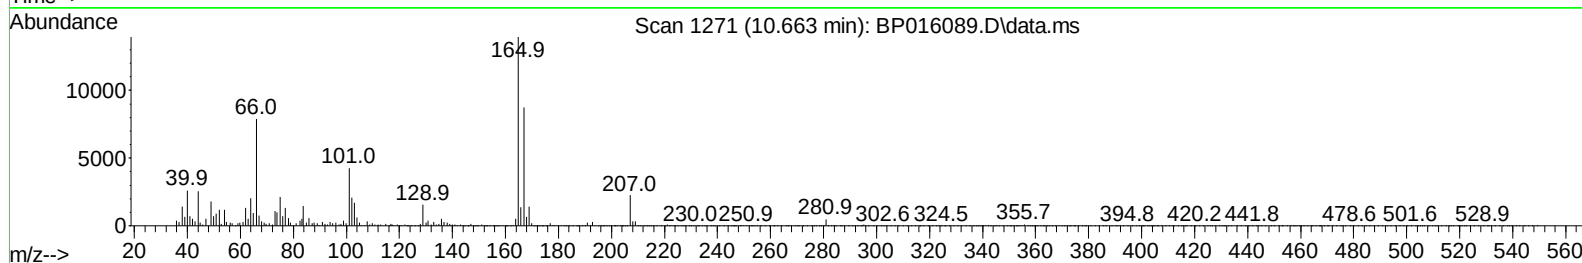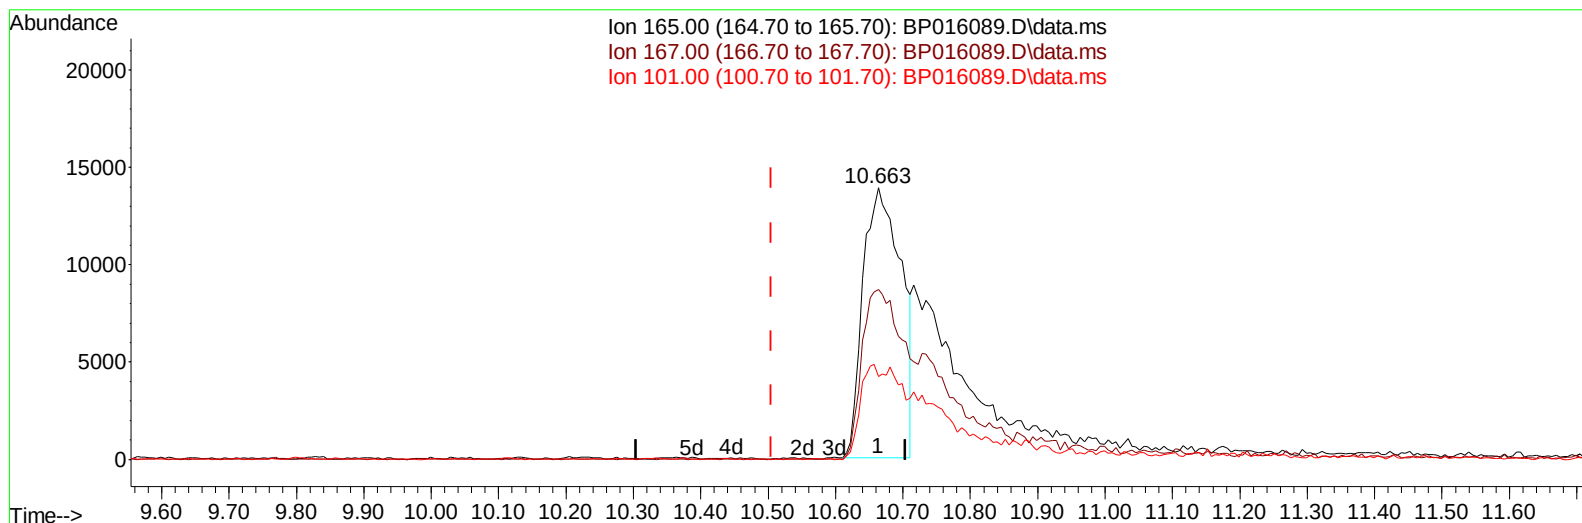

TIC: BP016089.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.663min (+ 0.159) 5.82 ng/ul

response 54669

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	62.69
101.00	37.30	30.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:18:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

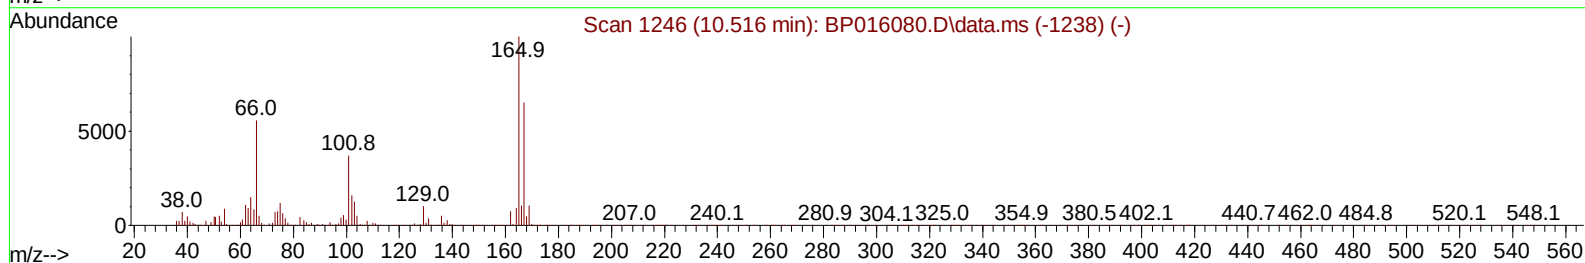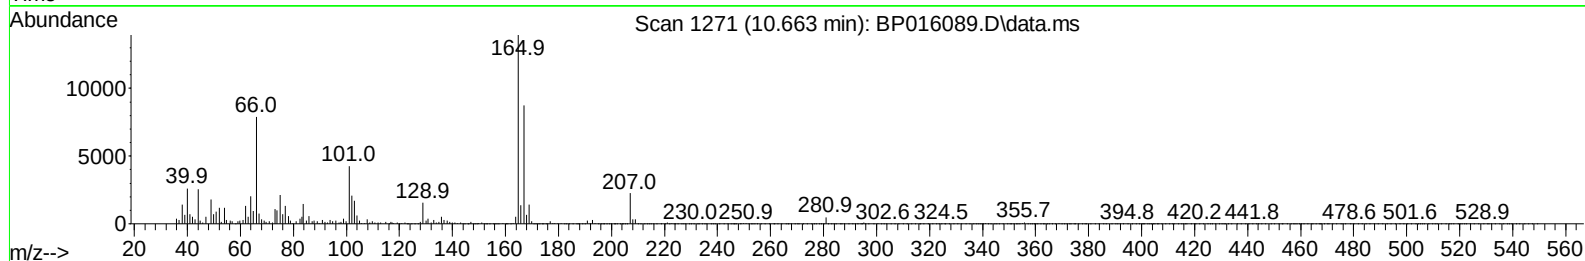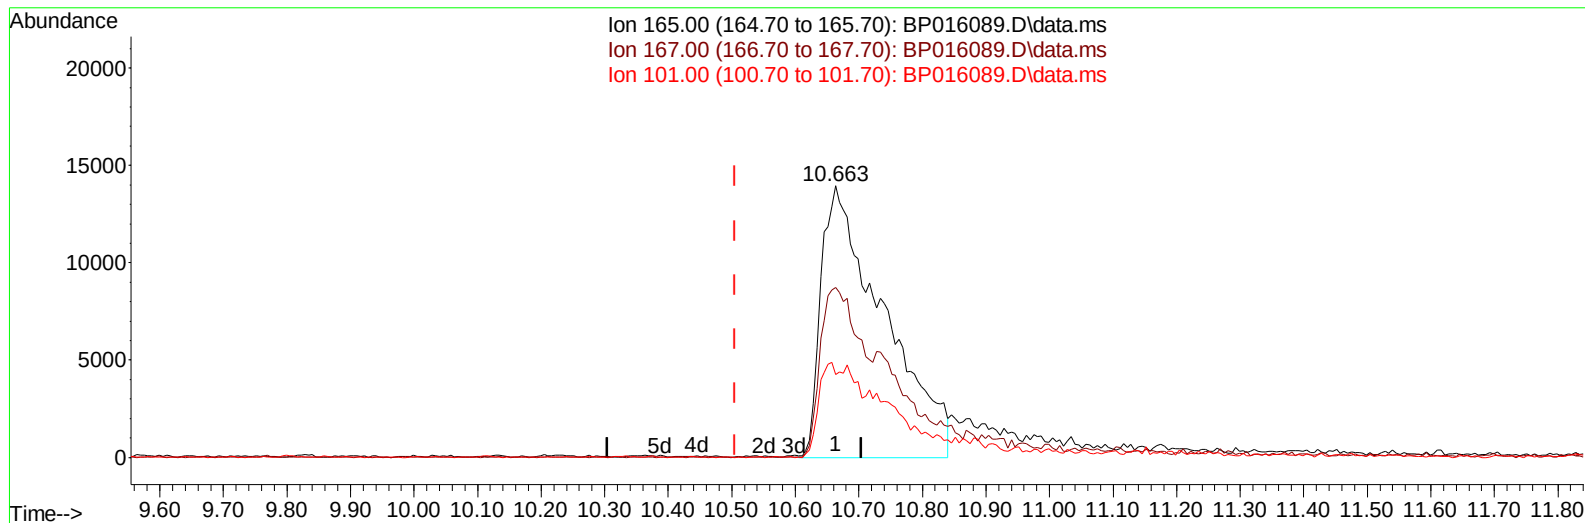

TIC: BP016089.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.663min (+ 0.159) 10.13 ng/ul m

response 95050

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	62.69
101.00	37.30	30.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:19:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

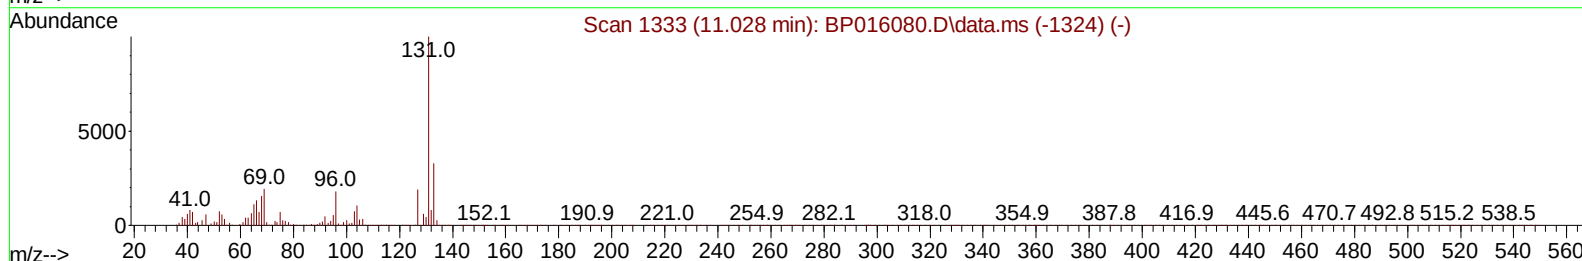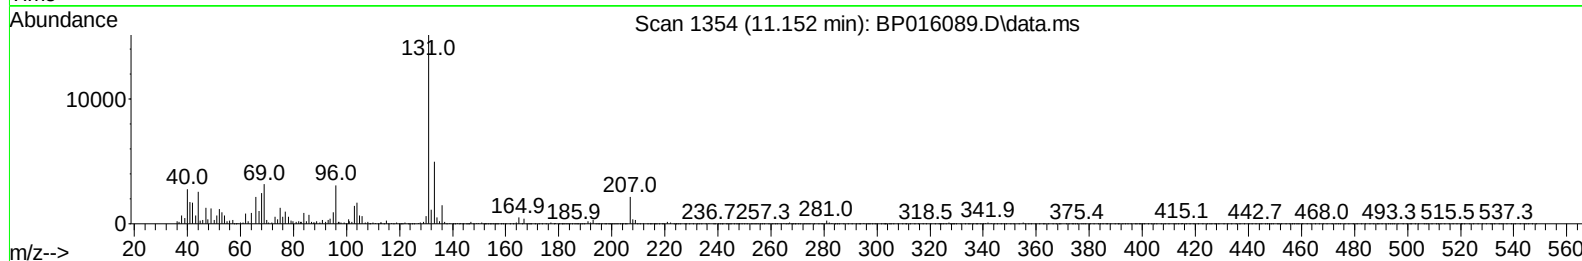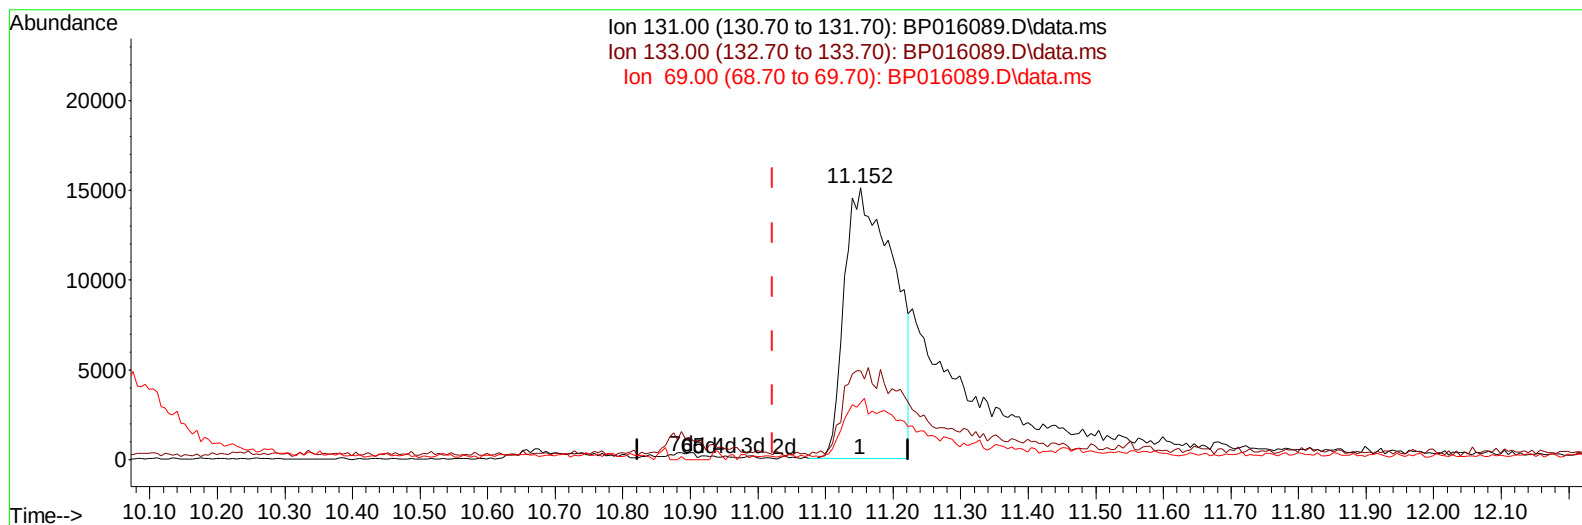

TIC: BP016089.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.152min (+ 0.130) 6.33 ng/u1

response 76321

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	32.77
69.00	22.20	20.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:19:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

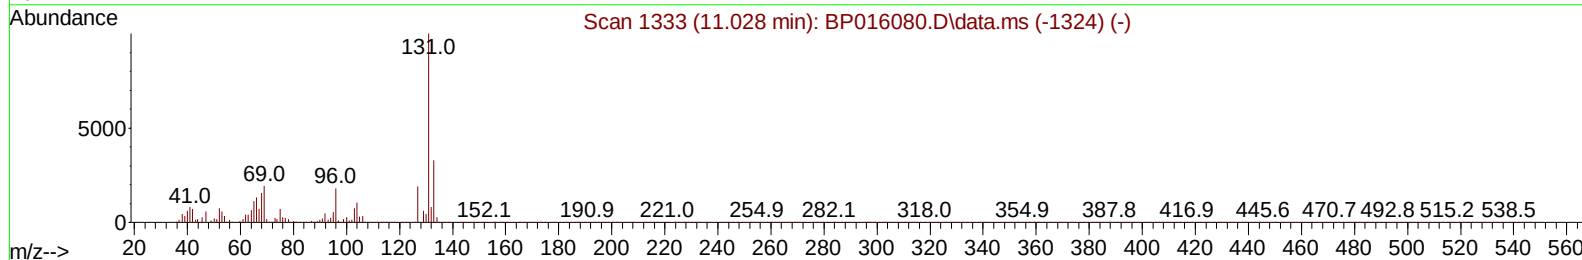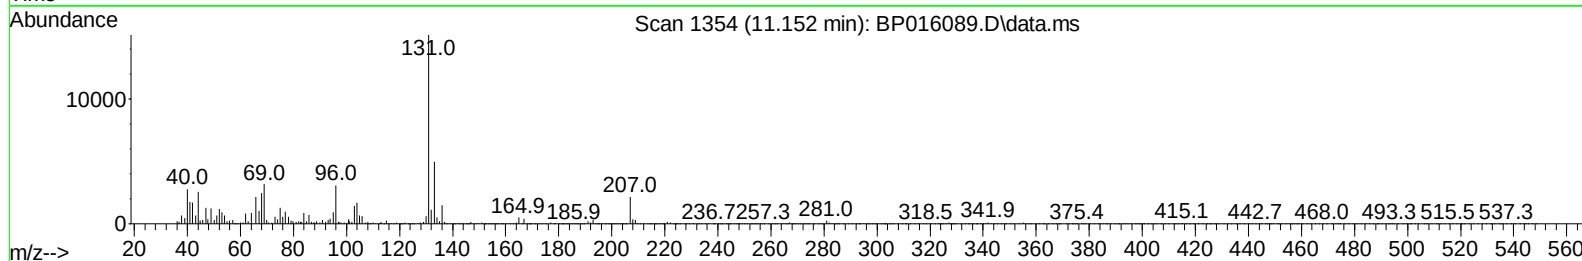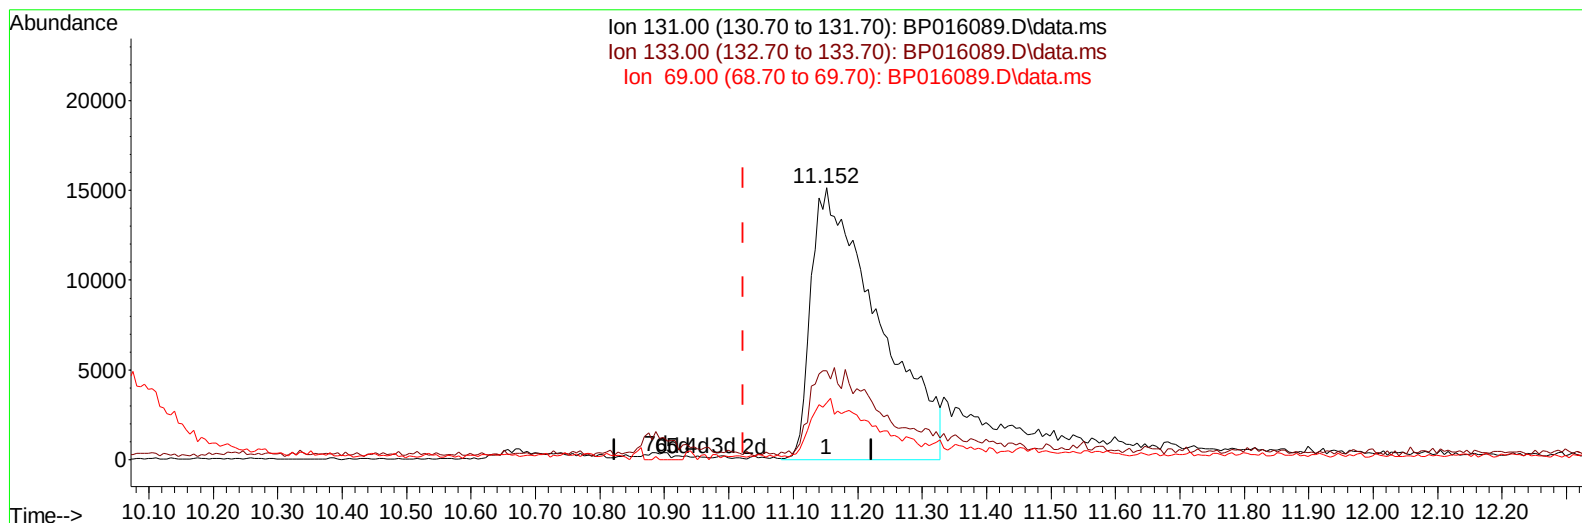

TIC: BP016089.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.152min (+ 0.130) 9.06 ng/ul m

response 109254

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	32.77
69.00	22.20	20.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

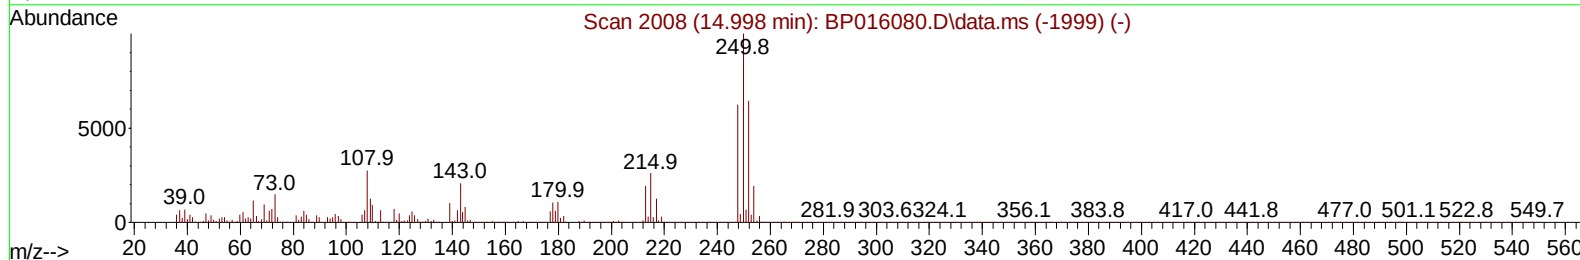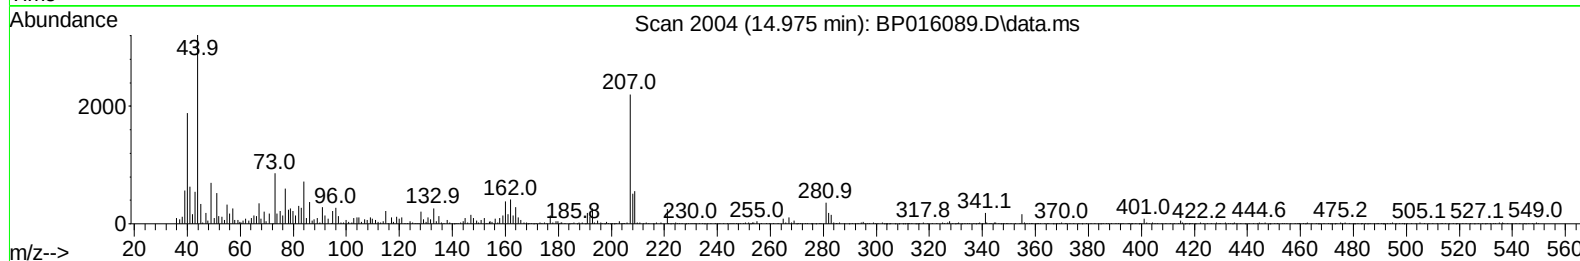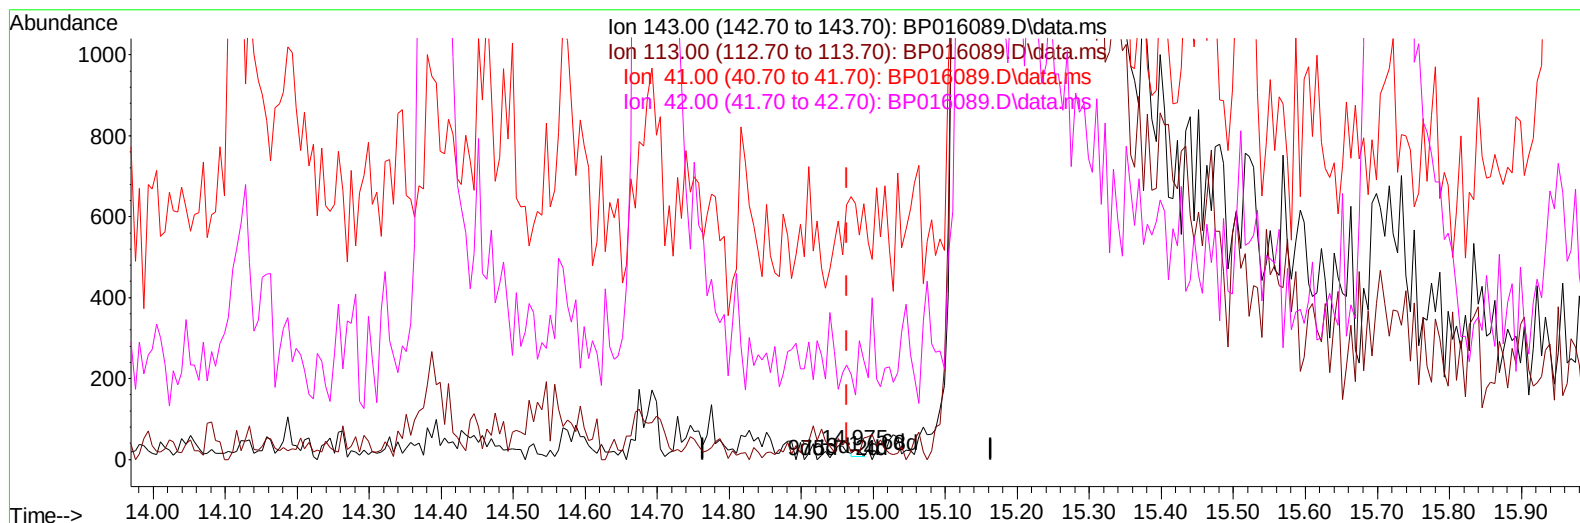

TIC: BP016089.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.975min (+ 0.012) 0.00 ng/ul

response 11

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	95.83
41.00	45.70	2633.33#
42.00	31.20	662.50#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

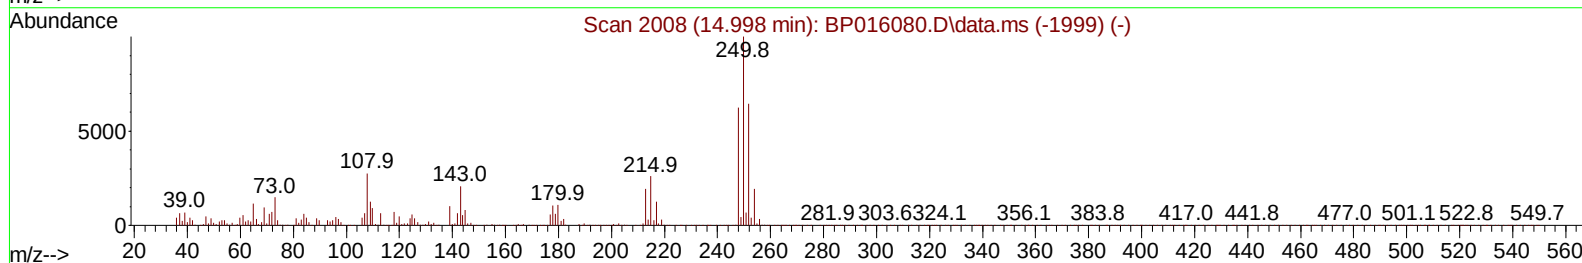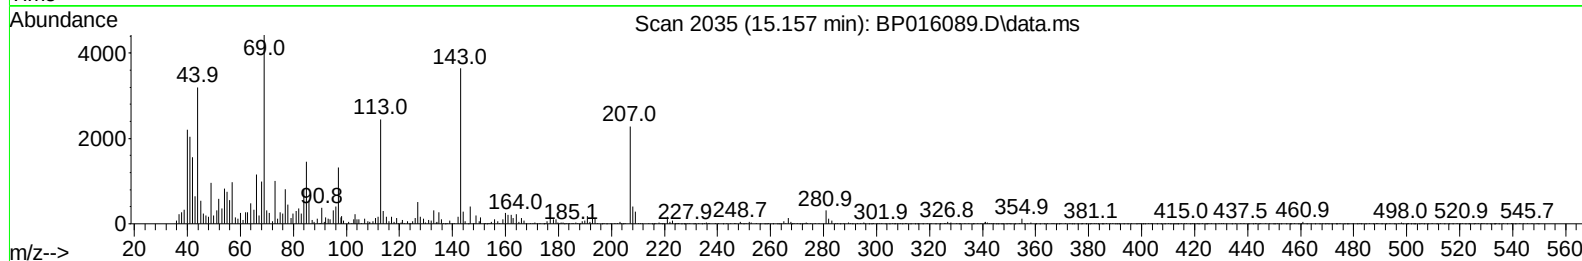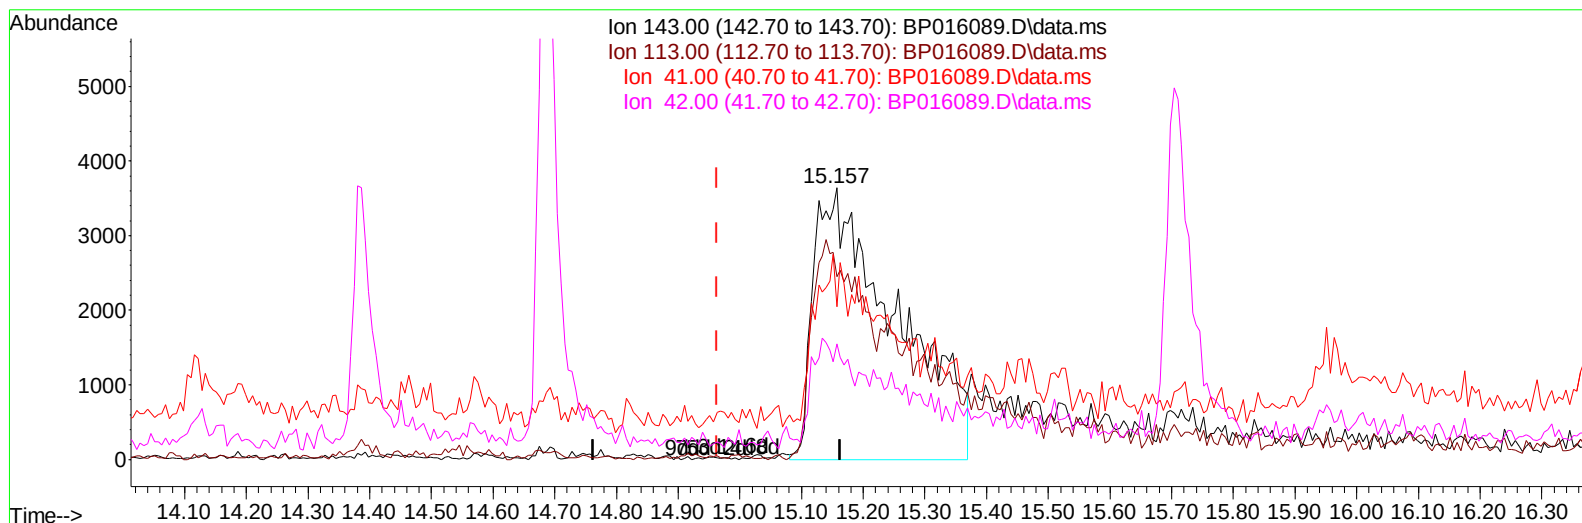

TIC: BP016089.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.157min (+ 0.194) 7.98 ng/ul m

response 33755

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	67.24#
41.00	45.70	56.14#
42.00	31.20	42.68#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

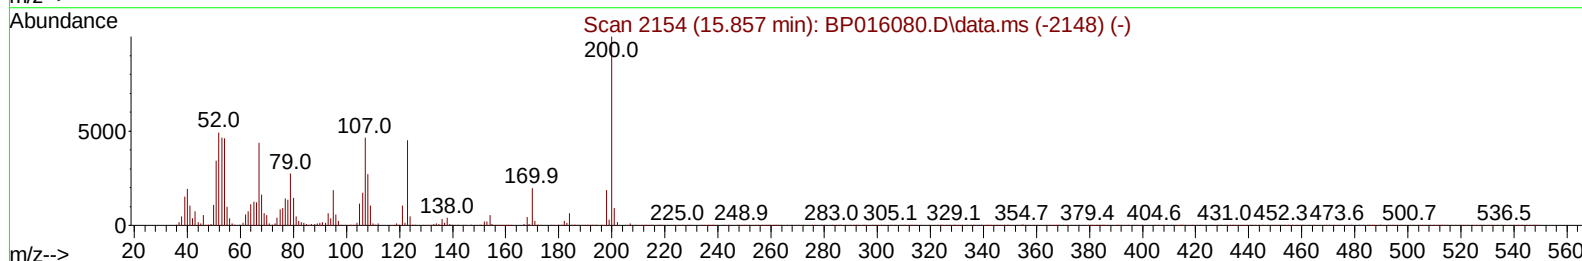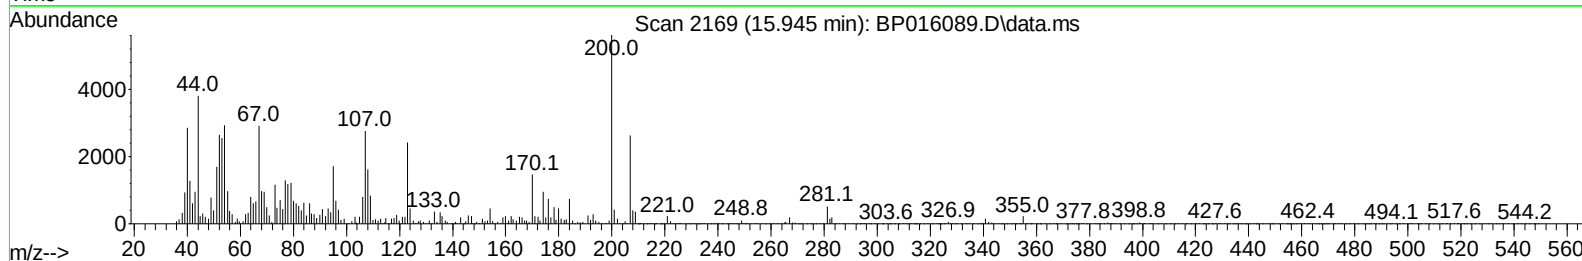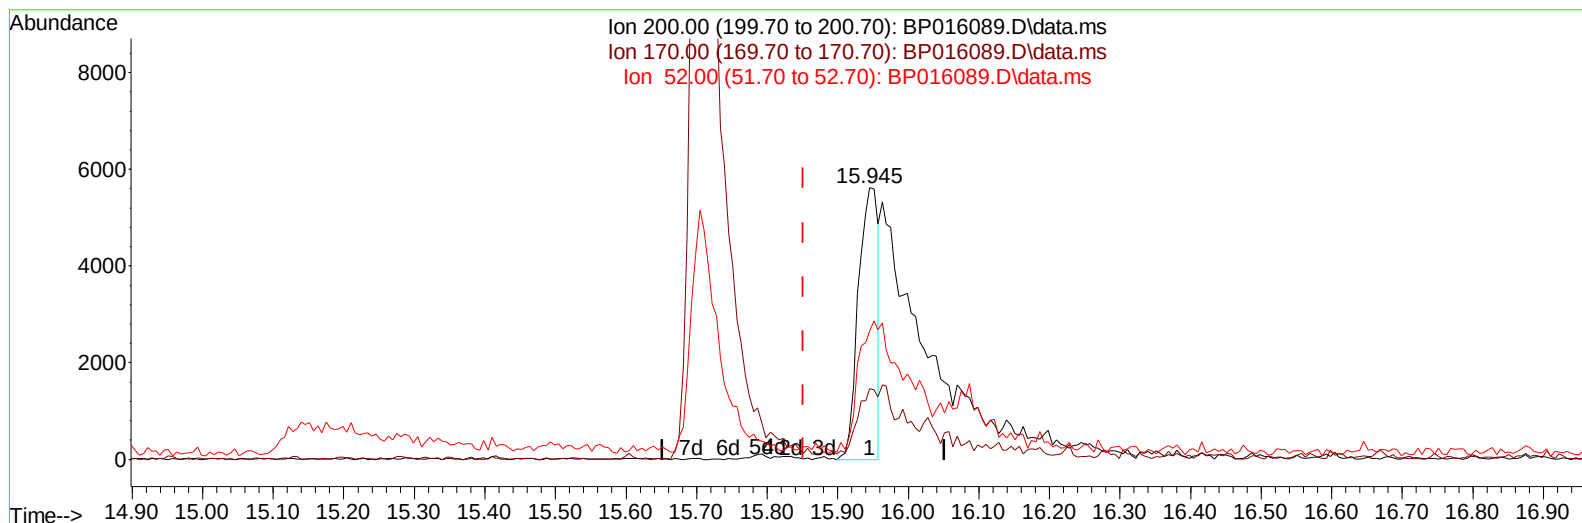

TIC: BP016089.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.945min (+ 0.094) 1.90 ng/ul

response 10970

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.30	26.08
52.00	52.20	47.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Quant Time: Jul 08 23:19:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

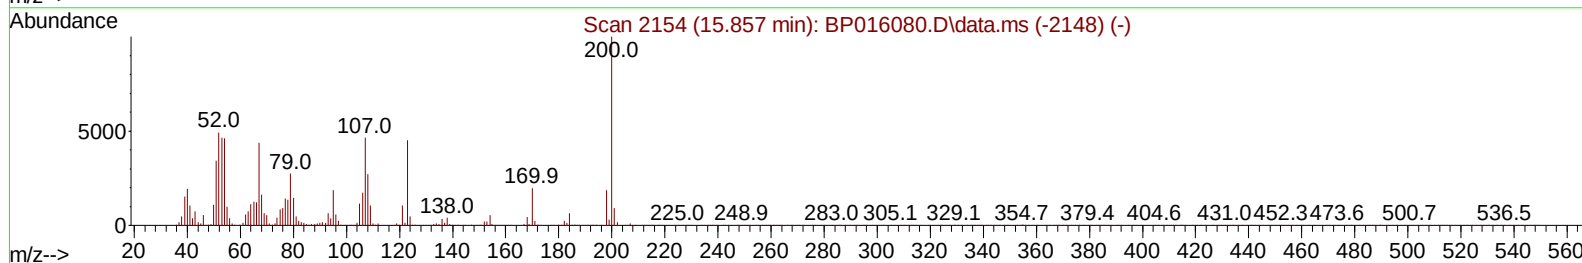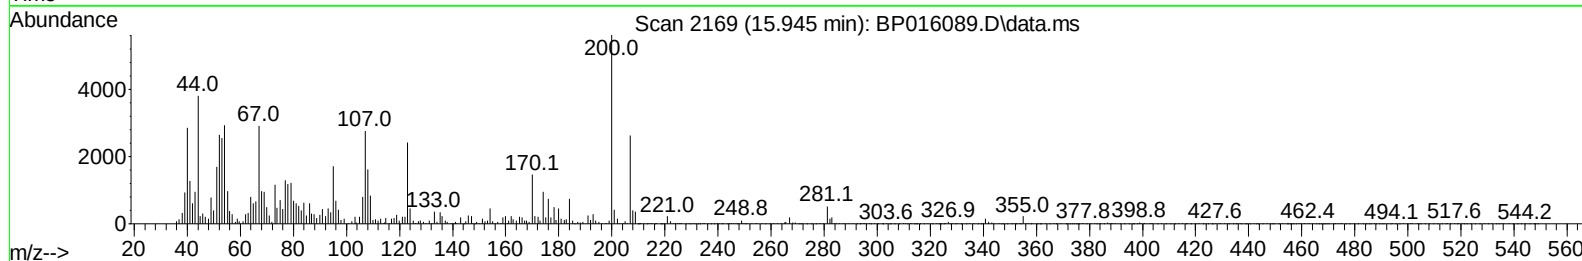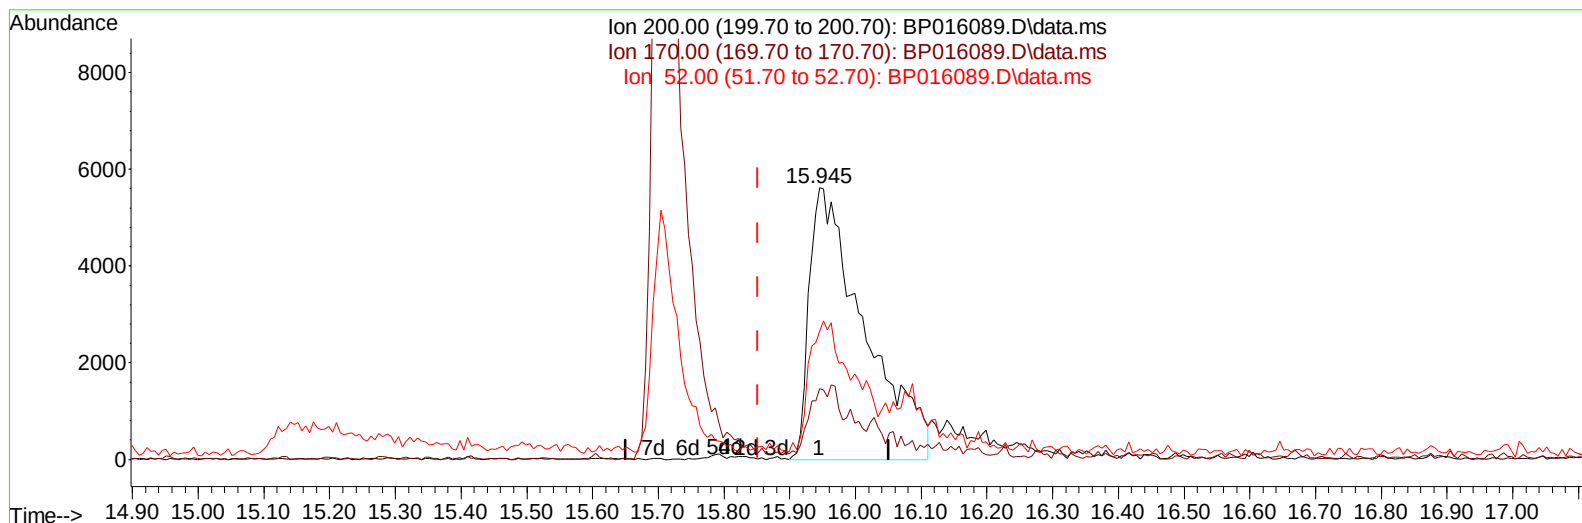

TIC: BP016089.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.945min (+ 0.094) 5.65 ng/ul m

response 32636

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.30	26.08
52.00	52.20	47.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016089.D
 Acq On : 08 Jul 2023 13:00
 Operator : MA/JU
 Sample : 03332-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTY7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

Quant Time: Jul 08 23:20:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.052	152	111188	20.000	ng/ul	0.02
20) Naphthalene-d8	10.881	136	590601	20.000	ng/ul	0.03
38) Acenaphthene-d10	14.687	164	414951	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.451	188	939129	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	1068771	20.000	ng/ul	# 0.00
88) Perylene-d12	24.074	264	1201522	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	9177m	2.970	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.287	99	106945m	11.242	ng/ul	0.07
9) Bis-(2-Chloroethyl)eth...	7.399	67	89932m	15.280	ng/ul	0.04
11) 2-Chlorophenol-d4	7.617	132	99238	13.819	ng/ul	0.05
15) 4-Methylphenol-d8	8.869	113	98585m	13.118	ng/ul	0.10
21) Nitrobenzene-d5	9.299	128	47344	10.489	ng/ul	0.08
24) 2-Nitrophenol-d4	10.046	143	56043m	10.639	ng/ul	0.10
28) 2,4-Dichlorophenol-d3	10.663	165	95050m	10.125	ng/ul	0.16
31) 4-Chloroaniline-d4	11.152	131	109254m	9.060	ng/ul	0.13
46) Dimethylphthalate-d6	14.122	166	464196	14.473	ng/ul	0.04
49) Acenaphthylene-d8	14.387	160	481102	13.344	ng/ul	0.01
54) 4-Nitrophenol-d4	15.157	143	33755m	7.975	ng/ul	0.19
60) Fluorene-d10	15.704	176	402630	15.246	ng/ul	0.03
65) 4,6-Dinitro-2-methylph...	15.945	200	32636m	5.651	ng/ul	0.09
73) Anthracene-d10	17.569	188	646291	15.066	ng/ul	0.02
81) Pyrene-d10	19.786	212	925605	13.263	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.904	264	946130	15.610	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016089.D
Acq On : 08 Jul 2023 13:00
Operator : MA/JU
Sample : 03332-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTY7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

Quant Time: Jul 08 23:20:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

