




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:33:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

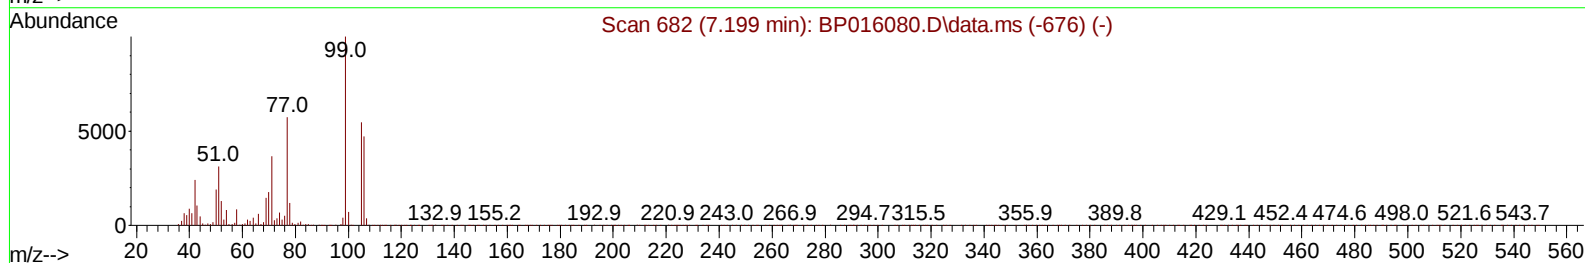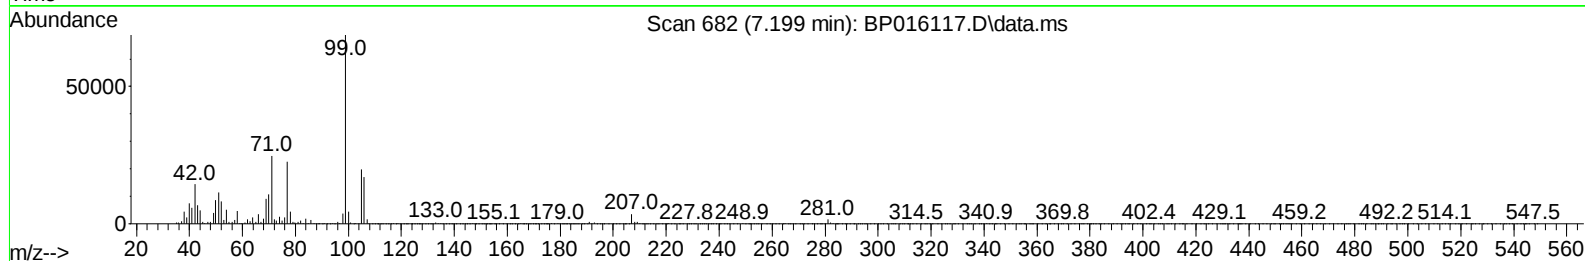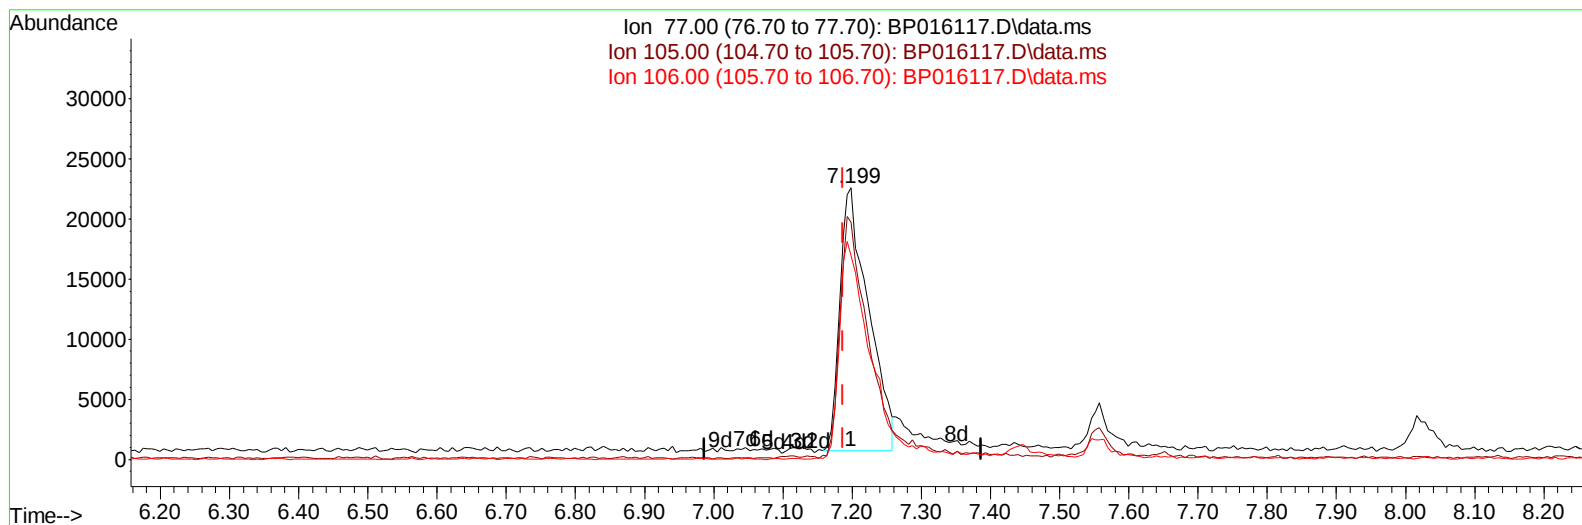

TIC: BP016117.D\data.ms

(6) Benzaldehyde

7.199min (+ 0.012) 11.64 ng/u1

response 62466

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	91.70	87.31
106.00	83.30	75.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:33:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

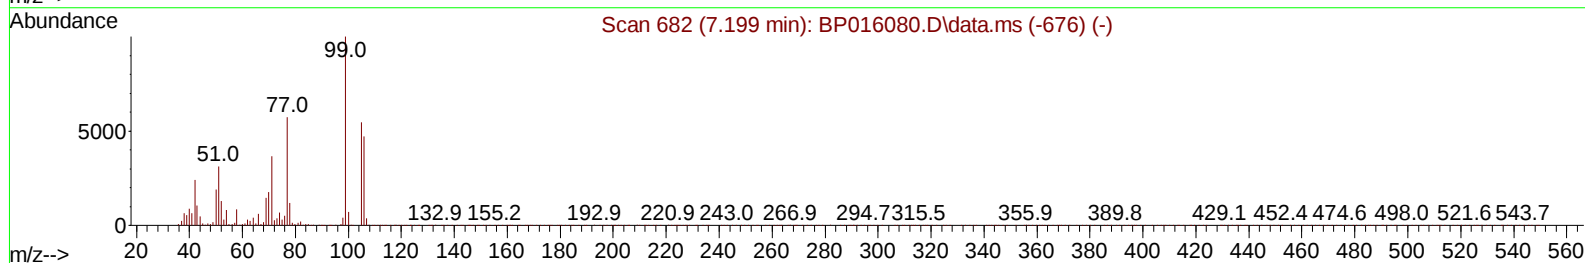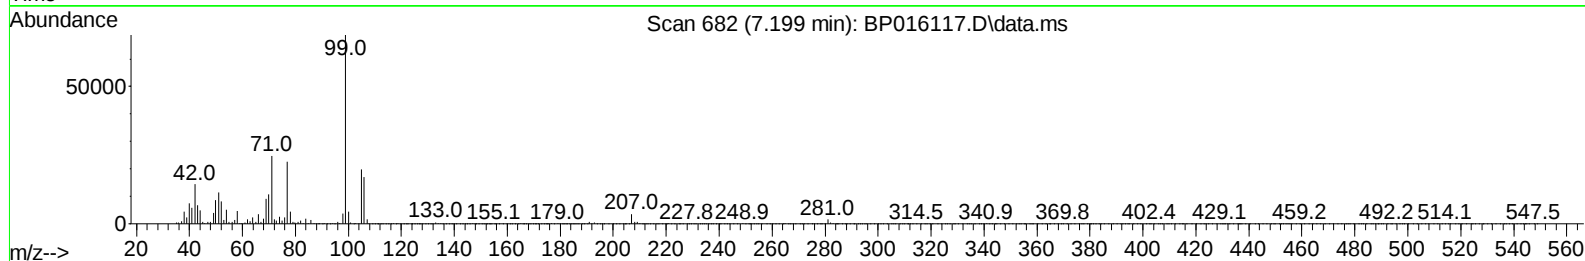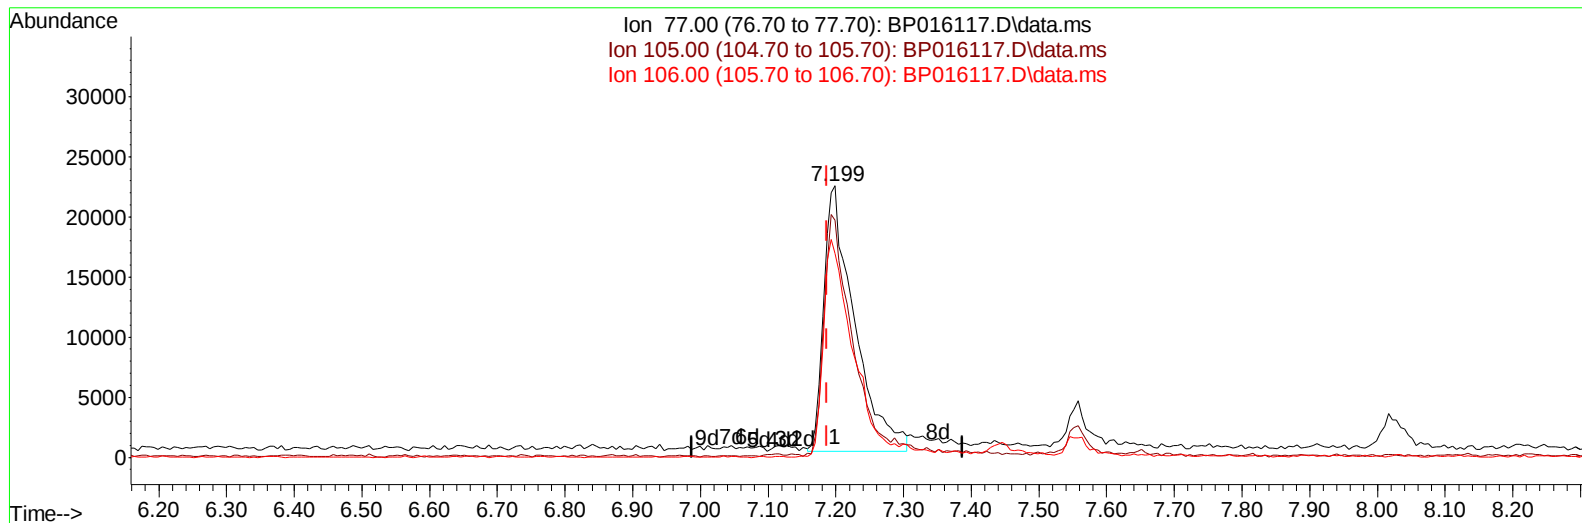

TIC: BP016117.D\data.ms

(6) Benzaldehyde

7.199min (+ 0.012) 12.96 ng/ul m

response 69519

Ion	Exp%	Act%
77.00	100.00	100.00
105.00	91.70	87.31
106.00	83.30	75.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:33:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

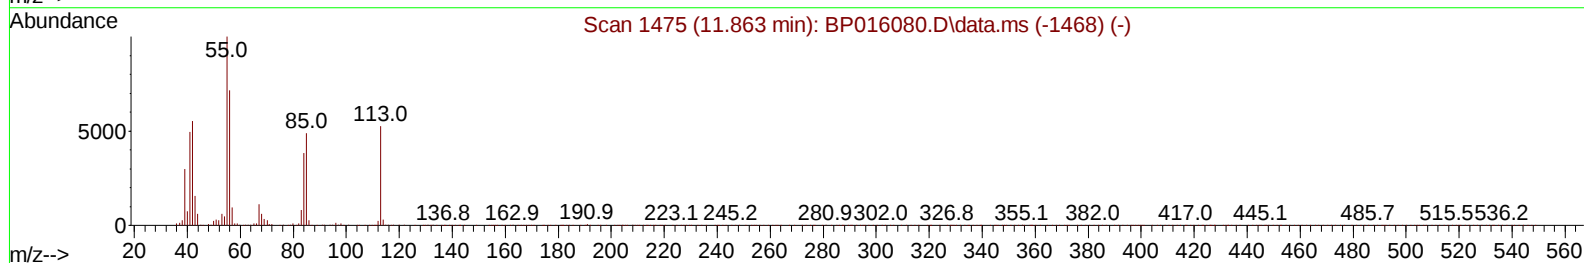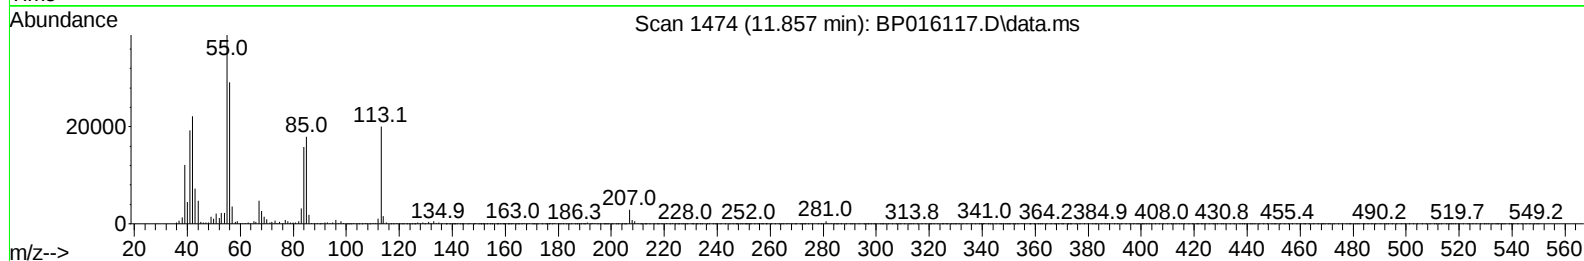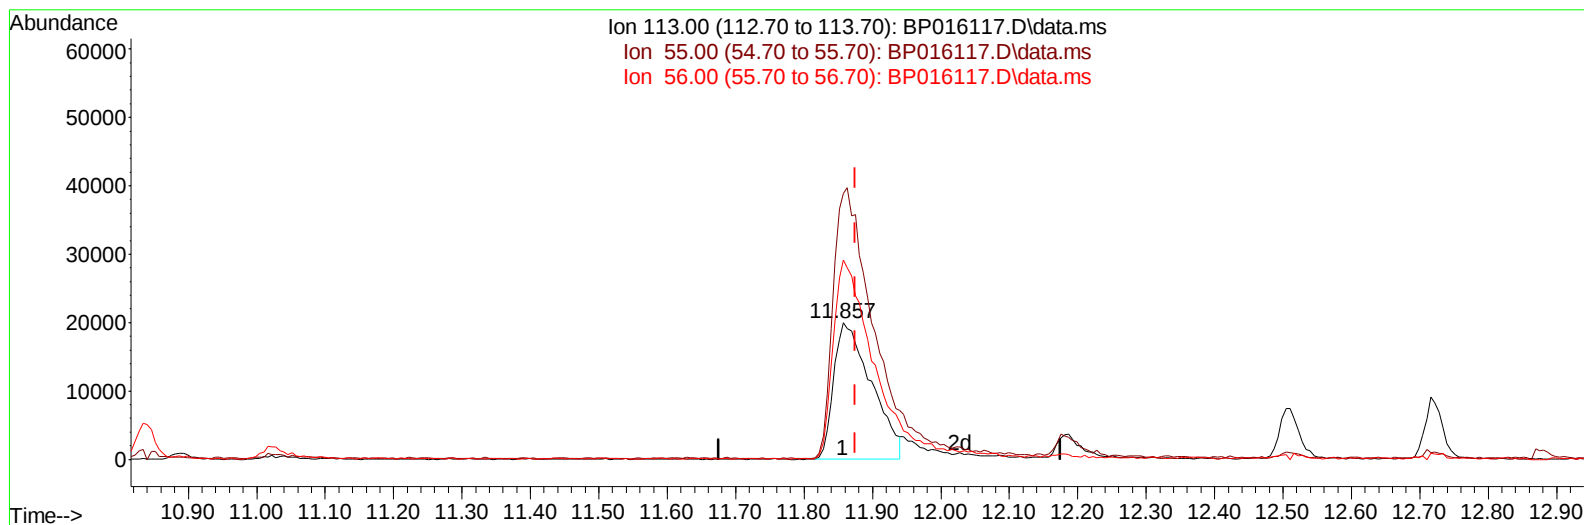

TIC: BP016117.D\data.ms

(34) Caprolactam

11.857min (-0.018) 22.18 ng/ul

response 76256

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	178.50	194.48
56.00	146.10	145.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:33:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

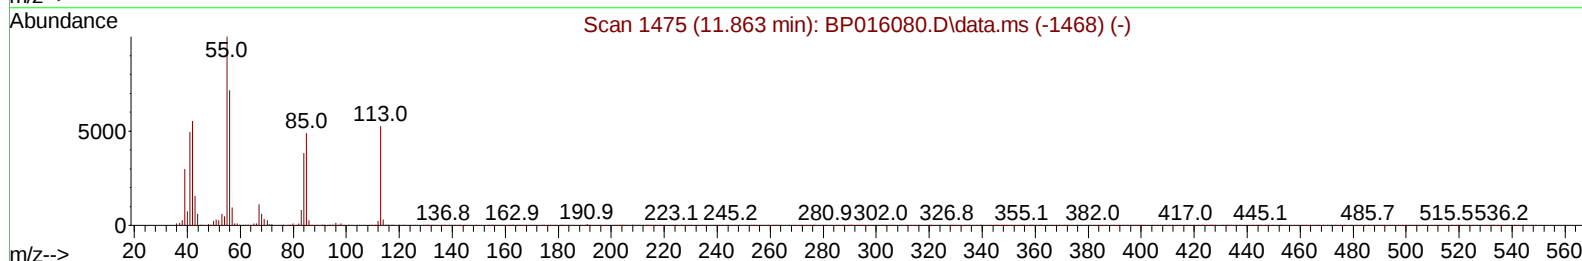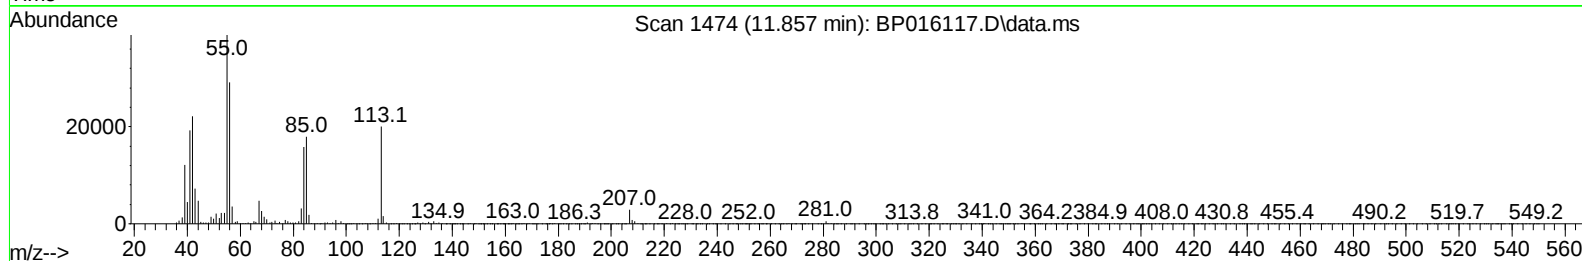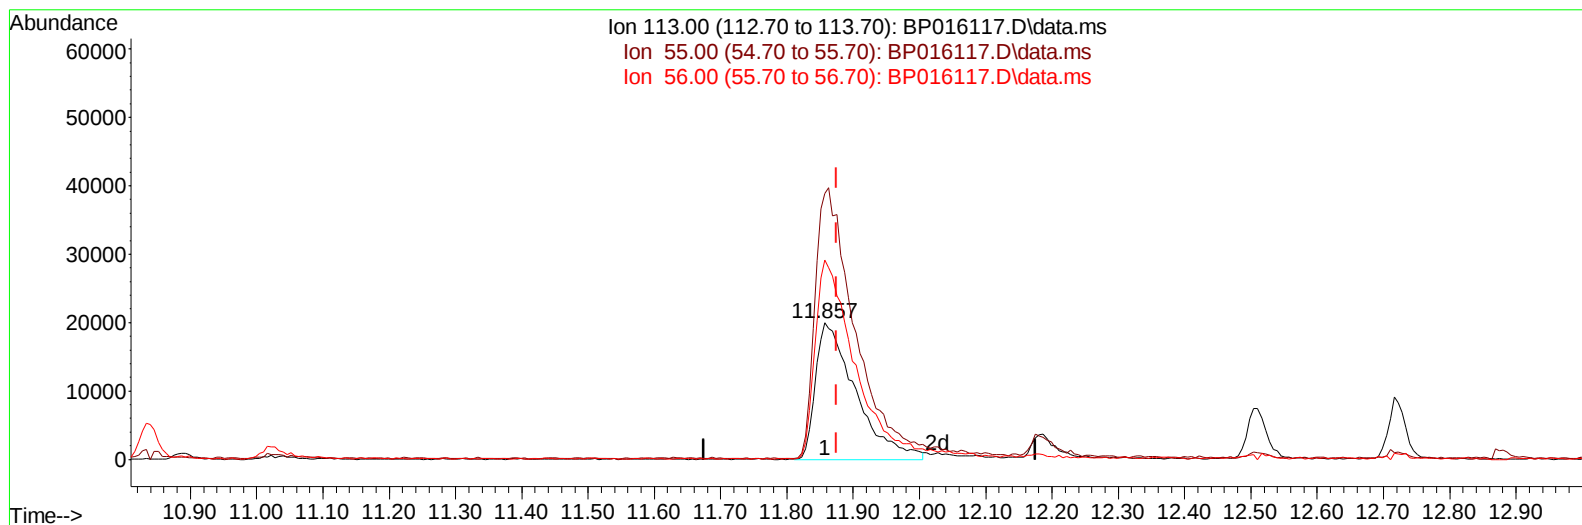

TIC: BP016117.D\data.ms

(34) Caprolactam

11.857min (-0.018) 24.40 ng/ul m

response 83891

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	178.50	194.48
56.00	146.10	145.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:35:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

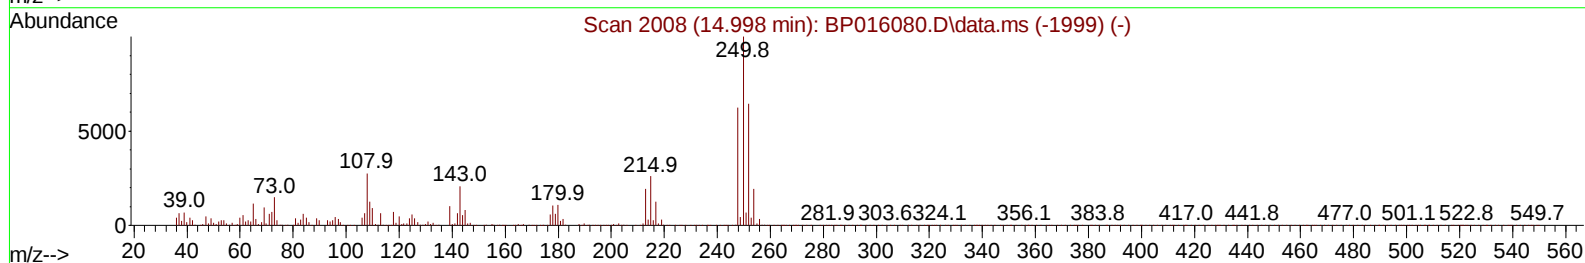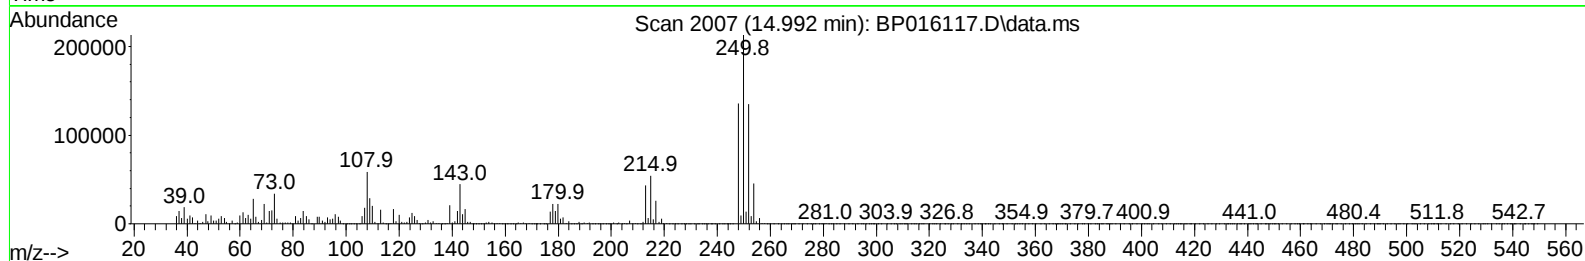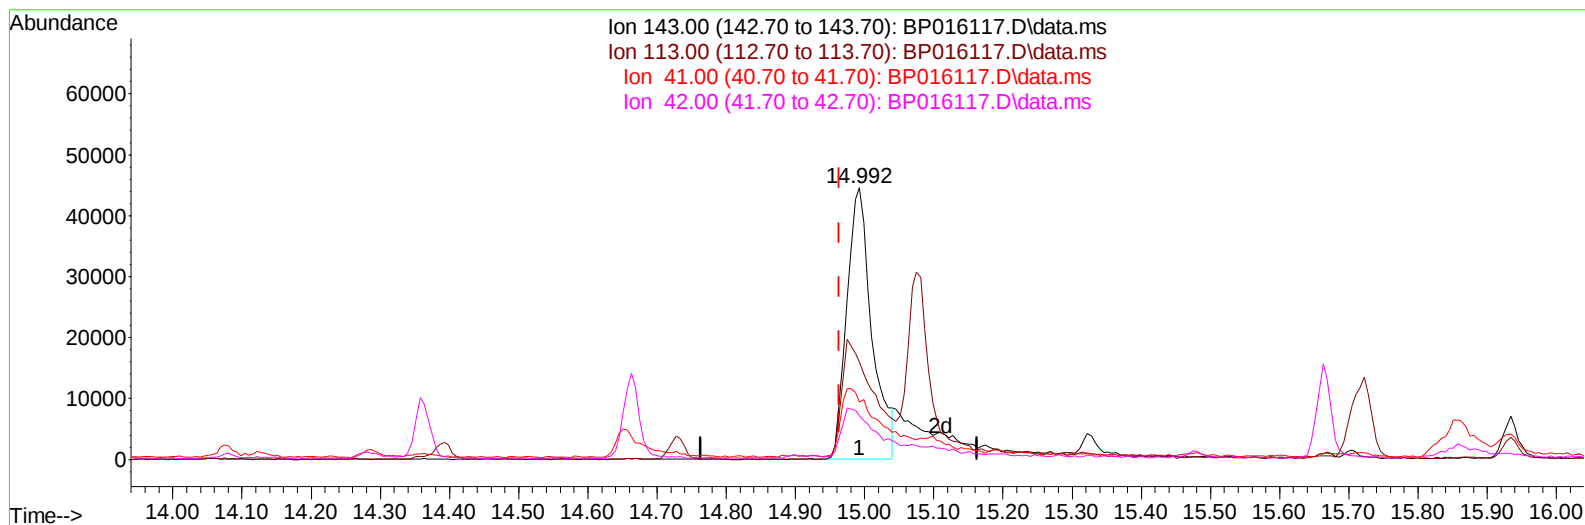

TIC: BP016117.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.992min (+ 0.029) 23.54 ng/u1

response 111853

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	35.99#
41.00	45.70	21.05#
42.00	31.20	16.12#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016117.D
Acq On : 09 Jul 2023 06:02
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:35:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

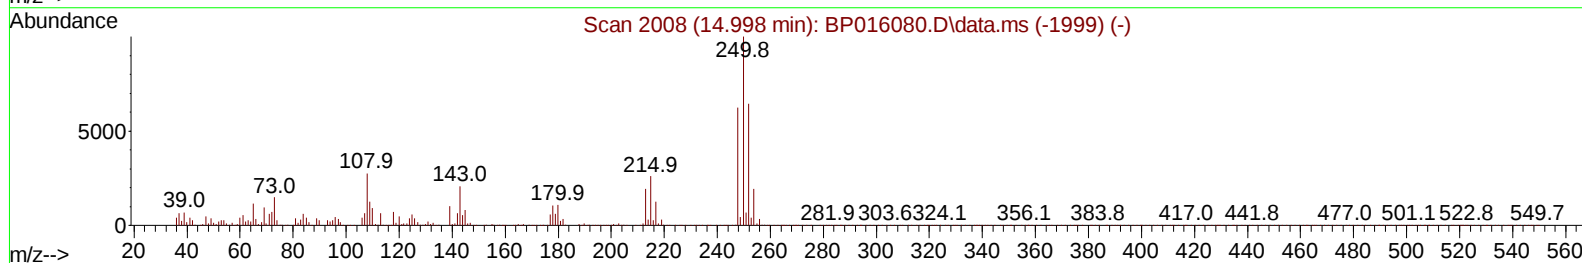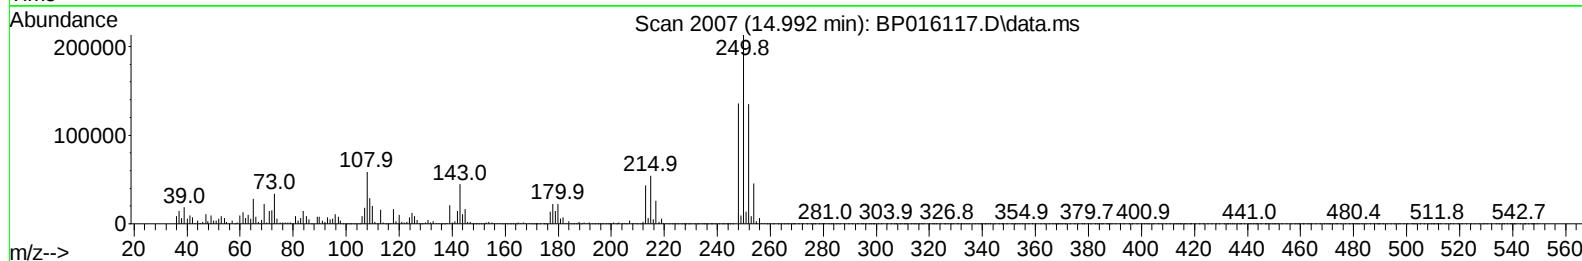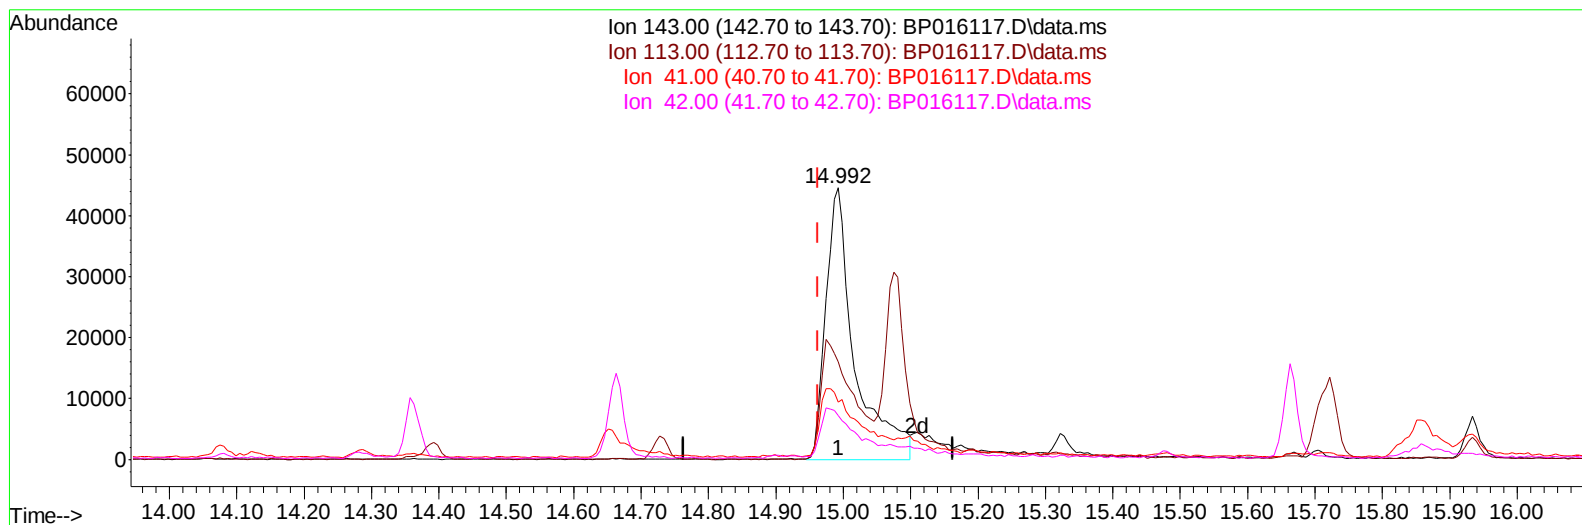

TIC: BP016117.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.992min (+ 0.029) 27.87 ng/ul m

response 132437

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	35.99#
41.00	45.70	21.05#
42.00	31.20	16.12#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:36:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

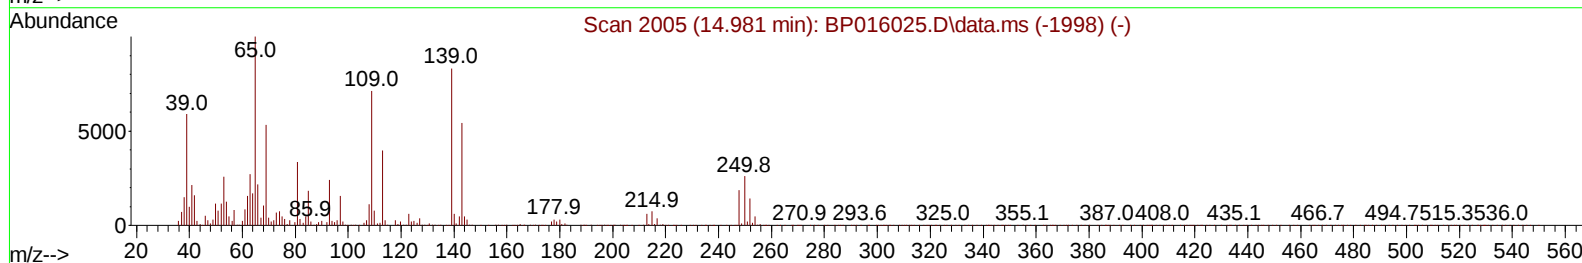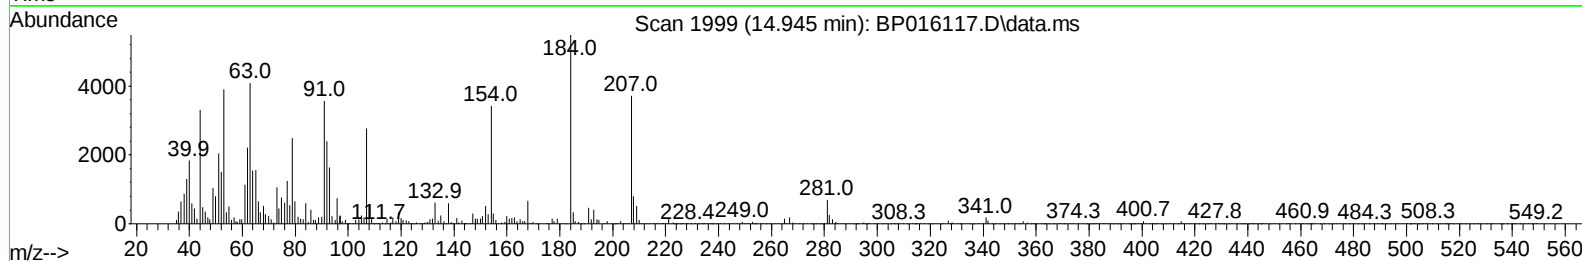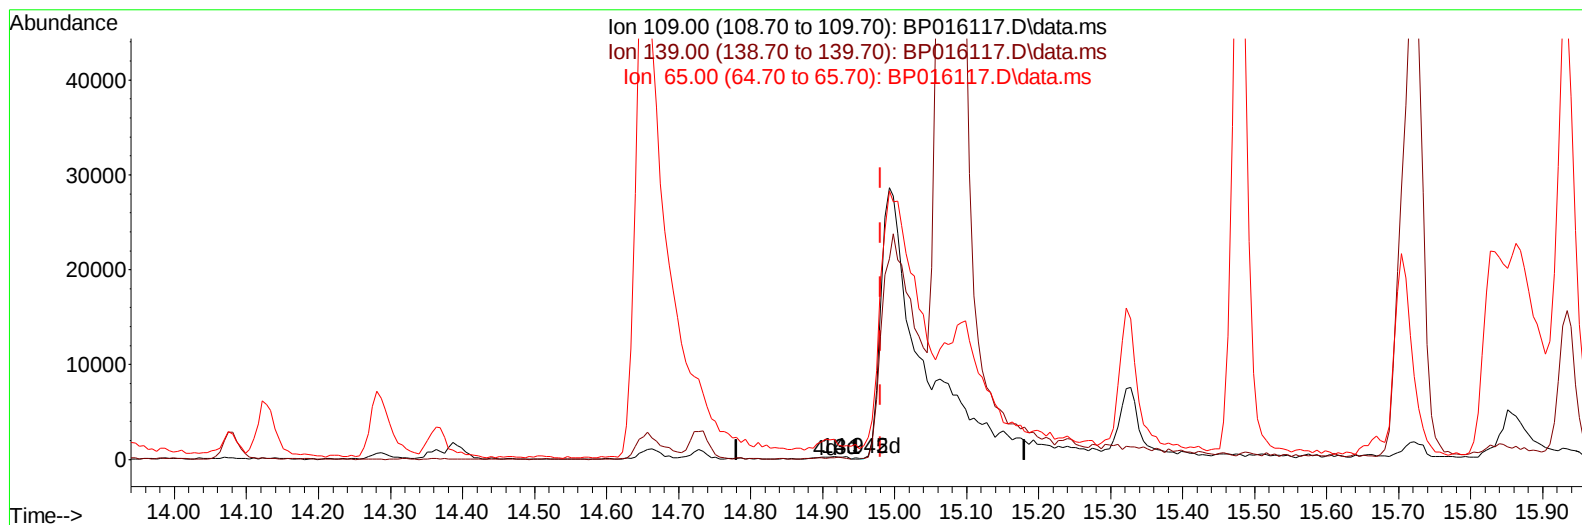

TIC: BP016117.D\data.ms

(55) 4-Nitrophenol

14.945min (-0.035) 0.02 ng/ul

response 82

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	101.60	46.26#
65.00	124.90	1061.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:36:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

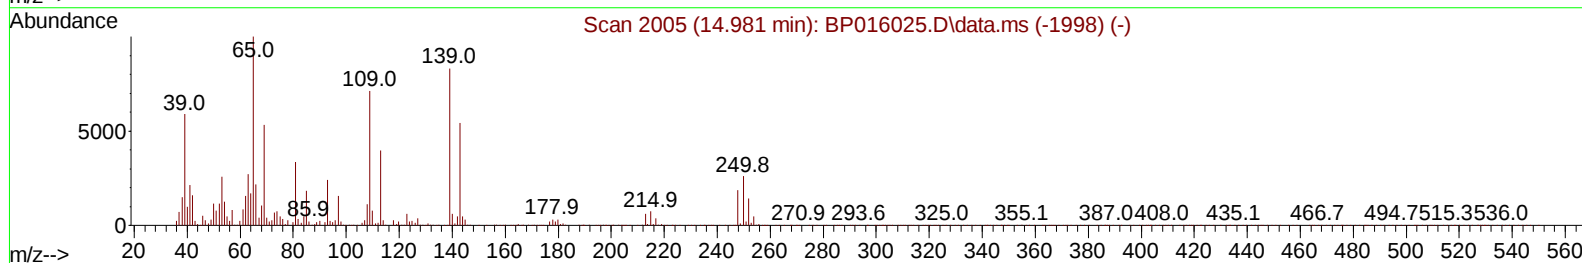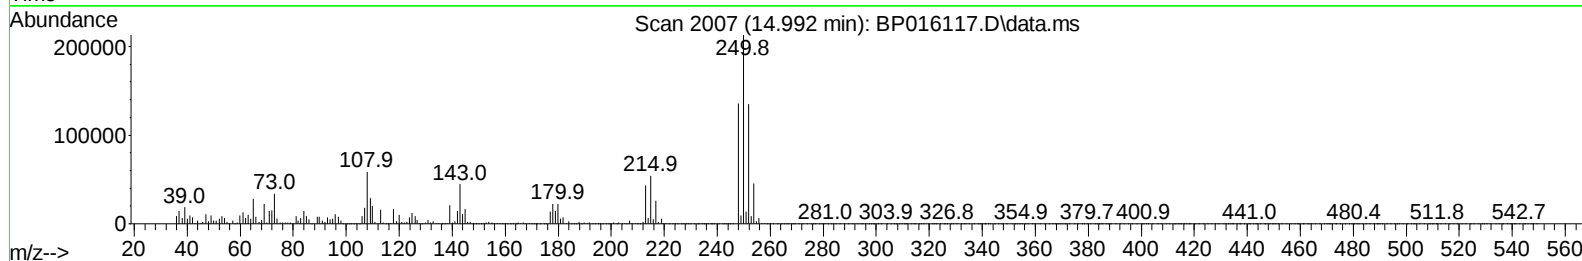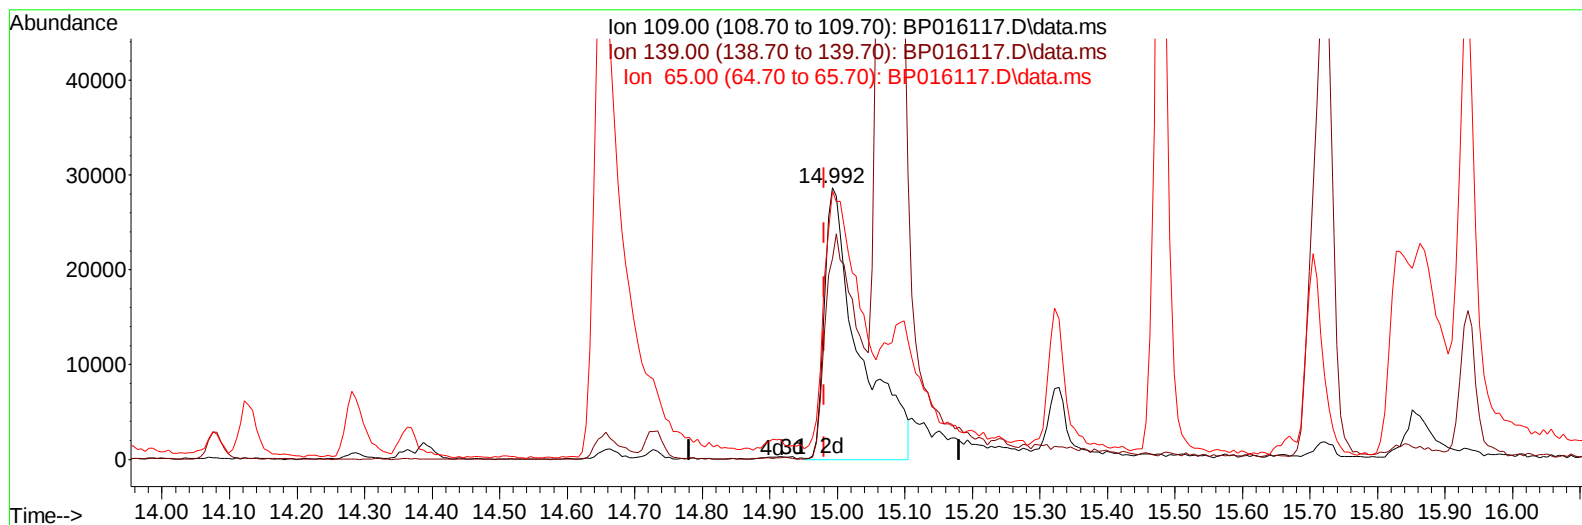

TIC: BP016117.D\data.ms

(55) 4-Nitrophenol

14.992min (+ 0.012) 20.73 ng/ul m

response 102064

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	101.60	74.01#
65.00	124.90	98.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:36:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

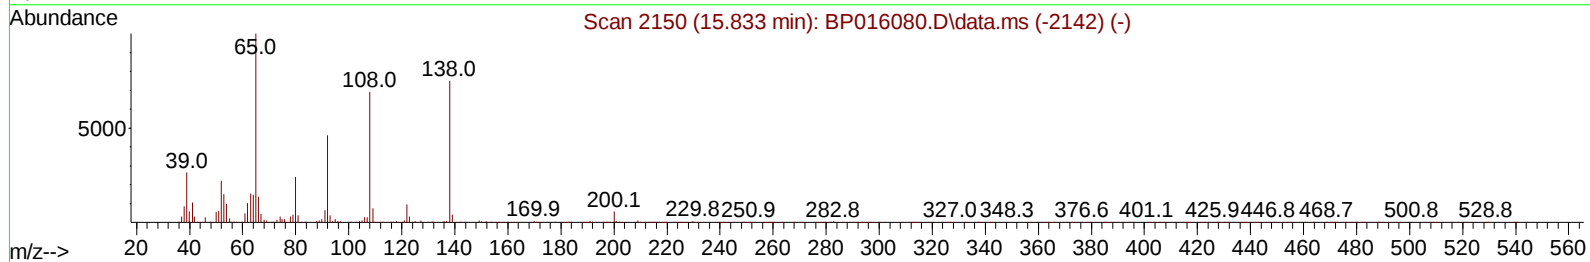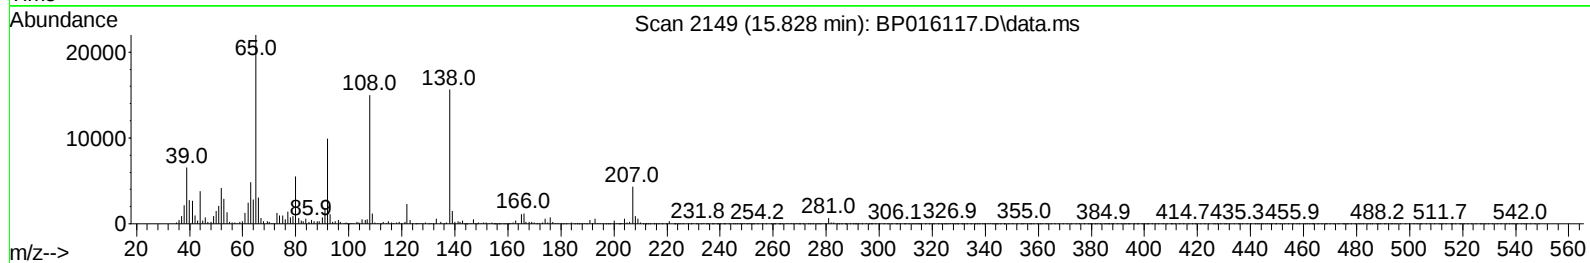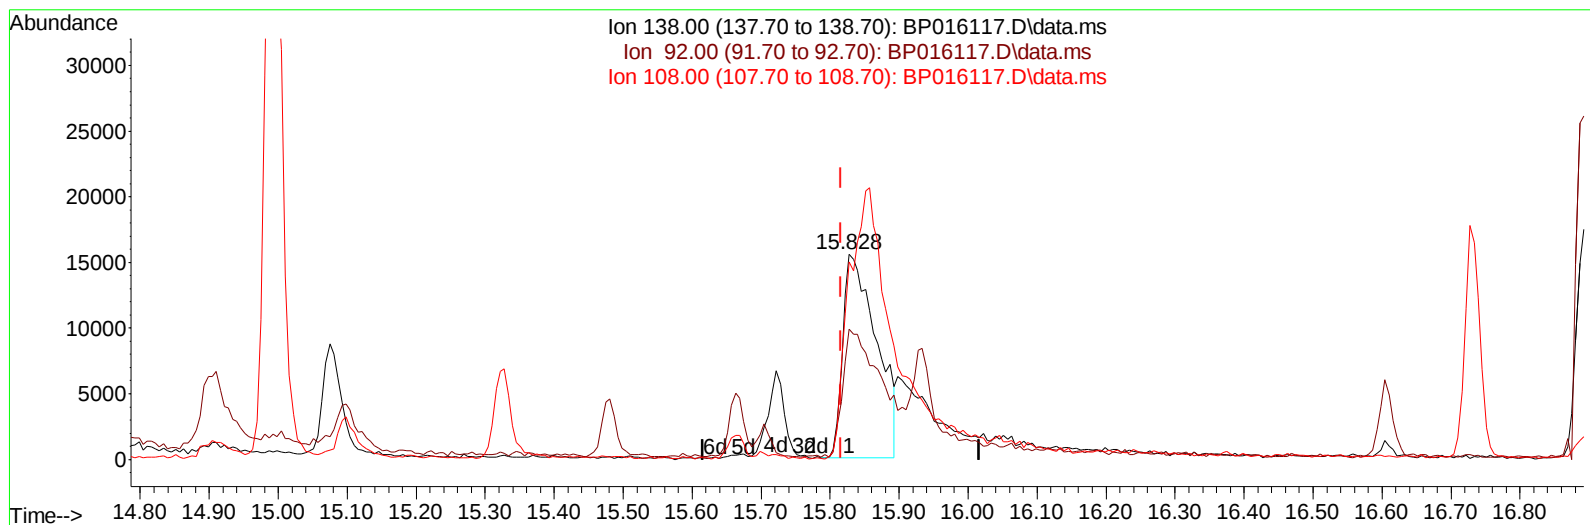

TIC: BP016117.D\data.ms

(63) 4-Nitroaniline

15.828min (+ 0.012) 12.98 ng/ul

response 52642

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	62.60	63.35
108.00	106.90	96.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:36:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

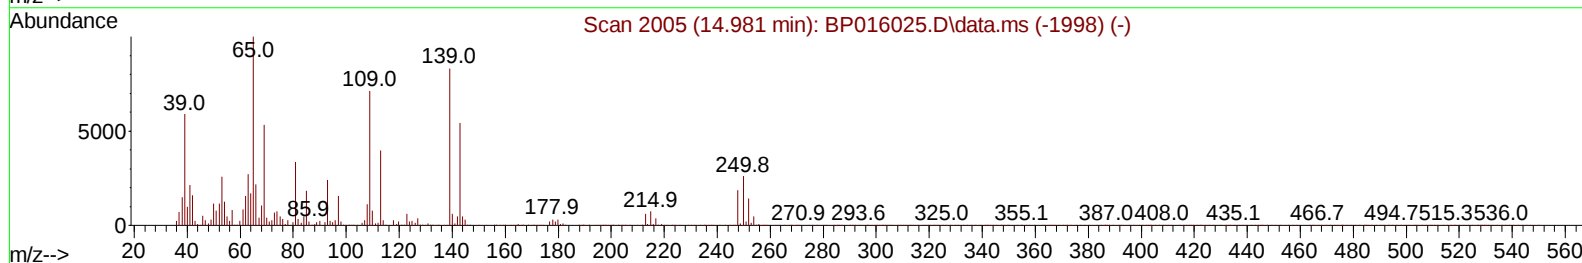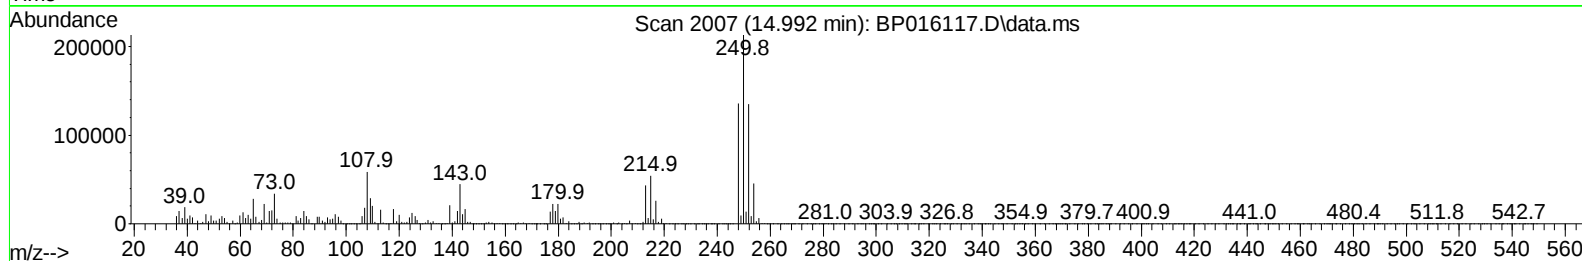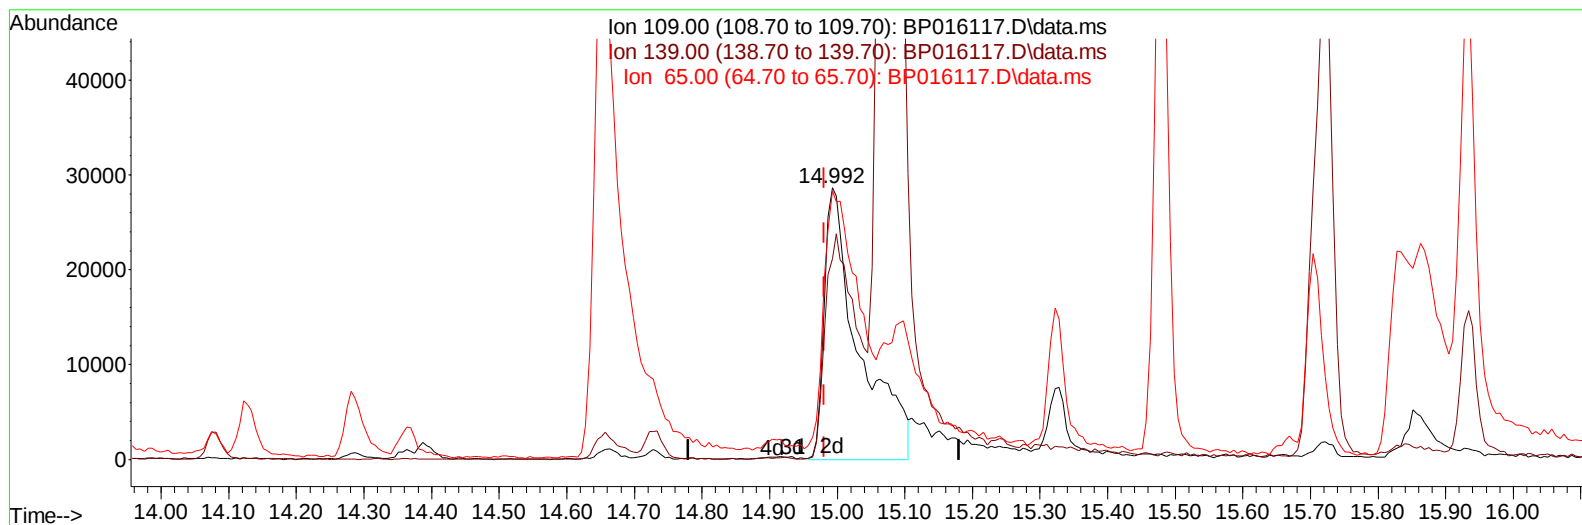

TIC: BP016117.D\data.ms

(55) 4-Nitrophenol

14.992min (+ 0.012) 20.72 ng/ul m

response 102016

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	101.60	74.01#
65.00	124.90	98.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:37:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

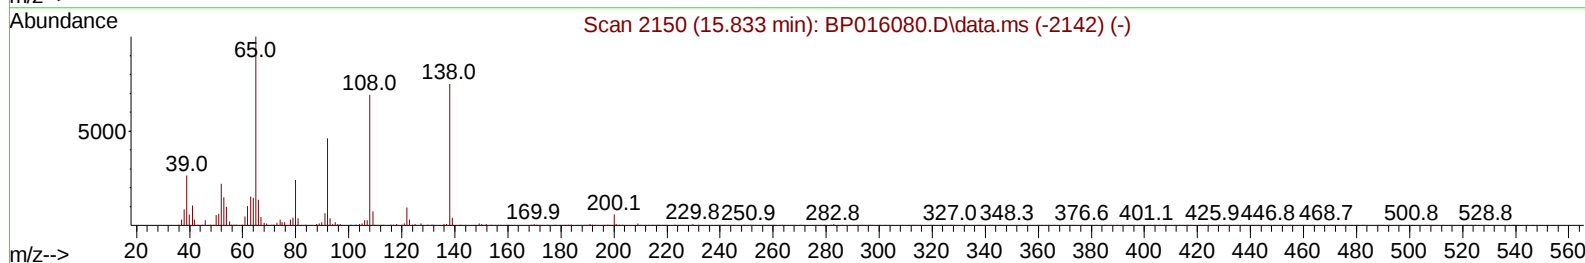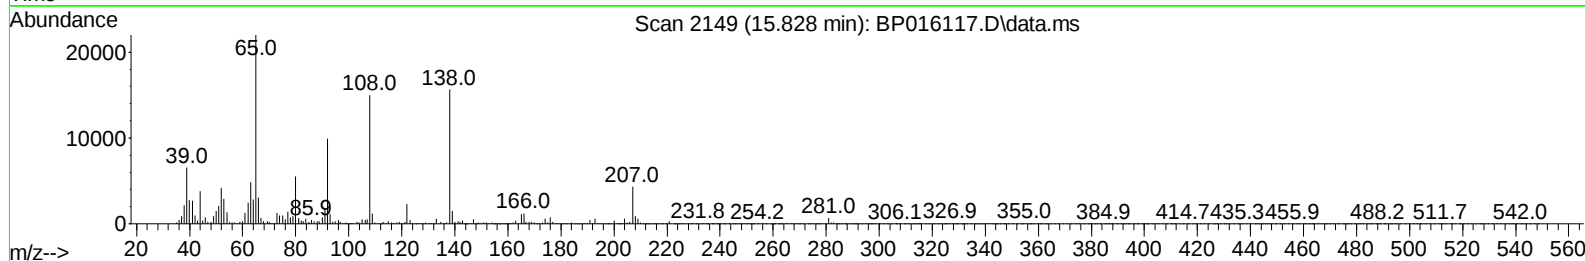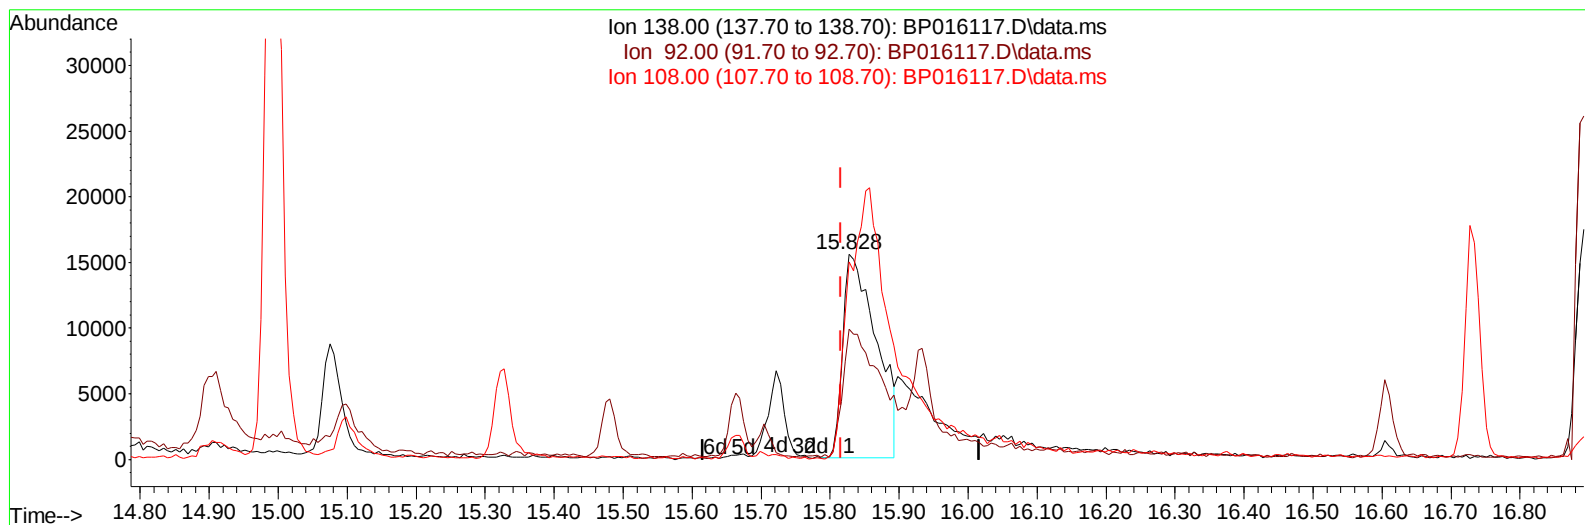

TIC: BP016117.D\data.ms

(63) 4-Nitroaniline

15.828min (+ 0.012) 12.98 ng/ul

response 52642

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	62.60	63.35
108.00	106.90	96.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:37:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

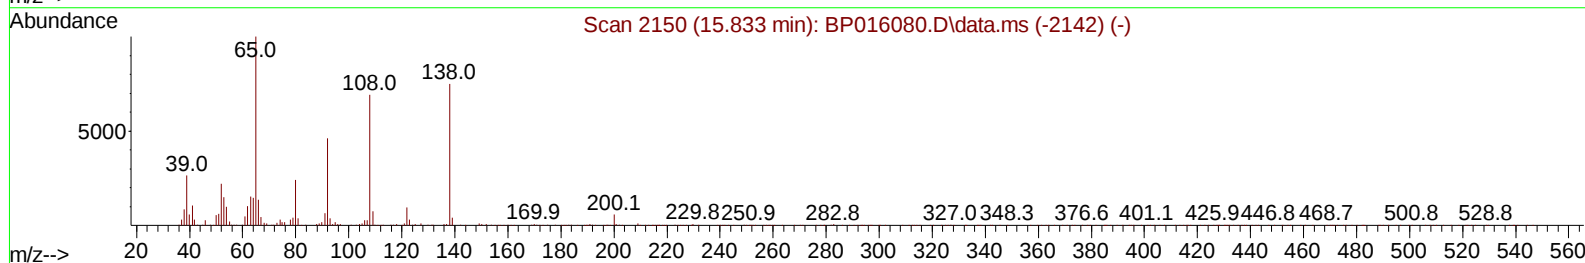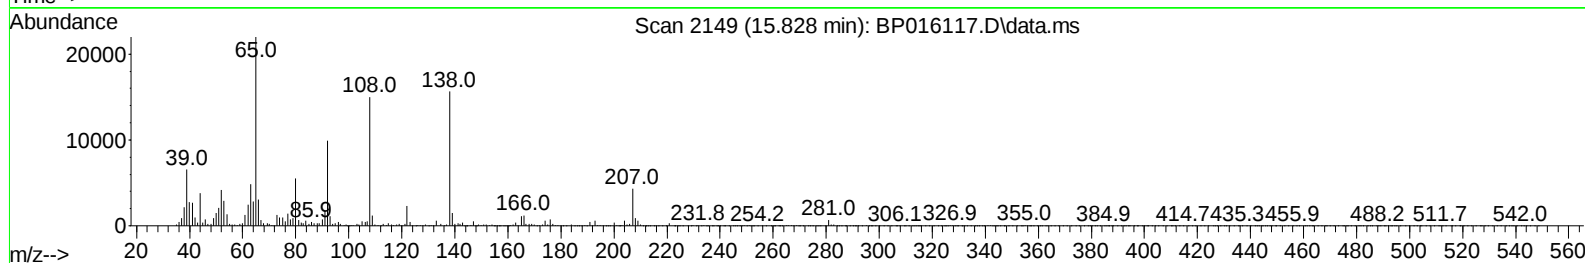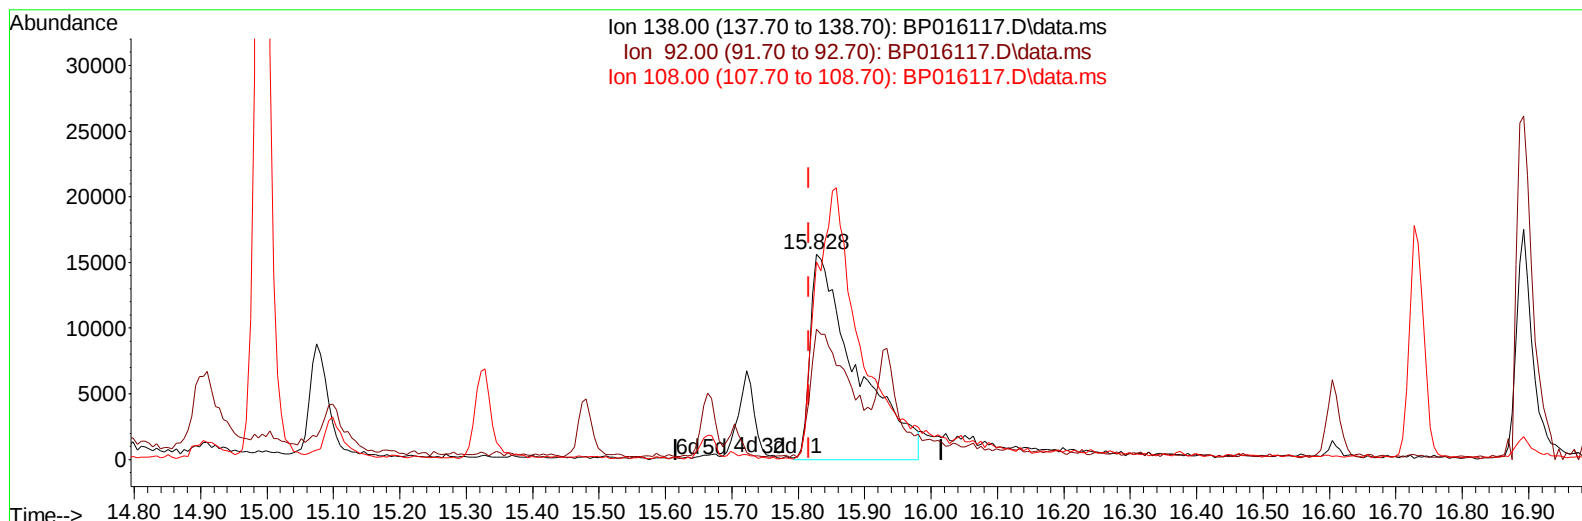

TIC: BP016117.D\data.ms

(63) 4-Nitroaniline

15.828min (+ 0.012) 18.46 ng/ul m

response 74883

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	62.60	63.35
108.00	106.90	96.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:37:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	155115	20.000	ng/ul	0.00
20) Naphthalene-d8	10.840	136	711329	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.663	164	465835	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.428	188	1093559	20.000	ng/ul	#-0.02
79) Chrysene-d12	21.527	240	1117236	20.000	ng/ul	#-0.01
88) Perylene-d12	24.074	264	1190332	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	38992	9.044	ng/uL	0.00
4) Pyridine-d5	3.799	84	224445	20.652	ng/ul	0.00
7) Phenol-d5	7.211	99	294483	22.189	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	194293	23.663	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.552	132	222264	22.185	ng/ul	-0.01
15) 4-Methylphenol-d8	8.763	113	225269	21.486	ng/ul	0.00
21) Nitrobenzene-d5	9.210	128	107006	19.684	ng/ul	0.00
24) 2-Nitrophenol-d4	9.946	143	128012	20.176	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	231185	20.447	ng/ul	0.00
31) 4-Chloroaniline-d4	11.022	131	346179	23.835	ng/ul	0.00
46) Dimethylphthalate-d6	14.081	166	777457	21.593	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	886375	21.899	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.992	143	132437m	27.873	ng/ul	0.03
60) Fluorene-d10	15.663	176	669697	22.589	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.857	200	110825	16.479	ng/ul	0.00
73) Anthracene-d10	17.534	188	1091316	21.847	ng/ul	-0.01
81) Pyrene-d10	19.769	212	1340786	18.379	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.898	264	1303121	21.702	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.381	88	41788	9.007	ng/uL	95
5) Pyridine	3.817	79	241535	21.244	ng/ul	99
6) Benzaldehyde	7.199	77	69519m	12.956	ng/ul	
8) Phenol	7.240	94	314679	22.848	ng/ul	93
10) Bis(2-Chloroethyl)ether	7.440	93	261689	23.881	ng/ul	96
12) 2-Chlorophenol	7.587	128	235981	22.171	ng/ul	95
13) 2-Methylphenol	8.493	108	244030	23.468	ng/ul	96
14) 2,2'-oxybis(1-Chloropr...	8.552	45	410859	27.452	ng/ul	99
16) Acetophenone	8.869	105	408025	23.674	ng/ul	91
17) N-Nitroso-di-n-propyla...	8.834	70	229208	23.945	ng/ul	97
18) 4-Methylphenol	8.840	108	267846	23.973	ng/ul	99
19) Hexachloroethane	9.081	117	109895	22.355	ng/ul	89
22) Nitrobenzene	9.258	77	329832	21.606	ng/ul	98
23) Isophorone	9.775	82	643369	22.023	ng/ul	99
25) 2-Nitrophenol	9.975	139	137936	20.485	ng/ul	97
26) 2,4-Dimethylphenol	10.040	107	308125	20.816	ng/ul	98
27) Bis(2-Chloroethoxy)met...	10.263	93	379817	23.031	ng/ul	100
29) 2,4-Dichlorophenol	10.540	162	233817	20.801	ng/ul	97
30) Naphthalene	10.887	128	857088	22.164	ng/ul	99
32) 4-Chloroaniline	11.052	127	372033	24.654	ng/ul	97
33) Hexachlorobutadiene	11.146	225	157293	18.530	ng/ul	99
34) Caprolactam	11.857	113	83891m	24.399	ng/ul	
35) 4-Chloro-3-methylphenol	12.181	107	280376	21.309	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016117.D
 Acq On : 09 Jul 2023 06:02
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 LabSampleId :
 SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:37:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 08 10:11:43 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/10/2023
 Supervised By :mohammad ahmed 07/10/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.510	142	562263	22.088	ng/ul	98
37) 1-Methylnaphthalene	12.722	142	576391	22.196	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.881	216	305196	19.881	ng/ul	97
40) Hexachlorocyclopentadiene	12.816	237	55134	12.005	ng/ul	94
41) 2,4,6-Trichlorophenol	13.140	196	190716	19.659	ng/ul	99
42) 2,4,5-Trichlorophenol	13.240	196	209108	20.321	ng/ul	99
43) 1,1'-Biphenyl	13.498	154	789940	21.409	ng/ul#	97
44) 2-Chloronaphthalene	13.557	162	611109	21.024	ng/ul	98
45) 2-Nitroaniline	13.804	65	199897	21.857	ng/ul	95
47) Dimethylphthalate	14.128	163	817275	21.933	ng/ul	99
48) 2,6-Dinitrotoluene	14.287	165	160945	21.293	ng/ul	99
50) Acenaphthylene	14.393	152	993247	22.271	ng/ul	99
51) 3-Nitroaniline	14.651	138	99729	16.825	ng/ul#	83
52) Acenaphthene	14.728	153	694729	22.464	ng/ul	98
53) 2,4-Dinitrophenol	14.904	184	54199	13.516	ng/ul	91
55) 4-Nitrophenol	14.992	109	102016m	20.719	ng/ul	
56) Dibenzofuran	15.075	168	971689	22.634	ng/ul	99
57) 2,4-Dinitrotoluene	15.098	165	239497	23.252	ng/ul	89
58) 2,3,4,6-Tetrachlorophenol	15.328	232	190620	21.567	ng/ul	98
59) Diethylphthalate	15.481	149	862740	22.879	ng/ul	99
61) Fluorene	15.722	166	800454	22.987	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.704	204	385585	21.640	ng/ul	97
63) 4-Nitroaniline	15.828	138	74883m	18.459	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.875	198	116868	17.175	ng/ul#	89
67) N-Nitrosodiphenylamine	15.934	169	669128	20.439	ng/ul	98
68) 4-Bromophenyl-phenylether	16.610	248	234423	18.772	ng/ul	91
69) Hexachlorobenzene	16.734	284	287826	19.534	ng/ul	96
70) Atrazine	16.892	200	245325	19.577	ng/ul	98
71) Pentachlorophenol	17.116	266	127346	18.007	ng/ul	93
72) Phenanthrene	17.475	178	1322203	22.256	ng/ul	100
74) Anthracene	17.575	178	1344069	22.516	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.475	216	316946	17.812	ng/uL	99
76) Pentachlorobenzene	14.992	250	329520	18.348	ng/uL	99
77) Carbazole	17.869	167	1206931	23.988	ng/ul	99
78) Di-n-butylphthalate	18.363	149	1571832	23.565	ng/ul	99
80) Fluoranthene	19.445	202	1633543	18.017	ng/ul#	95
82) Pyrene	19.804	202	1735131	18.761	ng/ul#	92
83) Butylbenzylphthalate	20.639	149	790482	20.950	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.451	252	501527	19.858	ng/ul	99
85) Benzo(a)anthracene	21.510	228	1640593	20.875	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.380	149	1160590	22.382	ng/ul	99
87) Chrysene	21.574	228	1706788	22.890	ng/ul	99
89) Di-n-octyl phthalate	22.333	149	1994599	22.929	ng/ul	100
90) Benzo(b)fluoranthene	23.280	252	1596384	20.872	ng/ul#	97
91) Benzo(k)fluoranthene	23.333	252	1780945	23.046	ng/ul#	98
93) Benzo(a)pyrene	23.957	252	1476369	22.091	ng/ul#	96
94) Indeno(1,2,3-cd)pyrene	26.762	276	1723238	18.994	ng/ul#	93
95) Dibenzo(a,h)anthracene	26.762	278	1433632	19.238	ng/ul#	94
96) Benzo(g,h,i)perylene	27.609	276	1377614	18.458	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_P
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/10/2023
Supervised By :mohammad ahmed 07/10/2023

Manual IntegrationsAPPROVED

Quant Time: Jul 09 06:37:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 08 10:11:43 2023
Response via : Initial Calibration

