

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016081.D
 Acq On : 08 Jul 2023 08:27
 Operator : MA/JU
 Sample : PB153818BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK818

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	36	rVB2	29083	47900	0.52%	0.071%
2	3.805	102	105	125	rBV	305726	696999	7.54%	1.039%
3	7.246	683	690	706	rBV2	248477	909696	9.84%	1.356%
4	7.369	706	711	718	rBV	174626	379427	4.10%	0.566%
5	7.581	740	747	777	rVB	287072	804555	8.70%	1.200%
6	8.034	815	824	852	rBV	292910	1035219	11.20%	1.544%
7	8.793	945	953	979	rBV	411792	1616445	17.49%	2.410%
8	9.240	1022	1029	1058	rBV	359082	1142692	12.36%	1.704%
9	9.981	1146	1155	1178	rBV2	257430	1068081	11.55%	1.593%
10	10.557	1246	1253	1272	rBV	296404	1363909	14.75%	2.034%
11	10.857	1297	1304	1322	rBV	569231	1543008	16.69%	2.301%
12	11.057	1330	1338	1373	rBV	398431	1907552	20.64%	2.844%
13	12.457	1570	1576	1580	rBV8	9566	22313	0.24%	0.033%
14	12.528	1583	1588	1595	rVB5	9288	23170	0.25%	0.035%
15	14.022	1837	1842	1847	rBV7	5561	9247	0.10%	0.014%
16	14.093	1847	1854	1883	rBV	2030107	4606134	49.83%	6.868%
17	14.375	1894	1902	1930	rBV	2586005	4583203	49.58%	6.834%
18	14.675	1946	1953	1972	rBV	1286298	2209561	23.90%	3.295%
19	14.998	1999	2008	2043	rBV2	252106	1606205	17.38%	2.395%
20	15.687	2117	2125	2149	rBV	2747812	6293572	68.08%	9.385%
21	15.863	2149	2155	2186	rVV	571994	1983194	21.45%	2.957%
22	16.469	2255	2258	2263	rBV7	7616	13594	0.15%	0.020%
23	17.116	2364	2368	2374	rBV9	8271	15347	0.17%	0.023%
24	17.439	2416	2423	2435	rBV	1837493	2804175	30.34%	4.181%
25	17.545	2435	2441	2476	rVB2	2958543	7506513	81.21%	11.193%
26	19.357	2745	2749	2754	rBV2	65433	90272	0.98%	0.135%
27	19.433	2759	2762	2768	rVV	41308	62719	0.68%	0.094%
28	19.775	2814	2820	2854	rBV	4100071	9243805	100.00%	13.784%
29	21.557	3118	3123	3138	rBV	1295577	3068579	33.20%	4.576%
30	23.910	3516	3523	3545	rVB2	2815907	7552660	81.71%	11.262%
31	24.086	3547	3553	3576	rVB	769142	2853056	30.86%	4.254%




Sum of corrected areas: 67062802

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016081.D
Acq On : 08 Jul 2023 08:27
Operator : MA/JU
Sample : PB153818BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

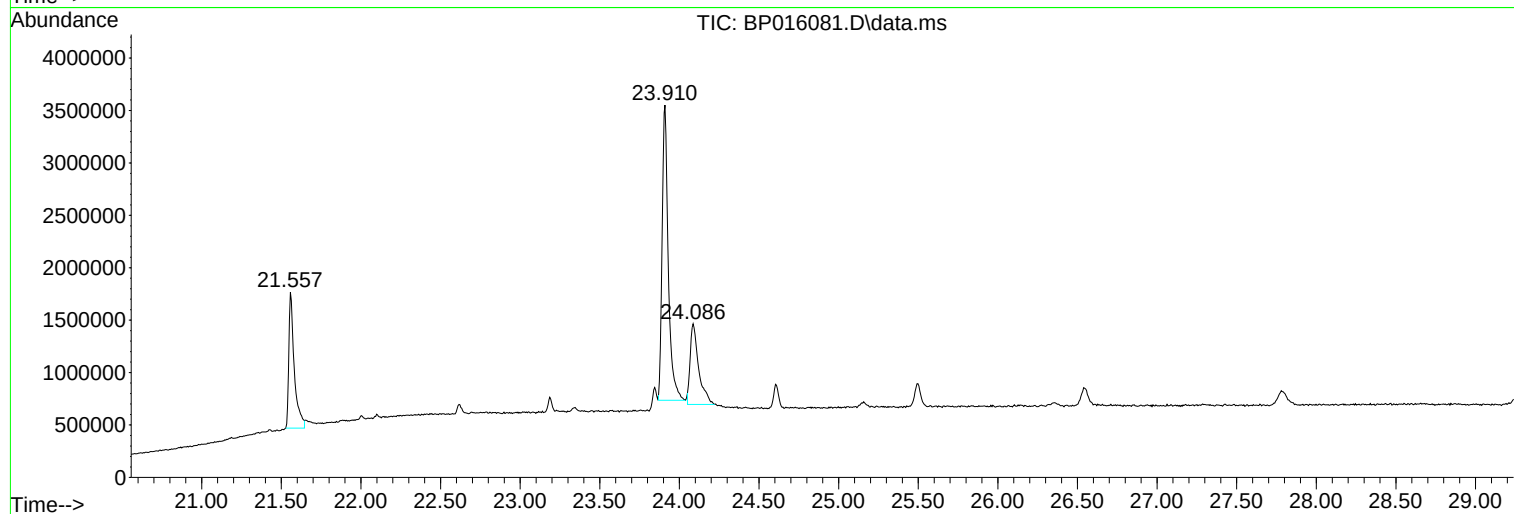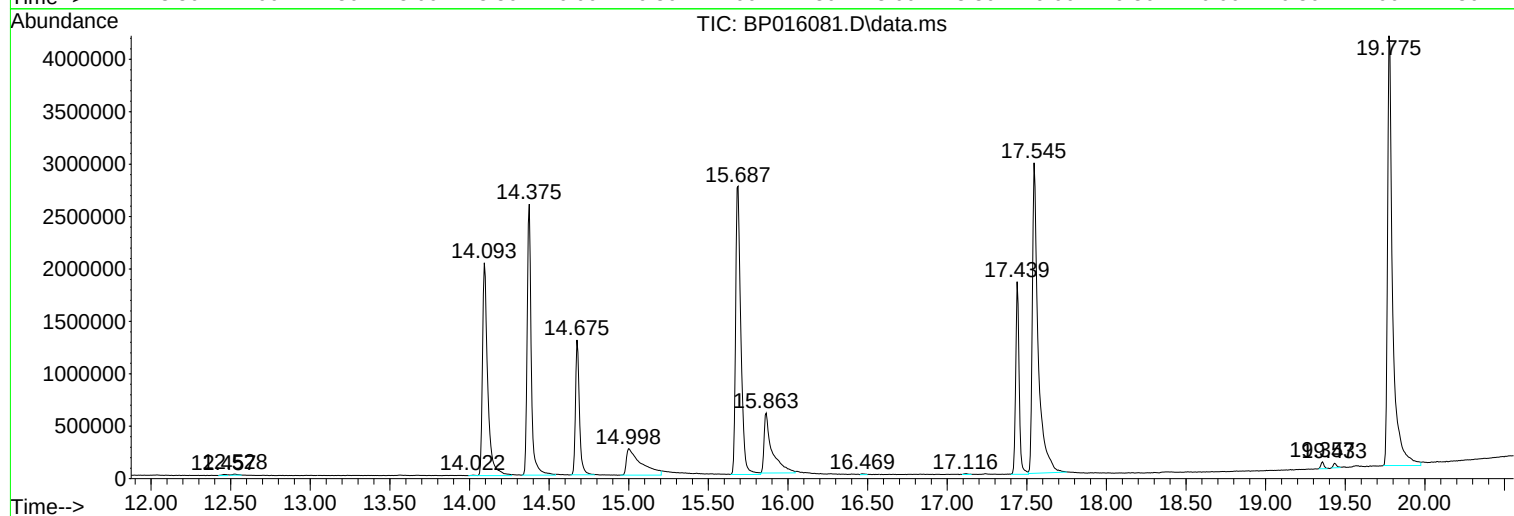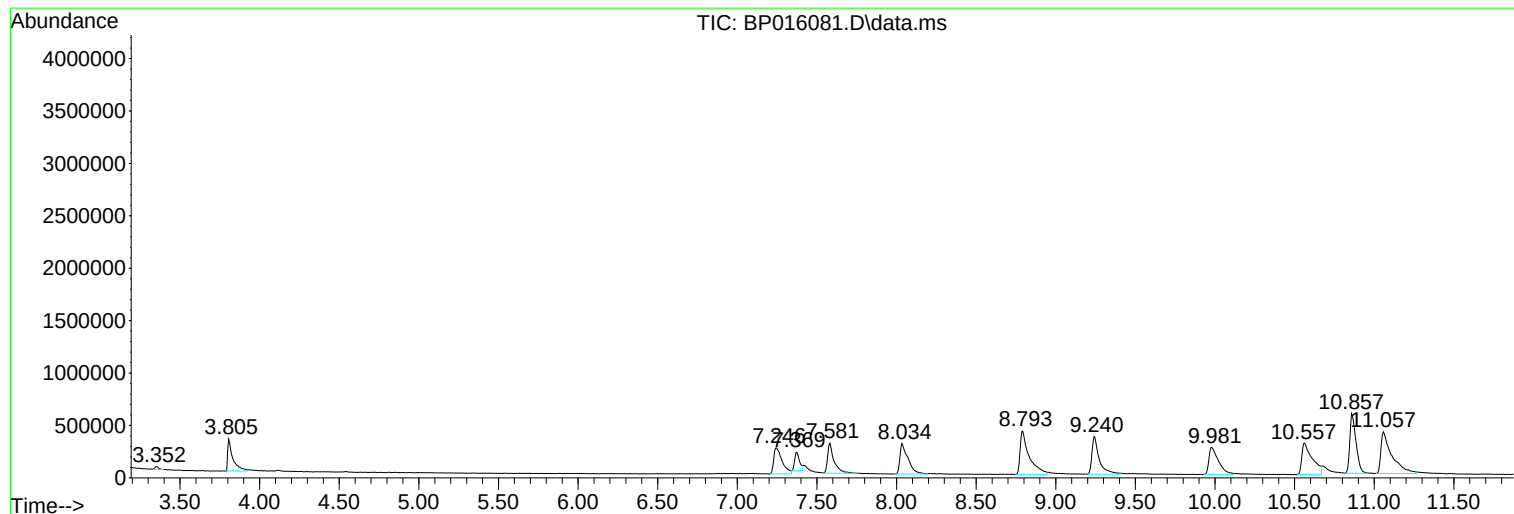

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016081.D
Acq On : 08 Jul 2023 08:27
Operator : MA/JU
Sample : PB153818BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016081.D
Acq On : 08 Jul 2023 08:27
Operator : MA/JU
Sample : PB153818BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc