

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016099.D
 Acq On : 08 Jul 2023 19:16
 Operator : MA/JU
 Sample : PB153818BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK818

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	38	rVB2	34862	59562	0.54%	0.072%
2	3.805	102	105	119	rBV	341226	718236	6.56%	0.874%
3	4.111	155	157	163	rBV4	8515	11509	0.11%	0.014%
4	7.234	681	688	705	rBV2	313816	1062433	9.70%	1.293%
5	7.369	705	711	737	rVV	245055	827746	7.55%	1.007%
6	7.575	739	746	772	rVB	345043	932110	8.51%	1.135%
7	8.028	816	823	843	rBV	348143	1151342	10.51%	1.401%
8	8.781	944	951	990	rBV	539904	1974737	18.02%	2.404%
9	9.234	1017	1028	1061	rBV	458726	1377868	12.58%	1.677%
10	9.969	1145	1153	1182	rBV	329813	1322730	12.07%	1.610%
11	10.546	1243	1251	1283	rBV	367334	1920387	17.53%	2.337%
12	10.857	1296	1304	1322	rVB	699743	1820872	16.62%	2.216%
13	11.046	1329	1336	1379	rBV	499955	2325832	21.23%	2.831%
14	12.457	1568	1576	1581	rBV6	11615	33806	0.31%	0.041%
15	12.522	1583	1587	1598	rVB5	12267	34671	0.32%	0.042%
16	13.557	1759	1763	1767	rBV5	7213	12716	0.12%	0.015%
17	14.087	1846	1853	1885	rBV	2435013	5540373	50.57%	6.743%
18	14.369	1892	1901	1922	rBV2	3132196	5509741	50.29%	6.706%
19	14.675	1946	1953	1972	rBV	1559202	2655701	24.24%	3.232%
20	14.993	2000	2007	2043	rBV2	330753	2008316	18.33%	2.444%
21	15.681	2116	2124	2146	rBV	3457190	7565910	69.05%	9.209%
22	15.857	2148	2154	2192	rVV	756412	2583876	23.58%	3.145%
23	16.263	2220	2223	2231	rVB8	6346	11400	0.10%	0.014%
24	16.469	2253	2258	2264	rBV10	7433	11864	0.11%	0.014%
25	17.110	2364	2367	2372	rVB7	9350	14496	0.13%	0.018%
26	17.434	2416	2422	2434	rBV	2142192	3322798	30.33%	4.044%
27	17.545	2434	2441	2469	rVV2	3678576	8912308	81.34%	10.848%
28	19.351	2744	2748	2753	rBV3	79149	112246	1.02%	0.137%
29	19.428	2758	2761	2768	rVV	49570	74406	0.68%	0.091%
30	19.775	2813	2820	2854	rBV	4756169	10956761	100.00%	13.336%
31	21.557	3117	3123	3148	rBV	1505015	4045930	36.93%	4.925%
32	23.845	3508	3512	3514	rBV	185810	292968	2.67%	0.357%
33	23.904	3514	3522	3543	rVV2	3414897	9585266	87.48%	11.667%
34	24.080	3545	3552	3576	rVB	943513	3367845	30.74%	4.099%

Sum of corrected areas: 82158762




Instrument :
BNA_P
ClientSampleId :
SBLK818

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016099.D
Acq On : 08 Jul 2023 19:16
Operator : MA/JU
Sample : PB153818BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

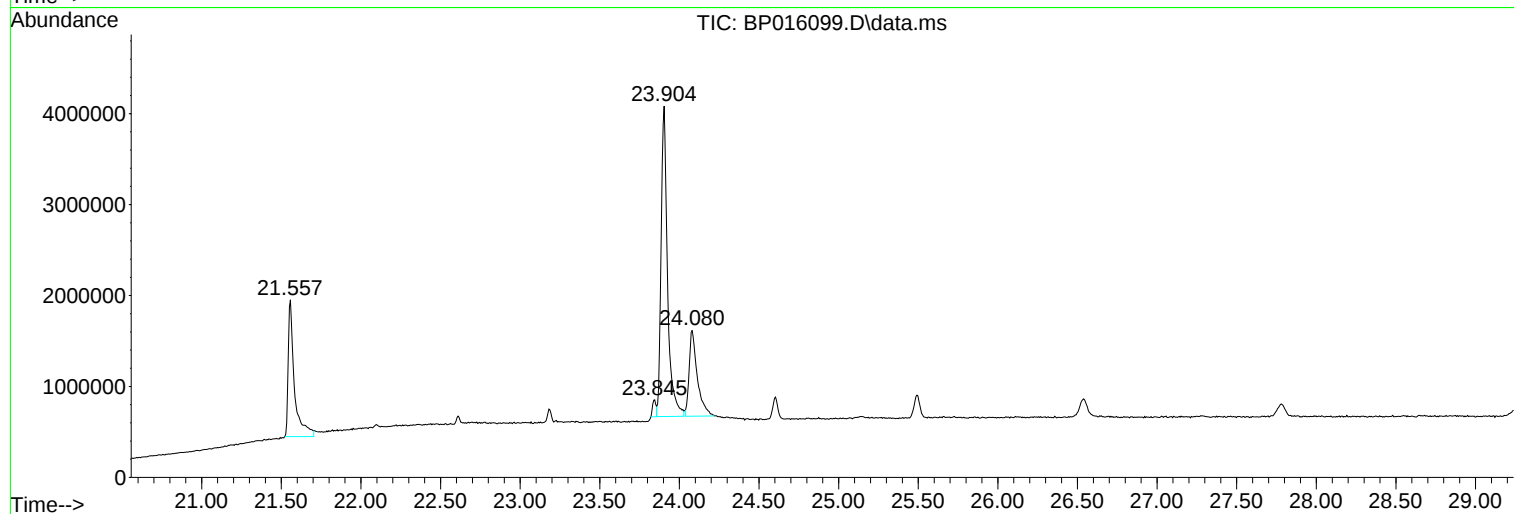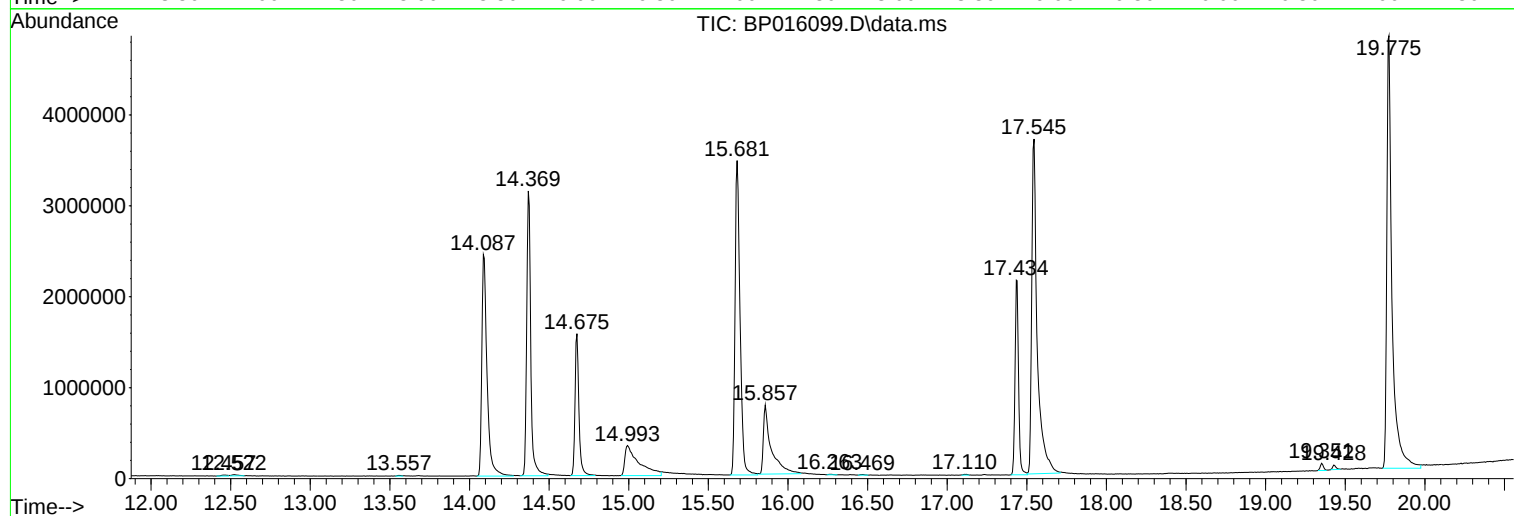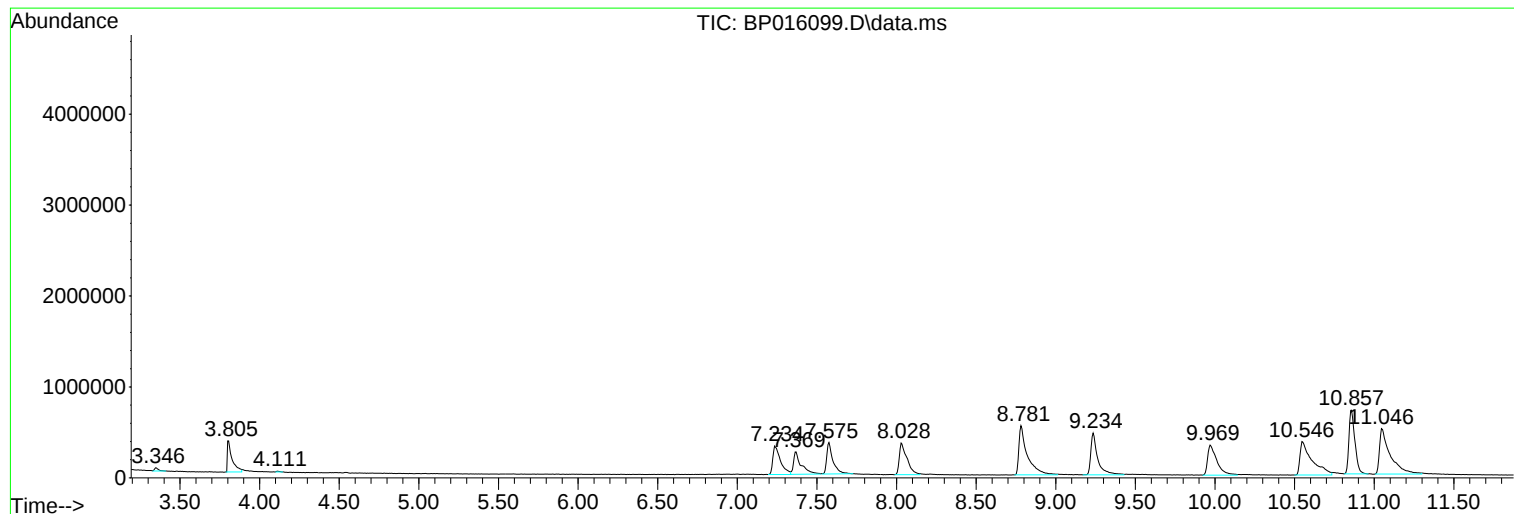

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016099.D
Acq On : 08 Jul 2023 19:16
Operator : MA/JU
Sample : PB153818BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016099.D
Acq On : 08 Jul 2023 19:16
Operator : MA/JU
Sample : PB153818BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc