

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016100.D
 Acq On : 08 Jul 2023 19:50
 Operator : MA/JU
 Sample : PB153847BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK847

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	36	rVB	28610	47806	0.56%	0.070%
2	3.805	103	105	122	rBV	251143	577848	6.76%	0.843%
3	7.246	683	690	707	rBV3	215664	814237	9.52%	1.188%
4	7.375	707	712	720	rBV	155838	355980	4.16%	0.519%
5	7.581	741	747	769	rBV	247712	680457	7.96%	0.993%
6	8.034	817	824	850	rBV	358182	1240091	14.50%	1.809%
7	8.793	946	953	988	rBV2	363585	1513700	17.70%	2.208%
8	9.246	1021	1030	1061	rBV	317907	1068032	12.49%	1.558%
9	9.981	1144	1155	1180	rBV2	217261	1005306	11.75%	1.467%
10	10.569	1245	1255	1272	rBV2	259947	1214297	14.20%	1.772%
11	10.857	1296	1304	1321	rBV	755721	2019404	23.61%	2.946%
12	11.057	1331	1338	1368	rBV	337522	1664495	19.46%	2.428%
13	12.469	1569	1578	1579	rBV9	7990	13658	0.16%	0.020%
14	13.557	1759	1763	1772	rBV10	7393	18462	0.22%	0.027%
15	14.093	1847	1854	1878	rBV	1867887	4253322	49.73%	6.206%
16	14.375	1894	1902	1931	rBV	2351292	4292709	50.19%	6.263%
17	14.675	1946	1953	1980	rBV	1962498	3341051	39.07%	4.875%
18	15.010	2003	2010	2046	rBV4	200051	1384935	16.19%	2.021%
19	15.681	2117	2124	2148	rBV	2496298	5893525	68.91%	8.599%
20	15.863	2149	2155	2187	rVV	442289	1760462	20.58%	2.569%
21	17.110	2364	2367	2374	rVB9	6047	11527	0.13%	0.017%
22	17.228	2384	2387	2397	rVB7	7030	14721	0.17%	0.021%
23	17.439	2416	2423	2434	rBV	2710210	4247130	49.66%	6.197%
24	17.545	2434	2441	2478	rVB2	2659961	6980465	81.62%	10.184%
25	19.357	2745	2749	2754	rBV2	51082	73996	0.87%	0.108%
26	19.433	2759	2762	2767	rBV	35577	52666	0.62%	0.077%
27	19.775	2814	2820	2854	rBV	3496751	8552280	100.00%	12.478%
28	21.551	3117	3122	3141	rBV	1865962	4655364	54.43%	6.792%
29	23.904	3515	3522	3542	rVB2	2546996	6663526	77.92%	9.722%
30	24.080	3545	3552	3575	rVB	1189227	4128978	48.28%	6.024%




Sum of corrected areas: 68540430

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016100.D
Acq On : 08 Jul 2023 19:50
Operator : MA/JU
Sample : PB153847BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK847

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

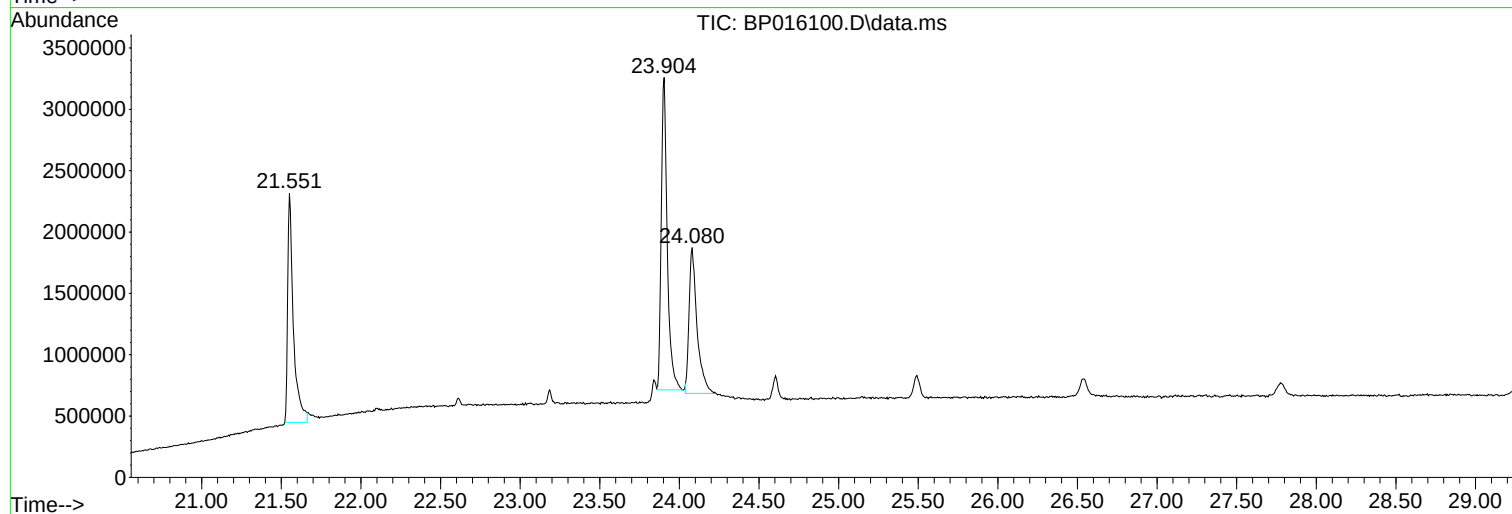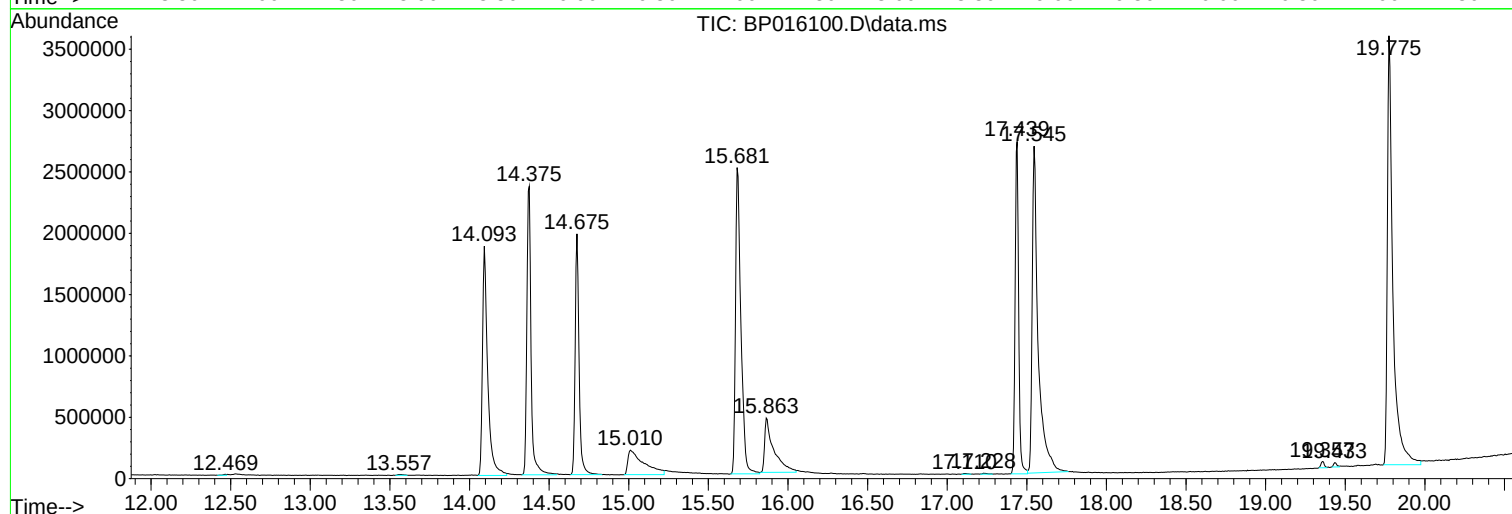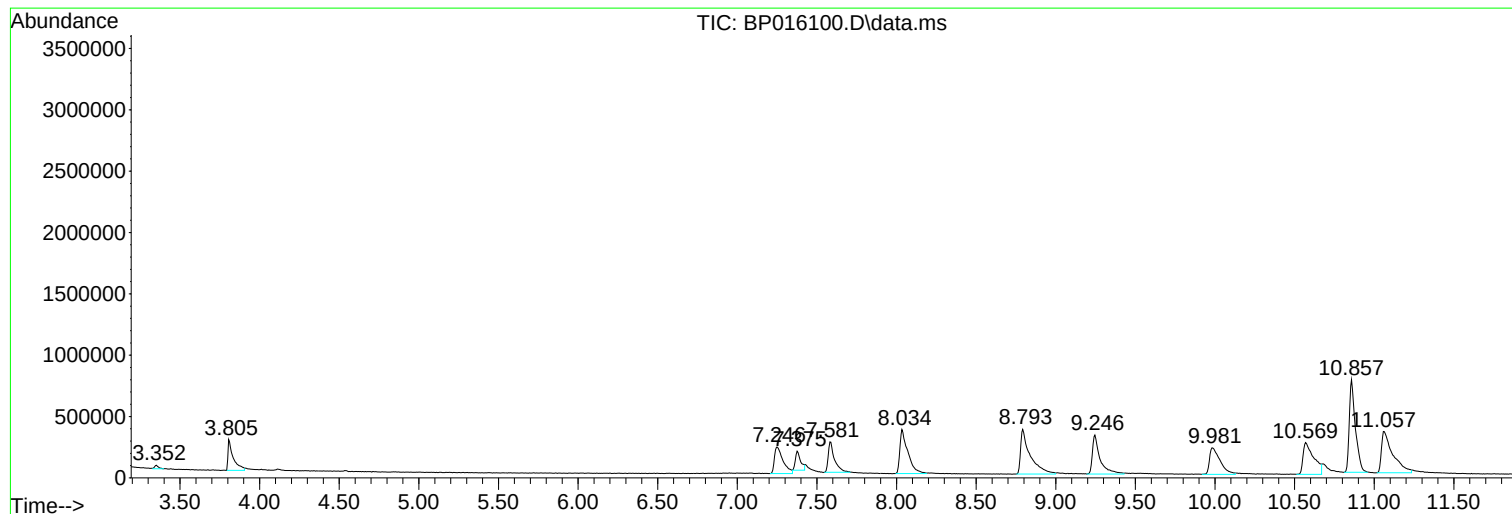

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016100.D
Acq On : 08 Jul 2023 19:50
Operator : MA/JU
Sample : PB153847BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK847

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016100.D
Acq On : 08 Jul 2023 19:50
Operator : MA/JU
Sample : PB153847BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK847

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc