

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016118.D
 Acq On : 09 Jul 2023 06:36
 Operator : MA/JU
 Sample : PB153850BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK850

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	37	rVB	33433	49896	0.52%	0.065%
2	3.805	103	105	128	rBV	313947	759122	7.92%	0.996%
3	4.117	154	158	163	rVB3	11516	18316	0.19%	0.024%
4	7.234	681	688	705	rBV2	281961	1003071	10.47%	1.316%
5	7.364	705	710	717	rBV	206234	423909	4.42%	0.556%
6	7.575	739	746	767	rBV	320590	841607	8.78%	1.104%
7	8.028	816	823	848	rBV	487237	1539364	16.06%	2.020%
8	8.781	944	951	983	rBV2	460832	1791125	18.69%	2.351%
9	9.234	1020	1028	1055	rBV	398438	1224324	12.77%	1.607%
10	9.969	1146	1153	1184	rBV	261945	1133889	11.83%	1.488%
11	10.552	1244	1252	1270	rBV	320299	1445983	15.09%	1.898%
12	10.846	1295	1302	1322	rVB	902053	2335043	24.36%	3.064%
13	11.052	1329	1337	1377	rBV	424259	1979256	20.65%	2.597%
14	12.463	1571	1577	1579	rBV7	8903	18227	0.19%	0.024%
15	12.528	1586	1588	1595	rVB8	8512	11459	0.12%	0.015%
16	13.557	1756	1763	1773	rBV2	19463	46062	0.48%	0.060%
17	14.087	1846	1853	1883	rBV	1903468	4473870	46.68%	5.871%
18	14.369	1893	1901	1918	rBV	2612702	4588214	47.87%	6.021%
19	14.669	1945	1952	1977	rBV	1913723	3226277	33.66%	4.234%
20	14.998	2001	2008	2045	rBV2	256171	1703465	17.77%	2.235%
21	15.675	2116	2123	2143	rBV	2797034	6321647	65.96%	8.296%
22	15.857	2149	2154	2195	rBV	493799	1910180	19.93%	2.507%
23	16.469	2254	2258	2262	rVB7	6087	10015	0.10%	0.013%
24	17.110	2364	2367	2371	rBV5	8018	10626	0.11%	0.014%
25	17.228	2384	2387	2393	rVB5	8579	15949	0.17%	0.021%
26	17.434	2415	2422	2434	rBV	2735673	4099108	42.77%	5.379%
27	17.540	2434	2440	2471	rVB2	3133657	7618957	79.50%	9.999%
28	19.351	2744	2748	2753	rBV2	68874	104911	1.09%	0.138%
29	19.428	2758	2761	2766	rBV	42921	69789	0.73%	0.092%
30	19.769	2813	2819	2848	rBV	4243983	9584128	100.00%	12.577%
31	21.545	3116	3121	3143	rBV2	1980676	5026516	52.45%	6.596%
32	23.898	3513	3521	3541	rVB2	3273551	8327306	86.89%	10.928%
33	24.074	3544	3551	3576	rVB	1288309	4489381	46.84%	5.891%




Sum of corrected areas: 76200992

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016118.D
Acq On : 09 Jul 2023 06:36
Operator : MA/JU
Sample : PB153850BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK850

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

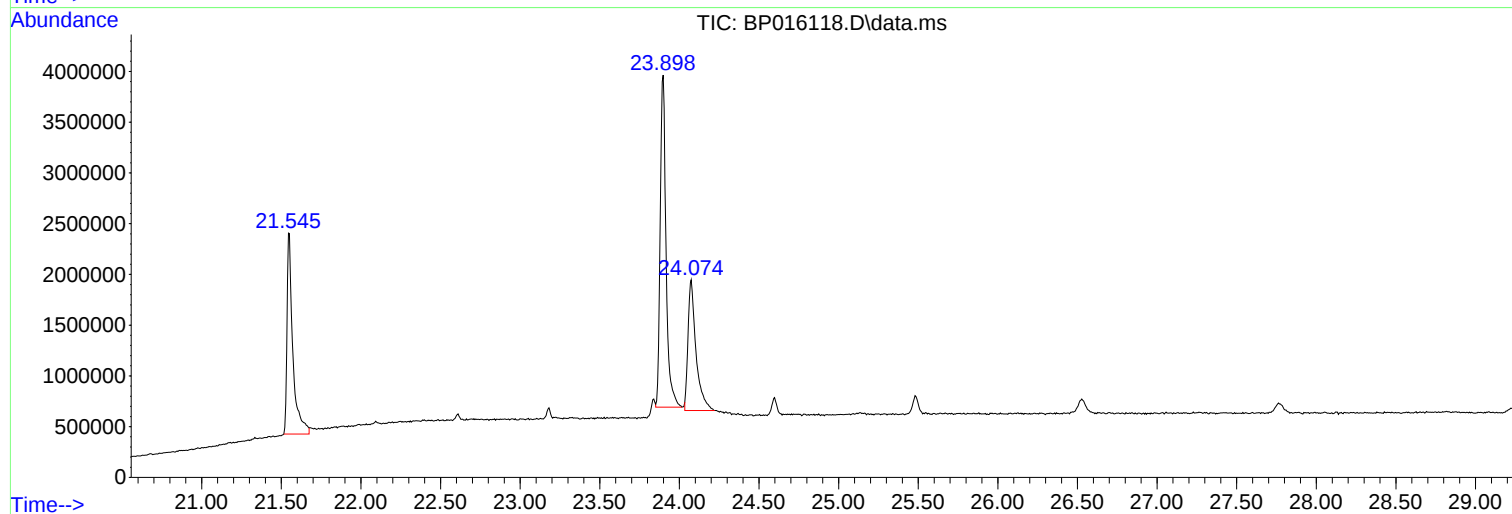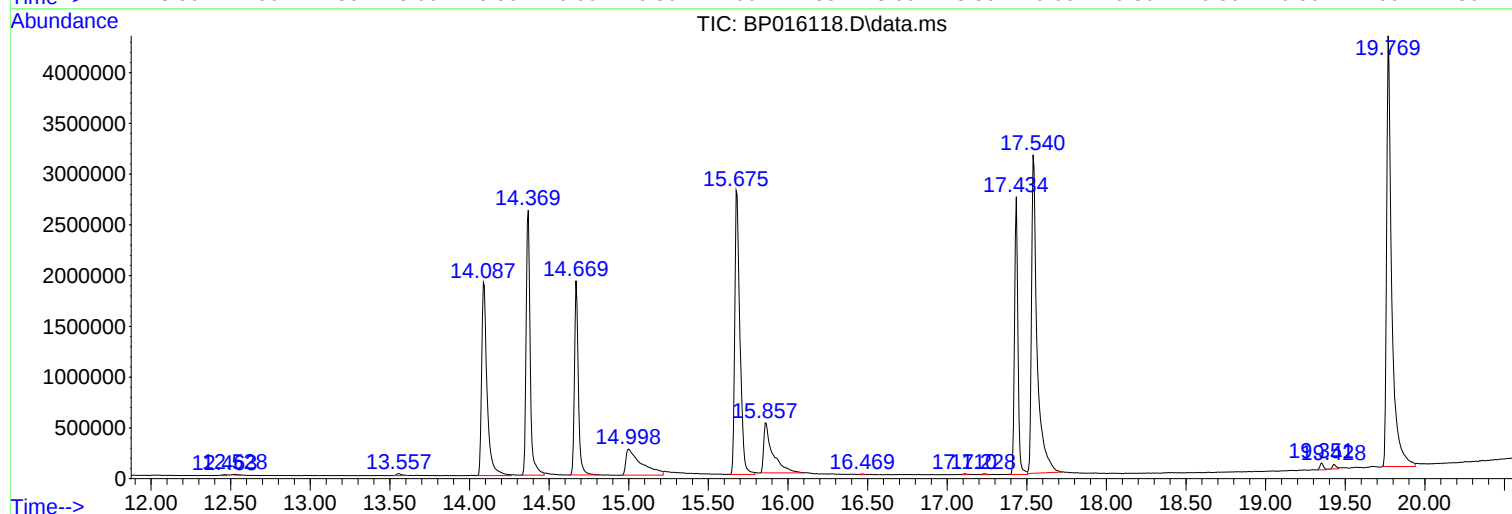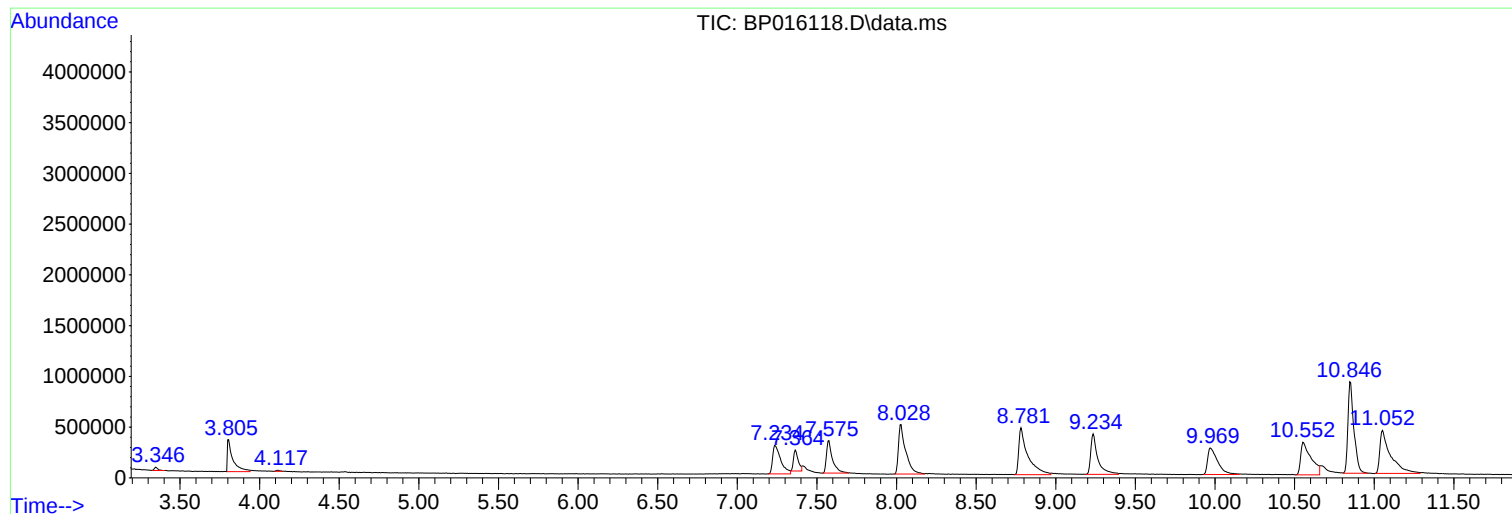

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016118.D
Acq On : 09 Jul 2023 06:36
Operator : MA/JU
Sample : PB153850BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK850

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016118.D
Acq On : 09 Jul 2023 06:36
Operator : MA/JU
Sample : PB153850BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK850

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc