

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016119.D
 Acq On : 09 Jul 2023 07:10
 Operator : MA/JU
 Sample : PB153890BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK890

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	35	rVB	62089	87505	1.46%	0.148%
2	3.793	101	103	126	rBV	543921	1184624	19.81%	2.006%
3	4.110	155	157	162	rVB2	10926	14822	0.25%	0.025%
4	7.222	680	686	703	rBV	399484	1401018	23.42%	2.372%
5	7.351	703	708	716	rBV	416333	837625	14.00%	1.418%
6	7.557	737	743	771	rVB	568864	1455099	24.33%	2.463%
7	8.022	815	822	844	rBV	431859	1294626	21.64%	2.192%
8	8.781	943	951	983	rBV2	472104	1875764	31.36%	3.176%
9	9.228	1017	1027	1053	rBV	477279	1485969	24.84%	2.516%
10	9.969	1146	1153	1183	rBV2	279210	1258296	21.04%	2.130%
11	10.563	1246	1254	1273	rBV	303359	1424623	23.82%	2.412%
12	10.851	1296	1303	1320	rBV	741652	1988260	33.24%	3.366%
13	11.057	1331	1338	1379	rBV	327224	1679186	28.07%	2.843%
14	12.469	1572	1578	1579	rBV6	7303	11252	0.19%	0.019%
15	12.533	1582	1589	1594	rVV8	8437	21535	0.36%	0.036%
16	13.569	1758	1765	1774	rBV3	17015	46335	0.77%	0.078%
17	14.098	1848	1855	1894	rBV	1133623	3034084	50.73%	5.137%
18	14.369	1894	1901	1923	rBV2	1909482	3479284	58.17%	5.890%
19	14.674	1946	1953	1972	rBV	1746939	3075362	51.42%	5.207%
20	15.045	2009	2016	2033	rBV4	108525	628668	10.51%	1.064%
21	15.574	2103	2106	2111	rVB6	5946	6965	0.12%	0.012%
22	15.686	2118	2125	2153	rBV	1702707	4463685	74.63%	7.557%
23	15.892	2153	2160	2194	rBV3	169268	976370	16.32%	1.653%
24	17.110	2365	2367	2373	rVB7	5426	8702	0.15%	0.015%
25	17.239	2384	2389	2392	rBV6	7189	10220	0.17%	0.017%
26	17.439	2416	2423	2434	rBV	2292956	3790856	63.38%	6.418%
27	17.545	2435	2441	2478	rVB2	1645907	4990613	83.44%	8.449%
28	18.351	2575	2578	2579	rBV3	6457	7015	0.12%	0.012%
29	19.362	2746	2750	2756	rBV3	38358	59164	0.99%	0.100%
30	19.439	2759	2763	2768	rBV3	27116	55795	0.93%	0.094%
31	19.780	2814	2821	2848	rBV	2304141	5981426	100.00%	10.127%
32	21.551	3117	3122	3142	rBV	1608371	4181499	69.91%	7.079%
33	23.903	3515	3522	3542	rBV2	1722954	4589330	76.73%	7.770%
34	24.080	3545	3552	3576	rVB	968061	3661407	61.21%	6.199%

Sum of corrected areas: 59066984

Instrument :

BNA_P

ClientSampleId :


SBLK890

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016119.D
Acq On : 09 Jul 2023 07:10
Operator : MA/JU
Sample : PB153890BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK890

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

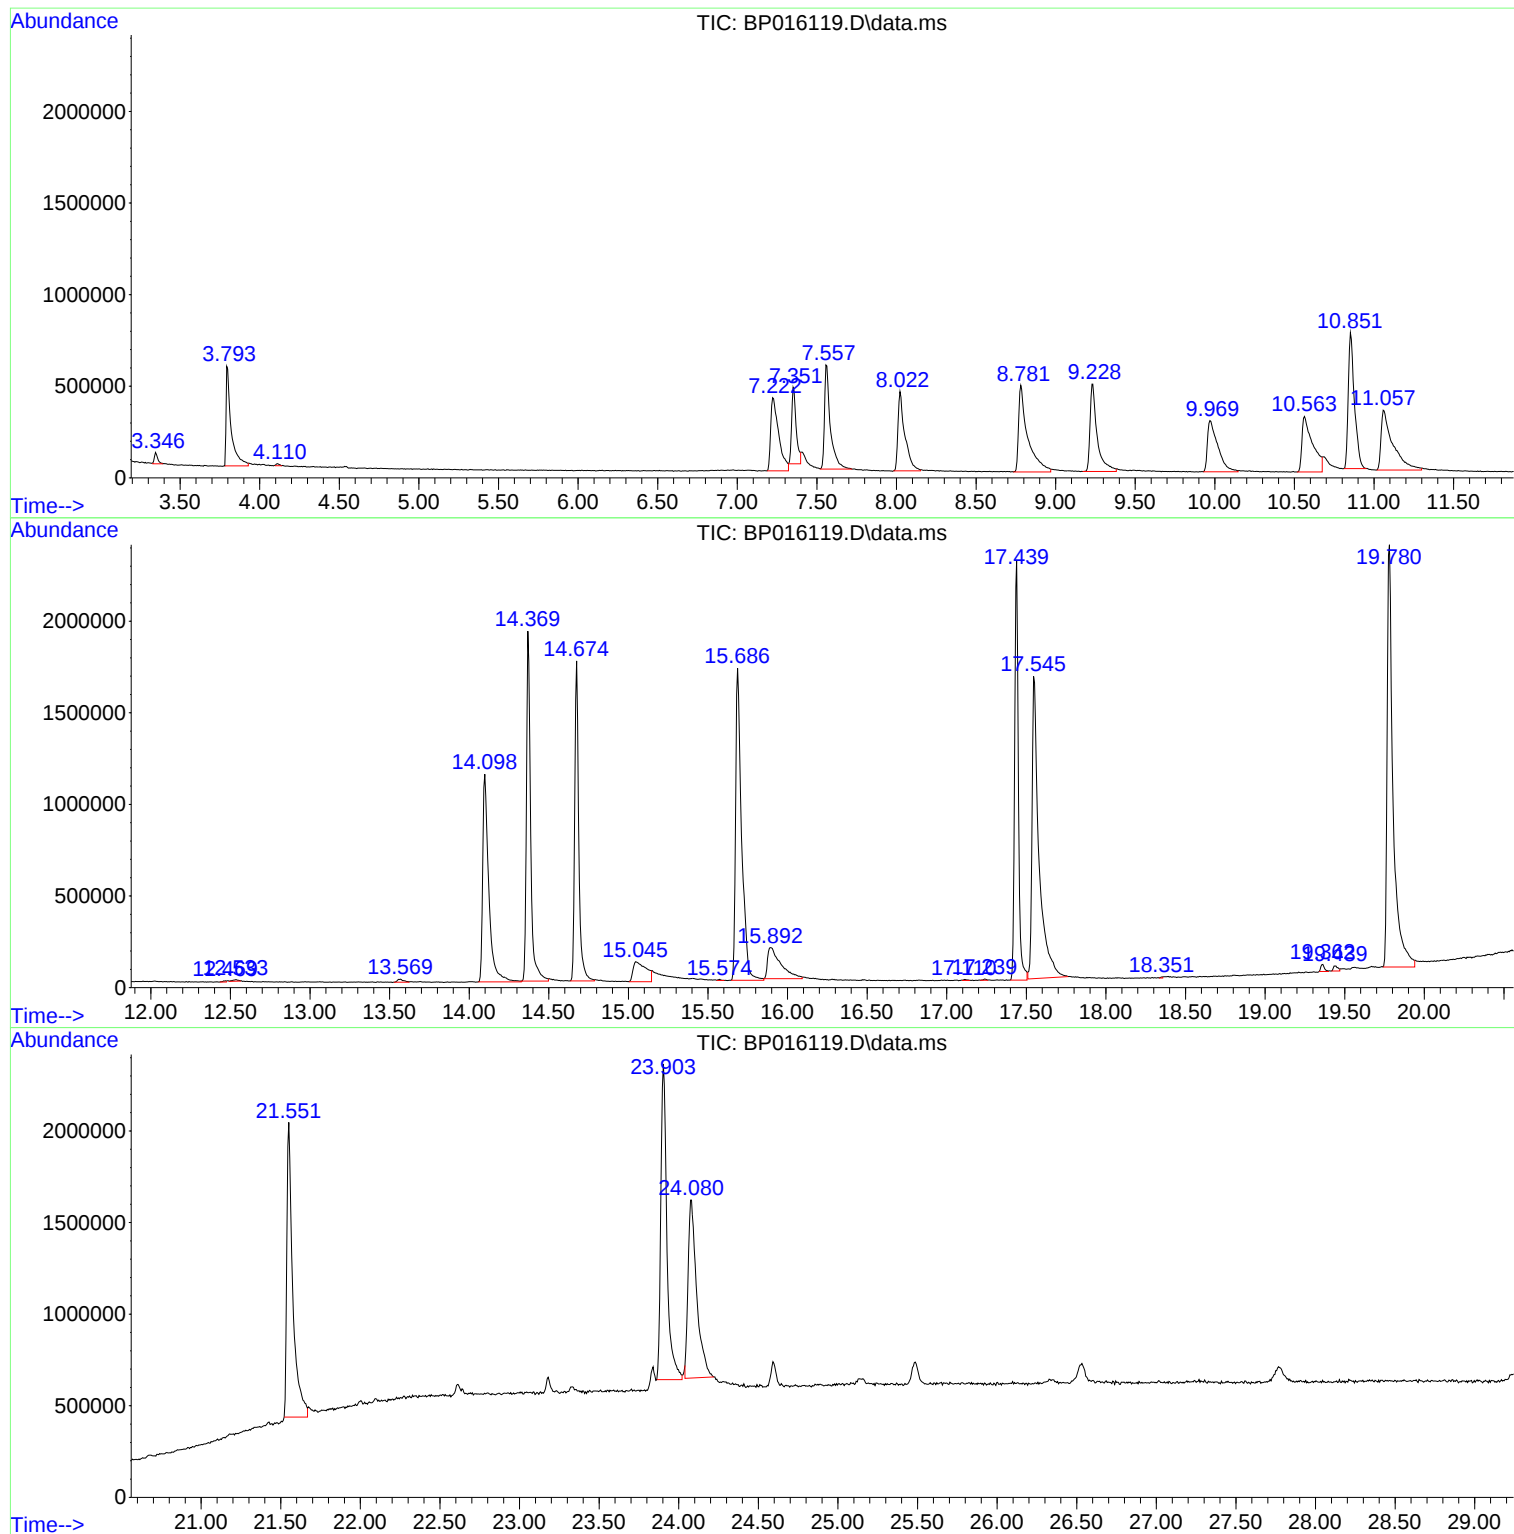

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016119.D
Acq On : 09 Jul 2023 07:10
Operator : MA/JU
Sample : PB153890BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK890

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016119.D
Acq On : 09 Jul 2023 07:10
Operator : MA/JU
Sample : PB153890BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK890

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc