

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016128.D
 Acq On : 09 Jul 2023 12:16
 Operator : MA/JU
 Sample : 03332-20
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	38	rVB	46577	78523	1.60%	0.149%
2	3.805	103	105	124	rBV	342853	765916	15.61%	1.450%
3	4.110	155	157	162	rVB	17186	21804	0.44%	0.041%
4	5.746	432	435	439	rVB6	3274	5150	0.10%	0.010%
5	7.240	681	689	704	rBV	256789	960669	19.59%	1.819%
6	7.357	704	709	718	rBV	269395	583111	11.89%	1.104%
7	7.569	739	745	766	rBV	403672	1061500	21.64%	2.010%
8	8.022	815	822	851	rBV	618063	1879920	38.33%	3.560%
9	8.793	946	953	988	rBV	277597	1396184	28.46%	2.644%
10	9.240	1022	1029	1061	rBV	332773	1124016	22.92%	2.128%
11	9.528	1075	1078	1083	rVB6	8698	13711	0.28%	0.026%
12	9.987	1143	1156	1181	rBV3	173497	926280	18.88%	1.754%
13	10.587	1250	1258	1296	rBV	201474	1281527	26.13%	2.427%
14	10.851	1296	1303	1327	rVB	998687	2807726	57.24%	5.316%
15	11.069	1334	1340	1368	rBV2	219842	1156637	23.58%	2.190%
16	12.028	1501	1503	1510	rVB7	5601	6410	0.13%	0.012%
17	12.539	1583	1590	1596	rBV7	7082	22034	0.45%	0.042%
18	13.492	1747	1752	1757	rBV9	6705	13621	0.28%	0.026%
19	13.563	1760	1764	1772	rVB9	8602	21809	0.44%	0.041%
20	13.675	1780	1783	1787	rBV6	2876	5292	0.11%	0.010%
21	14.098	1848	1855	1879	rBV	898887	2417704	49.29%	4.578%
22	14.369	1894	1901	1920	rBV	1421154	2735769	55.77%	5.180%
23	14.551	1930	1932	1940	rVB9	11503	22166	0.45%	0.042%
24	14.675	1946	1953	1974	rBV	2090063	3823425	77.95%	7.240%
25	15.110	2016	2027	2031	rBV6	52118	180004	3.67%	0.341%
26	15.439	2081	2083	2090	rVB8	9690	15638	0.32%	0.030%
27	15.510	2090	2095	2099	rVV8	7382	15694	0.32%	0.030%
28	15.686	2118	2125	2151	rBV	1380923	3506713	71.49%	6.640%
29	15.916	2157	2164	2183	rBV5	101740	529535	10.80%	1.003%
30	16.069	2184	2190	2204	rVB	364302	761674	15.53%	1.442%
31	16.322	2230	2233	2238	rVB3	12485	15357	0.31%	0.029%
32	16.616	2279	2283	2290	rBV2	18873	30183	0.62%	0.057%
33	16.927	2333	2336	2340	rVB5	5923	7453	0.15%	0.014%
34	17.104	2360	2366	2370	rBV9	9992	20099	0.41%	0.038%
35	17.233	2386	2388	2396	rVB5	7469	14029	0.29%	0.027%
36	17.439	2417	2423	2436	rBV	2591345	4382695	89.35%	8.299%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016128.D
 Acq On : 09 Jul 2023 12:16
 Operator : MA/JU
 Sample : 03332-20
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBTZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	17.551	2436	2442	2470	rVB2	1156690	3648890	74.39%	6.909%
38	18.298	2564	2569	2576	rBV	157676	341813	6.97%	0.647%
39	19.363	2747	2750	2754	rVB4	27009	33509	0.68%	0.063%
40	19.527	2774	2778	2790	rBV6	54852	146456	2.99%	0.277%
41	19.780	2815	2821	2844	rBV	1726672	4308153	87.83%	8.157%
42	21.227	3063	3067	3077	rVB5	155769	361010	7.36%	0.684%
43	21.545	3116	3121	3147	rBV	1618957	4905120	100.00%	9.288%
44	23.909	3517	3523	3542	rVB	1113082	2826477	57.62%	5.352%
45	24.080	3545	3552	3578	rVB	1046399	3630997	74.02%	6.875%




Sum of corrected areas: 52812403

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016128.D
Acq On : 09 Jul 2023 12:16
Operator : MA/JU
Sample : 03332-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

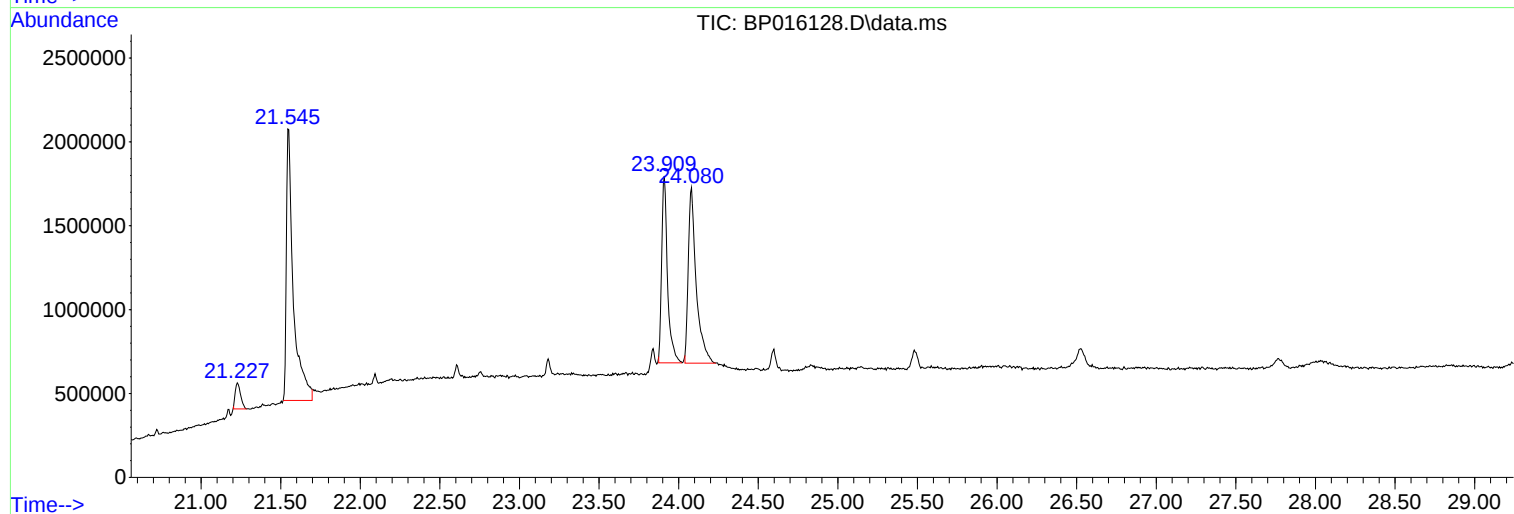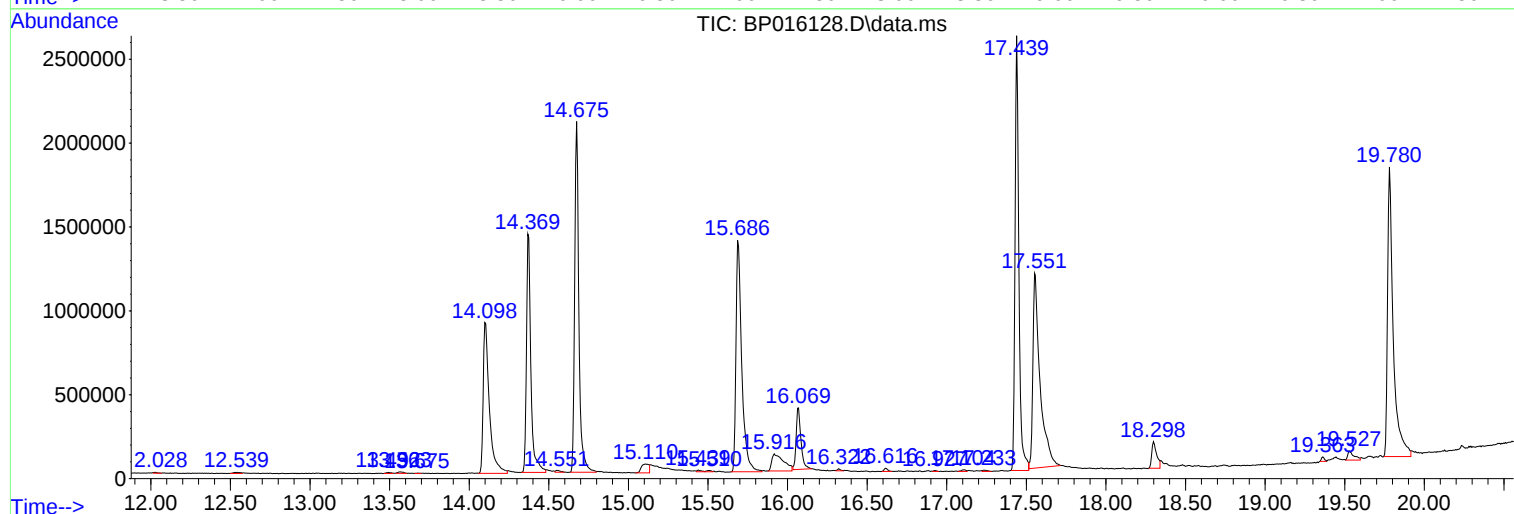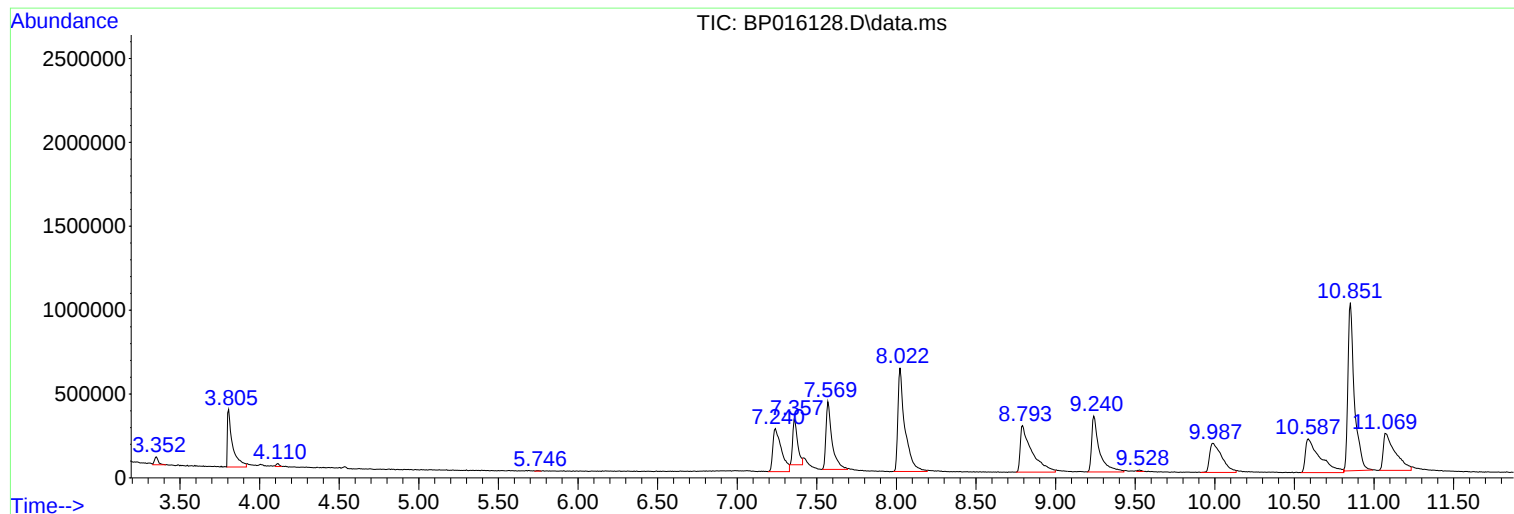

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016128.D
Acq On : 09 Jul 2023 12:16
Operator : MA/JU
Sample : 03332-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.069	3.48 ng/ul	761674	Phenanthrene-d10	17.439

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Methanone, phenyl-2-pyridinyl-	183	C12H9NO	000091-02-1	78

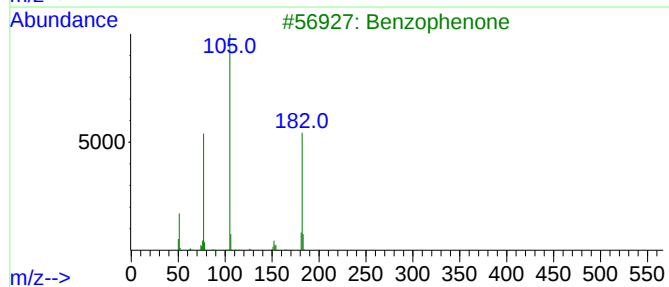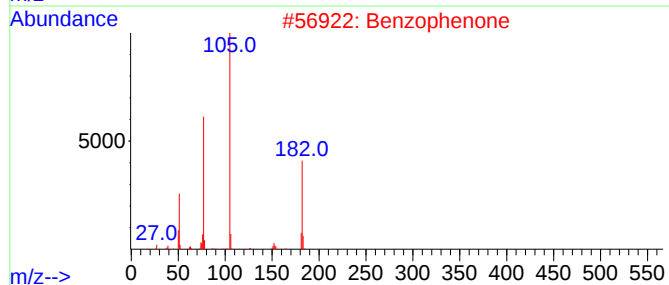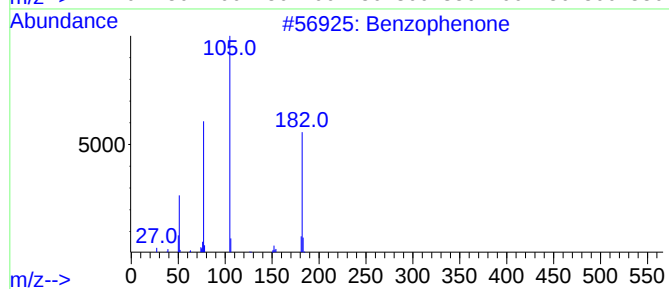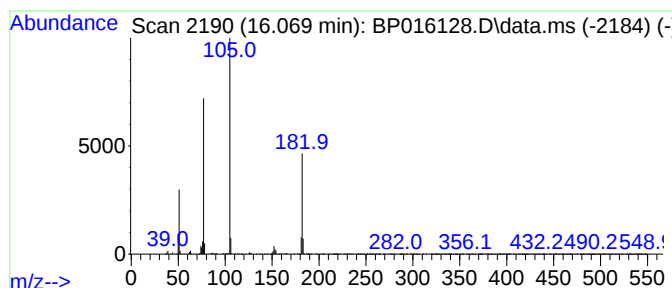

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016128.D
Acq On : 09 Jul 2023 12:16
Operator : MA/JU
Sample : 03332-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBTZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.069	3.5	ng/u1	761674	4	17.439	4382700	20.0