

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016137.D
 Acq On : 09 Jul 2023 17:56
 Operator : MA/JU
 Sample : PB153810BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	35	rVB	70480	100299	1.90%	0.169%
2	3.799	101	104	128	rBV	603968	1250766	23.64%	2.112%
3	4.111	154	157	164	rVB3	14695	26117	0.49%	0.044%
4	7.222	679	686	702	rBV	390516	1358286	25.68%	2.294%
5	7.352	702	708	736	rVV	479004	1284522	24.28%	2.169%
6	7.558	737	743	763	rVV	628090	1492723	28.22%	2.521%
7	8.016	814	821	849	rBV	632586	1892796	35.78%	3.197%
8	8.775	943	950	994	rBV	464524	1930799	36.50%	3.261%
9	9.228	1020	1027	1059	rBV	495144	1562696	29.54%	2.639%
10	9.969	1144	1153	1184	rBV2	273009	1295183	24.48%	2.187%
11	10.569	1246	1255	1272	rBV	289528	1364346	25.79%	2.304%
12	10.846	1295	1302	1324	rVB	1053777	2801879	52.97%	4.732%
13	11.057	1331	1338	1377	rBV	334389	1718830	32.49%	2.903%
14	12.534	1583	1589	1590	rBV5	9369	12828	0.24%	0.022%
15	13.569	1755	1765	1768	rBV4	15527	34832	0.66%	0.059%
16	14.010	1835	1840	1845	rVB8	4742	8062	0.15%	0.014%
17	14.098	1848	1855	1874	rBV	1144639	3079708	58.22%	5.201%
18	14.369	1893	1901	1935	rBV	1931640	3584605	67.76%	6.054%
19	14.669	1945	1952	1974	rBV	2059837	3801014	71.85%	6.420%
20	15.057	2009	2018	2021	rBV3	88912	214962	4.06%	0.363%
21	15.687	2118	2125	2151	rBV	1629709	4447622	84.08%	7.512%
22	15.887	2153	2159	2200	rVV3	196380	1085215	20.51%	1.833%
23	16.281	2224	2226	2230	rVB5	5619	6809	0.13%	0.011%
24	17.110	2362	2367	2373	rBV10	5360	11755	0.22%	0.020%
25	17.239	2386	2389	2394	rVB4	5306	7659	0.14%	0.013%
26	17.439	2416	2423	2436	rBV	2445257	4305553	81.39%	7.272%
27	17.551	2436	2442	2474	rVB2	1510613	4648203	87.87%	7.851%
28	19.363	2747	2750	2755	rBV2	34068	49060	0.93%	0.083%
29	19.445	2761	2764	2769	rBV4	16308	28109	0.53%	0.047%
30	19.780	2815	2821	2853	rBV	1905405	5289892	100.00%	8.934%
31	21.557	3117	3123	3144	rBV	1416608	4051379	76.59%	6.843%
32	23.910	3517	3523	3539	rBV2	1181999	3311936	62.61%	5.594%
33	24.080	3546	3552	3575	rVB	871210	3150447	59.56%	5.321%


Sum of corrected areas: 59208892

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016137.D
Acq On : 09 Jul 2023 17:56
Operator : MA/JU
Sample : PB153810BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

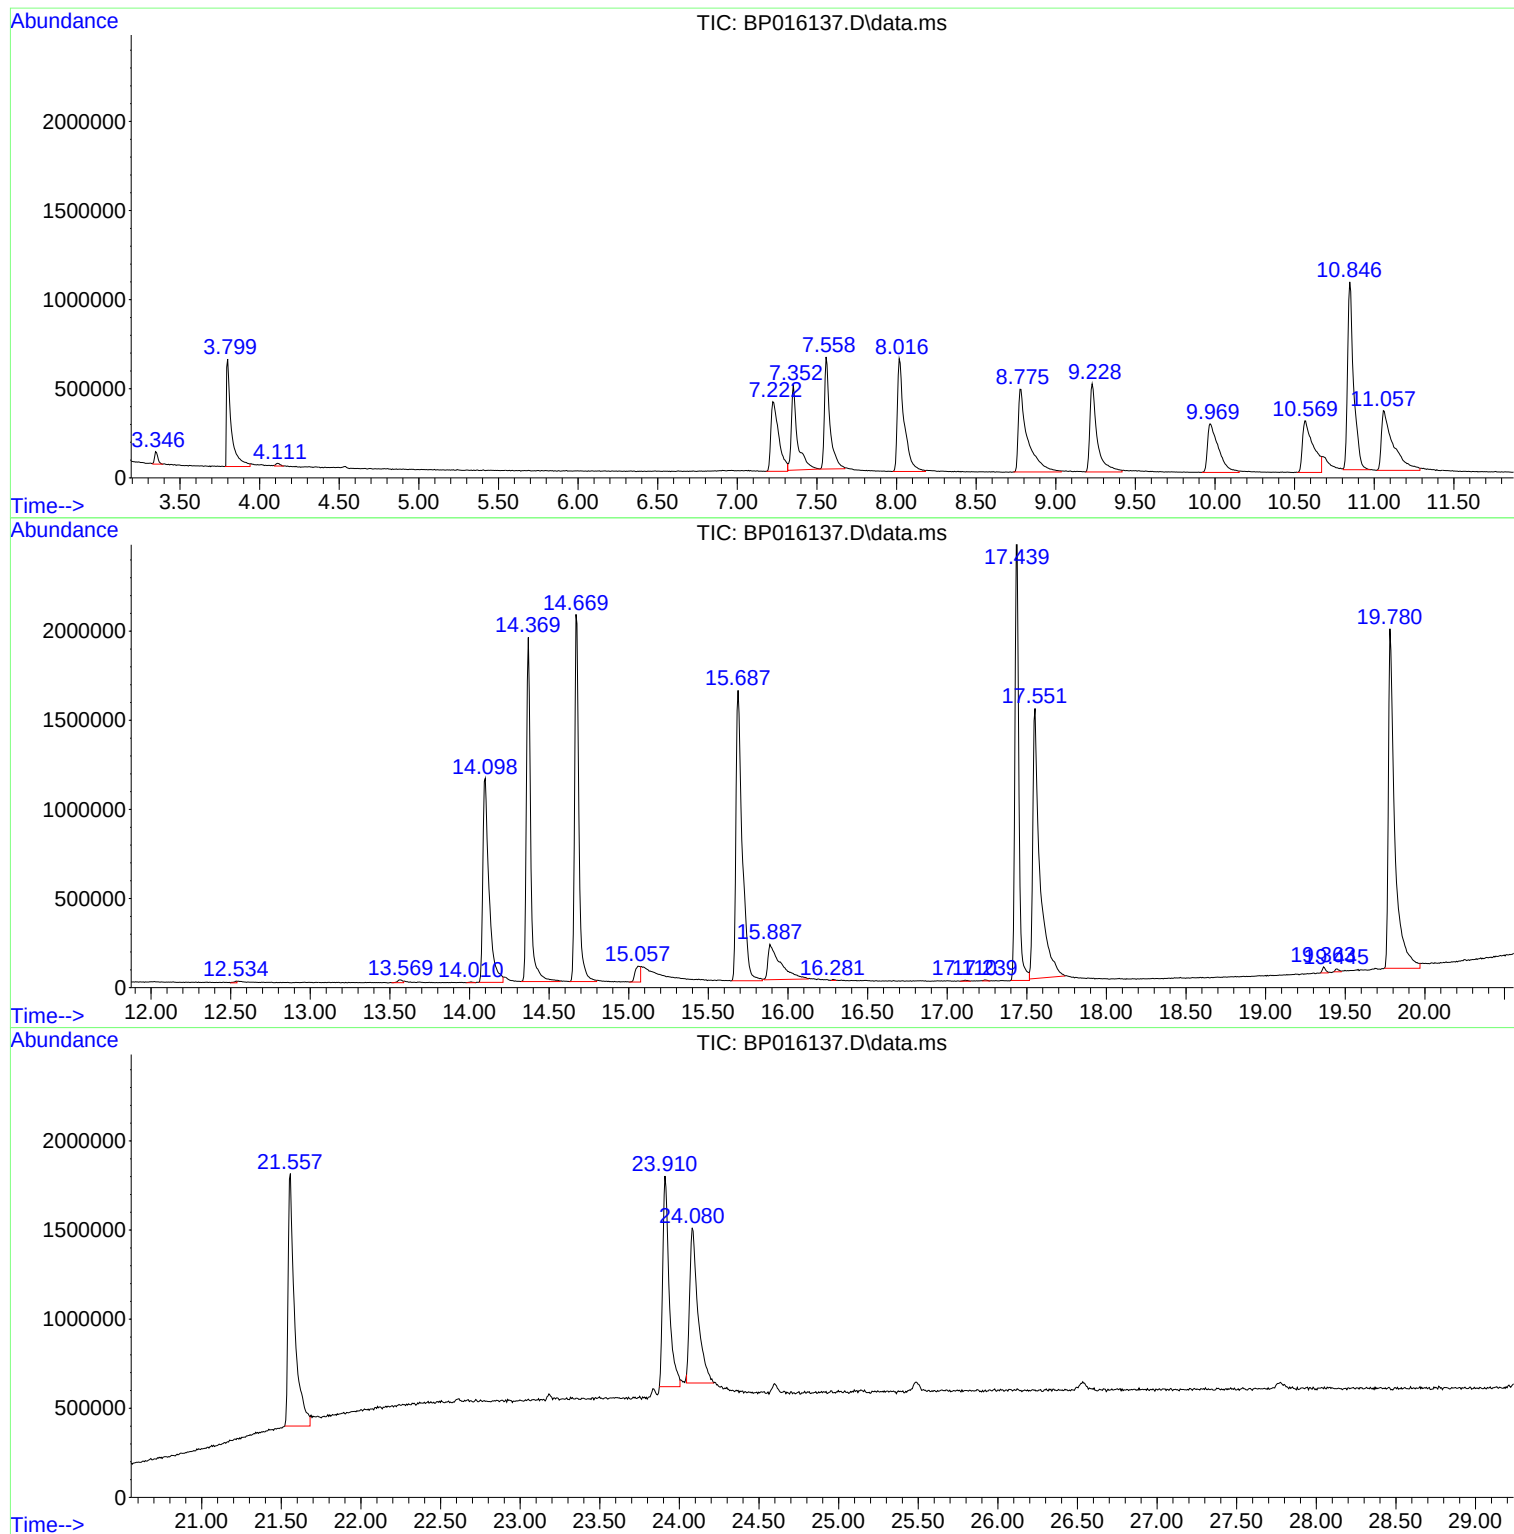

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016137.D
Acq On : 09 Jul 2023 17:56
Operator : MA/JU
Sample : PB153810BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016137.D
Acq On : 09 Jul 2023 17:56
Operator : MA/JU
Sample : PB153810BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc