

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016142.D
 Acq On : 09 Jul 2023 20:45
 Operator : MA/JU
 Sample : 03384-01
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBW82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	31	rBV2	23523	33626	0.55%	0.060%
2	3.816	106	107	128	rBV	101462	302434	4.97%	0.536%
3	4.005	134	139	145	rVB2	28882	49657	0.82%	0.088%
4	4.111	154	157	166	rVB2	15422	27557	0.45%	0.049%
5	6.158	502	505	508	rBV5	4050	6568	0.11%	0.012%
6	7.287	690	697	704	rBV2	53243	171832	2.83%	0.304%
7	7.363	704	710	735	rVB	294760	1028517	16.91%	1.822%
8	7.593	742	749	778	rVB	298166	982732	16.16%	1.741%
9	8.028	816	823	845	rBV	506417	1698499	27.93%	3.009%
10	8.810	950	956	957	rBV2	127935	187598	3.08%	0.332%
11	9.240	1022	1029	1064	rBV	402192	1336947	21.99%	2.368%
12	9.981	1147	1155	1182	rBV3	190129	1027664	16.90%	1.820%
13	10.581	1250	1257	1273	rBV2	228047	1039404	17.09%	1.841%
14	10.851	1295	1303	1326	rVB	905463	2607758	42.88%	4.619%
15	11.075	1334	1341	1367	rBV	206447	1114836	18.33%	1.975%
16	12.022	1500	1502	1507	rVB6	5717	6954	0.11%	0.012%
17	12.363	1553	1560	1563	rBV8	8057	16961	0.28%	0.030%
18	12.534	1586	1589	1590	rBV3	6655	6661	0.11%	0.012%
19	13.557	1755	1763	1773	rBV4	21251	57921	0.95%	0.103%
20	14.010	1835	1840	1843	rBV7	5747	9135	0.15%	0.016%
21	14.098	1848	1855	1877	rBV	1121794	2935446	48.27%	5.200%
22	14.369	1894	1901	1923	rBV	1767333	3283511	54.00%	5.816%
23	14.669	1943	1952	1979	rBV	2018876	3768926	61.98%	6.676%
24	15.233	2046	2048	2050	rBV3	4963	6150	0.10%	0.011%
25	15.263	2050	2053	2056	rVV5	4353	7999	0.13%	0.014%
26	15.369	2068	2071	2076	rVB7	4973	8360	0.14%	0.015%
27	15.522	2093	2097	2100	rBV6	5055	8140	0.13%	0.014%
28	15.686	2117	2125	2150	rBV	1611325	4344505	71.44%	7.695%
29	15.916	2158	2164	2186	rBV6	133181	730673	12.02%	1.294%
30	16.492	2259	2262	2268	rVB7	4398	6703	0.11%	0.012%
31	17.004	2344	2349	2355	rBV10	6540	14043	0.23%	0.025%
32	17.116	2365	2368	2375	rVB9	4159	8298	0.14%	0.015%
33	17.233	2387	2388	2394	rVB4	5720	8657	0.14%	0.015%
34	17.439	2416	2423	2436	rBV	2456792	4223017	69.45%	7.480%
35	17.551	2436	2442	2470	rVB	1596283	4726480	77.72%	8.372%
36	18.069	2525	2530	2542	rVB	219921	317767	5.23%	0.563%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016142.D
Acq On : 09 Jul 2023 20:45
Operator : MA/JU
Sample : 03384-01
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW82

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	18.333	2572	2575	2579	rBV6	14055	24673	0.41%	0.044%
38	19.145	2710	2713	2718	rVB4	20902	24962	0.41%	0.044%
39	19.357	2745	2749	2753	rBV	41785	60748	1.00%	0.108%
40	19.439	2760	2763	2771	rBV2	22039	42193	0.69%	0.075%
41	19.774	2814	2820	2848	rBV	2509302	6081045	100.00%	10.771%
42	21.545	3116	3121	3143	rBV2	1732263	4747401	78.07%	8.409%
43	23.898	3514	3521	3541	rBV2	1971457	5099707	83.86%	9.033%
44	24.068	3544	3550	3574	rVB	1191729	4262540	70.10%	7.550%


Sum of corrected areas: 56455205

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016142.D
Acq On : 09 Jul 2023 20:45
Operator : MA/JU
Sample : 03384-01
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

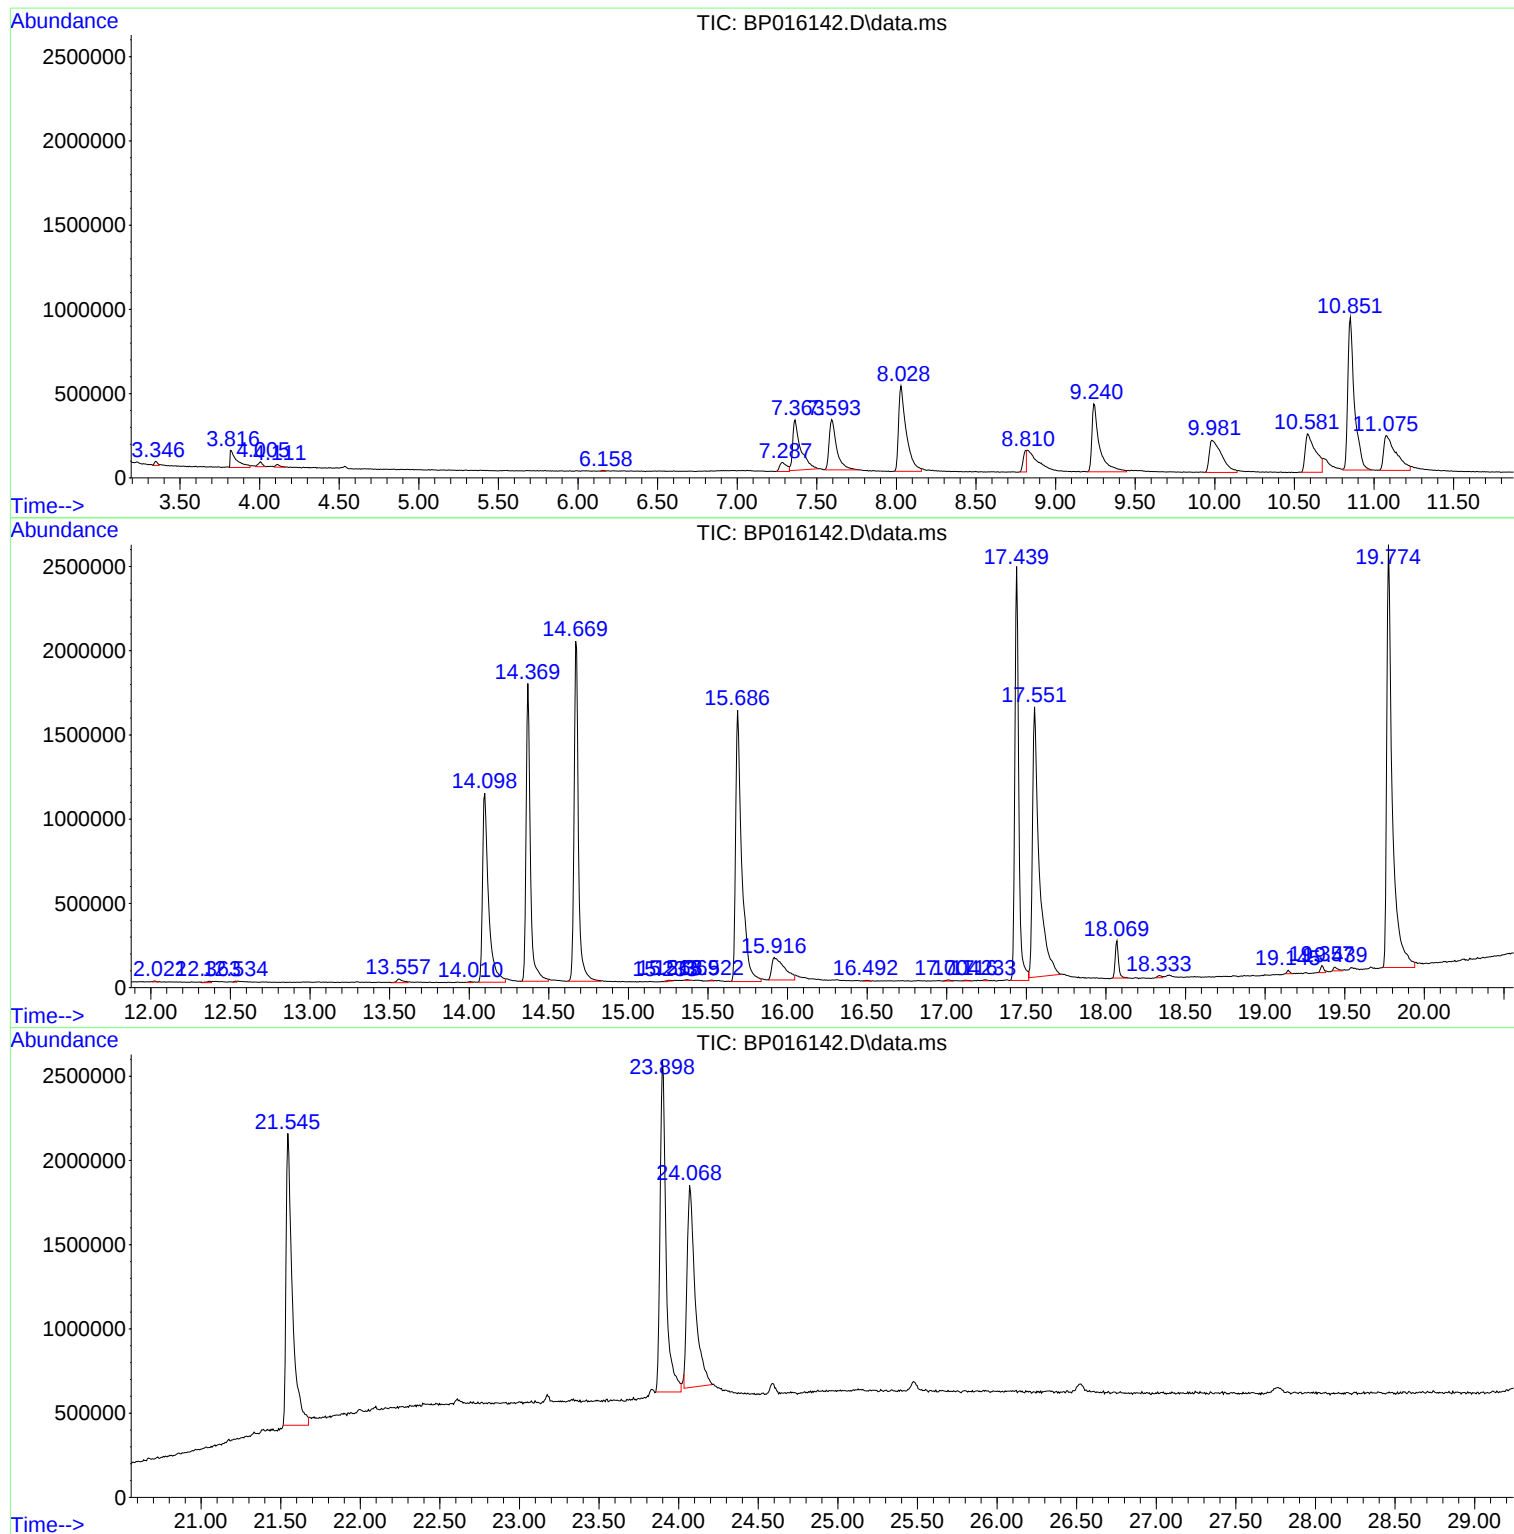

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016142.D
Acq On : 09 Jul 2023 20:45
Operator : MA/JU
Sample : 03384-01
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016142.D
Acq On : 09 Jul 2023 20:45
Operator : MA/JU
Sample : 03384-01
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW82

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------