

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
 Data File : BP016145.D
 Acq On : 09 Jul 2023 22:27
 Operator : MA/JU
 Sample : 03384-07
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YBW83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	25	28	33	rVB	28342	36723	0.59%	0.056%
2	3.816	104	107	121	rBV	110872	265322	4.25%	0.406%
3	4.005	134	139	144	rVB2	33780	55811	0.89%	0.085%
4	4.110	153	157	164	rVB2	22949	35161	0.56%	0.054%
5	6.093	488	494	496	rBV7	5358	10100	0.16%	0.015%
6	7.269	688	694	702	rBV	70978	214544	3.44%	0.329%
7	7.346	702	707	734	rVB	476072	1210606	19.40%	1.854%
8	7.587	739	748	768	rVV2	303293	1110953	17.80%	1.701%
9	8.016	813	821	852	rBV	874283	2558693	41.00%	3.918%
10	8.793	946	953	995	rBV	157170	915043	14.66%	1.401%
11	9.228	1020	1027	1060	rBV	464232	1442951	23.12%	2.209%
12	9.969	1144	1153	1182	rBV2	224119	1153456	18.48%	1.766%
13	10.575	1247	1256	1294	rBV2	250621	1491431	23.90%	2.284%
14	10.845	1294	1302	1325	rVB	1320799	3502470	56.12%	5.363%
15	11.063	1333	1339	1375	rBV	261012	1313250	21.04%	2.011%
16	12.351	1552	1558	1561	rBV7	6884	13701	0.22%	0.021%
17	12.528	1582	1588	1591	rBV8	7304	13706	0.22%	0.021%
18	12.716	1617	1620	1626	rBV7	3312	6797	0.11%	0.010%
19	13.563	1757	1764	1770	rBV2	19426	48259	0.77%	0.074%
20	14.092	1847	1854	1887	rBV	1171148	2973276	47.64%	4.553%
21	14.363	1894	1900	1925	rBV	1699213	3216613	51.54%	4.925%
22	14.669	1944	1952	1973	rBV	2566312	4670916	74.85%	7.152%
23	15.210	2035	2044	2046	rBV10	12205	29545	0.47%	0.045%
24	15.357	2067	2069	2080	rVB10	7733	16051	0.26%	0.025%
25	15.680	2118	2124	2151	rBV	1618345	4213660	67.52%	6.452%
26	15.898	2154	2161	2191	rBV3	223957	1181007	18.92%	1.808%
27	16.480	2257	2260	2267	rVB9	5001	8896	0.14%	0.014%
28	17.010	2345	2350	2357	rVB10	6690	13464	0.22%	0.021%
29	17.110	2363	2367	2370	rBV6	5034	6926	0.11%	0.011%
30	17.233	2385	2388	2392	rBV3	7669	9408	0.15%	0.014%
31	17.374	2407	2412	2415	rVB7	5770	9604	0.15%	0.015%
32	17.433	2415	2422	2435	rBV	3070633	5083968	81.46%	7.785%
33	17.545	2435	2441	2469	rVB	1867263	5096561	81.67%	7.804%
34	18.063	2524	2529	2538	rBV	307739	419772	6.73%	0.643%
35	18.304	2565	2570	2579	rBV2	63501	154534	2.48%	0.237%
36	18.380	2580	2583	2592	rVB2	17943	47504	0.76%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016145.D
Acq On : 09 Jul 2023 22:27
Operator : MA/JU
Sample : 03384-07
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW83

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	19.351	2744	2748	2752	rBV6	43762	65885	1.06%	0.101%
38	19.433	2759	2762	2770	rVB2	33664	59487	0.95%	0.091%
39	19.521	2773	2777	2784	rBV3	62065	115058	1.84%	0.176%
40	19.721	2807	2811	2813	rBV3	35699	47525	0.76%	0.073%
41	19.774	2814	2820	2846	rVV	2765633	6240772	100.00%	9.556%
42	21.074	3039	3041	3045	rVB3	59940	58761	0.94%	0.090%
43	21.539	3115	3120	3139	rBV	2242319	5493937	88.03%	8.412%
44	23.892	3514	3520	3540	rVB2	2254137	5286090	84.70%	8.094%
45	24.068	3542	3550	3576	rVB	1519229	5388678	86.35%	8.251%


Sum of corrected areas: 65306875

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016145.D
Acq On : 09 Jul 2023 22:27
Operator : MA/JU
Sample : 03384-07
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

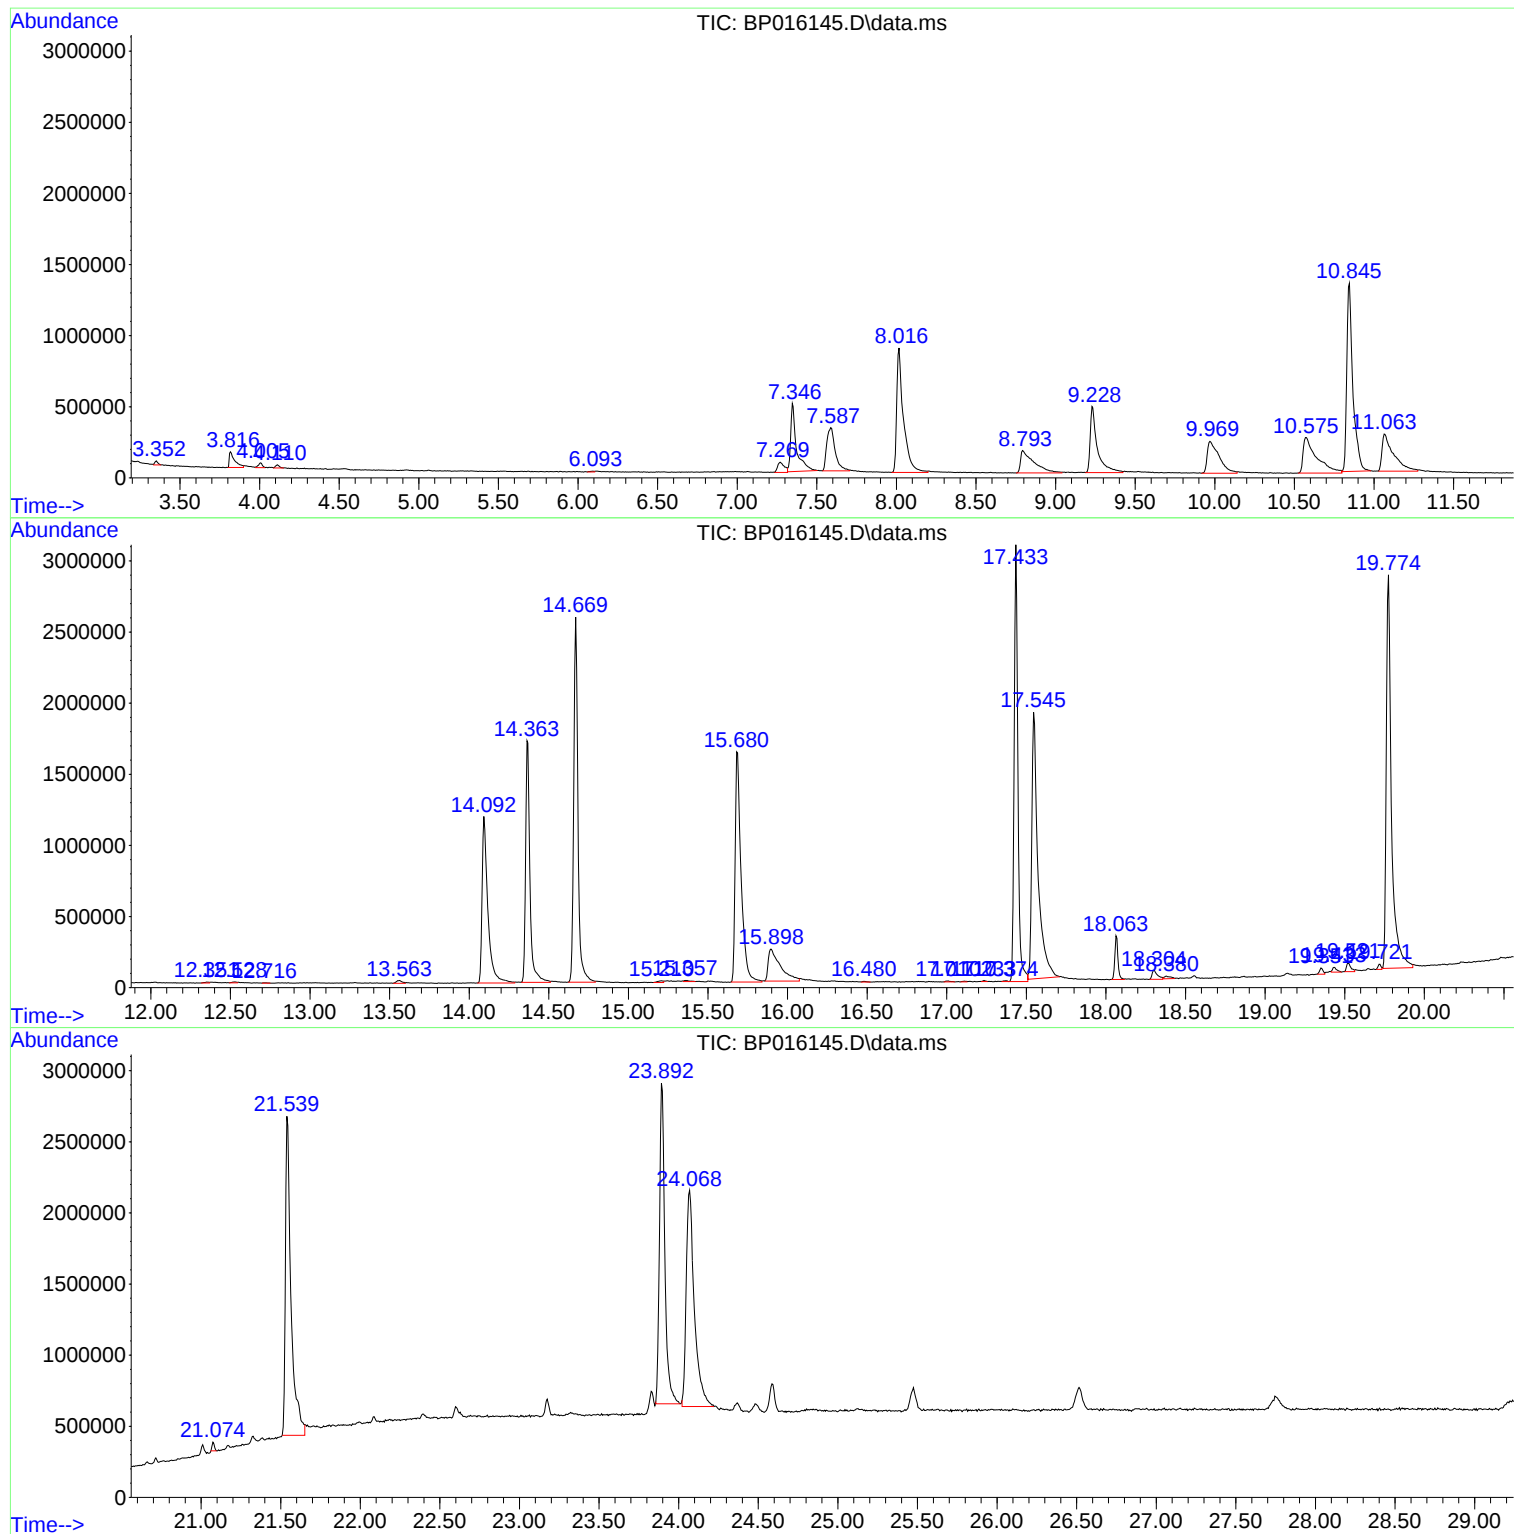

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016145.D
Acq On : 09 Jul 2023 22:27
Operator : MA/JU
Sample : 03384-07
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP070823\
Data File : BP016145.D
Acq On : 09 Jul 2023 22:27
Operator : MA/JU
Sample : 03384-07
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YBW83

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------