




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 10 23:22:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

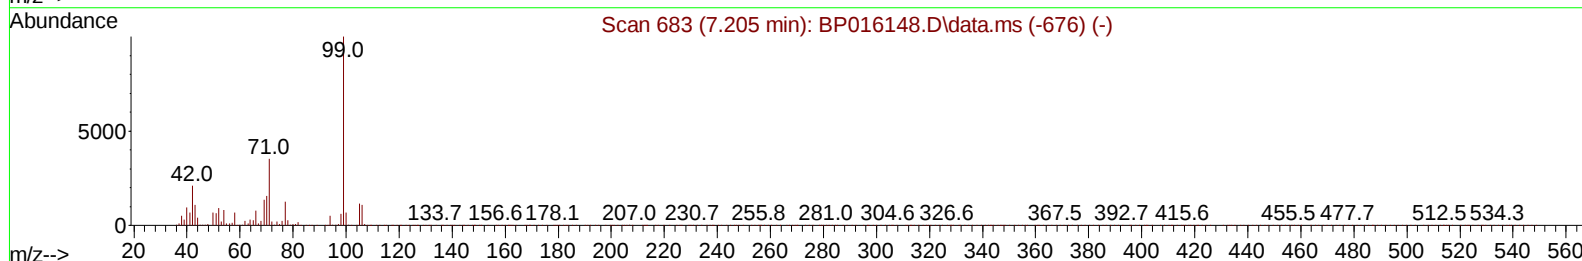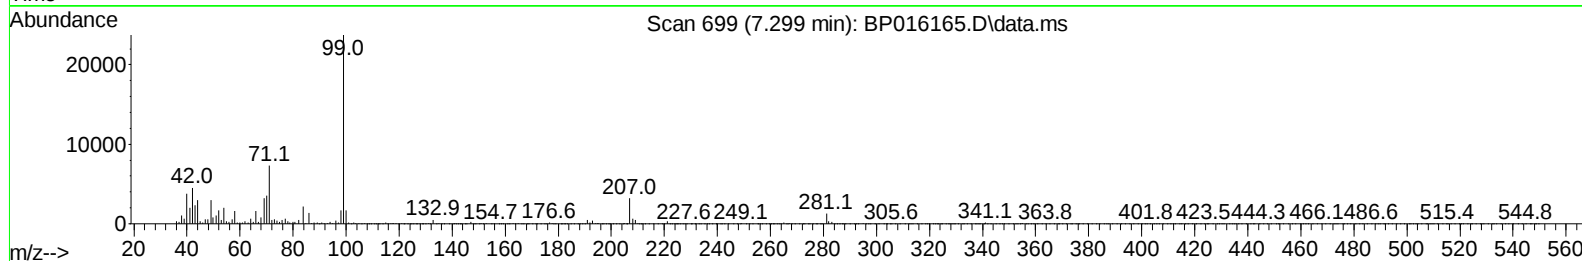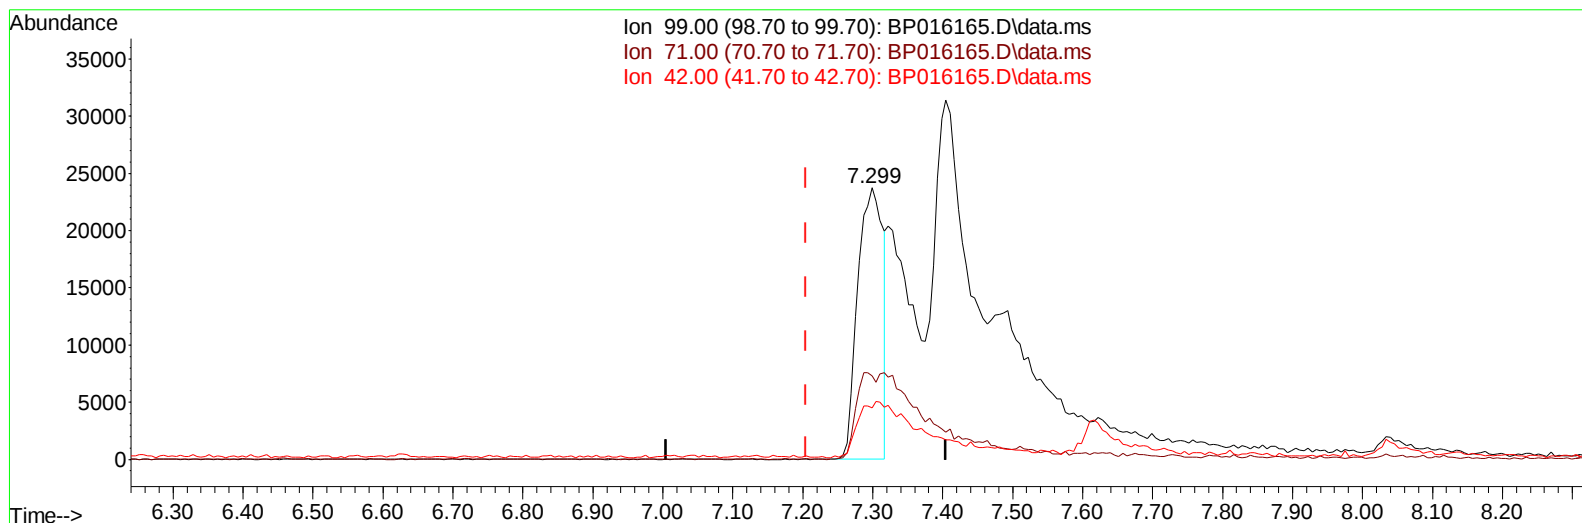

TIC: BP016165.D\data.ms

(7) Phenol-d5 (S)

7.299min (+ 0.094) 2.55 ng/ul

response 59298

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	30.77#
42.00	21.90	18.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 10 23:22:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

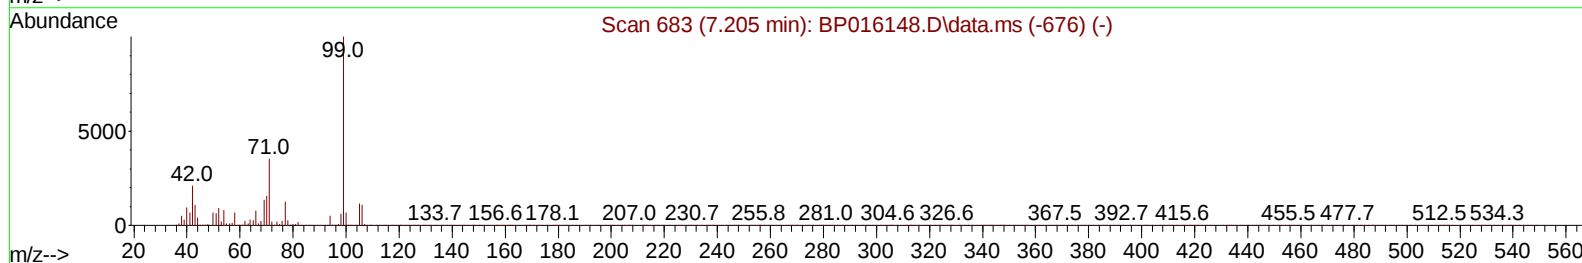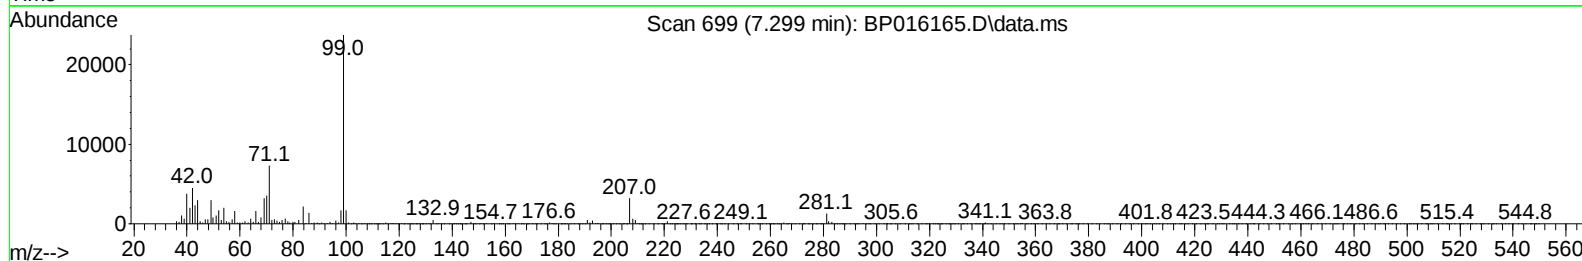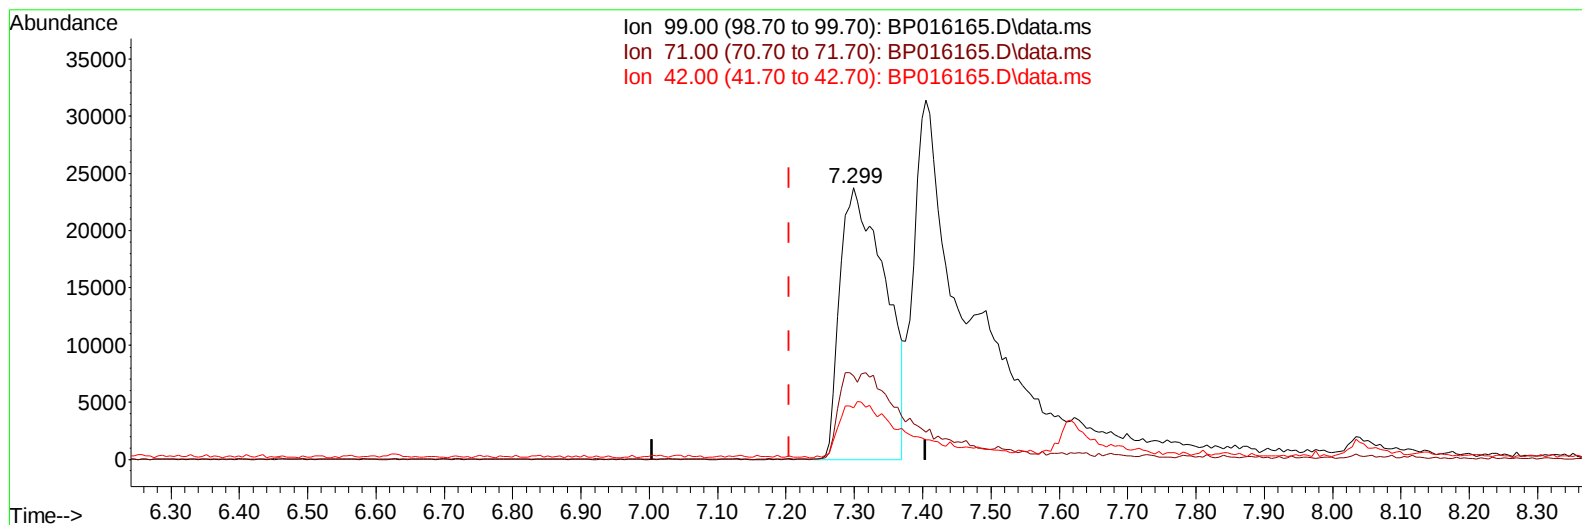

TIC: BP016165.D\data.ms

(7) Phenol-d5 (S)

7.299min (+ 0.094) 4.68 ng/u1 m

response 108902

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	42.70	30.77#
42.00	21.90	18.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:19:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

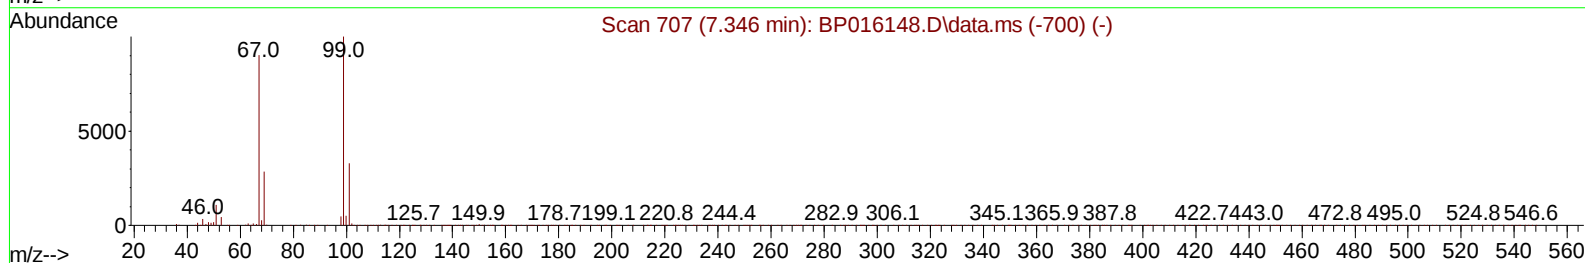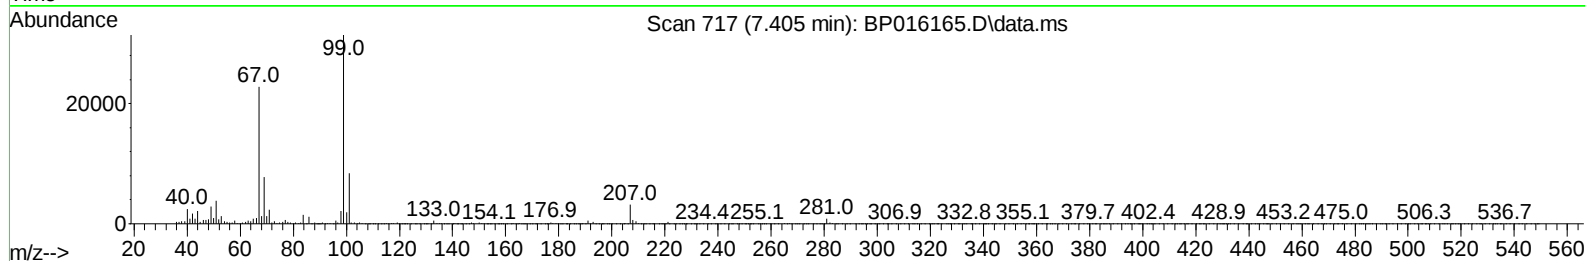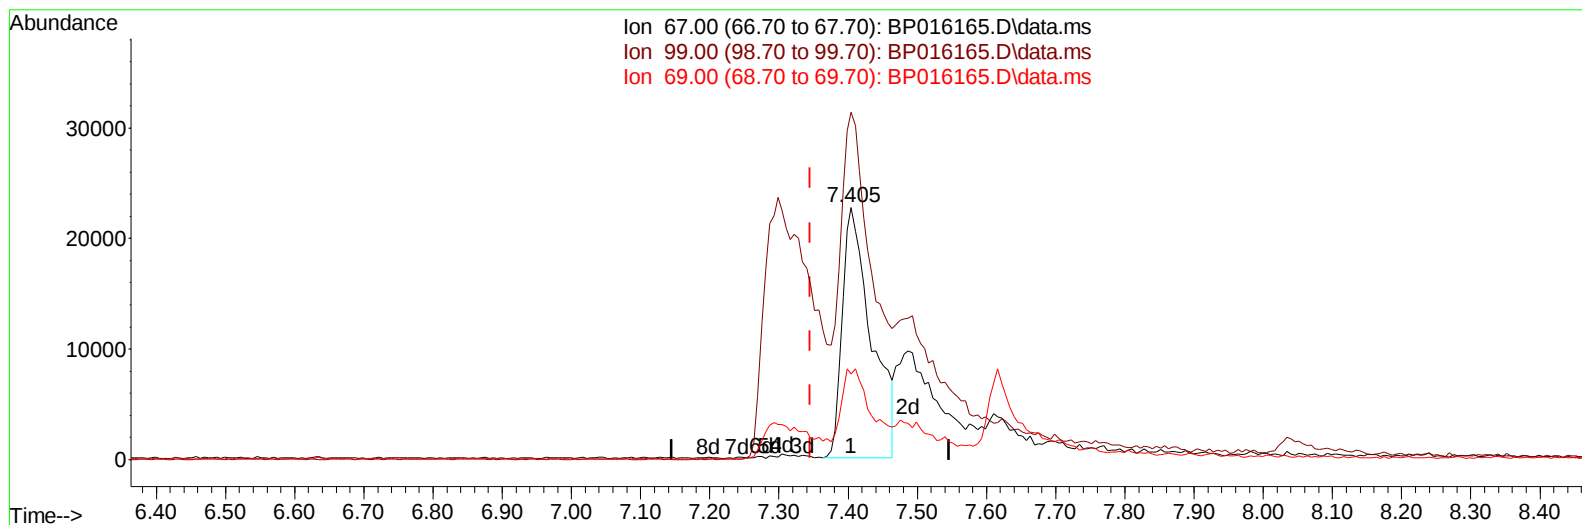

TIC: BP016165.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.405min (+ 0.059) 4.59 ng/u1

response 65981

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	137.69
69.00	32.10	33.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:19:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

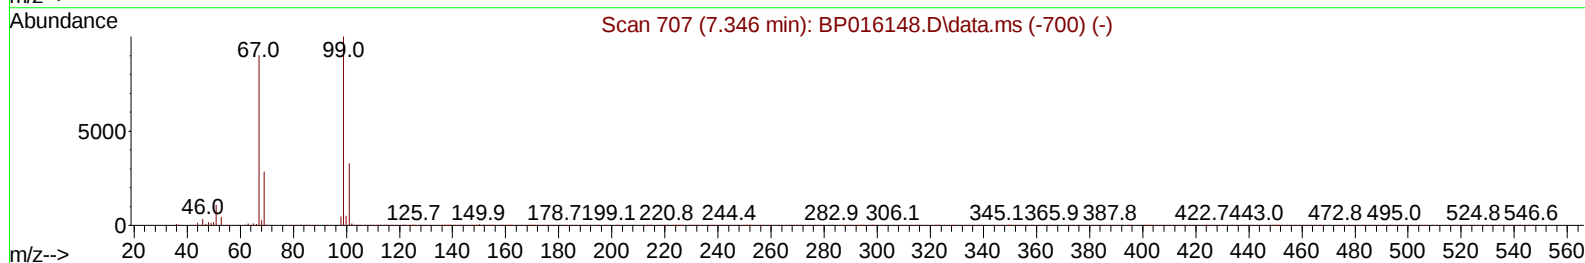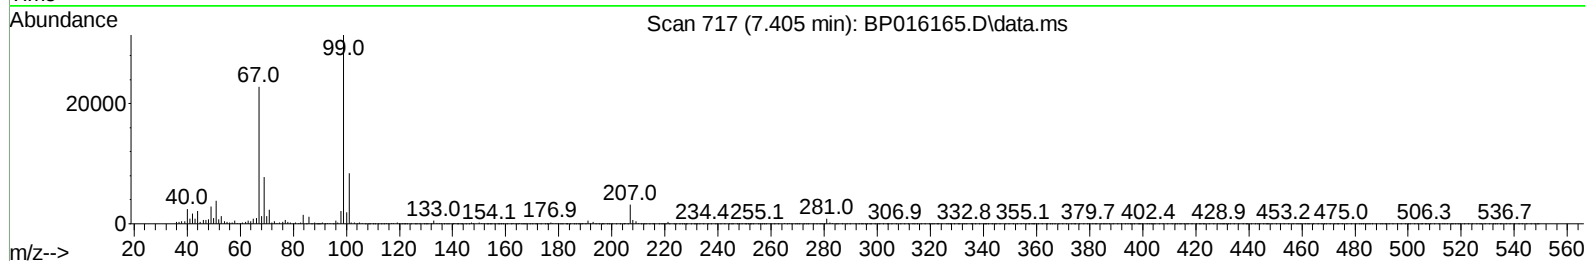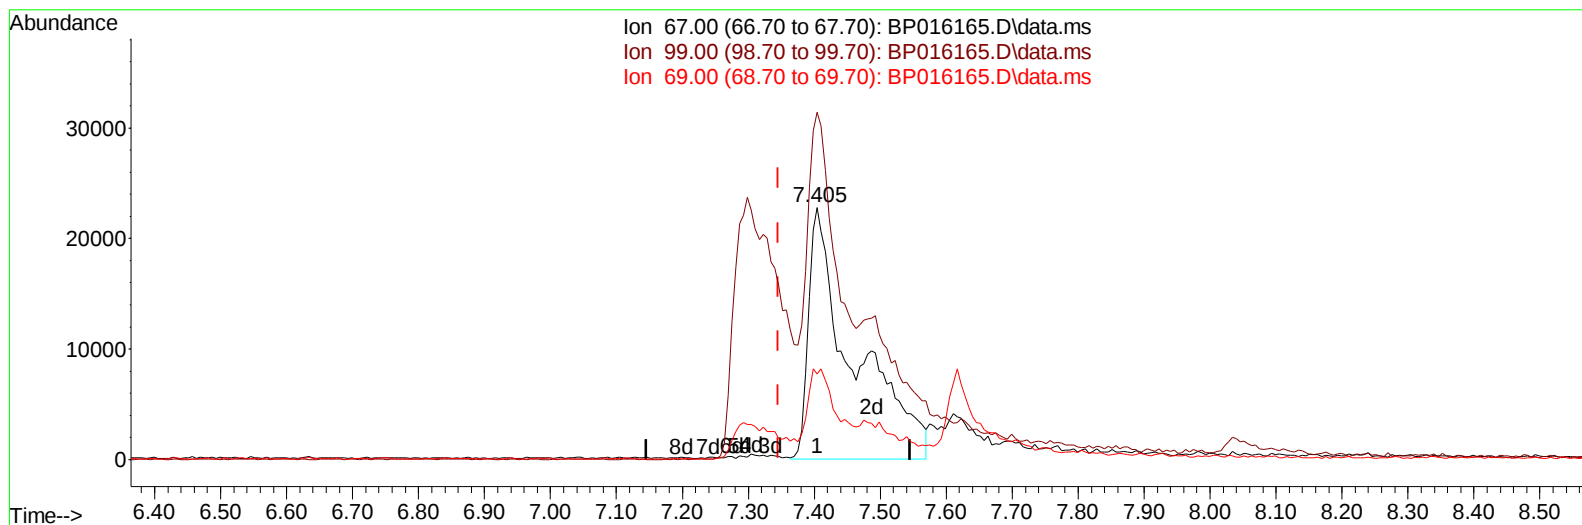

TIC: BP016165.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.405min (+ 0.059) 7.36 ng/ul m

response 105889

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.80	137.69
69.00	32.10	33.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:19:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

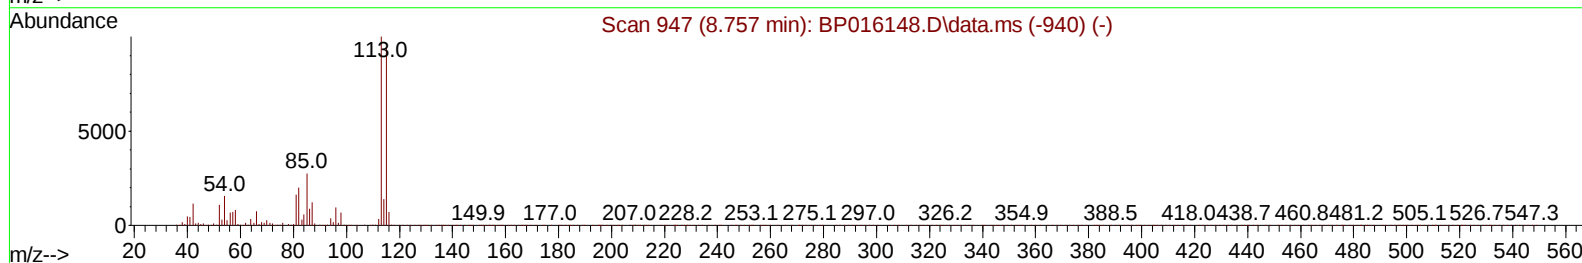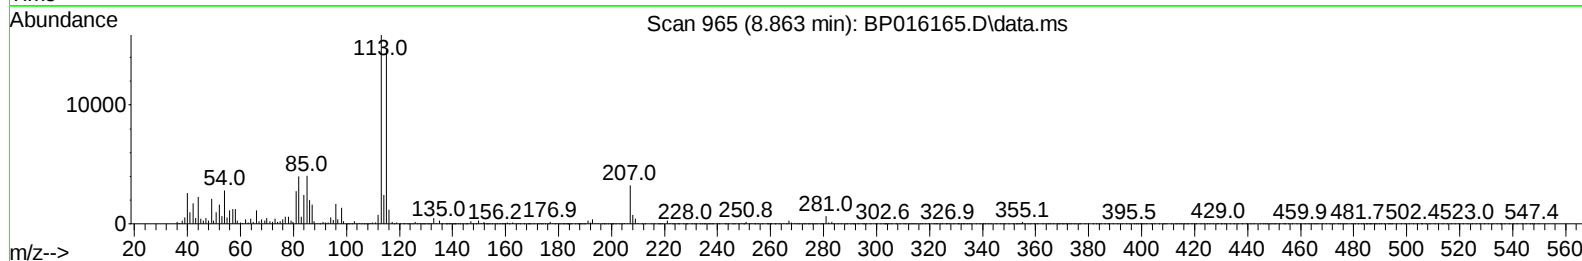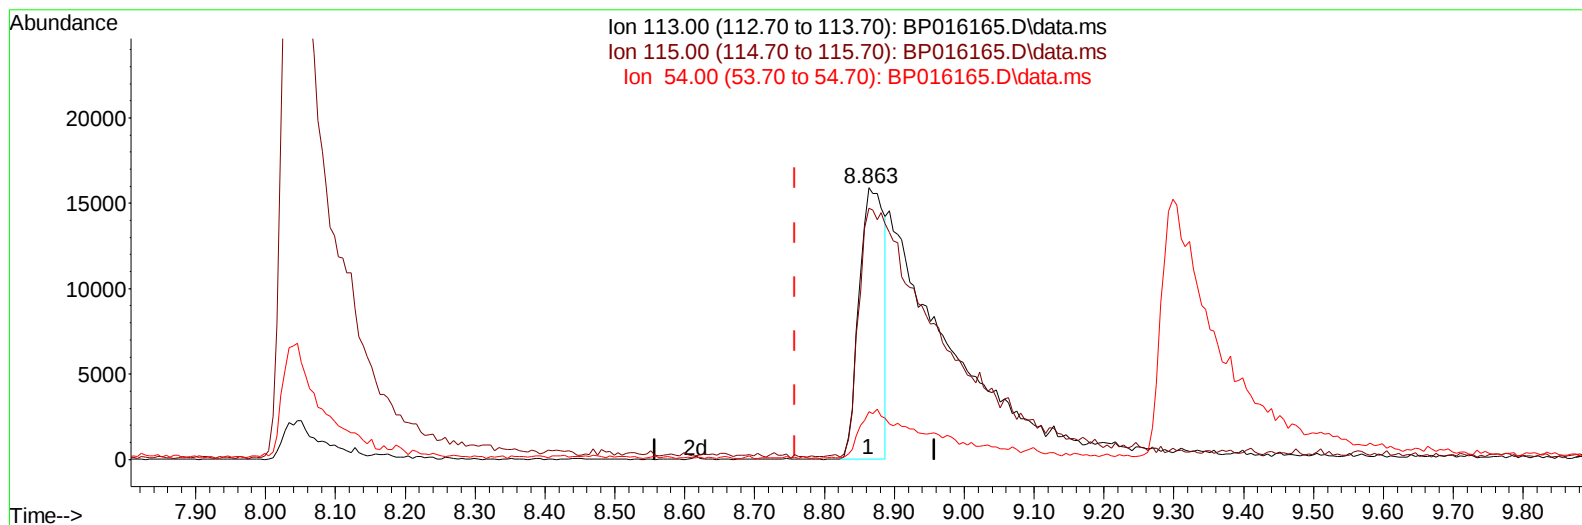

TIC: BP016165.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.863min (+ 0.106) 2.15 ng/u1

response 39568

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	92.62
54.00	16.10	17.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:19:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

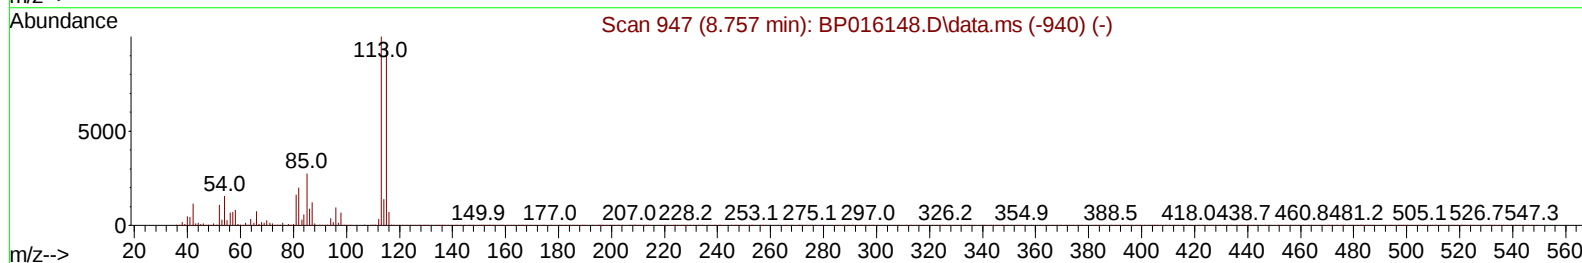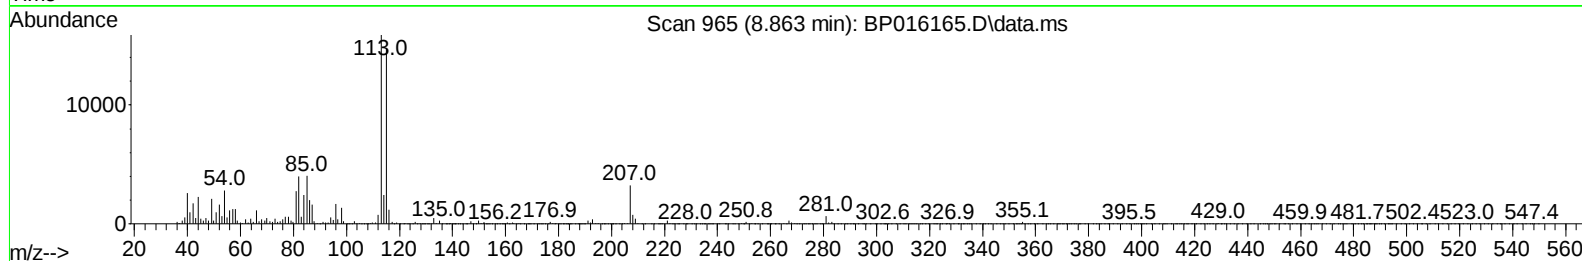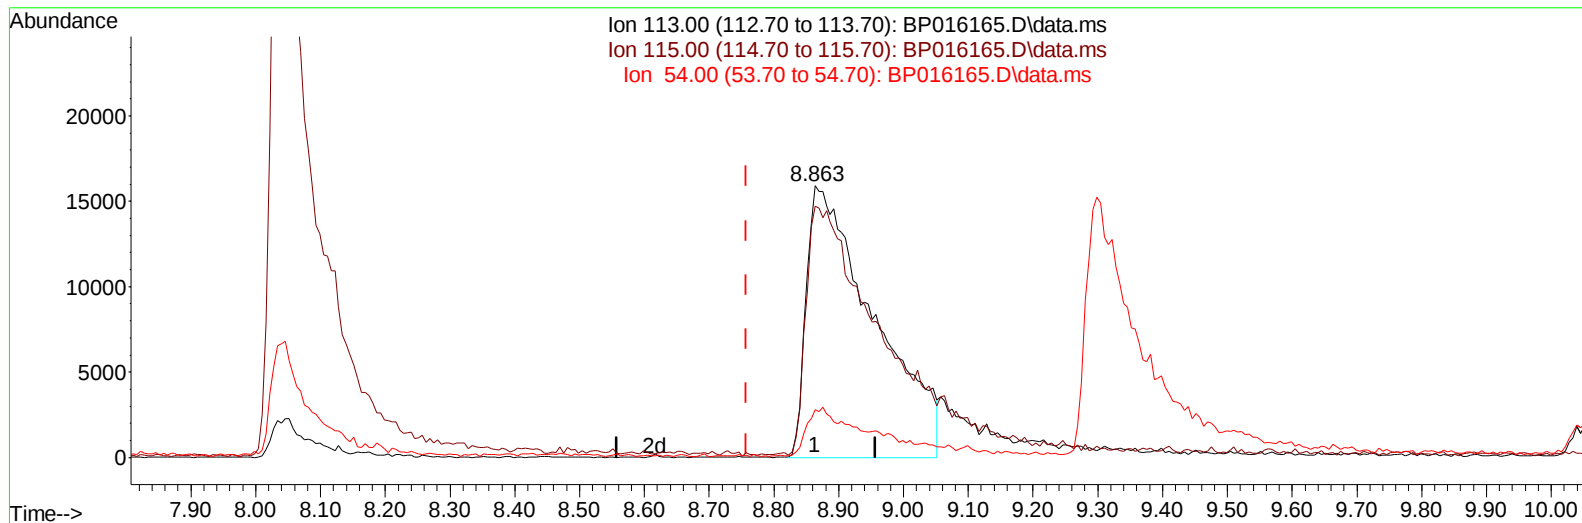

TIC: BP016165.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.863min (+ 0.106) 6.28 ng/ul m

response 115435

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.10	92.62
54.00	16.10	17.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:19:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

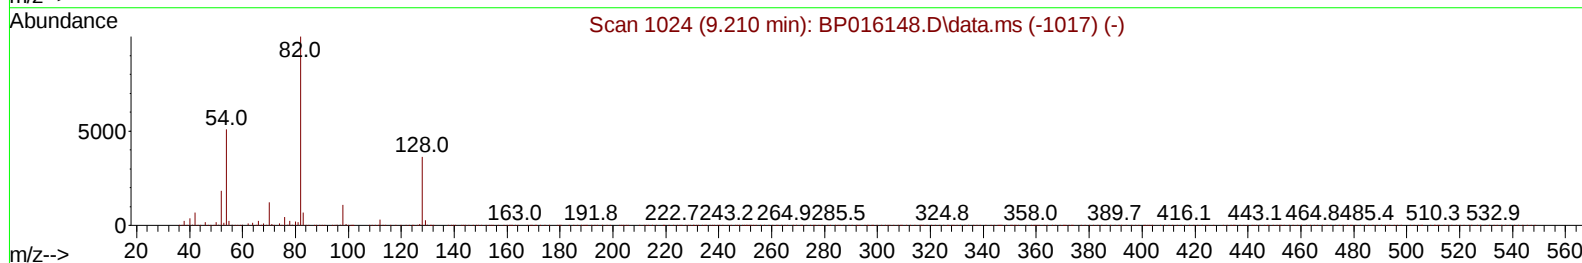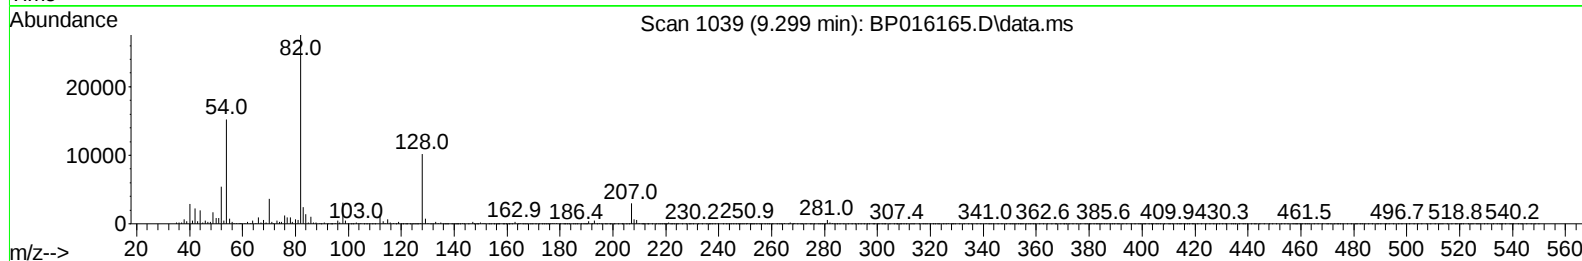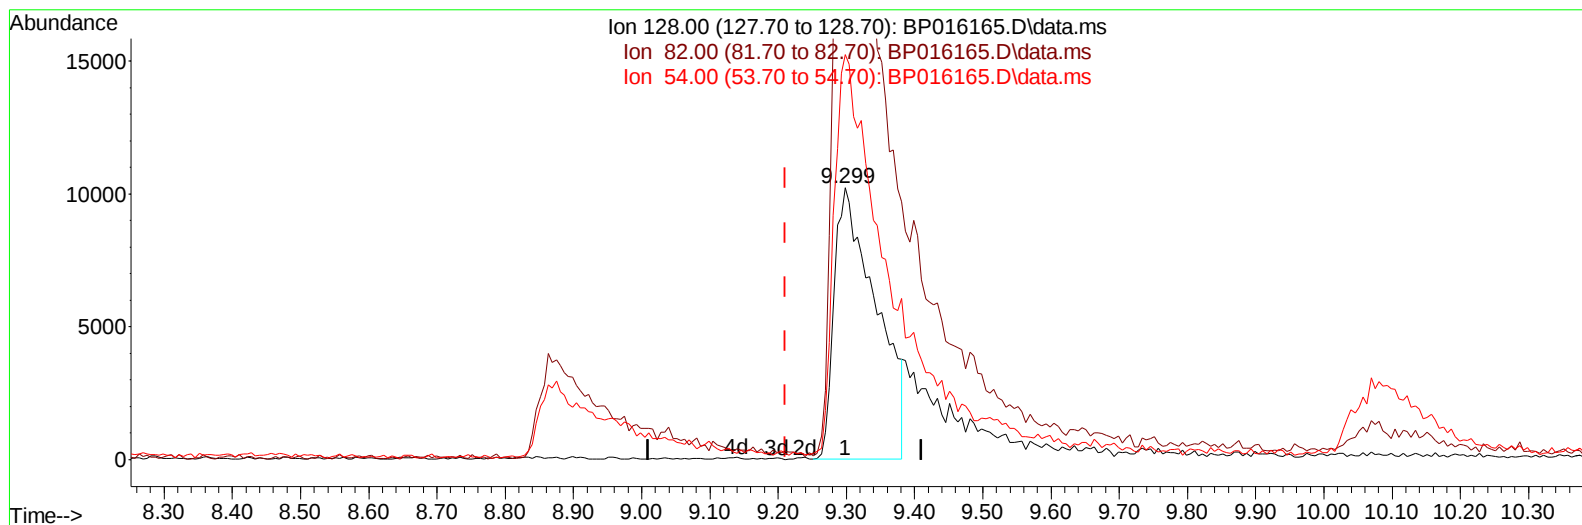

TIC: BP016165.D\data.ms

(21) Nitrobenzene-d5 (S)

9.299min (+ 0.088) 4.19 ng/u1

response 43626

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	269.56
54.00	141.60	149.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:19:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

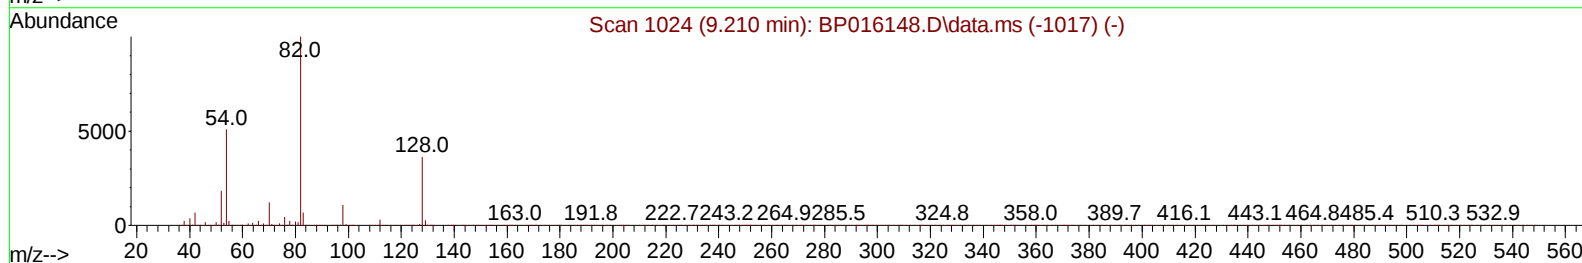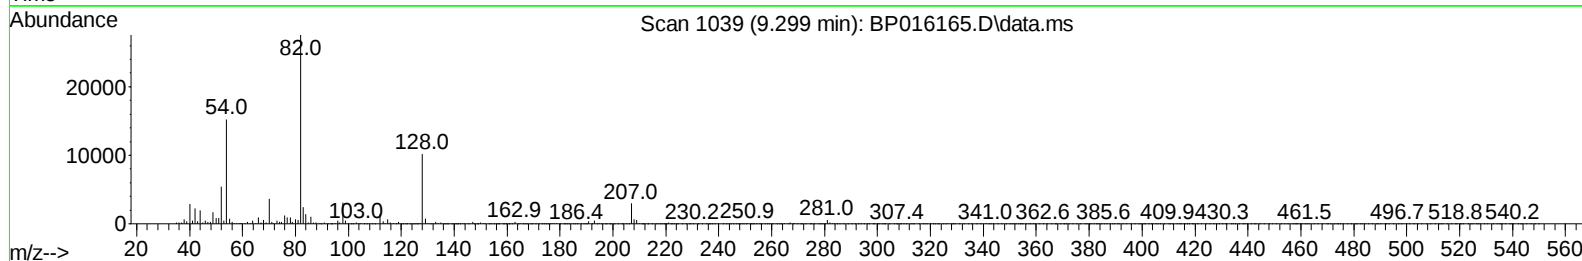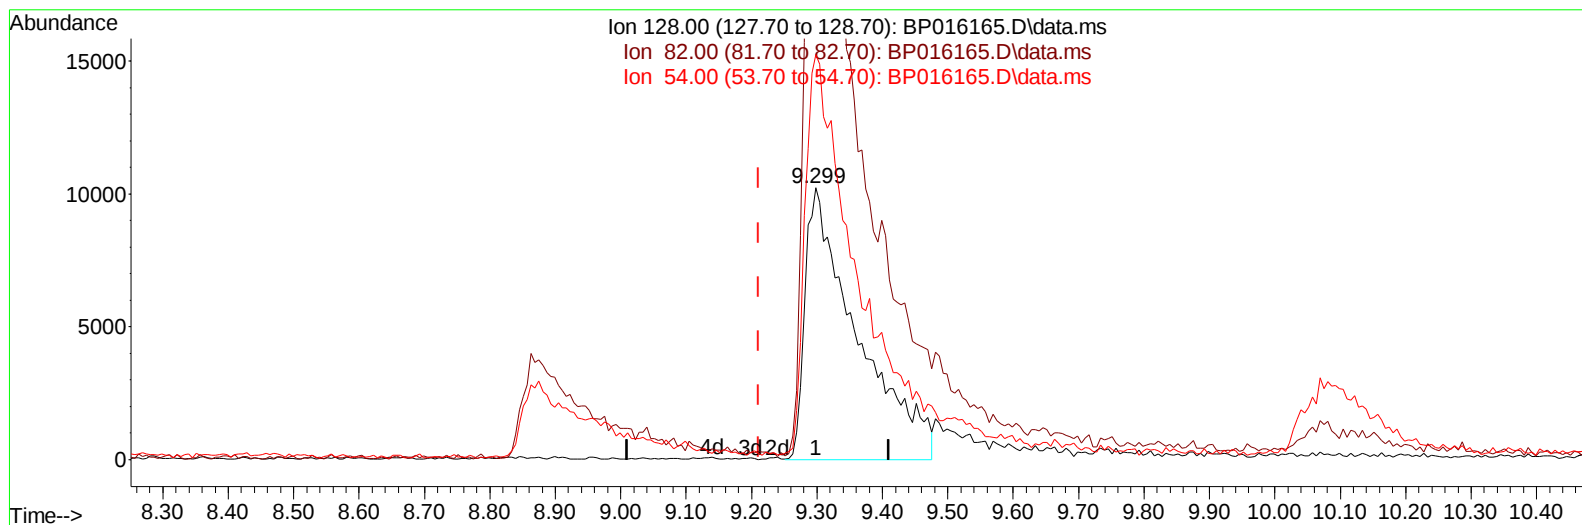

TIC: BP016165.D\data.ms

(21) Nitrobenzene-d5 (S)

9.299min (+ 0.088) 5.40 ng/ul m

response 56177

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	268.20	269.56
54.00	141.60	149.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:20:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

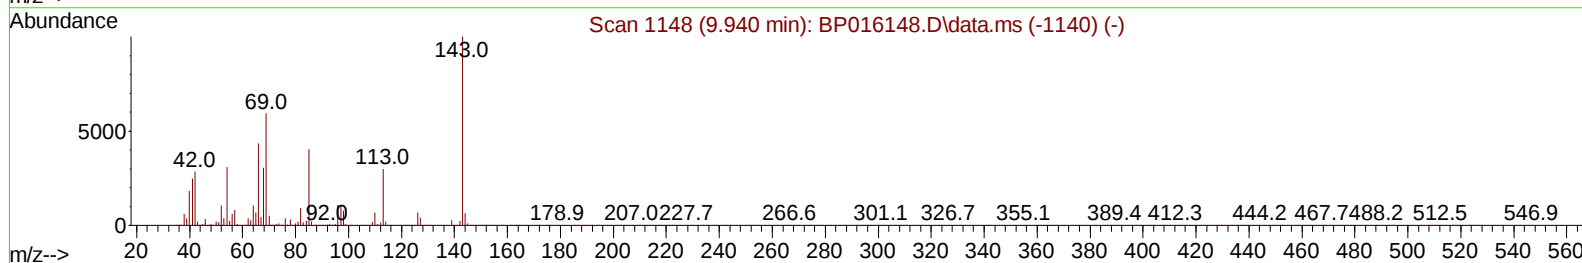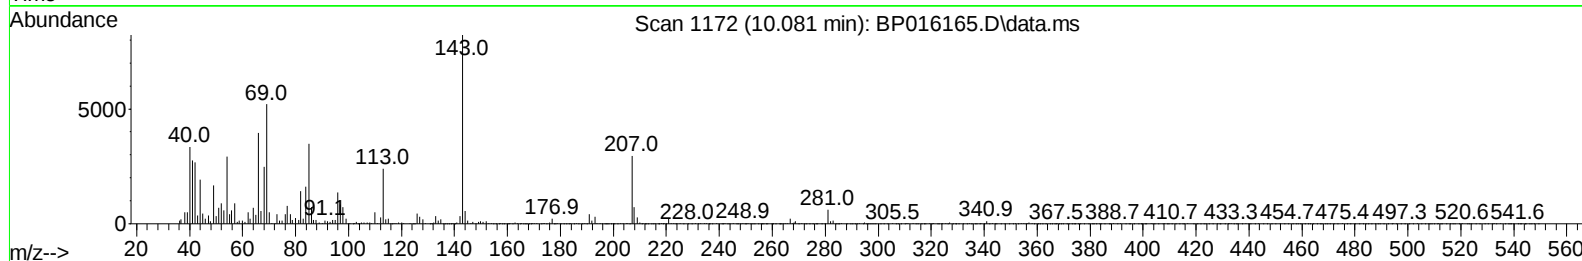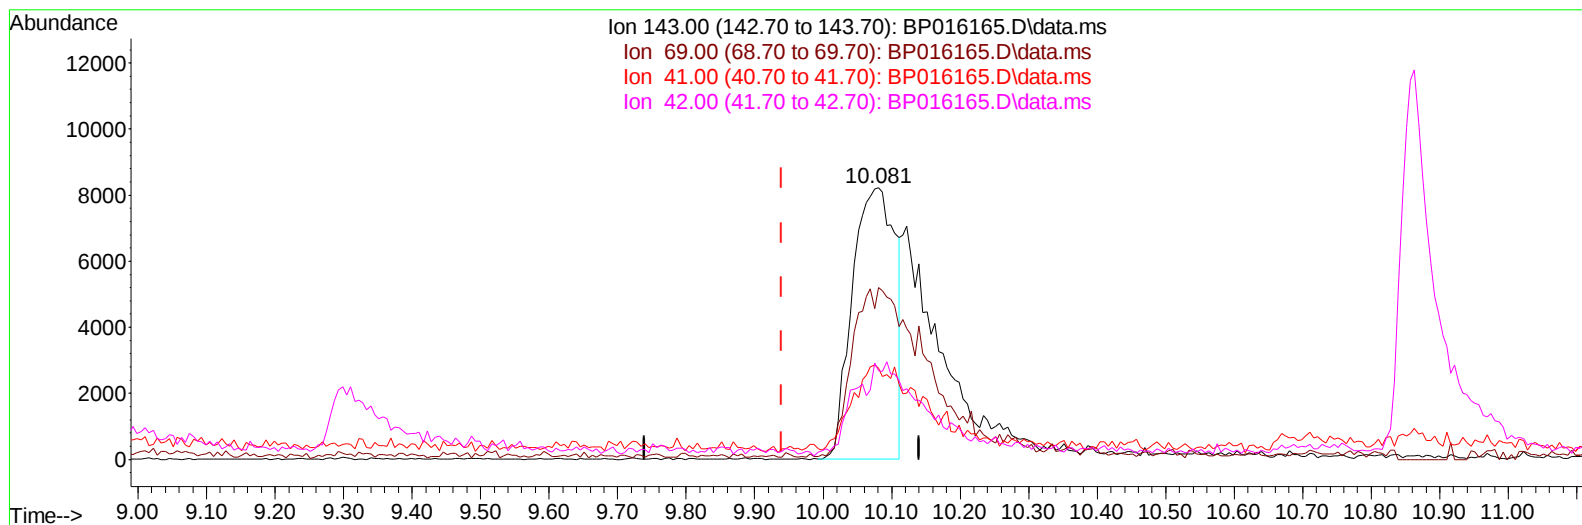

TIC: BP016165.D\data.ms

(24) 2-Nitrophenol-d4 (S)

10.081min (+ 0.141) 2.90 ng/u1

response 35273

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	63.27
41.00	26.80	33.54#
42.00	30.50	32.70




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:20:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

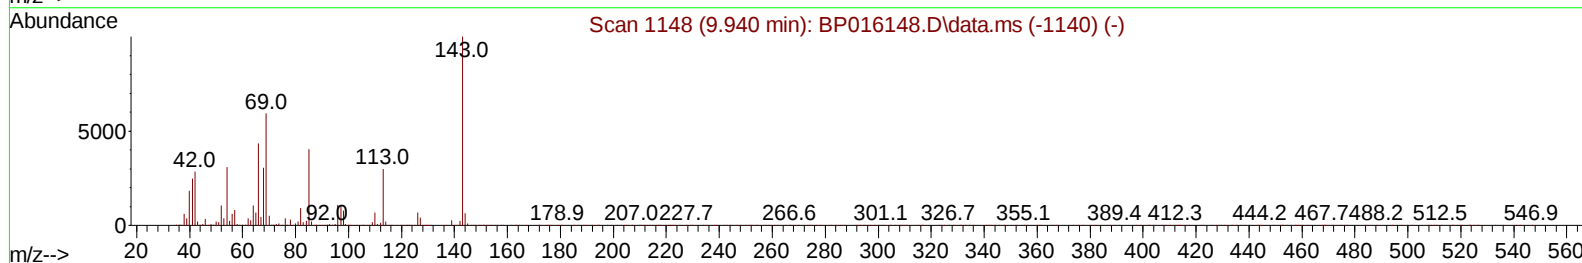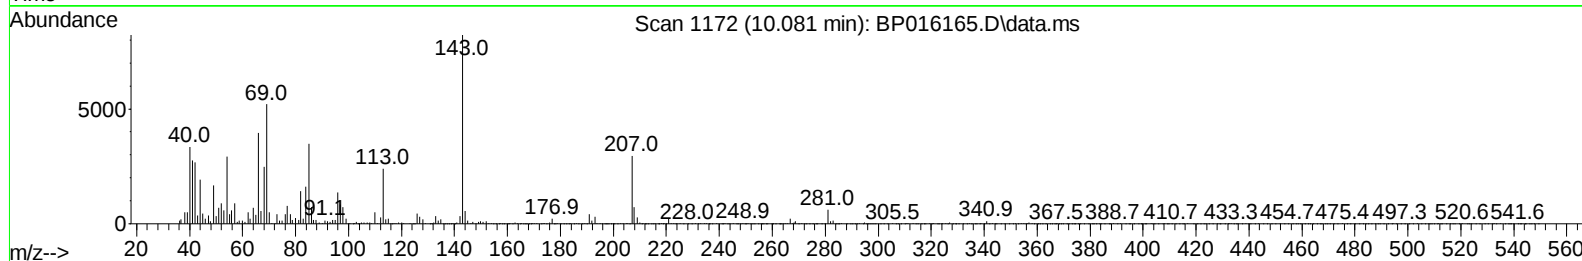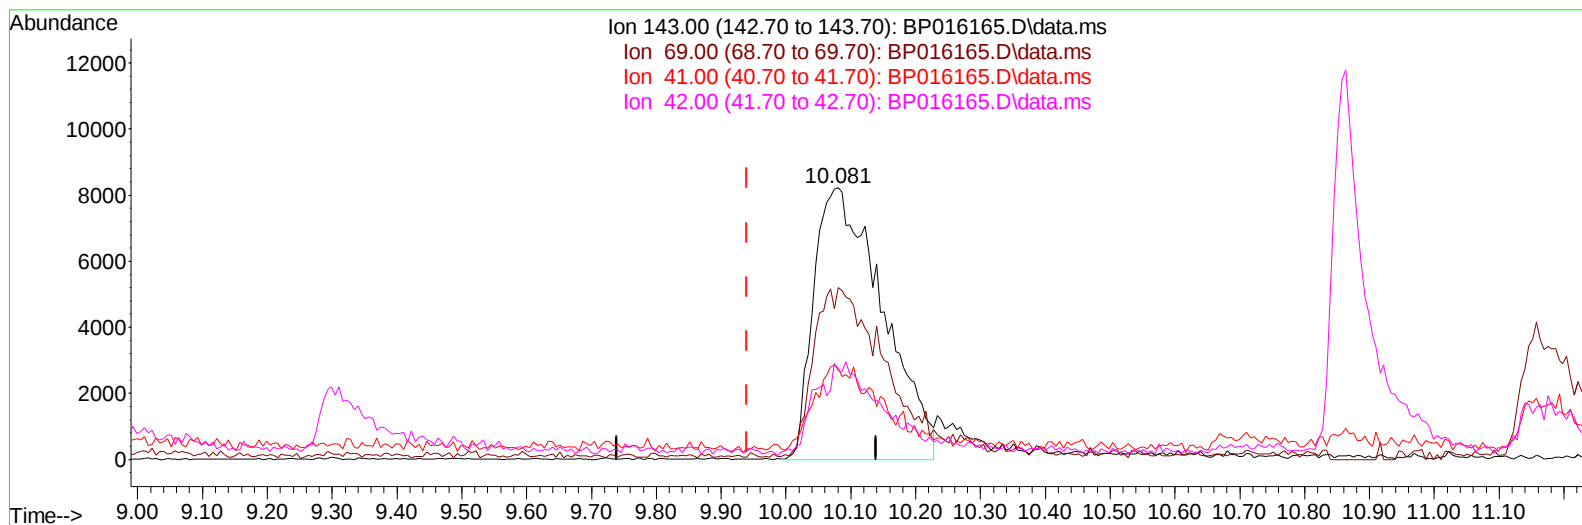

TIC: BP016165.D\data.ms

(24) 2-Nitrophenol-d4 (S)

10.081min (+ 0.141) 4.98 ng/ul m

response 60571

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	60.40	63.27
41.00	26.80	33.54#
42.00	30.50	32.70




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:20:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

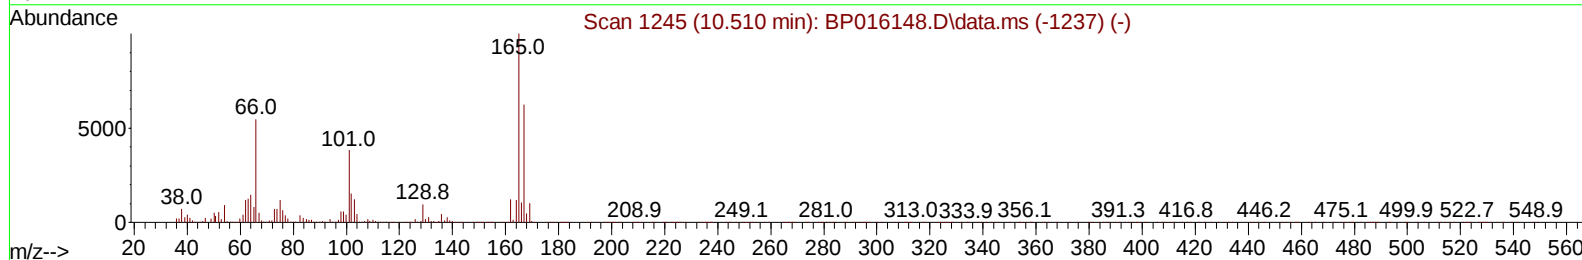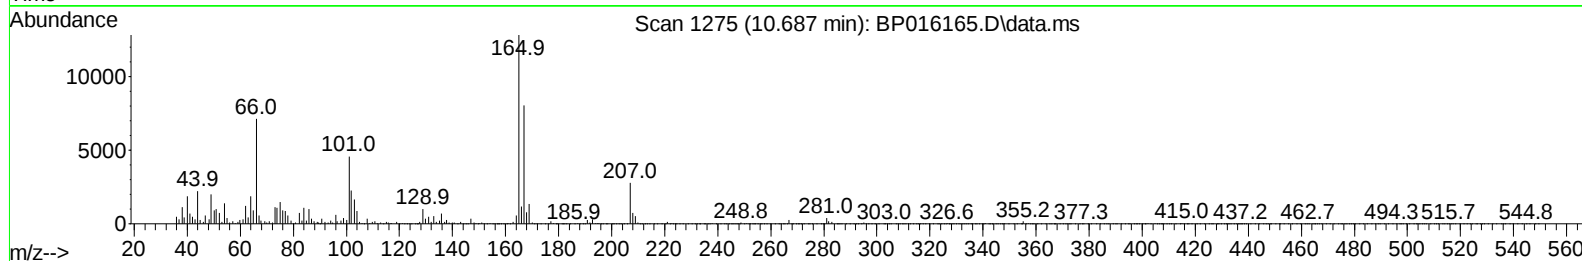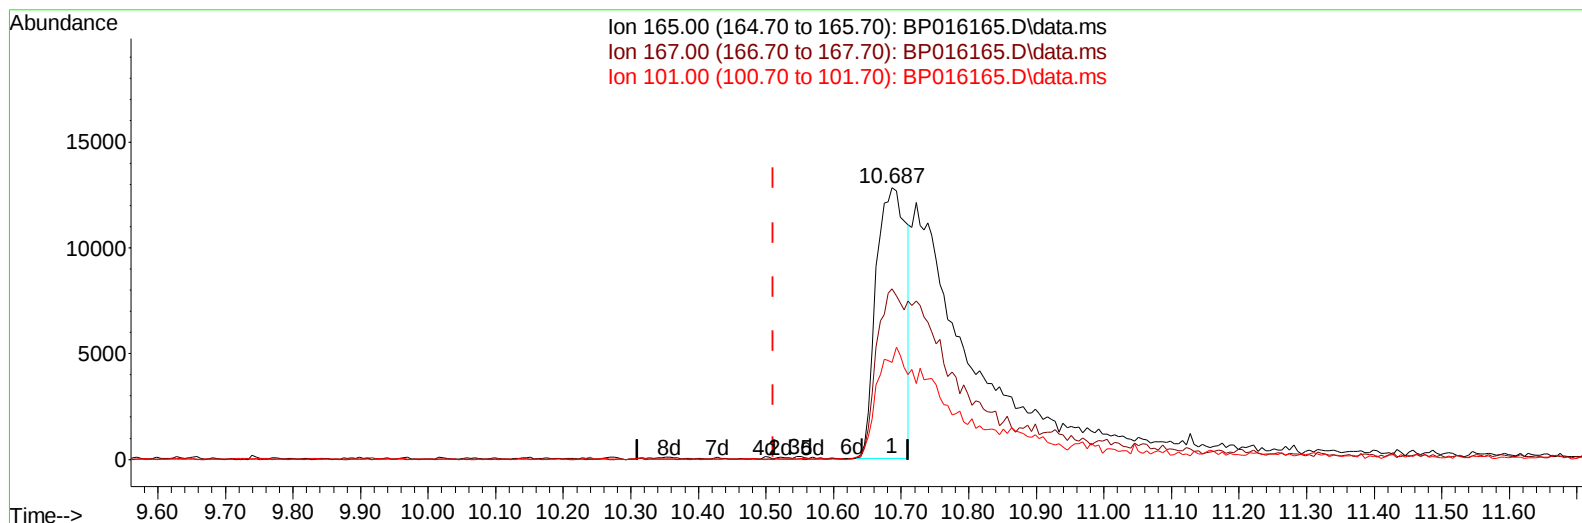

TIC: BP016165.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.687min (+ 0.176) 1.81 ng/ul

response 39193

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	62.82
101.00	37.30	35.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:20:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

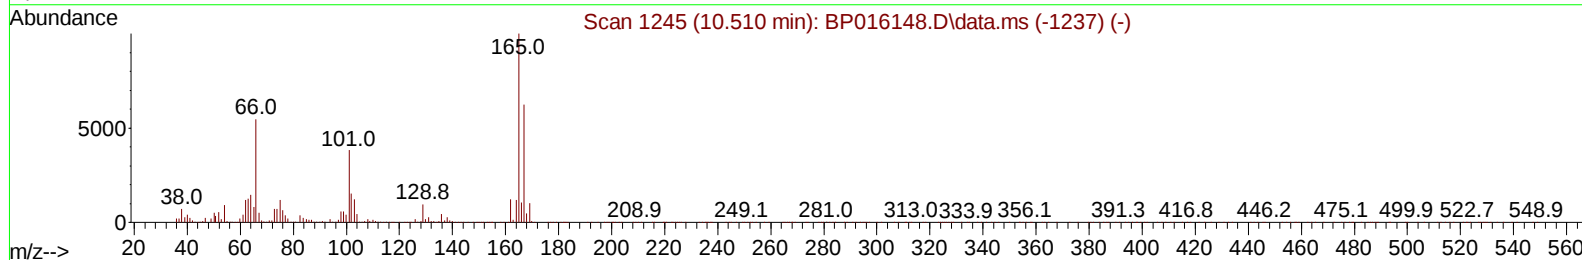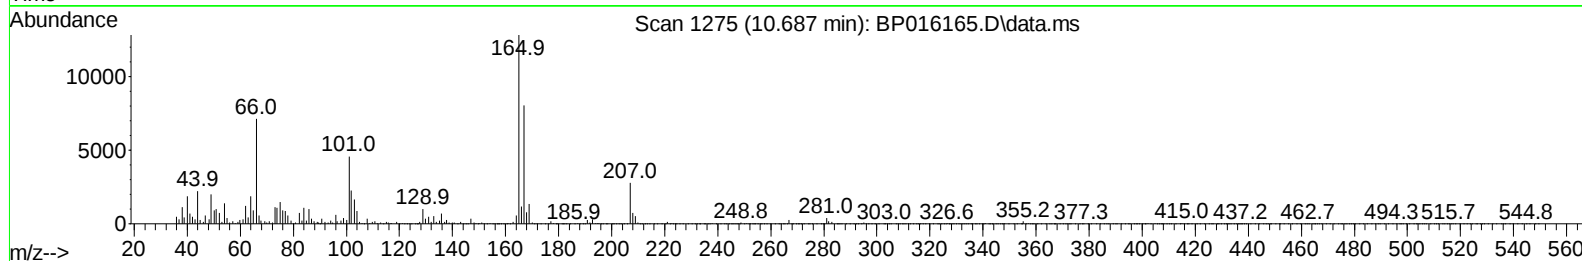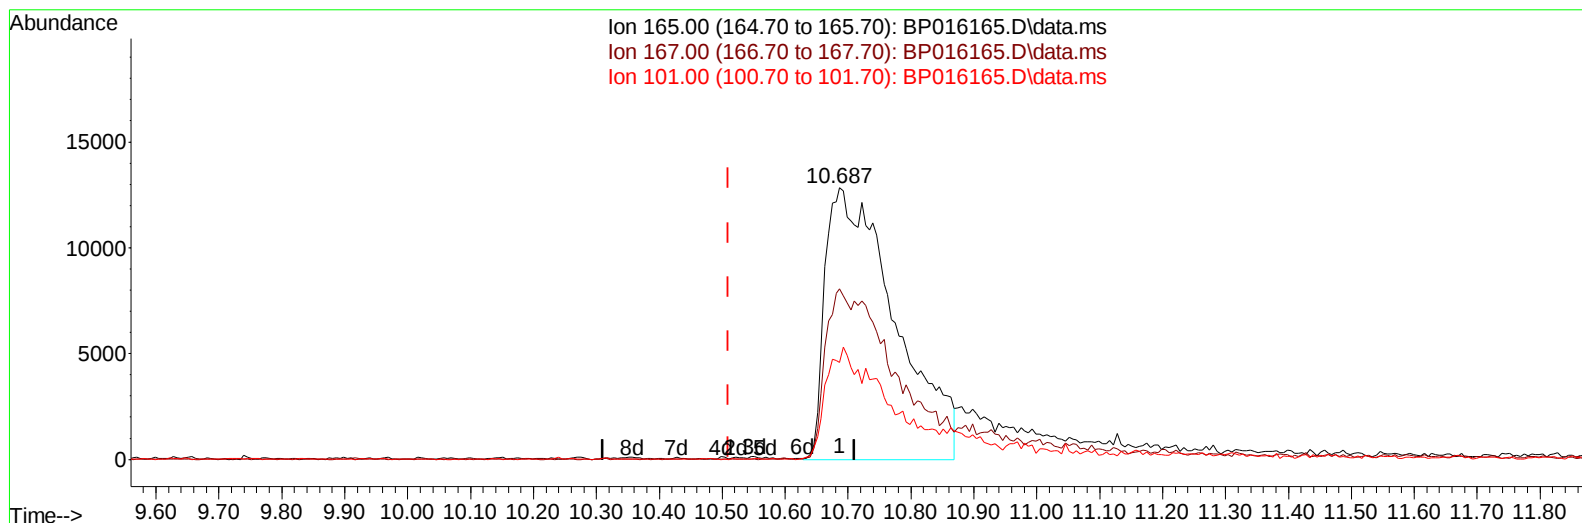

TIC: BP016165.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.687min (+ 0.176) 4.57 ng/ul m

response 98900

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	66.20	62.82
101.00	37.30	35.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:20:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

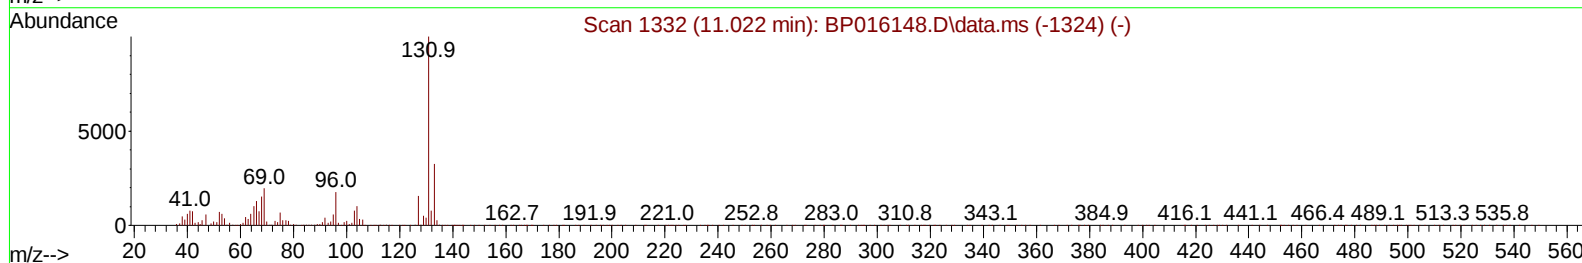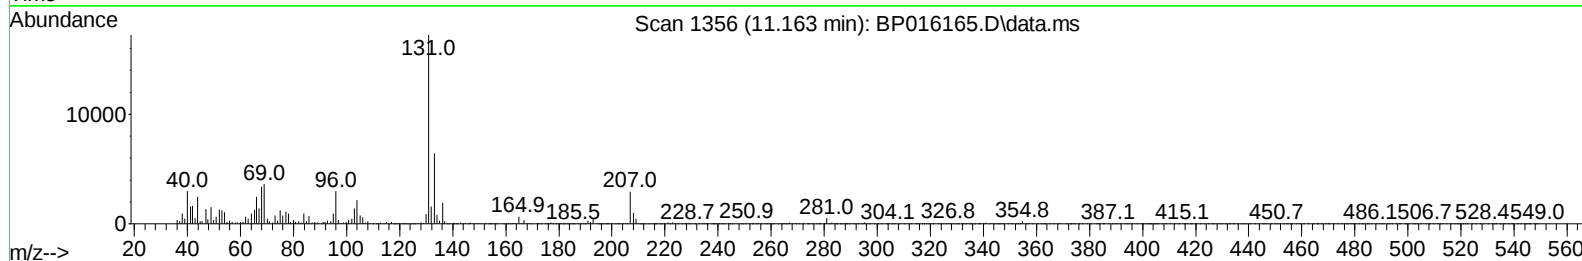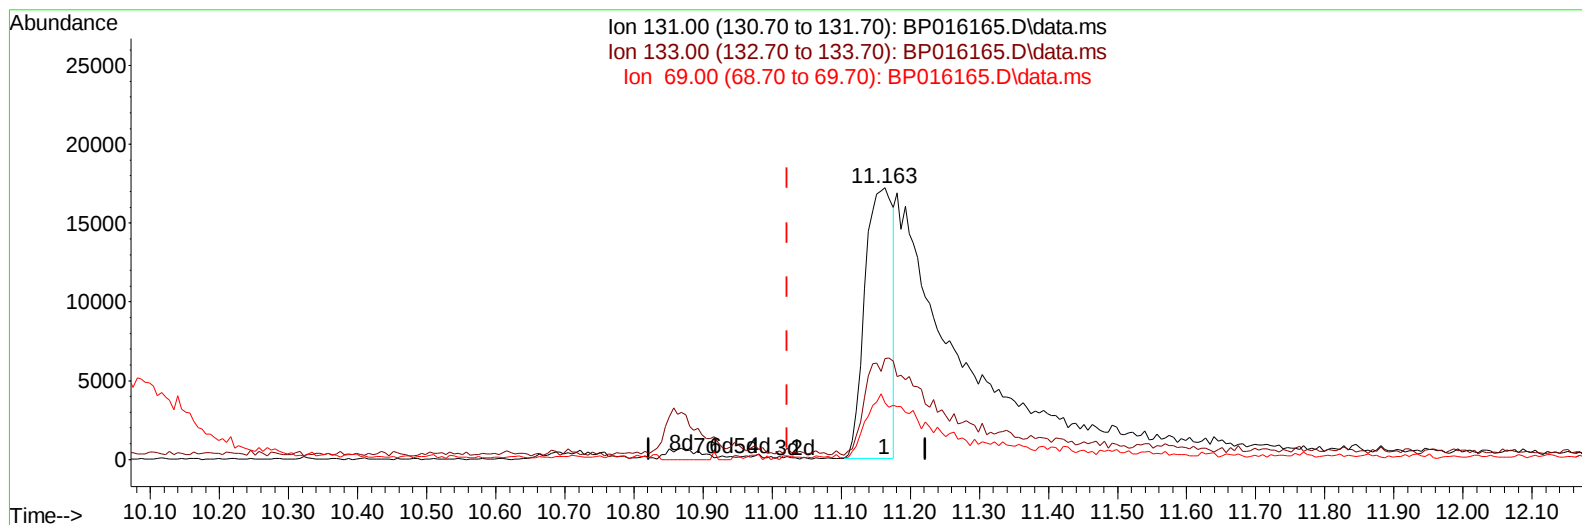

TIC: BP016165.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.163min (+ 0.141) 1.71 ng/ul

response 47561

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	37.23
69.00	22.20	20.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:20:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

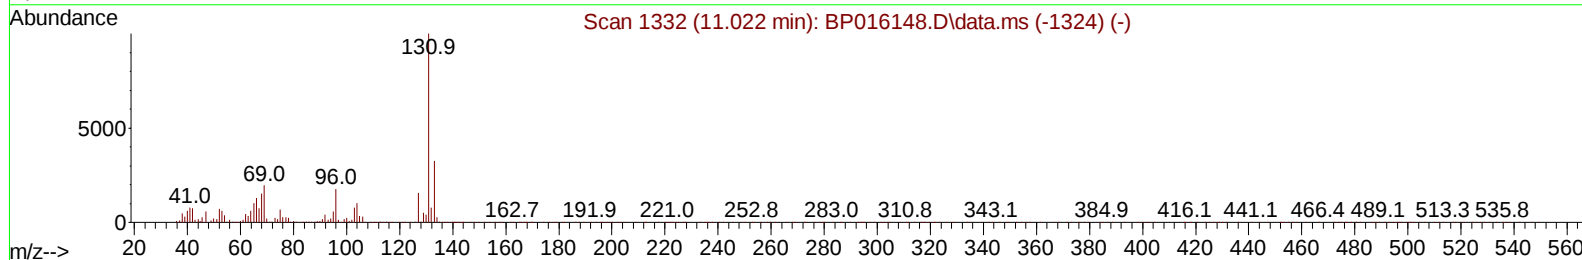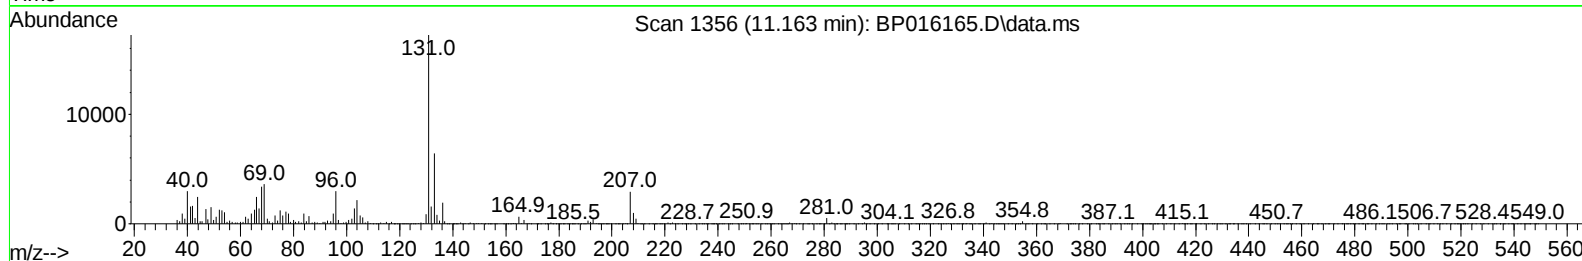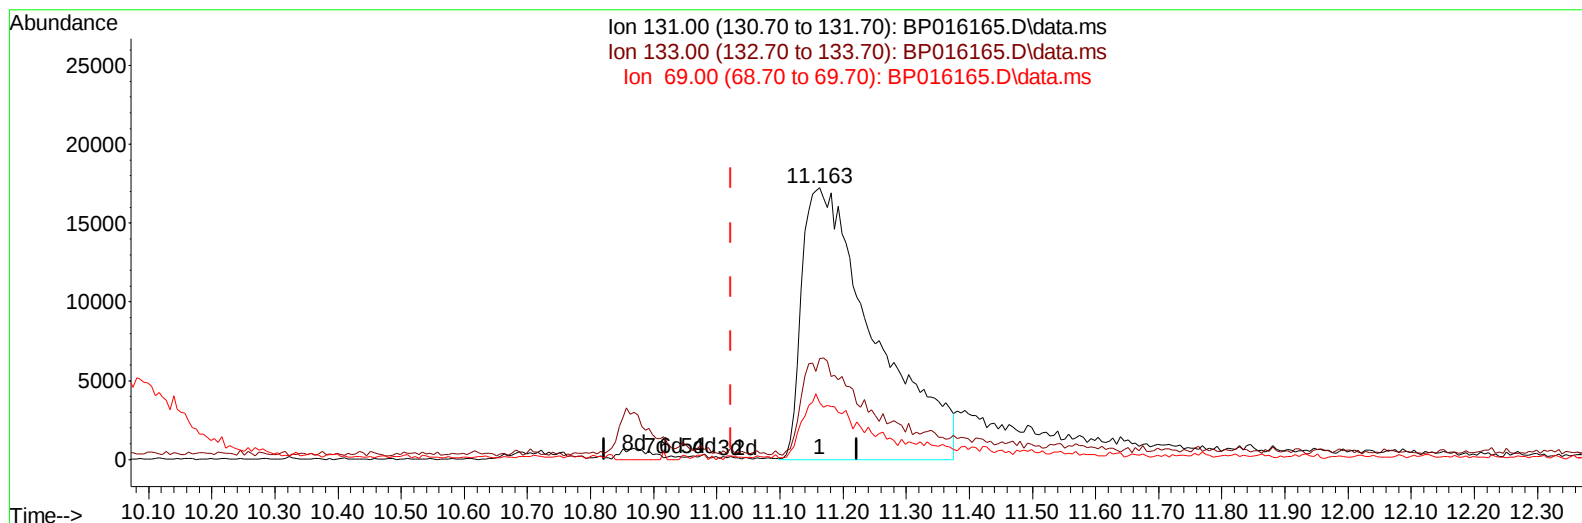

TIC: BP016165.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.163min (+ 0.141) 4.93 ng/ul m

response 137194

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	34.50	37.23
69.00	22.20	20.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:21:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

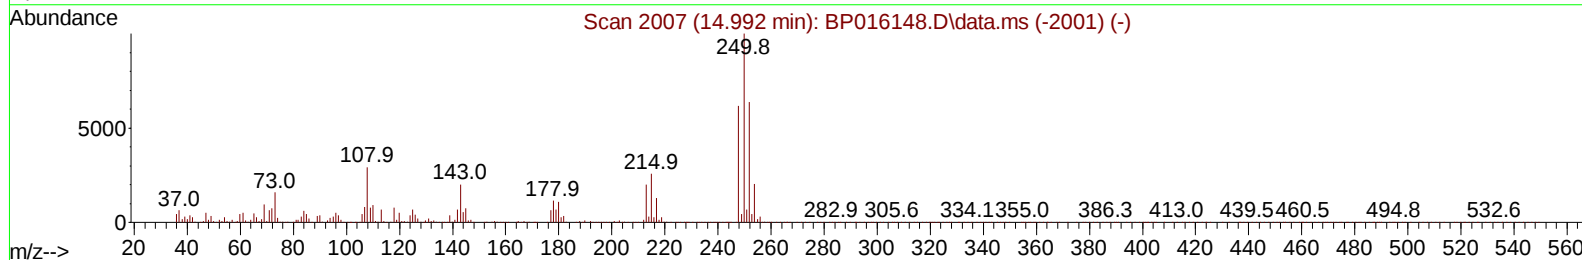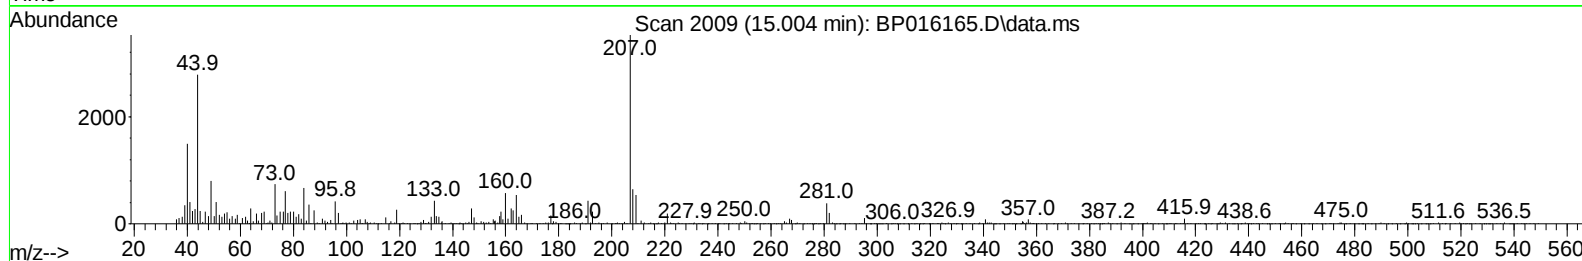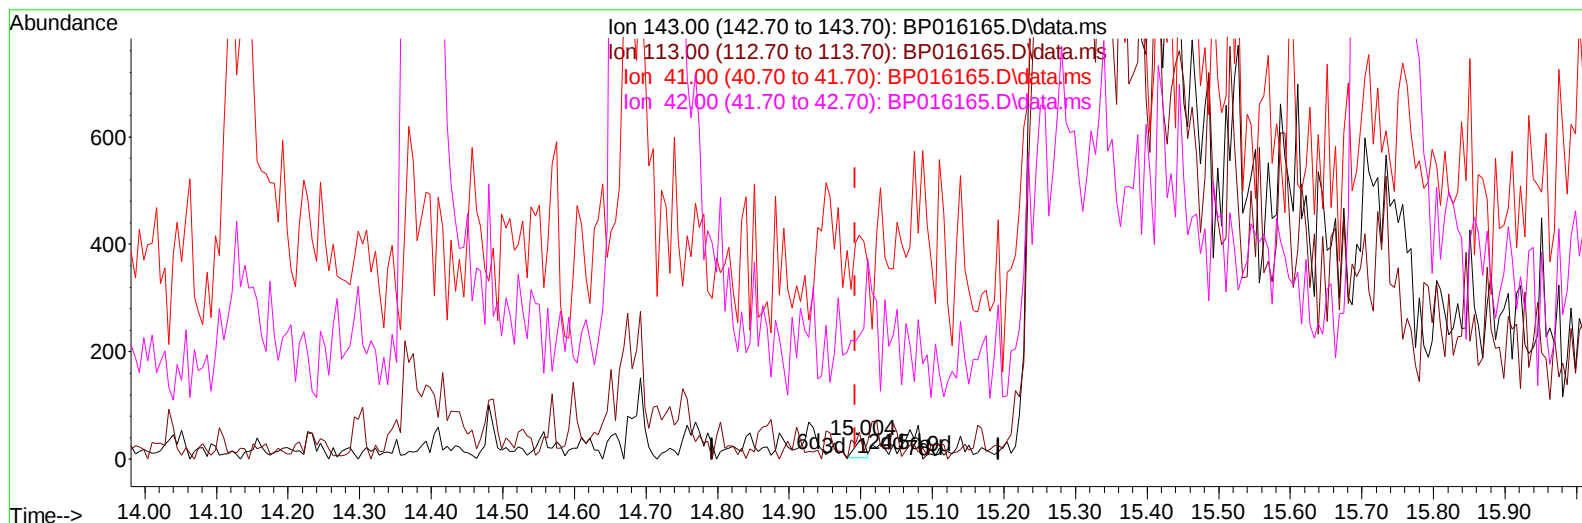

TIC: BP016165.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.004min (+ 0.012) 0.00 ng/u1

response 35

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	42.86#
41.00	45.70	1157.14#
42.00	31.20	694.29#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:21:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

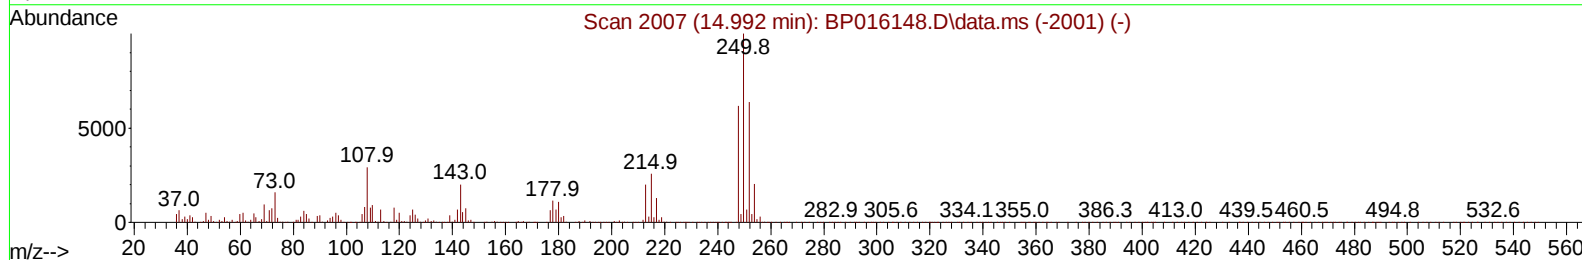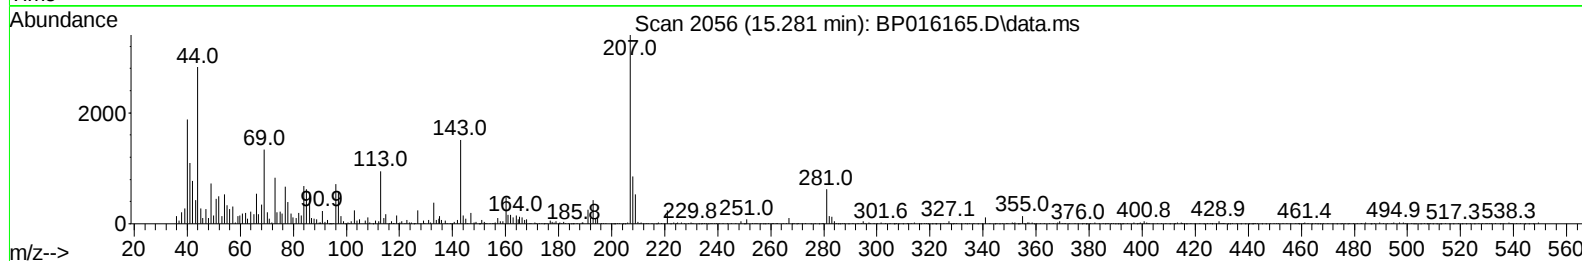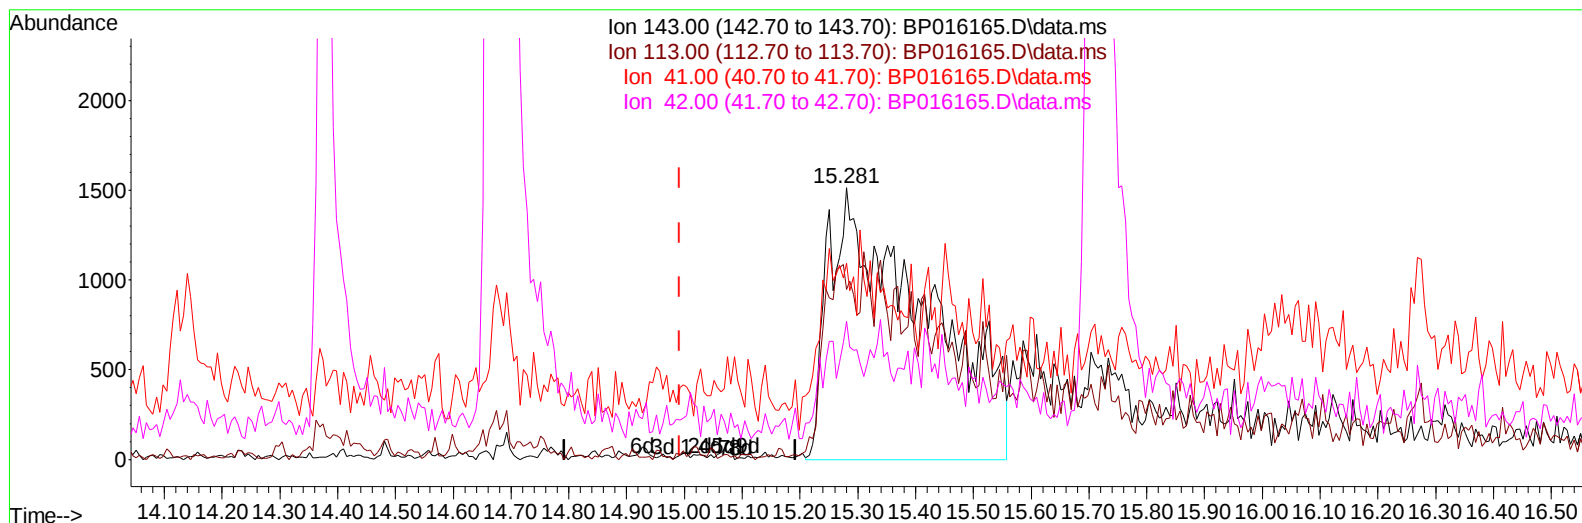

TIC: BP016165.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.281min (+ 0.288) 1.88 ng/ul m

response 17582

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.00	62.70#
41.00	45.70	72.22#
42.00	31.20	50.86#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:21:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

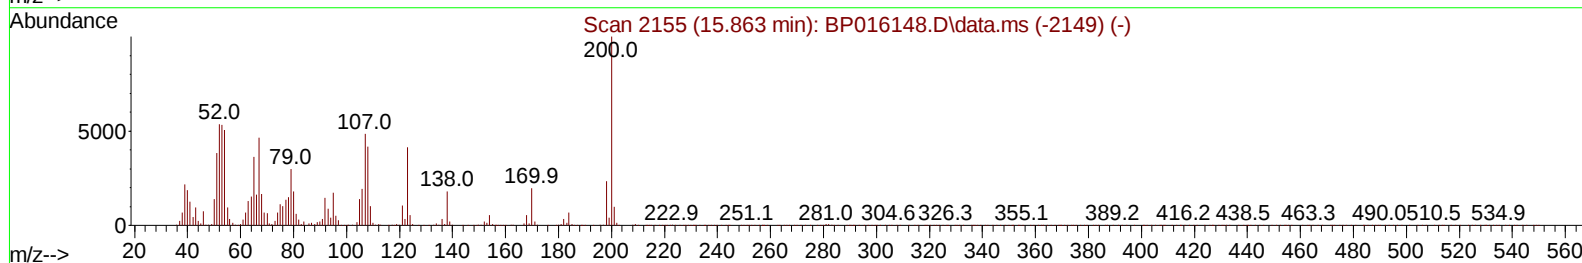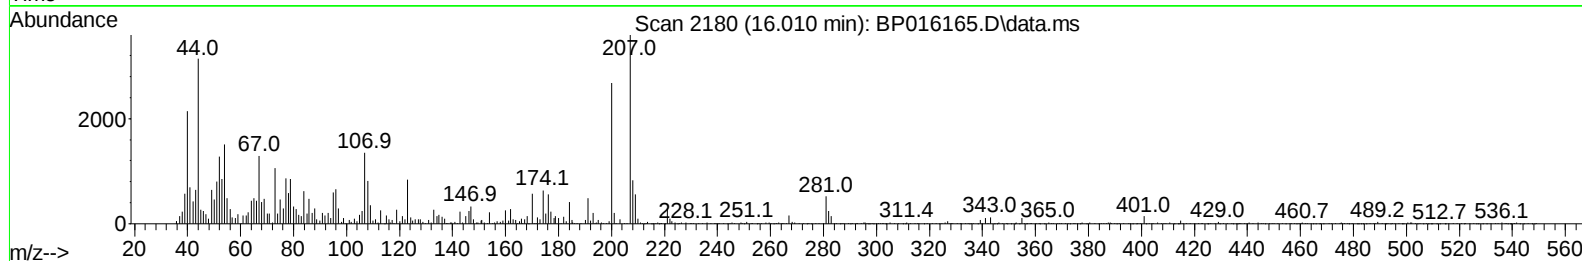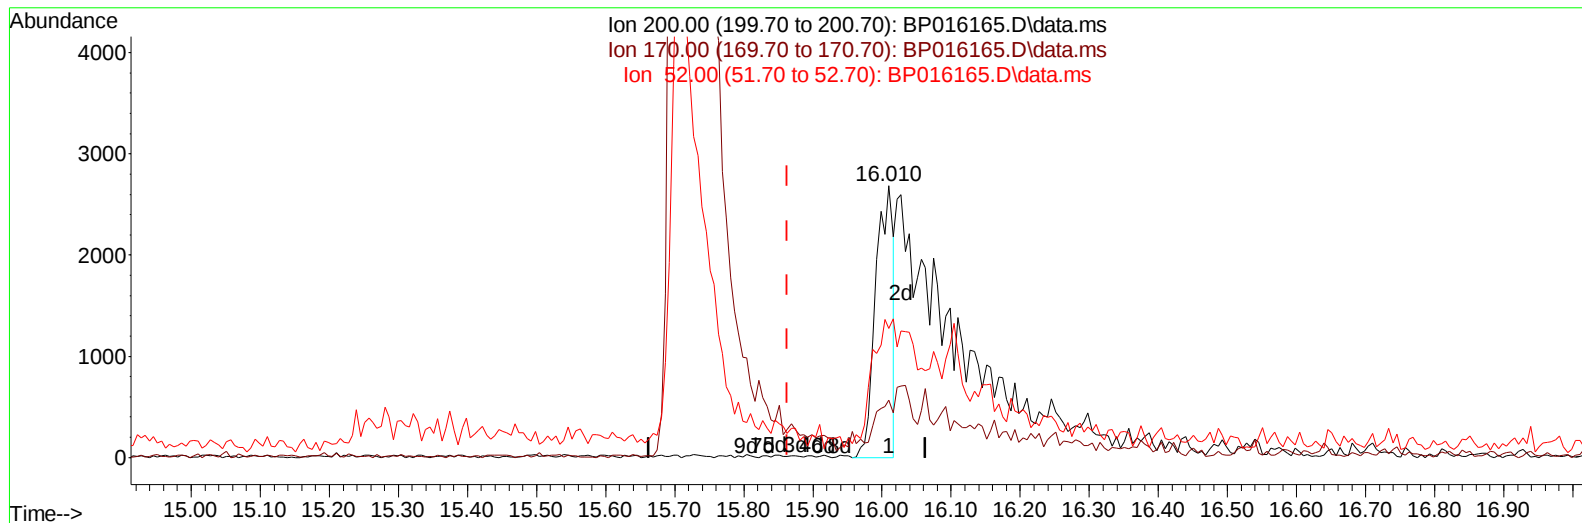

TIC: BP016165.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

16.010min (+ 0.147) 0.38 ng/u1

response 4679

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.30	21.17
52.00	52.20	47.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:21:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

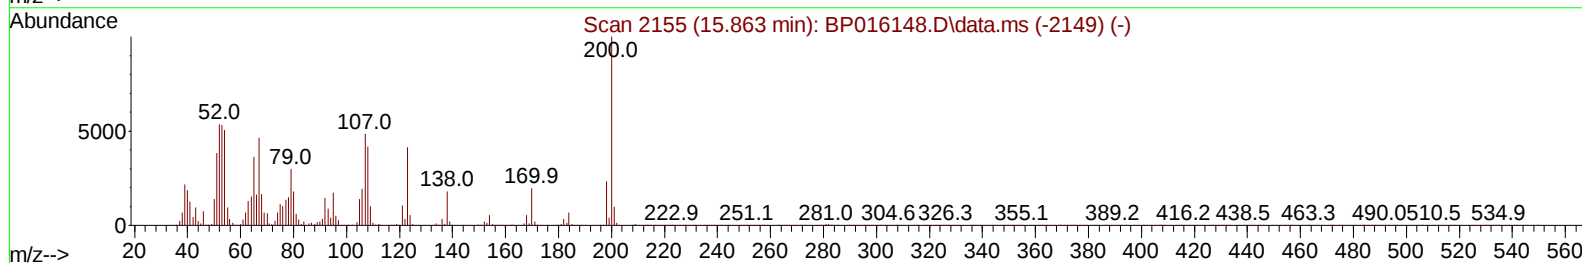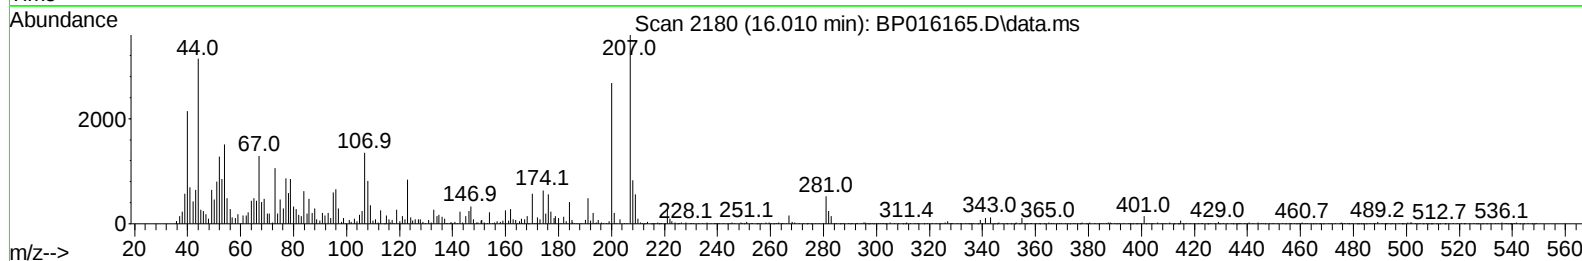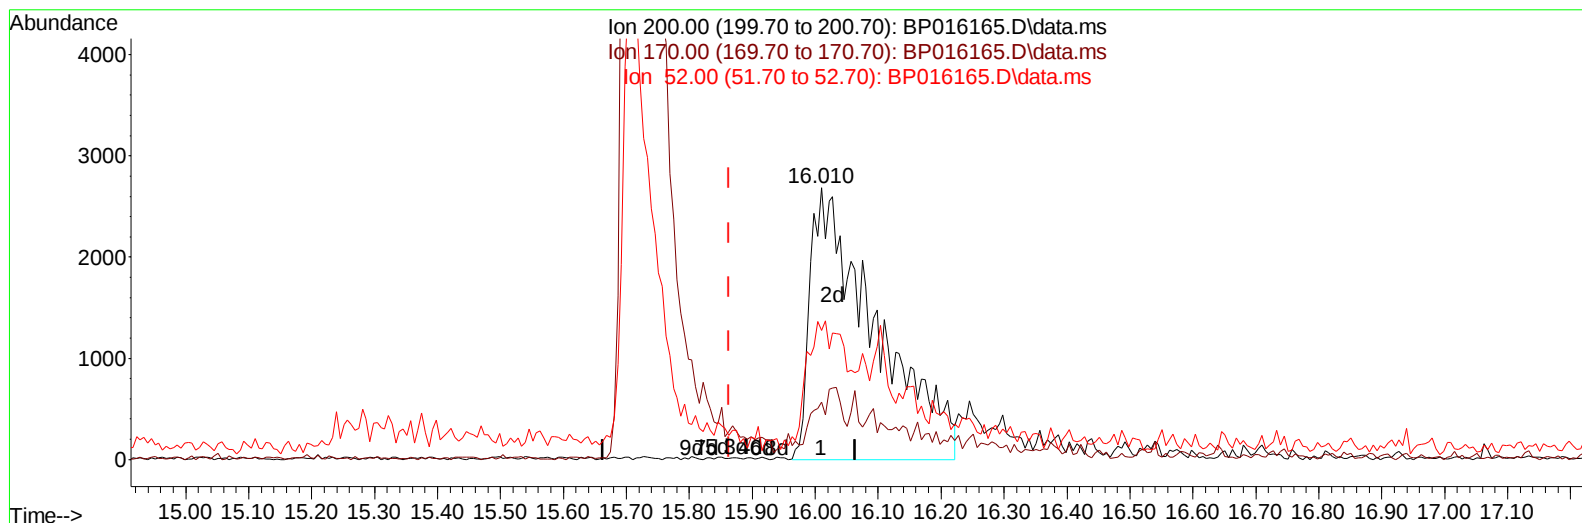

TIC: BP016165.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

16.010min (+ 0.147) 1.57 ng/ul m

response 19257

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	24.30	21.17
52.00	52.20	47.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/11/2023
 Supervised By :mohammad ahmed 07/11/2023

Quant Time: Jul 11 00:22:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 10 23:19:51 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.040	152		271770	20.000	ng/ul	0.02
20) Naphthalene-d8	10.857	136		1362432	20.000	ng/ul	# 0.02
38) Acenaphthene-d10	14.675	164		917997	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188		1990871	20.000	ng/ul	# 0.01
79) Chrysene-d12	21.545	240		1951505	20.000	ng/ul	0.00
88) Perylene-d12	24.074	264		1962053	20.000	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.346	96		10484	1.388	ng/uL	0.00
4) Pyridine-d5	3.816	84		77162	4.052	ng/ul	0.02
7) Phenol-d5	7.299	99		108902m	4.683	ng/ul	0.09
9) Bis-(2-Chloroethyl)eth...	7.405	67		105889m	7.360	ng/ul	0.06
11) 2-Chlorophenol-d4	7.616	132		113569	6.470	ng/ul	0.07
15) 4-Methylphenol-d8	8.863	113		115435m	6.284	ng/ul	0.11
21) Nitrobenzene-d5	9.299	128		56177m	5.395	ng/ul	0.09
24) 2-Nitrophenol-d4	10.081	143		60571m	4.984	ng/ul	0.14
28) 2,4-Dichlorophenol-d3	10.687	165		98900m	4.567	ng/ul	0.18
31) 4-Chloroaniline-d4	11.163	131		137194m	4.932	ng/ul	0.14
46) Dimethylphthalate-d6	14.128	166		472218	6.655	ng/ul	0.05
49) Acenaphthylene-d8	14.375	160		506887	6.355	ng/ul	0.01
54) 4-Nitrophenol-d4	15.281	143		17582m	1.878	ng/ul	0.29
60) Fluorene-d10	15.710	176		429557	7.352	ng/ul	0.04
65) 4,6-Dinitro-2-methylph...	16.010	200		19257m	1.573	ng/ul	0.15
73) Anthracene-d10	17.575	188		630550	6.934	ng/ul	0.04
81) Pyrene-d10	19.792	212		855842	6.716	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.910	264		671022	6.780	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Manual IntegrationsAPPROVED

Quant Time: Jul 11 00:22:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 10 23:19:51 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/11/2023
Supervised By :mohammad ahmed 07/11/2023

