

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016149.D
 Acq On : 10 Jul 2023 09:36
 Operator : MA/JU
 Sample : PB153948BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK948

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	38	rVB	82088	122446	2.26%	0.217%
2	3.793	100	103	133	rBV	720905	1507528	27.88%	2.677%
3	4.111	154	157	163	rVB3	15263	25547	0.47%	0.045%
4	7.222	679	686	702	rBV	485564	1661828	30.73%	2.951%
5	7.352	702	708	715	rBV	507421	997251	18.44%	1.771%
6	7.558	736	743	778	rVB	753288	1862195	34.44%	3.307%
7	8.016	814	821	850	rBV	486857	1480786	27.38%	2.629%
8	8.775	943	950	991	rBV2	538012	2219681	41.05%	3.941%
9	9.228	1020	1027	1058	rBV	539407	1746012	32.29%	3.100%
10	9.969	1145	1153	1182	rBV2	326146	1469636	27.18%	2.610%
11	10.563	1246	1254	1274	rBV2	347793	1680030	31.07%	2.983%
12	10.851	1295	1303	1331	rVB	770705	2174752	40.22%	3.862%
13	11.063	1331	1339	1388	rBV3	350473	1895606	35.05%	3.366%
14	12.010	1498	1500	1505	rVB6	3761	5928	0.11%	0.011%
15	12.504	1576	1584	1585	rBV7	7996	18371	0.34%	0.033%
16	12.546	1585	1591	1594	rVV7	8414	18276	0.34%	0.032%
17	13.563	1761	1764	1765	rBV3	7239	7378	0.14%	0.013%
18	14.010	1835	1840	1846	rVB9	5408	9343	0.17%	0.017%
19	14.098	1846	1855	1876	rBV	1185389	3213702	59.43%	5.707%
20	14.369	1894	1901	1926	rBV	1996678	3809433	70.45%	6.764%
21	14.675	1946	1953	1976	rBV	1566781	2806642	51.90%	4.984%
22	15.092	2016	2024	2026	rBV4	68908	174423	3.23%	0.310%
23	15.687	2118	2125	2156	rBV	1652124	4784656	88.48%	8.496%
24	15.910	2156	2163	2184	rBV5	130333	737585	13.64%	1.310%
25	17.445	2417	2424	2436	rBV	1678155	3005751	55.58%	5.337%
26	17.551	2436	2442	2474	rVB2	1461665	4712941	87.16%	8.369%
27	19.369	2747	2751	2758	rBV6	36144	67291	1.24%	0.119%
28	19.457	2762	2766	2770	rBV5	18051	35070	0.65%	0.062%
29	19.786	2816	2822	2856	rBV	1895924	5407530	100.00%	9.602%
30	21.569	3120	3125	3146	rBV	898965	2806606	51.90%	4.984%
31	23.921	3519	3525	3545	rBV2	1202284	3734465	69.06%	6.631%
32	24.098	3550	3555	3572	rVB	580767	2117588	39.16%	3.760%




Sum of corrected areas: 56316277

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016149.D
Acq On : 10 Jul 2023 09:36
Operator : MA/JU
Sample : PB153948BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK948

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

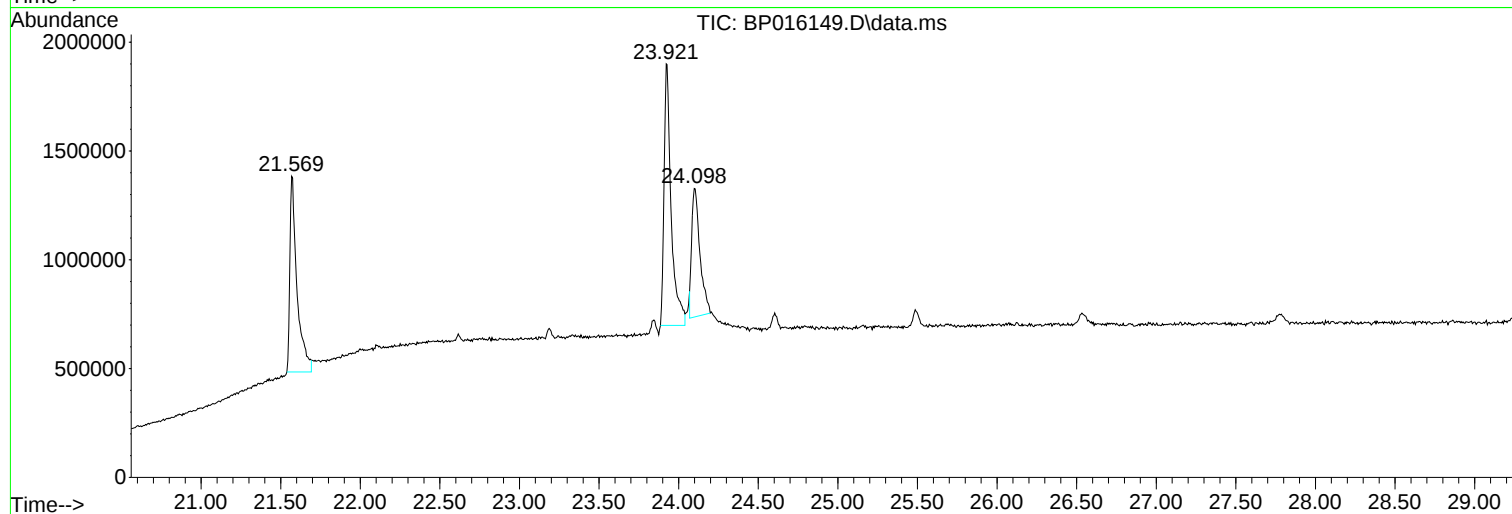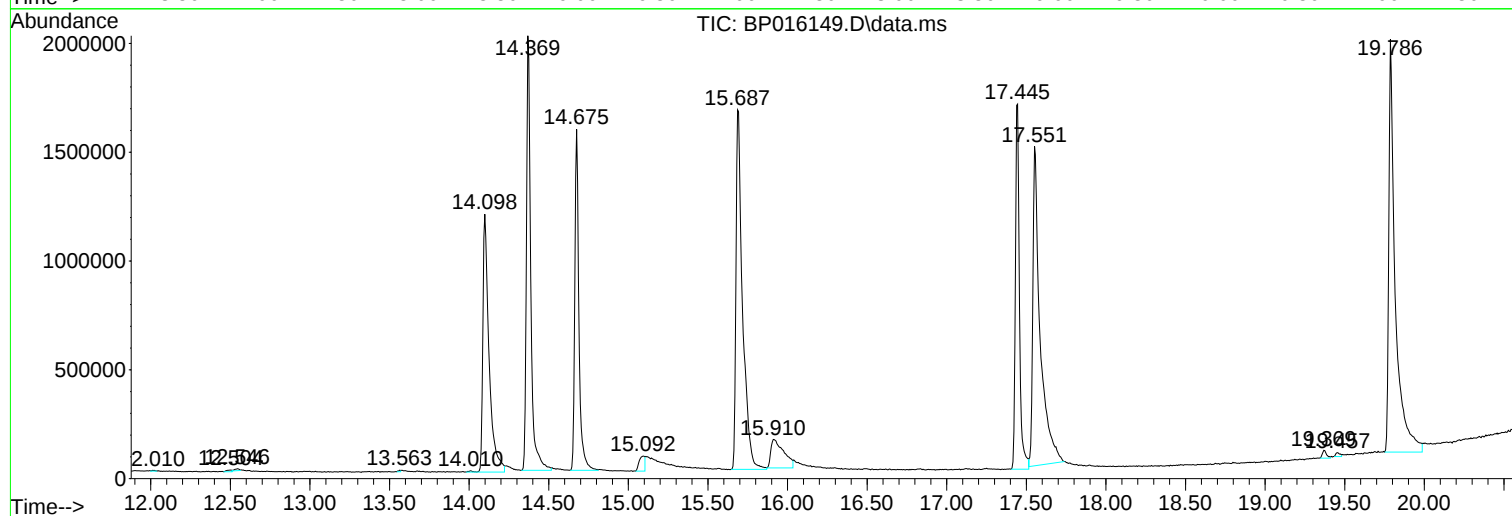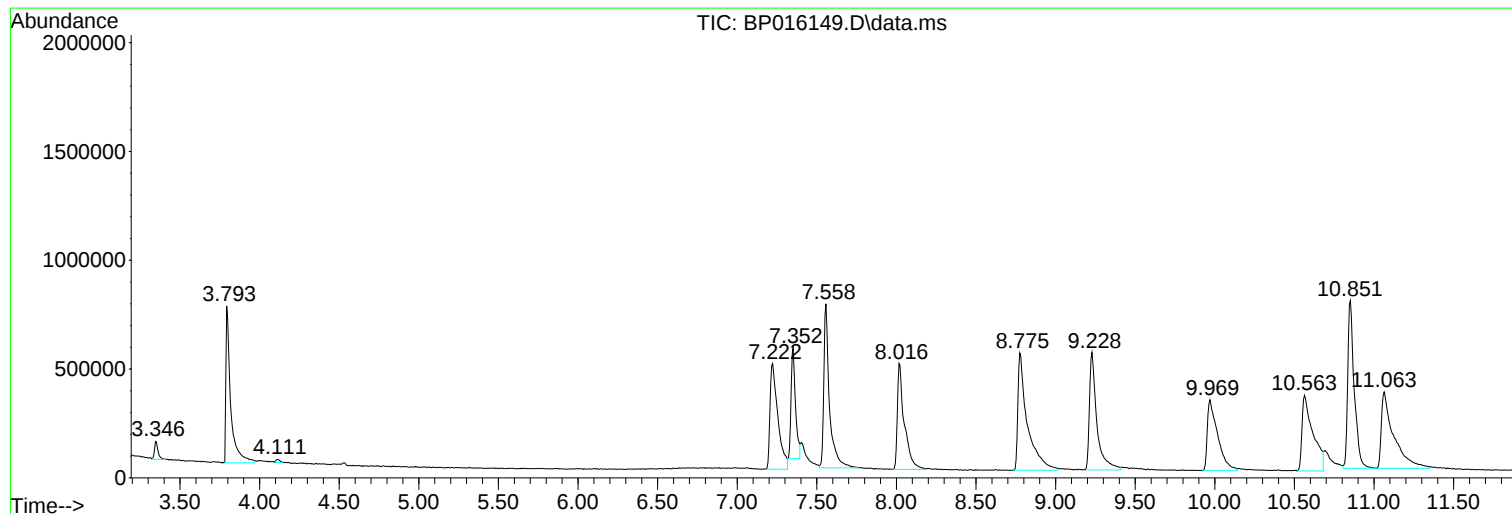

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016149.D
Acq On : 10 Jul 2023 09:36
Operator : MA/JU
Sample : PB153948BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK948

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016149.D
Acq On : 10 Jul 2023 09:36
Operator : MA/JU
Sample : PB153948BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK948

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc