

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016163.D
 Acq On : 10 Jul 2023 18:07
 Operator : MA/JU
 Sample : 03385-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	35	rVB4	19955	32332	0.75%	0.103%
2	3.817	106	107	126	rBV	90353	262857	6.06%	0.835%
3	4.111	152	157	165	rVB	44413	75380	1.74%	0.239%
4	7.293	691	698	712	rBV2	68776	353162	8.14%	1.122%
5	7.405	712	717	727	rVV	73093	196211	4.52%	0.623%
6	7.616	746	753	779	rVB	126781	418140	9.64%	1.329%
7	8.046	818	826	852	rBV	294836	1251254	28.85%	3.976%
8	8.863	957	965	966	rBV2	79843	145860	3.36%	0.463%
9	9.299	1032	1039	1056	rBV2	85842	387227	8.93%	1.230%
10	10.075	1159	1171	1175	rBV5	50405	189879	4.38%	0.603%
11	10.687	1265	1275	1284	rBV4	67134	298849	6.89%	0.950%
12	10.863	1298	1305	1336	rVB	539731	2033496	46.89%	6.461%
13	11.151	1347	1354	1357	rBV3	59957	141728	3.27%	0.450%
14	12.557	1590	1593	1597	rBV6	3750	7223	0.17%	0.023%
15	13.581	1762	1767	1780	rBV6	7553	24328	0.56%	0.077%
16	14.010	1836	1840	1842	rBV4	7796	9631	0.22%	0.031%
17	14.128	1852	1860	1892	rBV	303973	1135785	26.19%	3.609%
18	14.381	1896	1903	1920	rBV	523651	1194152	27.54%	3.794%
19	14.681	1946	1954	1979	rBV	1298451	3022298	69.69%	9.603%
20	15.287	2052	2057	2058	rBV5	6327	7375	0.17%	0.023%
21	15.563	2101	2104	2108	rVB6	5136	6502	0.15%	0.021%
22	15.710	2122	2129	2154	rBV	522027	1723466	39.74%	5.476%
23	15.957	2167	2171	2172	rBV4	3604	4337	0.10%	0.014%
24	16.022	2176	2182	2184	rBV7	16401	29292	0.68%	0.093%
25	16.092	2189	2194	2216	rVV	110609	339776	7.83%	1.080%
26	16.269	2220	2224	2232	rVB5	20781	34572	0.80%	0.110%
27	16.634	2280	2286	2296	rBV2	29034	57811	1.33%	0.184%
28	17.257	2388	2392	2396	rBV6	5294	8546	0.20%	0.027%
29	17.451	2419	2425	2440	rBV	1583698	3530311	81.40%	11.217%
30	17.575	2440	2446	2474	rVB	494125	1807056	41.67%	5.741%
31	18.304	2565	2570	2581	rBV3	92335	247850	5.72%	0.787%
32	19.375	2749	2752	2755	rBV5	13953	21724	0.50%	0.069%
33	19.528	2775	2778	2790	rBV5	37880	91276	2.10%	0.290%
34	19.792	2816	2823	2847	rBV	883315	2473024	57.03%	7.857%
35	20.233	2895	2898	2902	rBV	59267	74545	1.72%	0.237%
36	20.722	2978	2981	2984	rBV3	47407	53692	1.24%	0.171%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016163.D
Acq On : 10 Jul 2023 18:07
Operator : MA/JU
Sample : 03385-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Y4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	21.169	3055	3057	3060	rBV	77070	69180	1.60%	0.220%
38	21.545	3116	3121	3143	rBV	1569412	4336735	100.00%	13.779%
39	23.910	3518	3523	3540	rVB2	691494	1675352	38.63%	5.323%
40	24.080	3544	3552	3578	rVB	989168	3701815	85.36%	11.761%




Sum of corrected areas: 31474029

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016163.D
Acq On : 10 Jul 2023 18:07
Operator : MA/JU
Sample : 03385-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Y4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

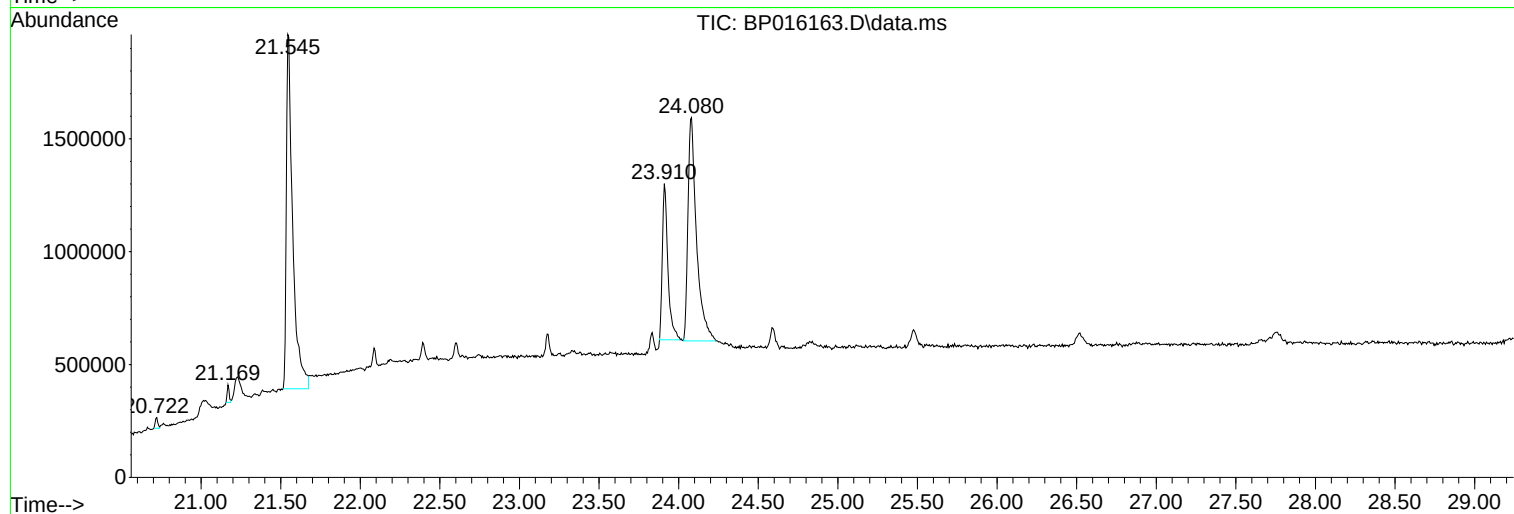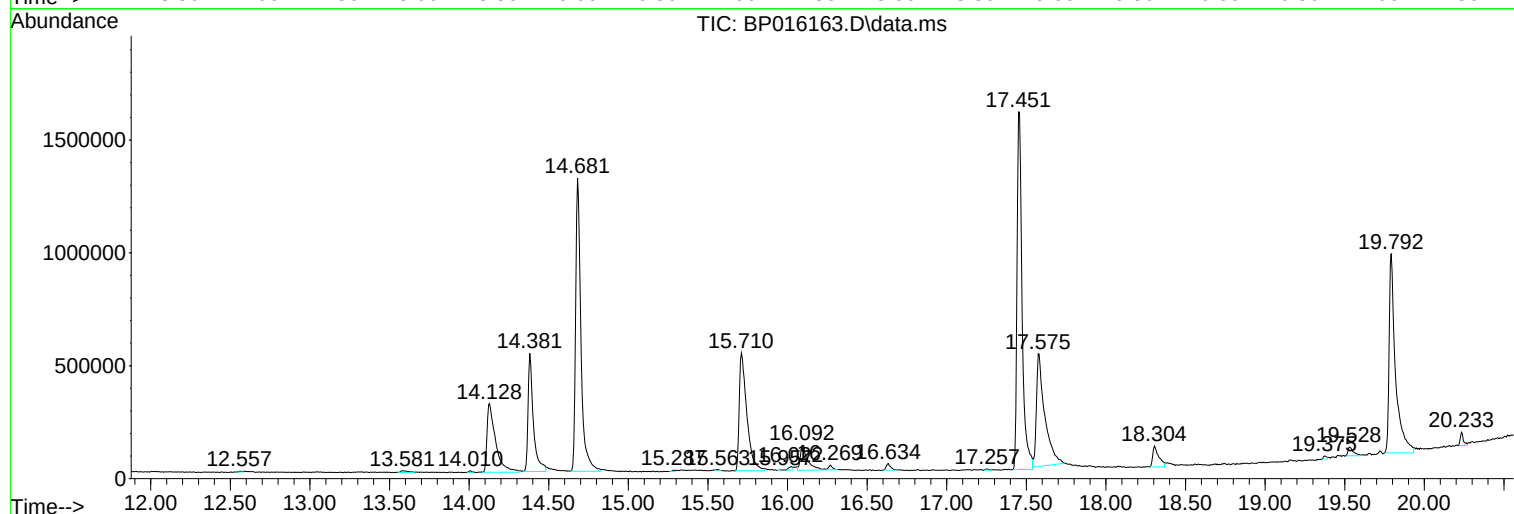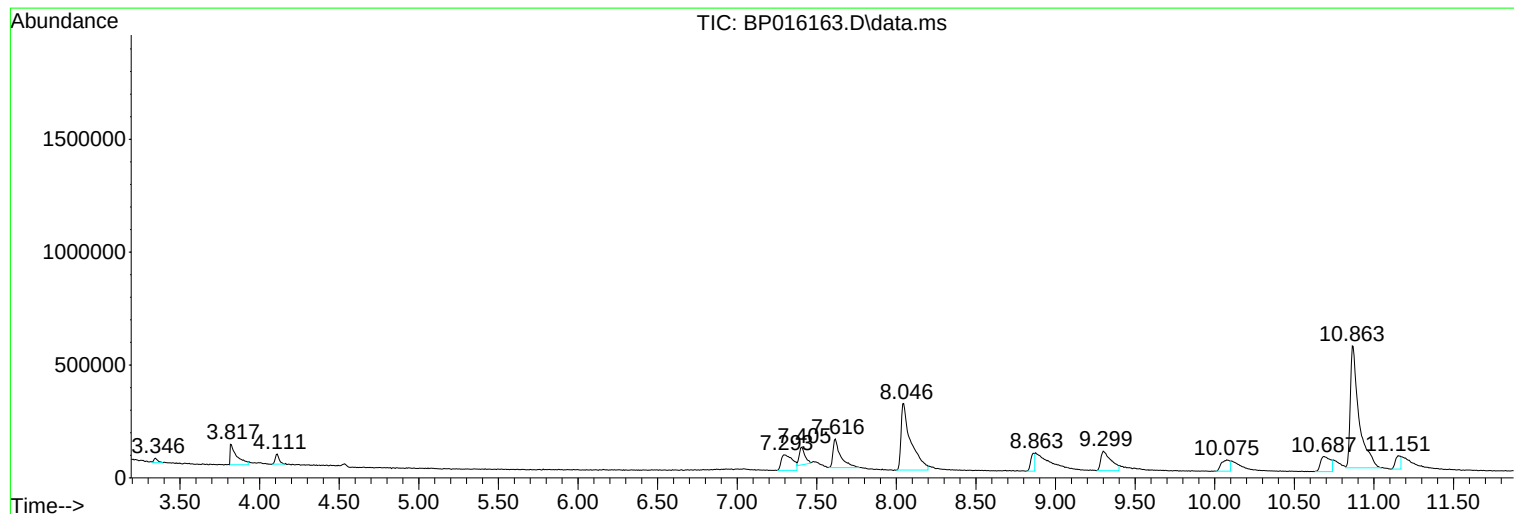

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016163.D
Acq On : 10 Jul 2023 18:07
Operator : MA/JU
Sample : 03385-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Y4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016163.D
Acq On : 10 Jul 2023 18:07
Operator : MA/JU
Sample : 03385-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7Y4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------