

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016164.D
 Acq On : 10 Jul 2023 19:15
 Operator : MA/JU
 Sample : 03385-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX802

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	33	rVB2	29179	41375	0.58%	0.071%
2	3.811	104	106	124	rBV	138739	351548	4.96%	0.604%
3	4.005	133	139	146	rVB	42672	78649	1.11%	0.135%
4	4.111	153	157	163	rVB2	18790	30744	0.43%	0.053%
5	5.058	314	318	324	rBV2	15787	29465	0.42%	0.051%
6	7.252	684	691	704	rBV2	173231	692232	9.77%	1.189%
7	7.358	704	709	720	rVV	188943	443119	6.25%	0.761%
8	7.575	739	746	765	rBV	258546	785006	11.08%	1.348%
9	8.016	813	821	851	rBV	797255	2564265	36.19%	4.404%
10	8.805	948	955	977	rBV2	158076	921422	13.00%	1.582%
11	9.252	1024	1031	1059	rBV	197032	786197	11.10%	1.350%
12	10.010	1150	1160	1161	rBV4	97950	228798	3.23%	0.393%
13	10.616	1255	1263	1275	rBV2	142781	642085	9.06%	1.103%
14	10.846	1295	1302	1330	rVB	1311391	3900250	55.04%	6.698%
15	11.110	1339	1347	1376	rBV2	122880	729166	10.29%	1.252%
16	13.046	1674	1676	1684	rVB9	4985	8956	0.13%	0.015%
17	13.281	1712	1716	1720	rBV6	8694	16615	0.23%	0.029%
18	13.563	1759	1764	1782	rVB2	20508	55873	0.79%	0.096%
19	14.004	1836	1839	1844	rBV6	5545	7892	0.11%	0.014%
20	14.104	1848	1856	1888	rBV	668291	1983542	27.99%	3.406%
21	14.369	1894	1901	1921	rBV	1099190	2127241	30.02%	3.653%
22	14.669	1945	1952	1976	rBV	2835263	5699926	80.44%	9.789%
23	15.163	2025	2036	2038	rBV6	38908	118967	1.68%	0.204%
24	15.445	2080	2084	2088	rVB6	7800	12117	0.17%	0.021%
25	15.534	2093	2099	2101	rBV7	6184	11051	0.16%	0.019%
26	15.692	2119	2126	2156	rBV	1103623	2956116	41.72%	5.077%
27	15.945	2162	2169	2185	rBV8	63987	325450	4.59%	0.559%
28	16.075	2186	2191	2205	rVB	122078	288471	4.07%	0.495%
29	16.263	2217	2223	2228	rBV	36996	52658	0.74%	0.090%
30	16.616	2278	2283	2288	rBV3	19317	32870	0.46%	0.056%
31	17.239	2384	2389	2393	rBV3	11190	18791	0.27%	0.032%
32	17.439	2416	2423	2437	rBV	3804722	6894753	97.31%	11.841%
33	17.557	2437	2443	2470	rVB2	948500	3142845	44.36%	5.397%
34	18.298	2564	2569	2579	rBV2	127013	294797	4.16%	0.506%
35	19.157	2712	2715	2719	rBV6	14025	21681	0.31%	0.037%
36	19.363	2746	2750	2752	rBV4	26636	38469	0.54%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016164.D
 Acq On : 10 Jul 2023 19:15
 Operator : MA/JU
 Sample : 03385-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX802

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

37	19.522	2773	2777	2783	rBV4	68871	125948	1.78%	0.216%
38	19.651	2796	2799	2802	rVB2	32774	35107	0.50%	0.060%
39	19.716	2807	2810	2814	rBV3	34880	45916	0.65%	0.079%
40	19.780	2814	2821	2841	rBV	1778578	4226975	59.66%	7.259%
41	20.233	2895	2898	2903	rBV	76532	79140	1.12%	0.136%
42	20.716	2977	2980	2984	rBV	114923	123996	1.75%	0.213%
43	21.169	3054	3057	3060	rBV	156124	158056	2.23%	0.271%
44	21.539	3114	3120	3131	rBV2	3056401	7085574	100.00%	12.168%
45	22.086	3210	3213	3219	rVB	167935	202103	2.85%	0.347%
46	23.898	3515	3521	3539	rBV2	1242591	3099061	43.74%	5.322%
47	24.068	3542	3550	3584	rVB	1857648	6714051	94.76%	11.530%


Sum of corrected areas: 58229329

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016164.D
Acq On : 10 Jul 2023 19:15
Operator : MA/JU
Sample : 03385-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX802

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

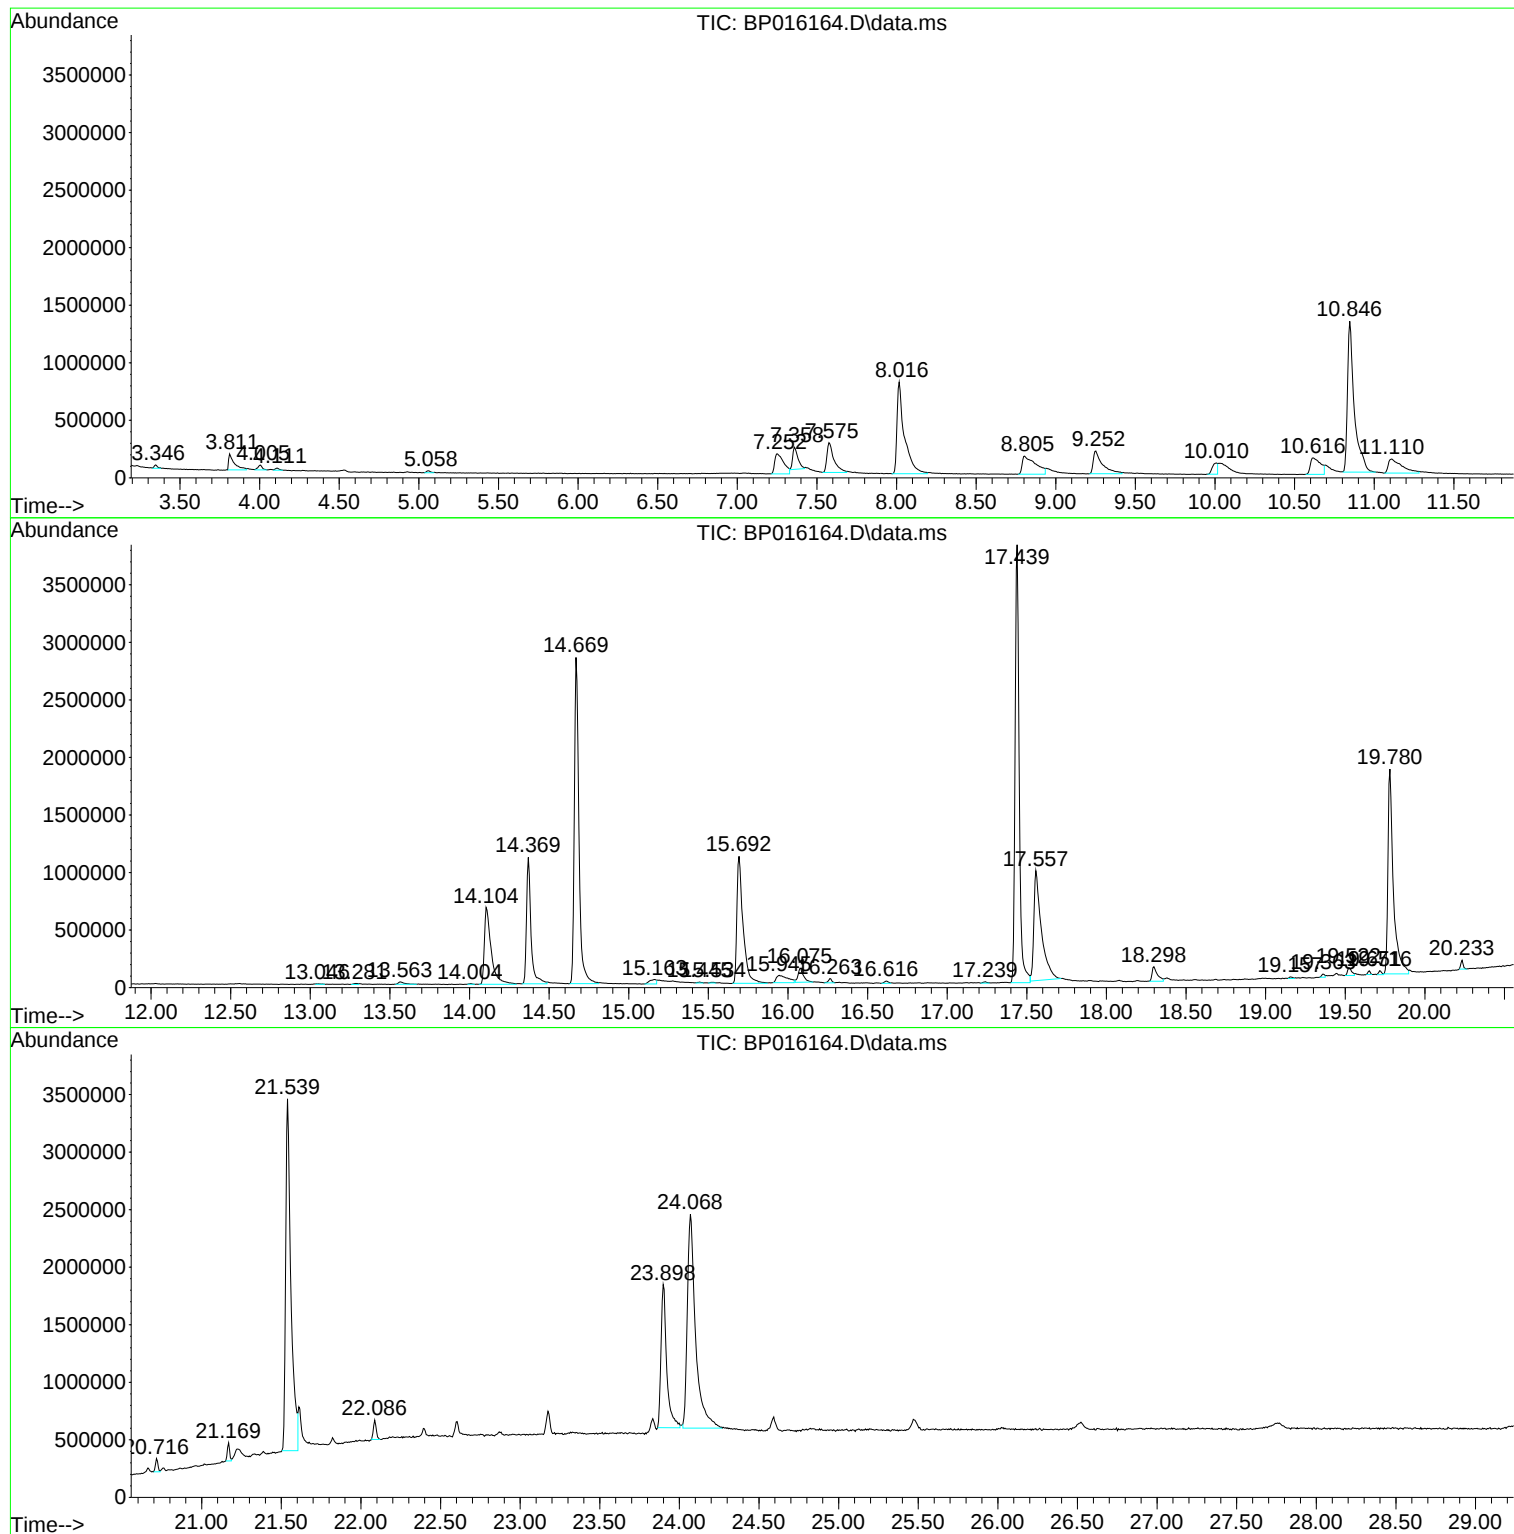

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016164.D
Acq On : 10 Jul 2023 19:15
Operator : MA/JU
Sample : 03385-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX802

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016164.D
Acq On : 10 Jul 2023 19:15
Operator : MA/JU
Sample : 03385-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX802

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------