

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
 Data File : BP016165.D
 Acq On : 10 Jul 2023 19:49
 Operator : MA/JU
 Sample : 03385-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX803

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	24	27	33	rVB2	16754	24650	0.44%	0.064%
2	3.816	106	107	122	rBV	89789	244105	4.38%	0.638%
3	4.111	154	157	162	rVB2	12637	18661	0.33%	0.049%
4	4.528	225	228	236	rVB2	14458	28320	0.51%	0.074%
5	7.299	690	699	712	rBV4	68341	339577	6.09%	0.888%
6	7.405	712	717	727	rVV2	65498	179254	3.21%	0.469%
7	7.616	747	753	765	rBV	127737	349248	6.26%	0.913%
8	8.040	817	825	853	rBV	471275	1784761	32.00%	4.667%
9	8.863	957	965	967	rBV2	72198	135672	2.43%	0.355%
10	9.299	1032	1039	1061	rBV	82213	417327	7.48%	1.091%
11	10.069	1158	1170	1197	rBV6	50368	381107	6.83%	0.997%
12	10.687	1266	1275	1296	rBV5	65312	446991	8.02%	1.169%
13	10.857	1296	1304	1340	rVB	820790	3013166	54.03%	7.880%
14	11.628	1432	1435	1440	rVB7	3512	6850	0.12%	0.018%
15	12.545	1586	1591	1592	rBV5	4783	6592	0.12%	0.017%
16	13.322	1719	1723	1728	rBV8	3160	5618	0.10%	0.015%
17	13.587	1764	1768	1774	rBV9	6834	15963	0.29%	0.042%
18	14.004	1835	1839	1844	rVB7	4129	6317	0.11%	0.017%
19	14.128	1853	1860	1892	rBV	296009	1113060	19.96%	2.911%
20	14.375	1895	1902	1931	rVV2	533968	1248978	22.40%	3.266%
21	14.675	1946	1953	1979	rBV	1806599	4292049	76.96%	11.224%
22	15.257	2046	2052	2055	rBV8	9990	24089	0.43%	0.063%
23	15.557	2099	2103	2110	rVB9	5035	9443	0.17%	0.025%
24	15.710	2121	2129	2158	rBV	548995	1743111	31.26%	4.558%
25	16.010	2172	2180	2183	rBV9	19541	54096	0.97%	0.141%
26	16.098	2190	2195	2208	rVB	44969	120790	2.17%	0.316%
27	16.269	2221	2224	2231	rVB6	10910	18001	0.32%	0.047%
28	17.245	2386	2390	2397	rBV4	7842	14404	0.26%	0.038%
29	17.363	2406	2410	2413	rBV6	4990	6778	0.12%	0.018%
30	17.445	2417	2424	2440	rBV	2317388	5107604	91.59%	13.357%
31	17.575	2440	2446	2479	rVB2	470328	1857963	33.32%	4.859%
32	18.310	2566	2571	2582	rBV4	62022	162928	2.92%	0.426%
33	18.563	2611	2614	2618	rBV6	5751	11266	0.20%	0.029%
34	19.792	2816	2823	2847	rBV2	872568	2380370	42.68%	6.225%
35	20.233	2895	2898	2903	rBV3	44163	49343	0.88%	0.129%
36	20.716	2978	2980	2984	rVB	56209	55453	0.99%	0.145%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Title : SVOA CALIBRATION

37	21.169	3054	3057	3060	rBV	99850	99514	1.78%	0.260%
38	21.545	3115	3121	3131	rBV	2188388	5331670	95.61%	13.943%
39	23.910	3517	3523	3538	rBV2	601478	1557573	27.93%	4.073%
40	24.074	3543	3551	3586	rVB	1474054	5576687	100.00%	14.584%




Sum of corrected areas: 38239349

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

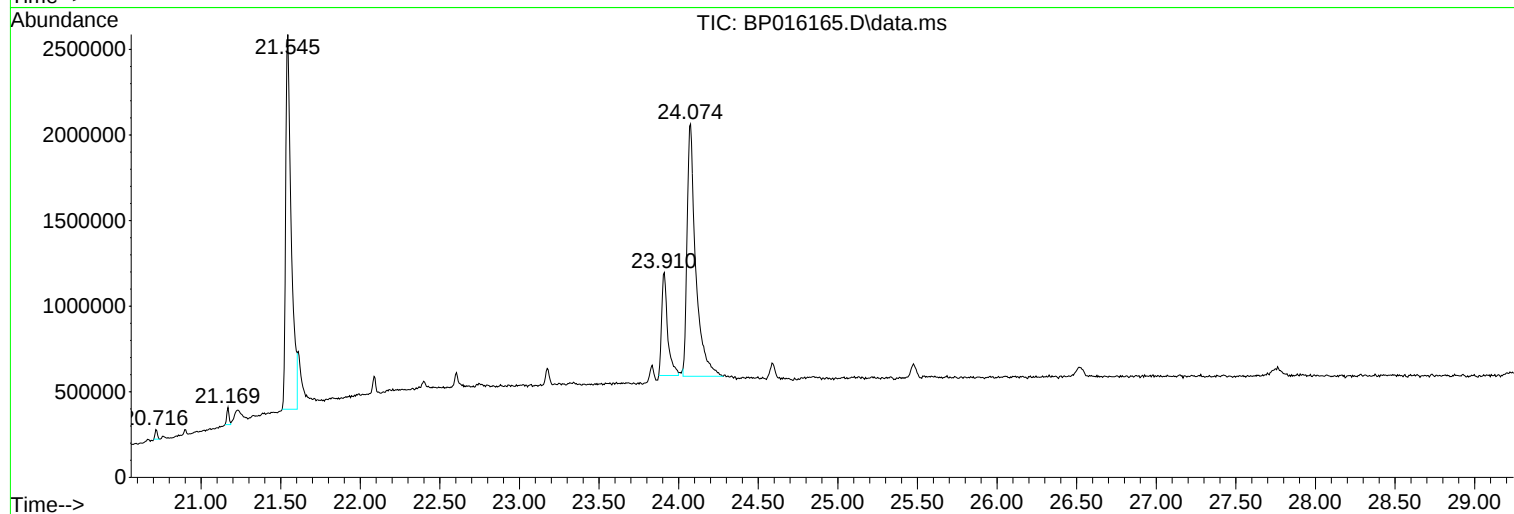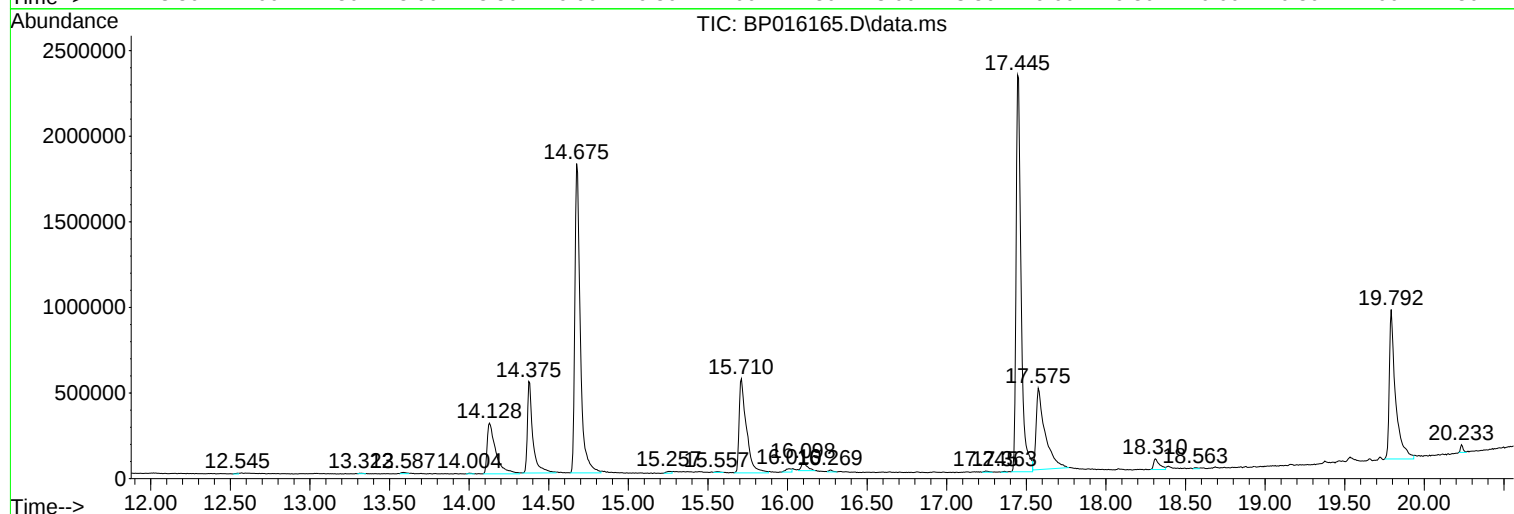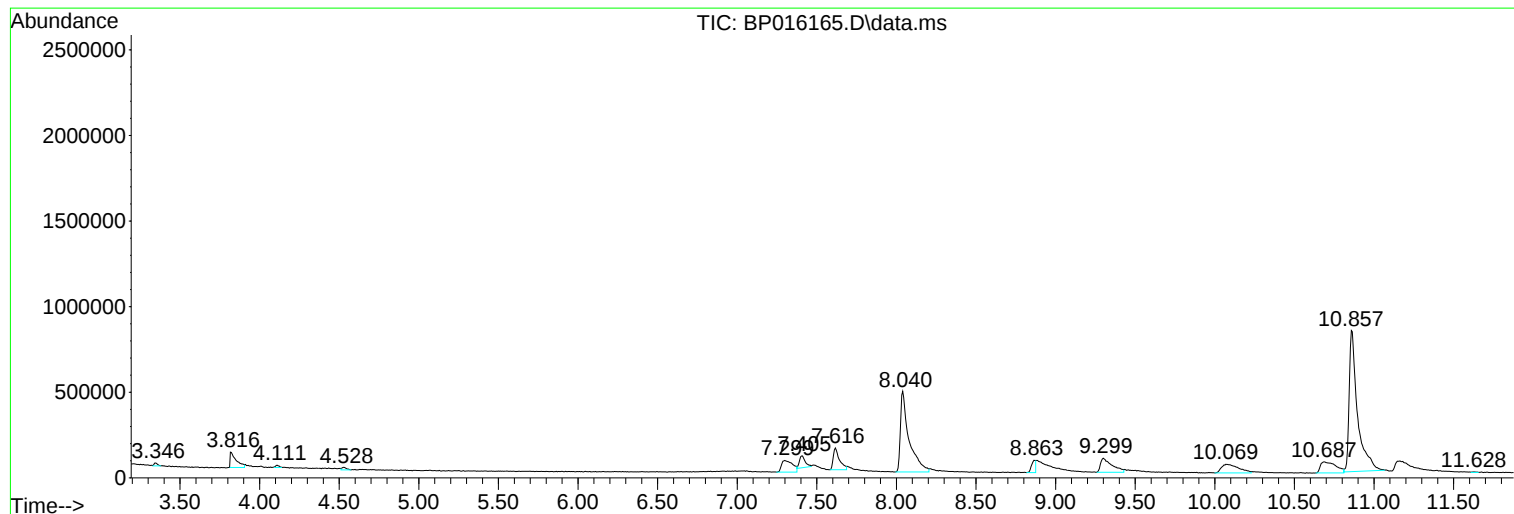

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071023\
Data File : BP016165.D
Acq On : 10 Jul 2023 19:49
Operator : MA/JU
Sample : 03385-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP062623.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------