


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071320\
 Data File : BP002725.D
 Acq On : 13 Jul 2020 08:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:54:03 2020

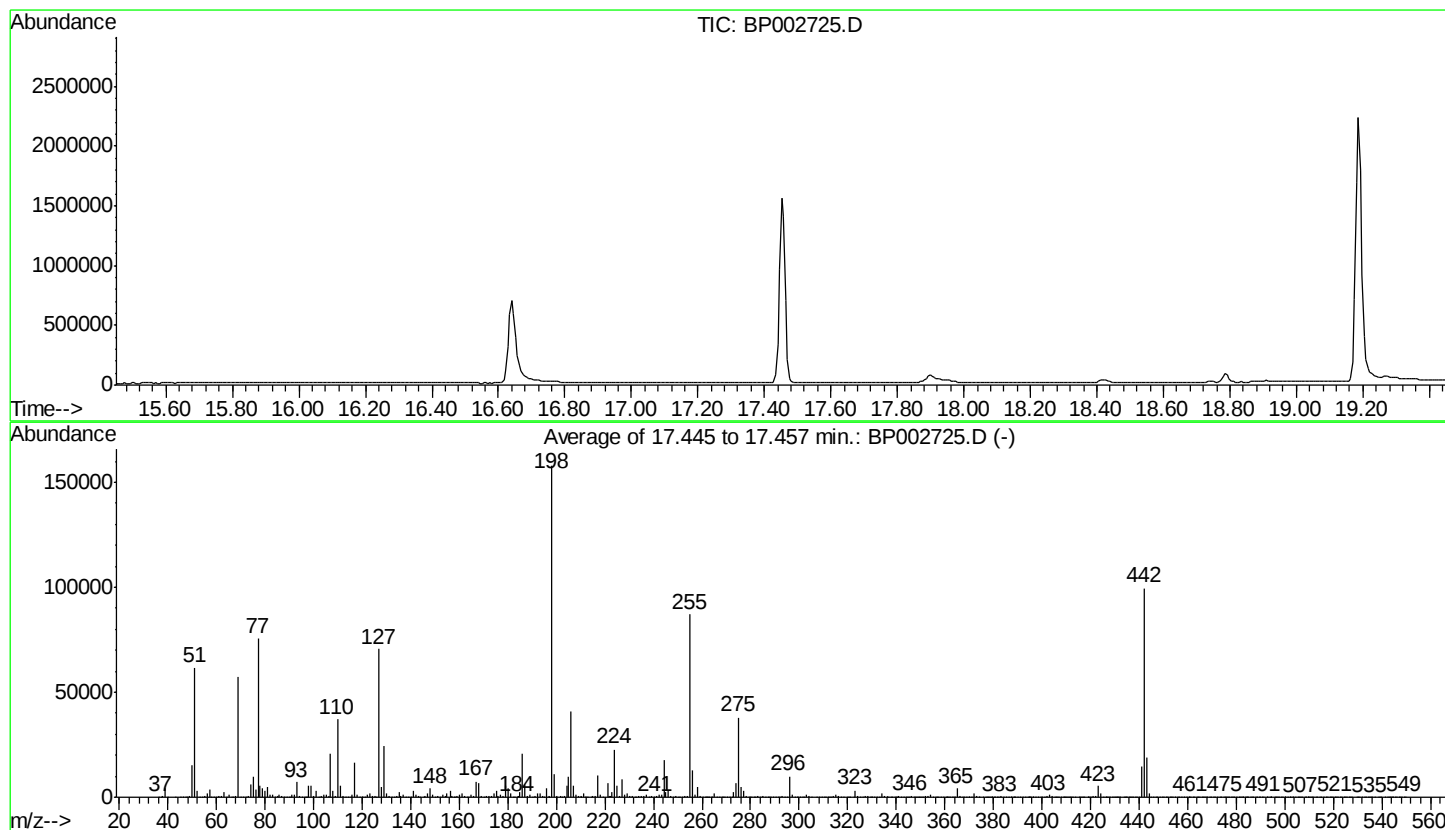

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	61707	PASS
68	69	0.00	2	1.4	790	PASS
69	198	0.00	100	36.2	57211	PASS
70	69	0.00	2	0.4	230	PASS
127	198	10	80	44.7	70543	PASS
197	198	0.00	2	0.3	419	PASS
198	198	100	100	100.0	157945	PASS
199	198	5	9	6.8	10728	PASS
275	198	10	60	24.0	37848	PASS
365	198	1	100	2.7	4236	PASS
441	198	0.01	100	9.5	14946	PASS
442	198	50	100	63.0	99512	PASS
443	442	15	24	18.9	18795	PASS