




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 19:41:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

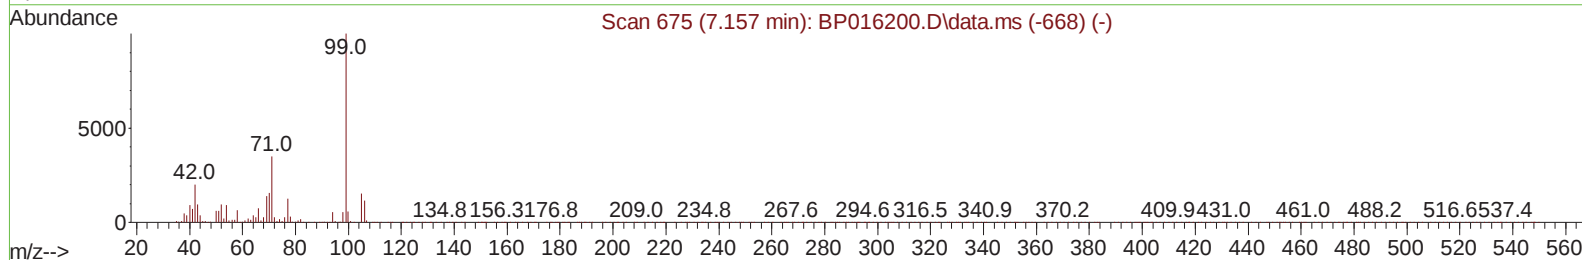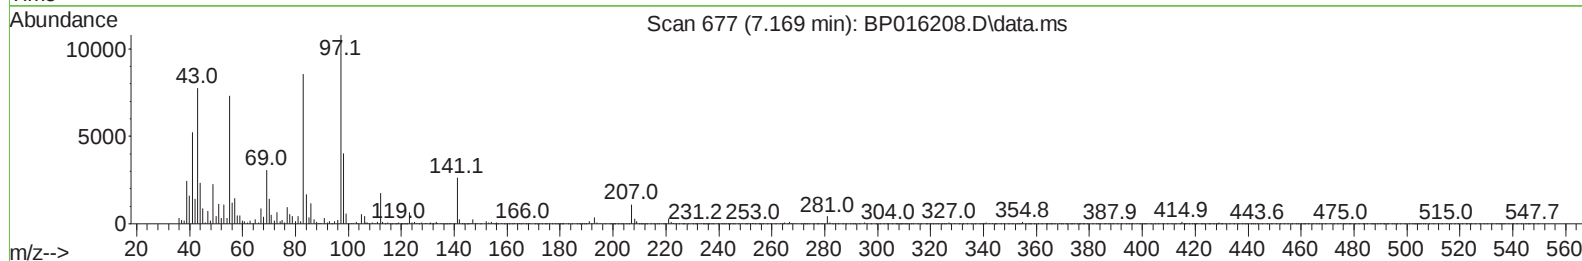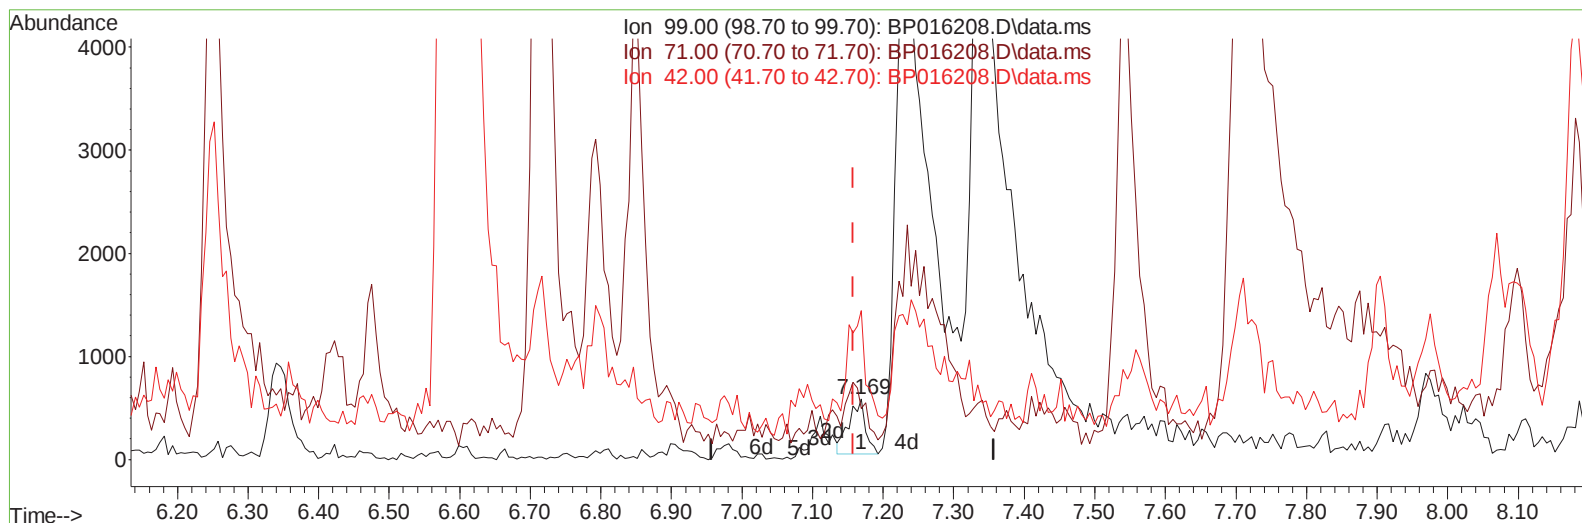

TIC: BP016208.D\data.ms

(7) Phenol-d5 (S)

7.169min (+ 0.012) 0.09 ng/u1

response 883

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.20	84.35#
42.00	21.40	245.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:00:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

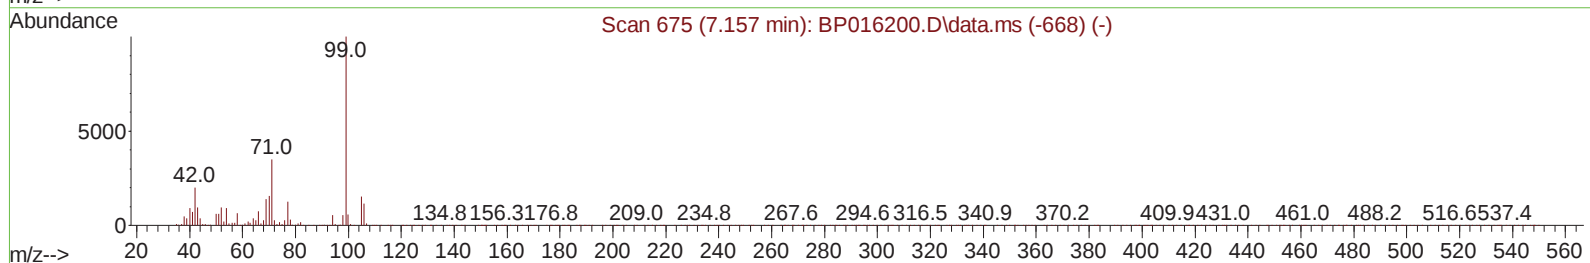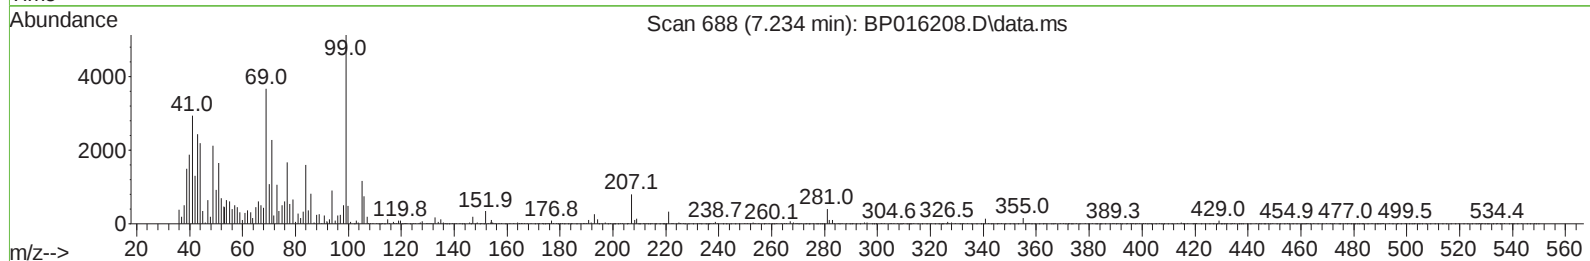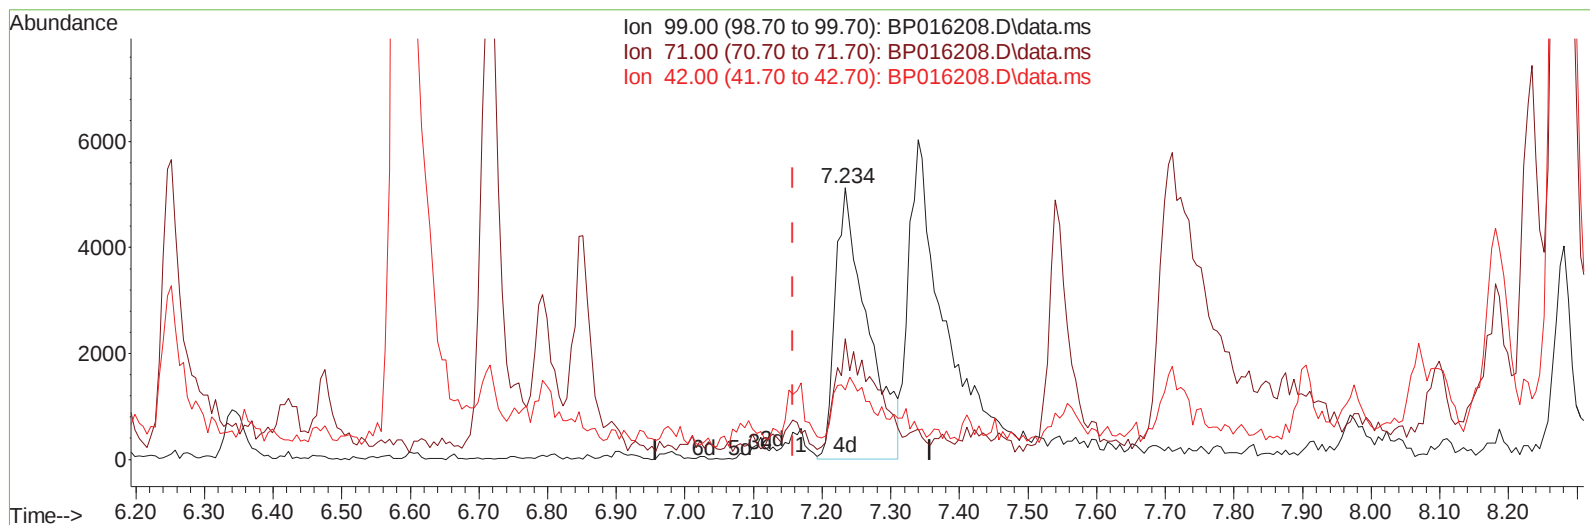

TIC: BP016208.D\data.ms

(7) Phenol-d5 (S)

7.234min (+ 0.077) 1.66 ng/ul m

response 16729

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.20	44.37#
42.00	21.40	25.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:01:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

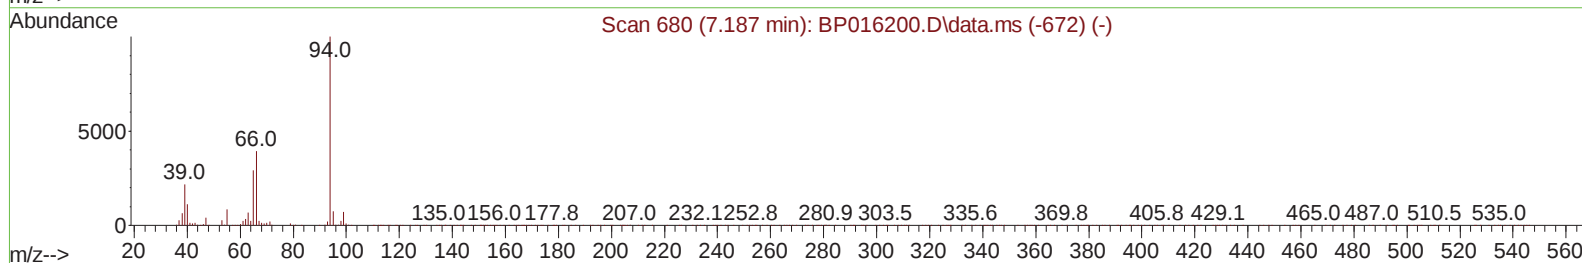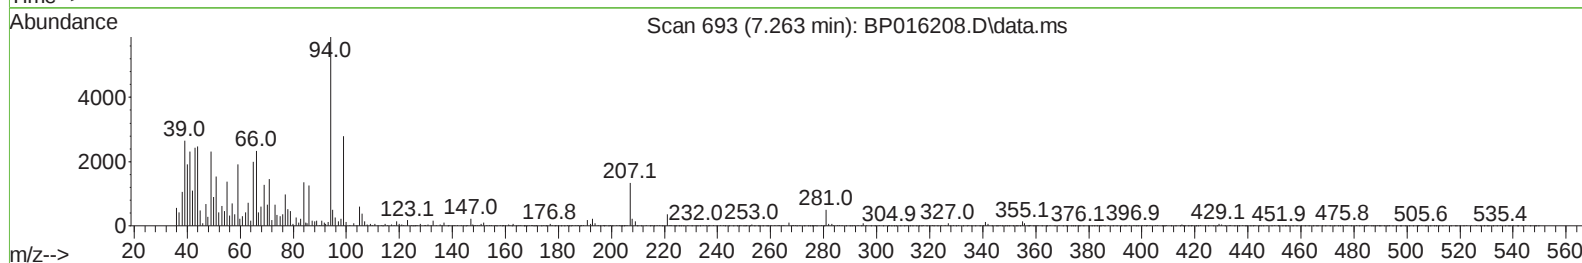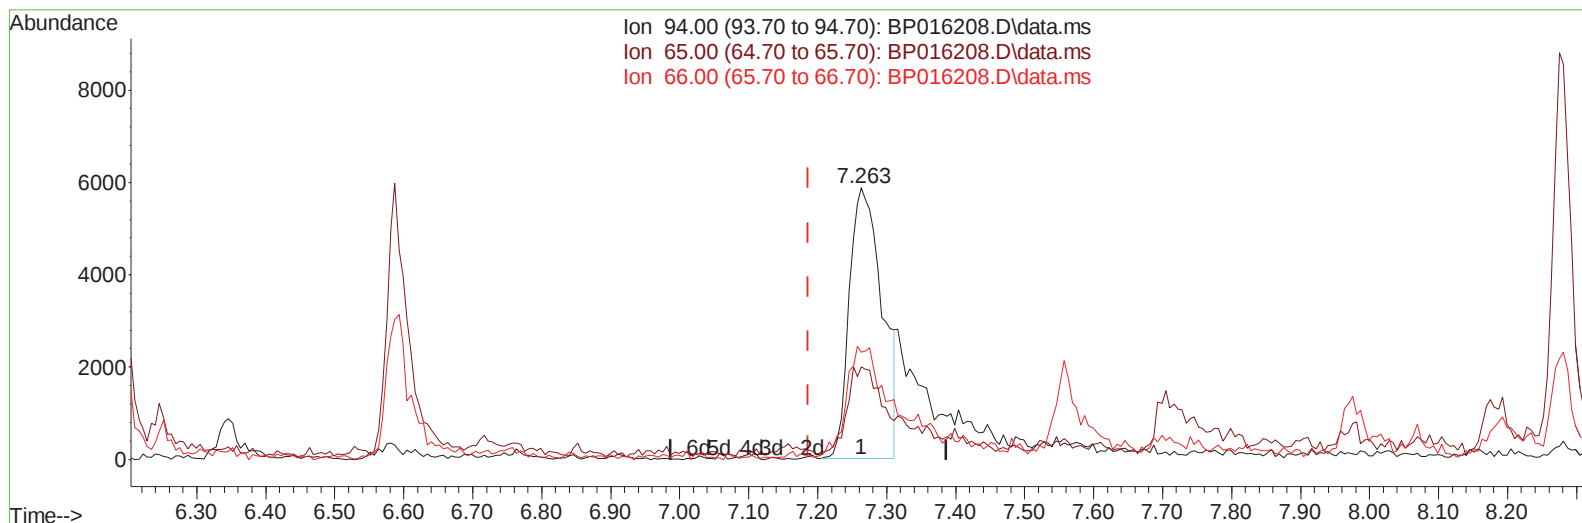

TIC: BP016208.D\data.ms

(8) Phenol

7.263min (+ 0.077) 1.80 ng/ul

response 19381

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	31.90	34.04
66.00	40.90	39.53
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:01:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

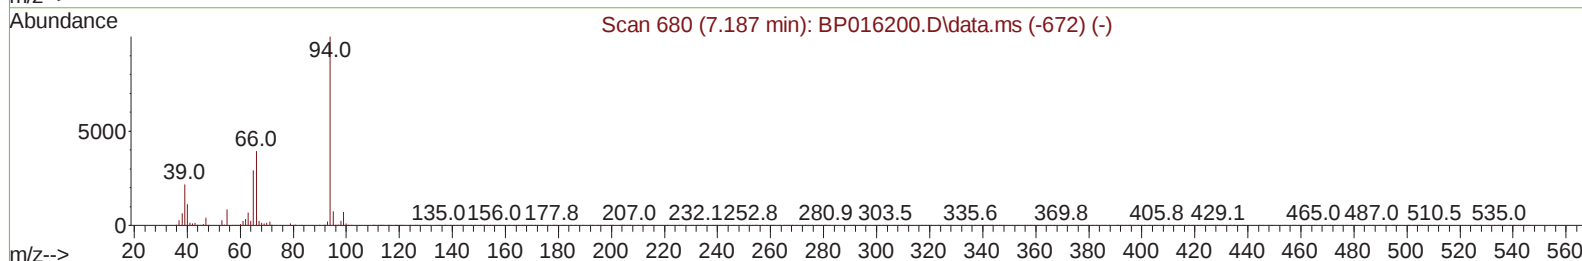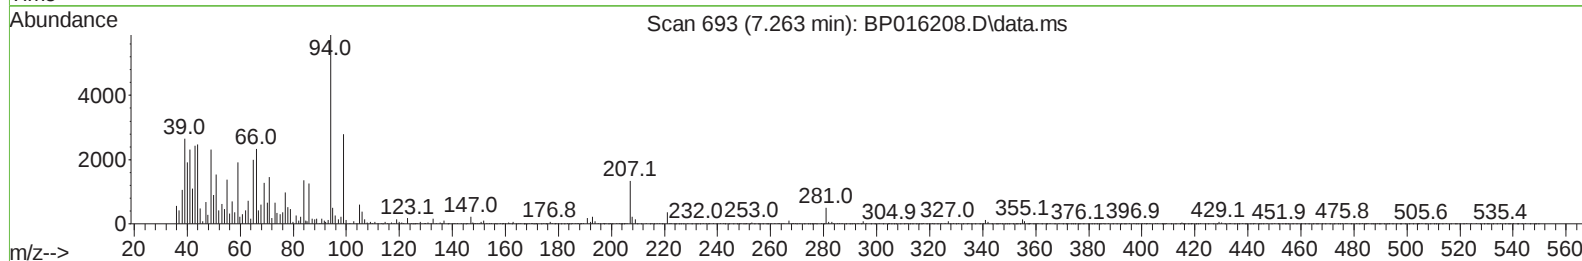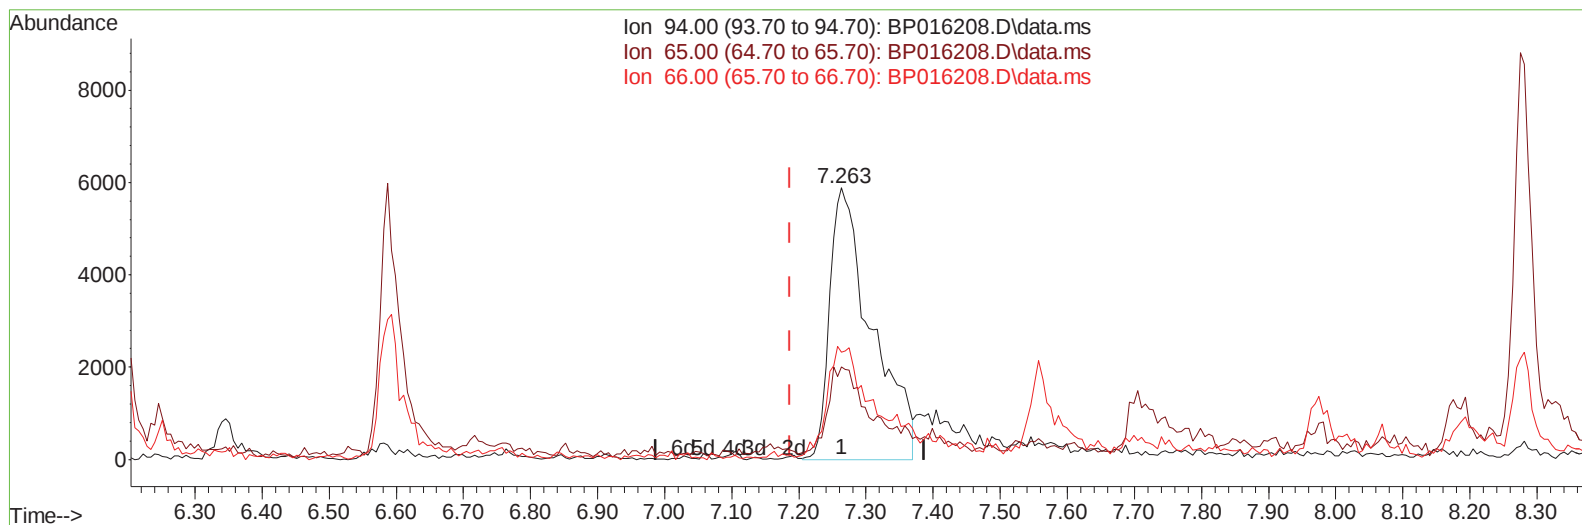

TIC: BP016208.D\data.ms

(8) Phenol

7.263min (+ 0.077) 2.38 ng/ul m

response 25647

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	31.90	34.04
66.00	40.90	39.53
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:19:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

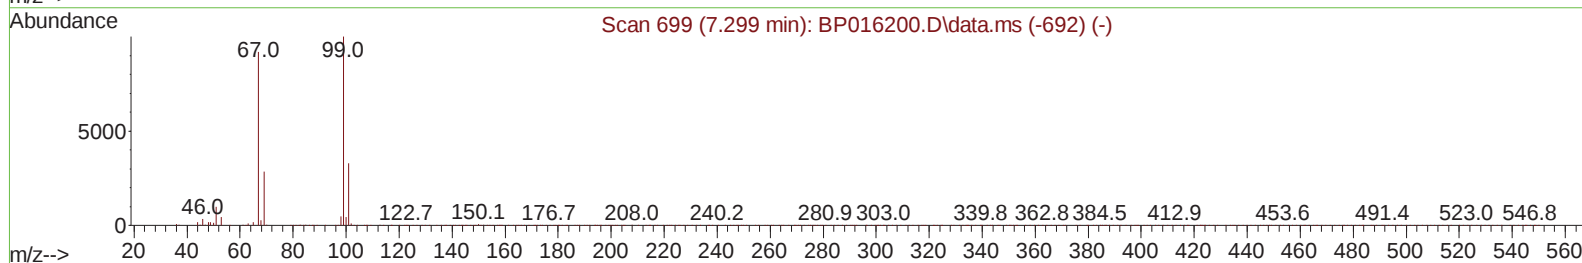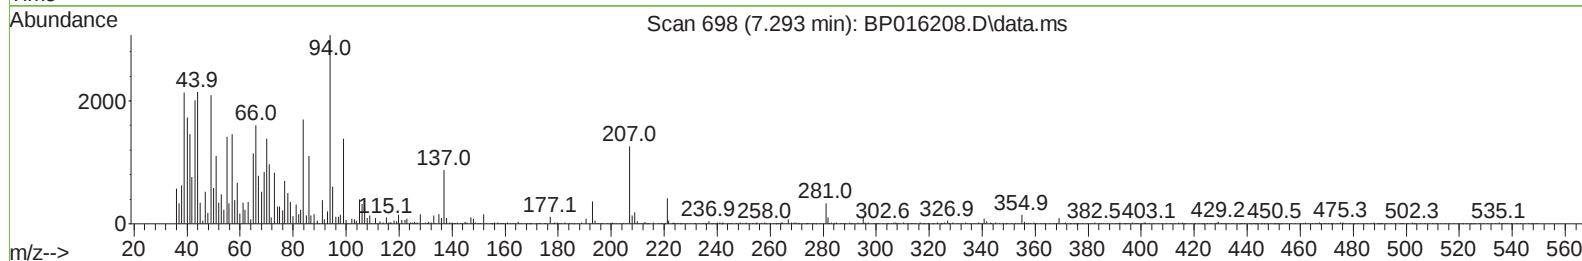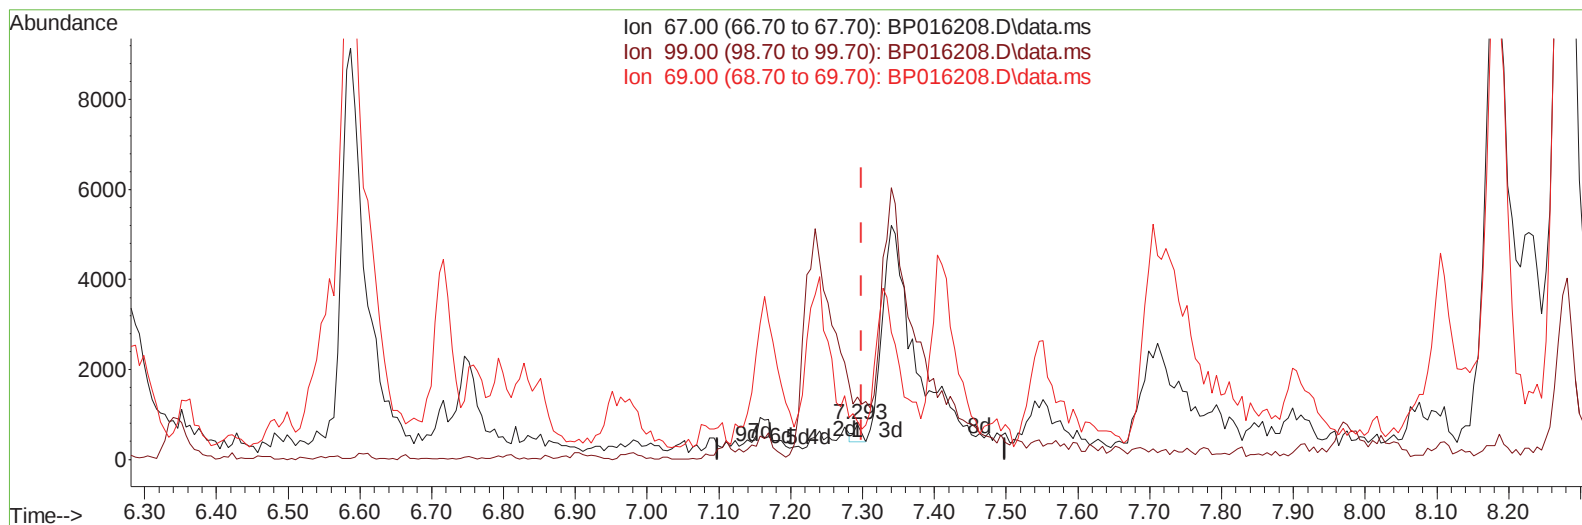

TIC: BP016208.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.293min (-0.006) 0.04 ng/u1

response 272

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	178.28#
69.00	33.10	108.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:19:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

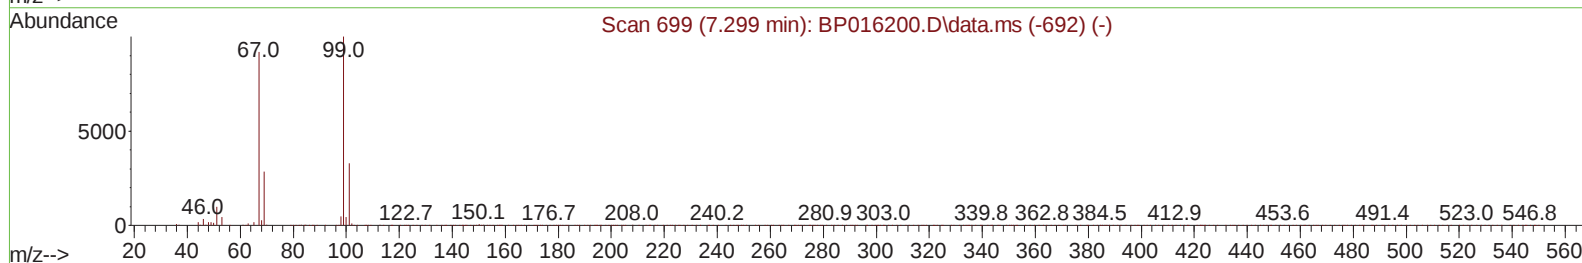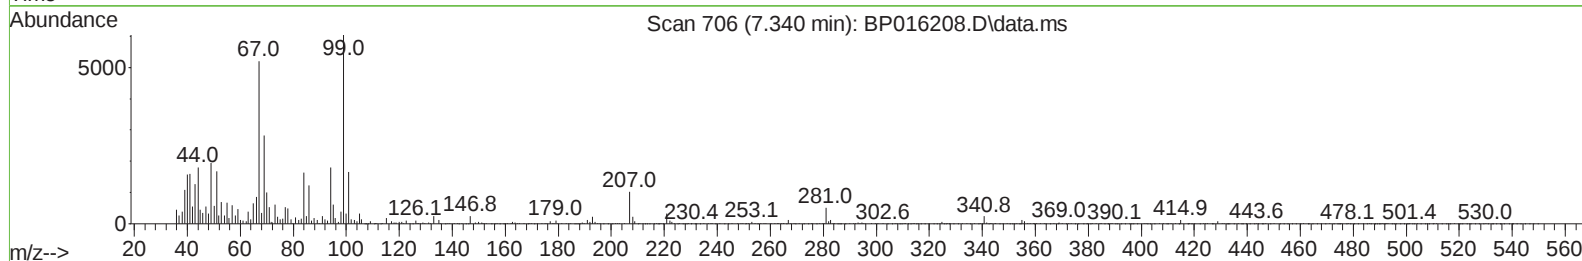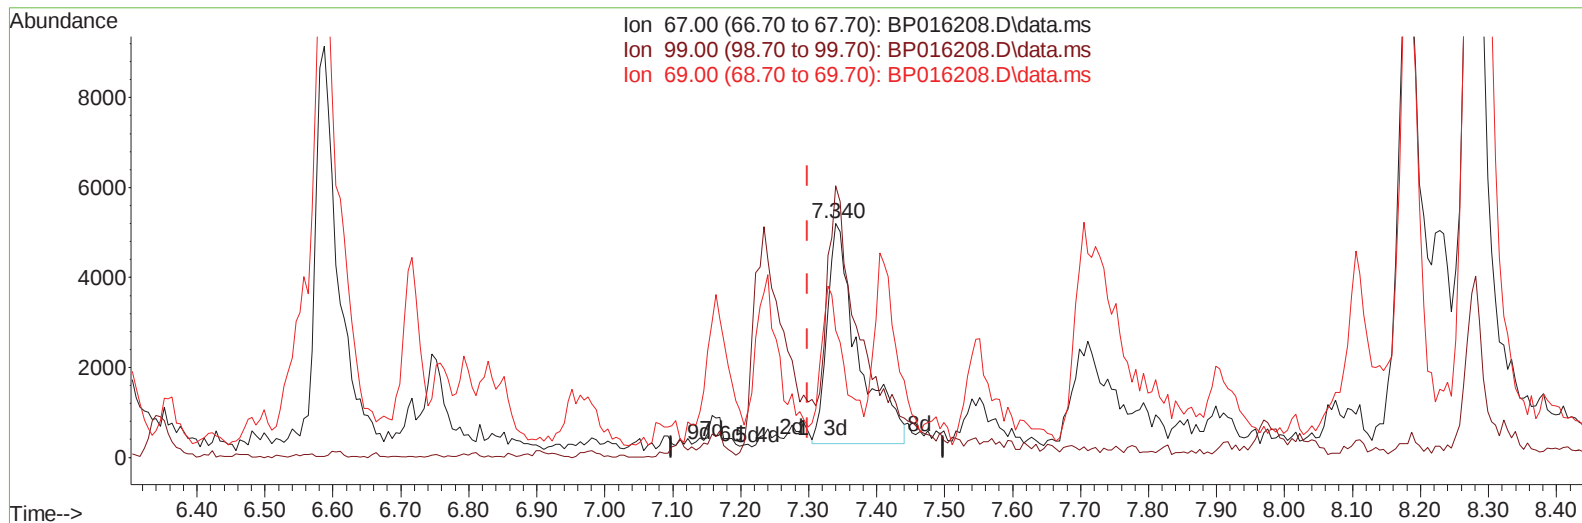

TIC: BP016208.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.340min (+ 0.041) 2.29 ng/ul m

response 15604

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	115.99
69.00	33.10	54.29#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 19:15:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

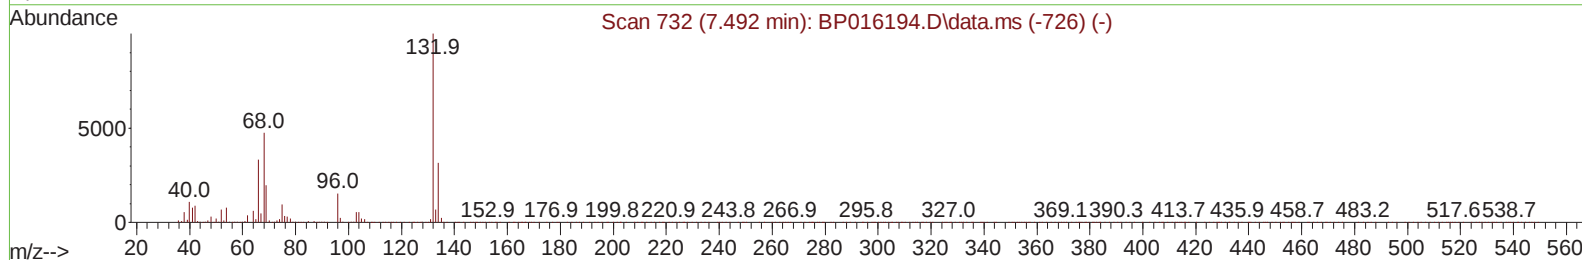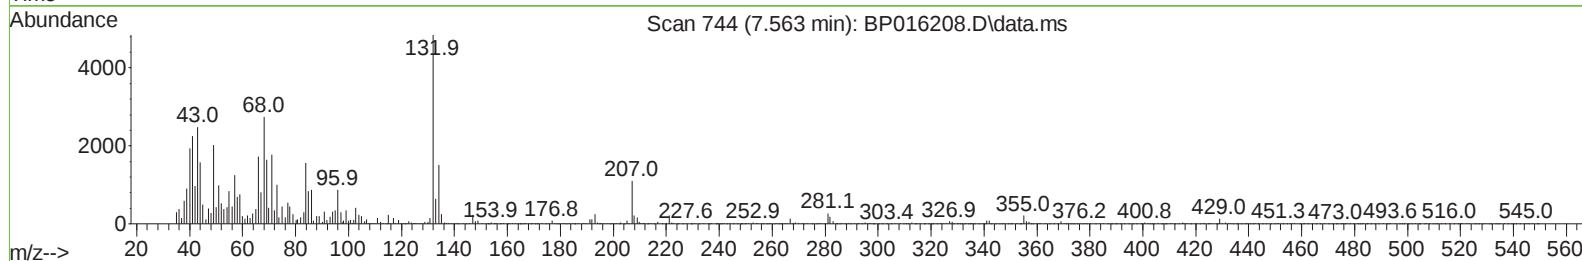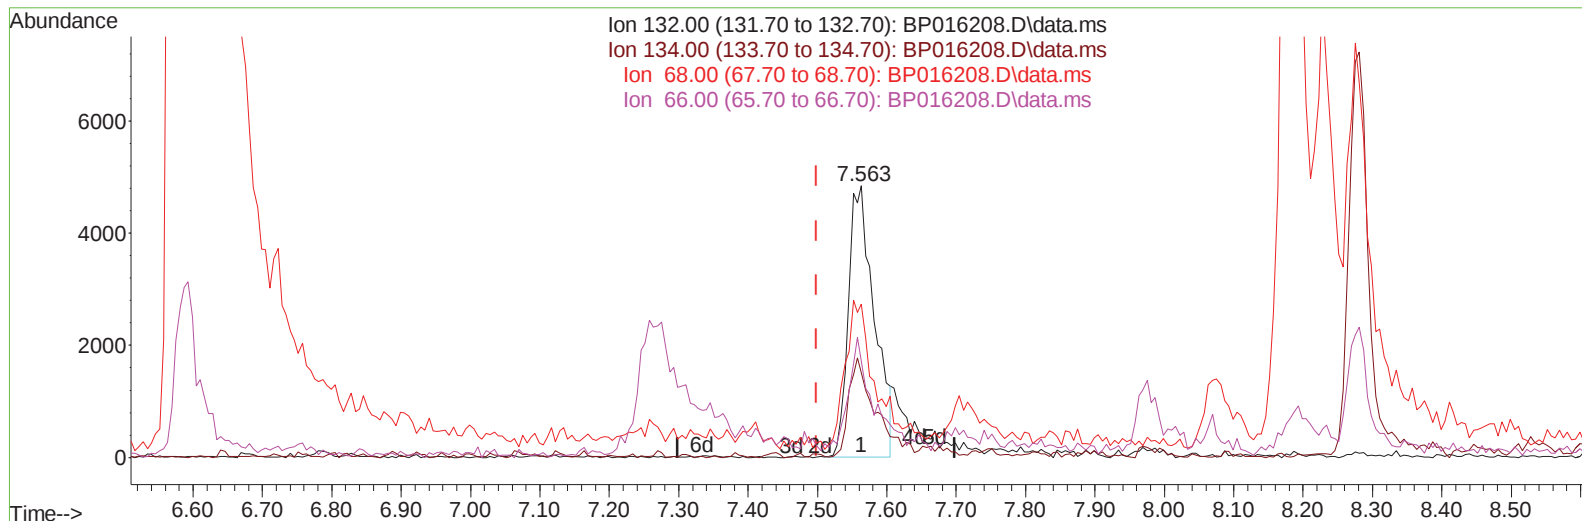

TIC: BP016208.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.563min (+ 0.065) 1.72 ng/u1

response 12476

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	31.50	31.30
68.00	47.30	56.59
66.00	33.60	35.59




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 19:15:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

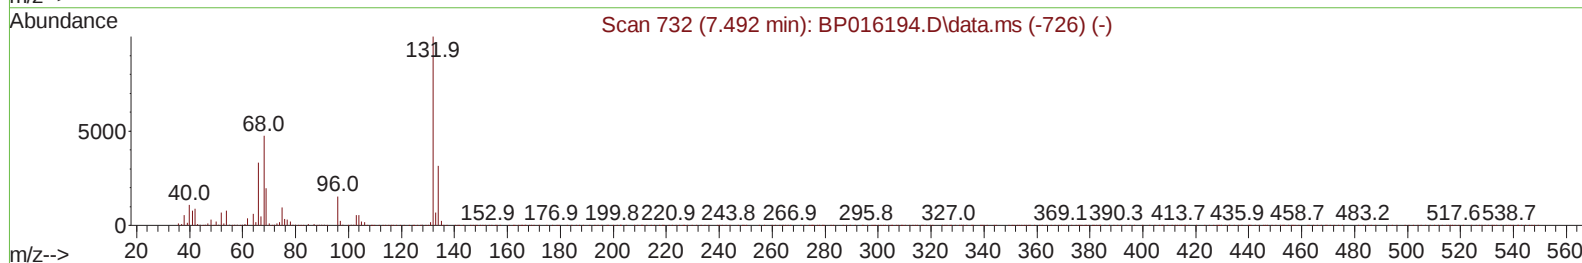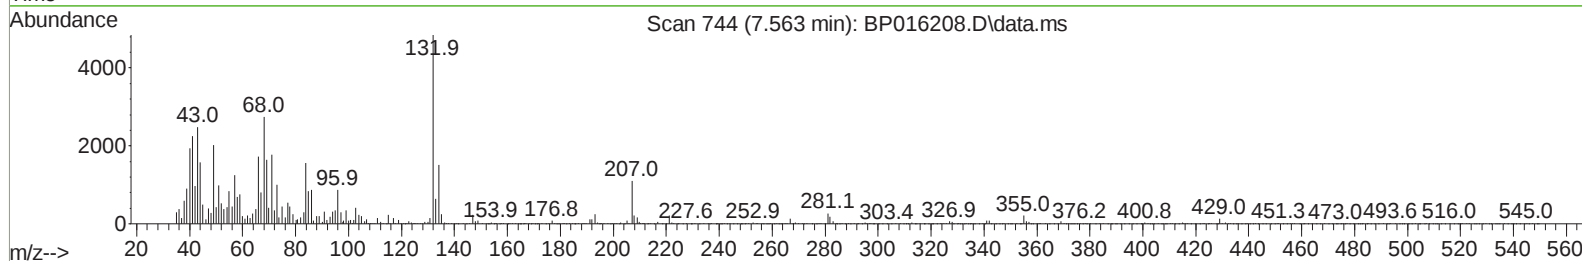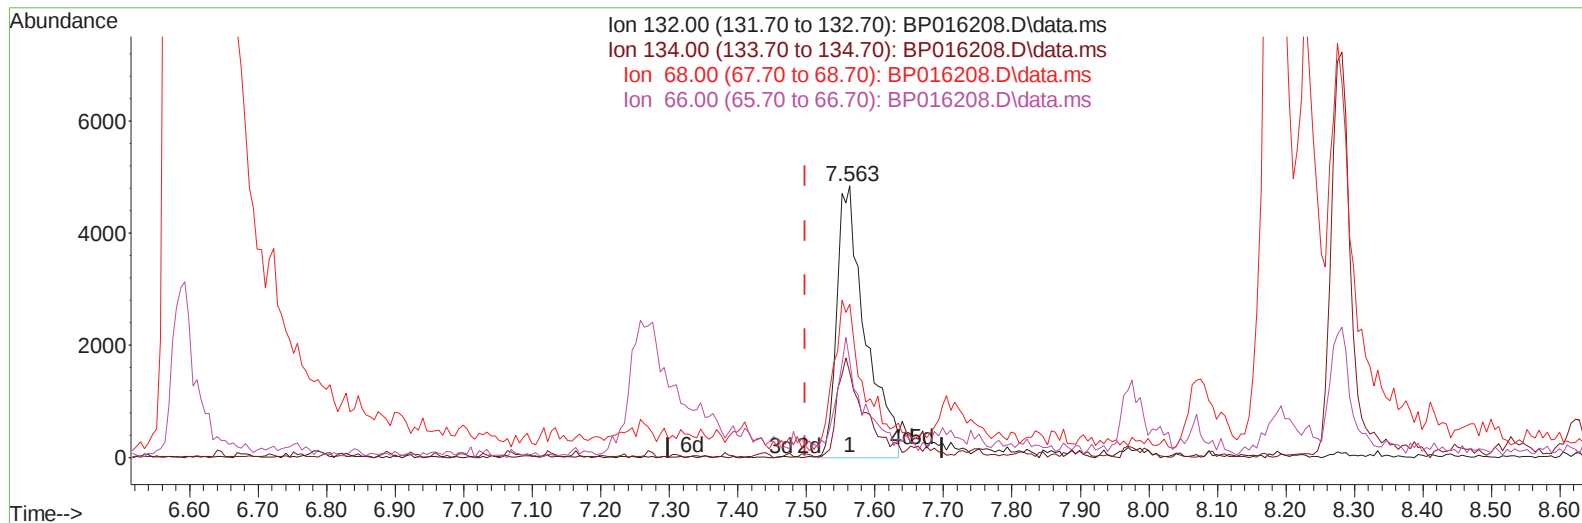

TIC: BP016208.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.563min (+ 0.065) 1.93 ng/ul m

response 13990

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	31.50	31.30
68.00	47.30	56.59
66.00	33.60	35.59




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 14 11:59:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

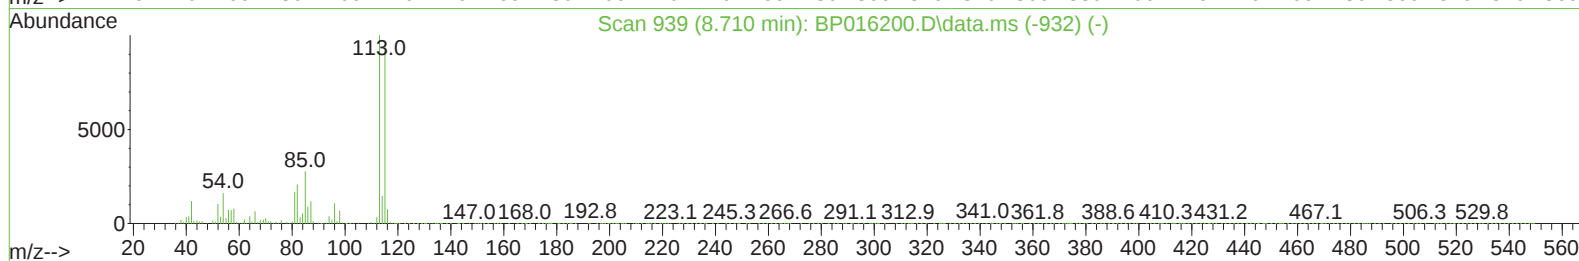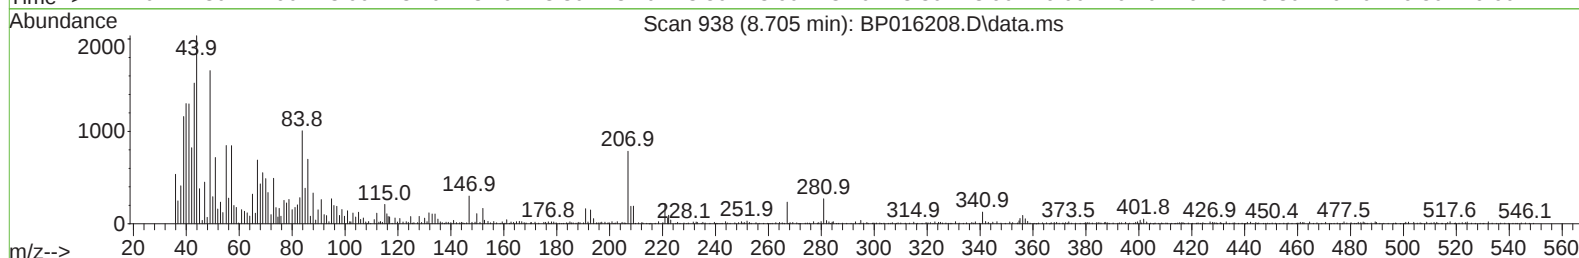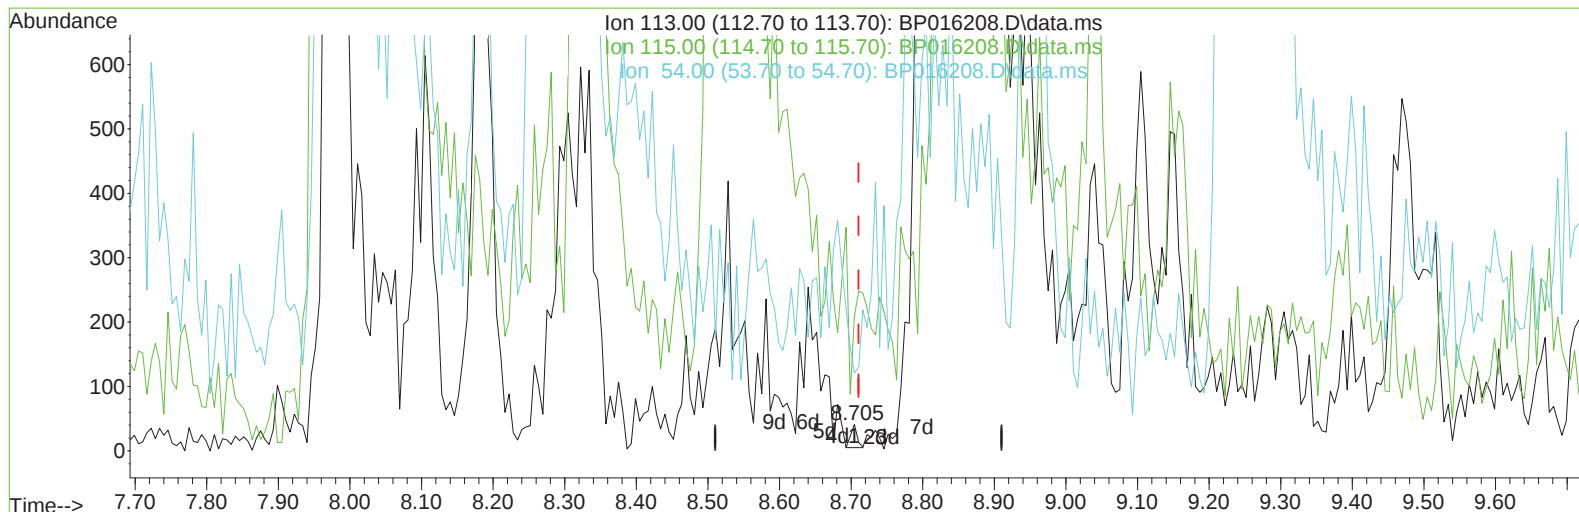

TIC: BP016208.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.705min (-0.006) 0.00 ng/u1

response 22

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	509.76#
54.00	16.30	295.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:21:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

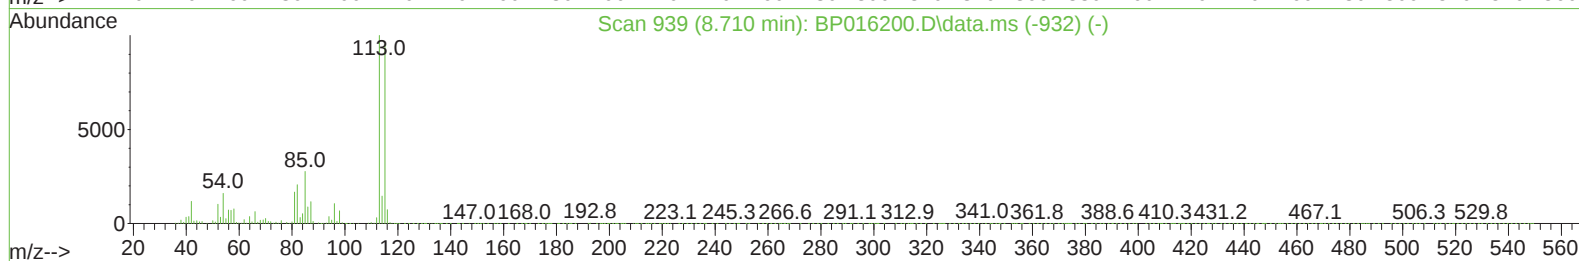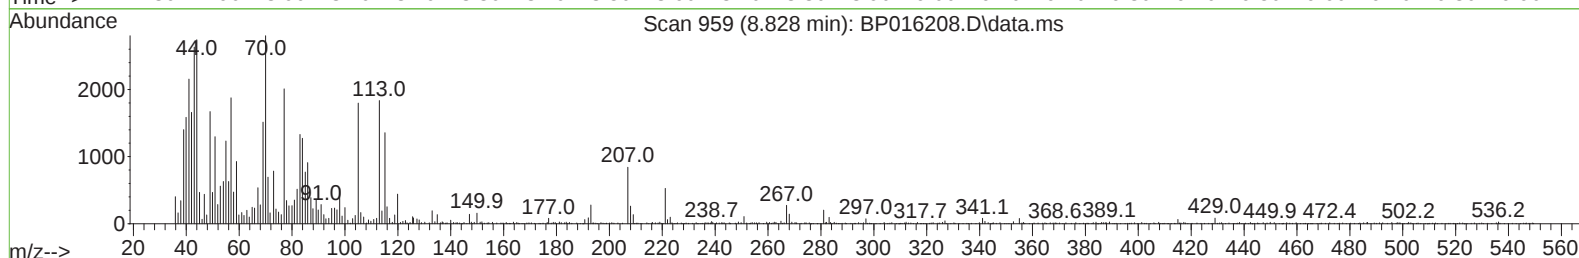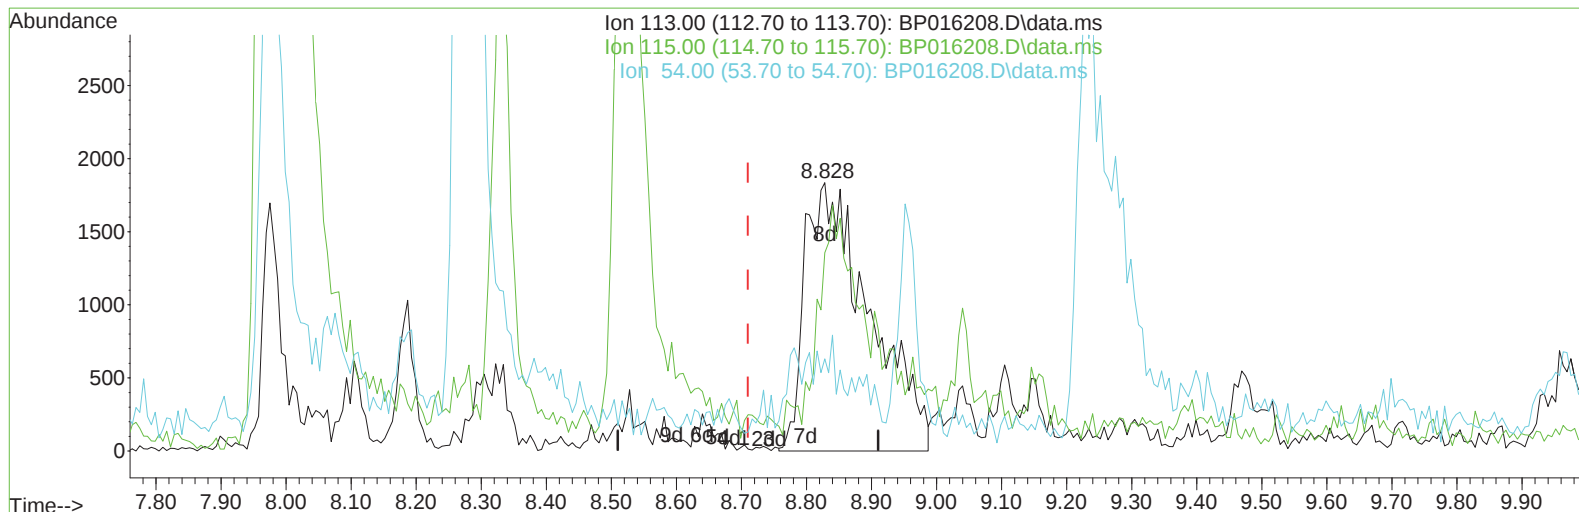

TIC: BP016208.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.828min (+ 0.118) 1.56 ng/u1 m

response 12661

Ion	Exp%	Act%
-----	------	------

113.00	100.00	100.00
--------	--------	--------

115.00	90.20	73.86
--------	-------	-------

54.00	16.30	34.31#
-------	-------	--------

0.00	0.00	0.00
------	------	------




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

Quant Time: Jul 14 11:59:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

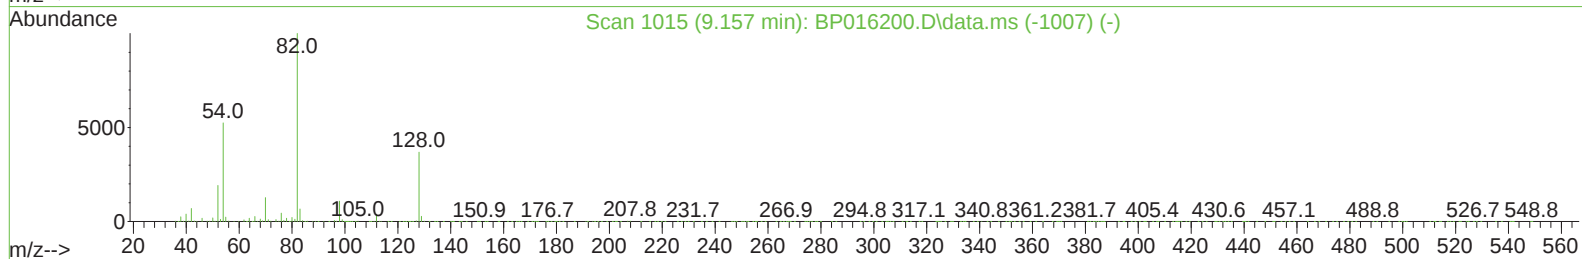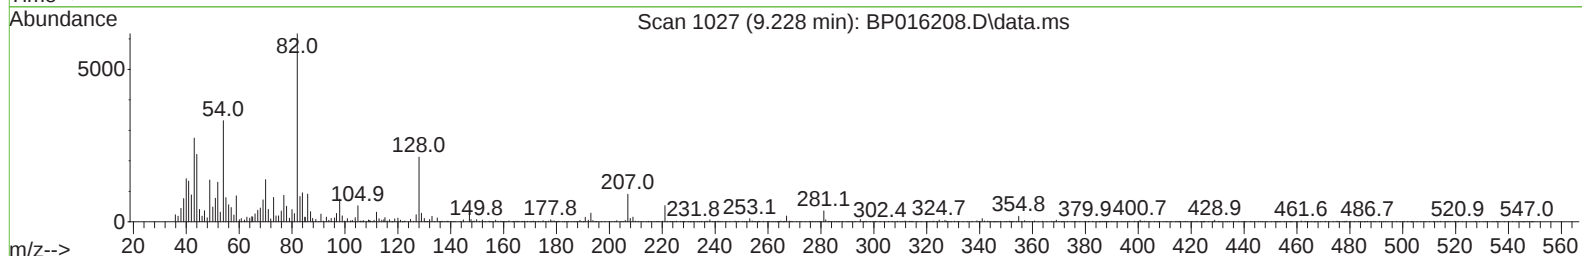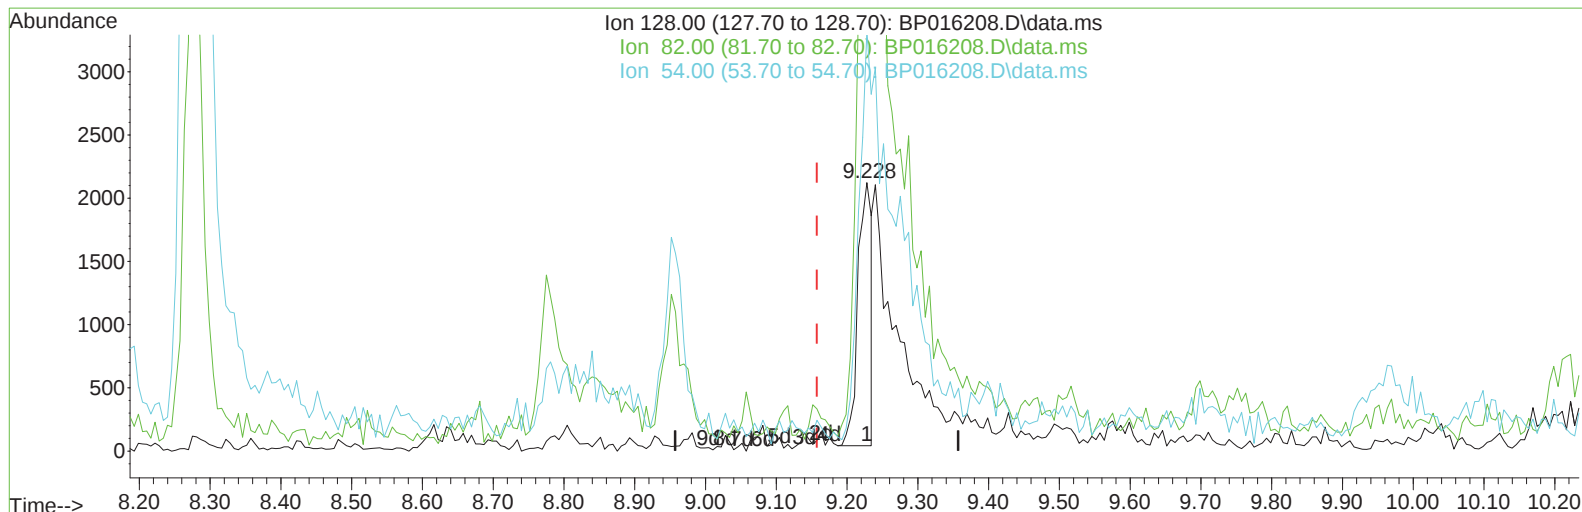

TIC: BP016208.D\data.ms

(21) Nitrobenzene-d5 (S)

9.228min (+ 0.071) 0.74 ng/u1

response	2806	
Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	290.58
54.00	136.80	156.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:21:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

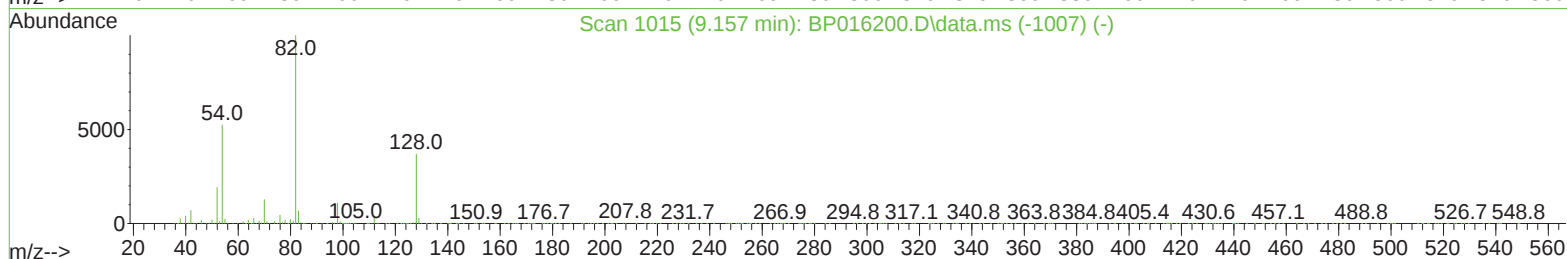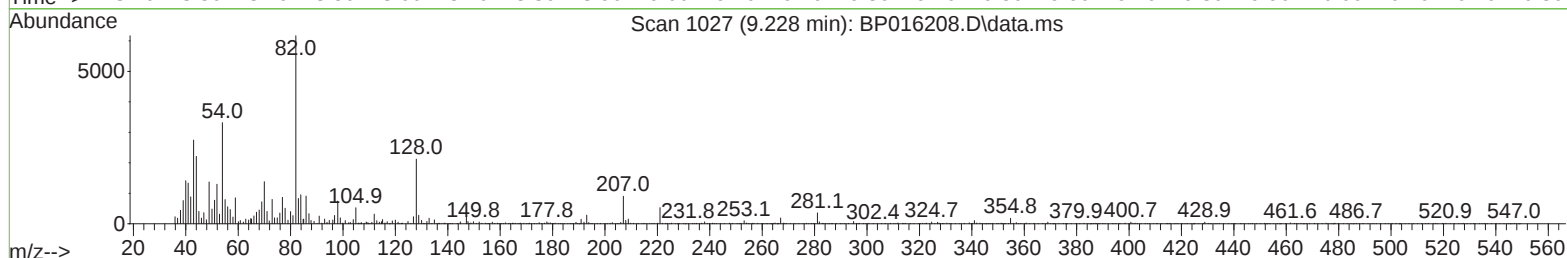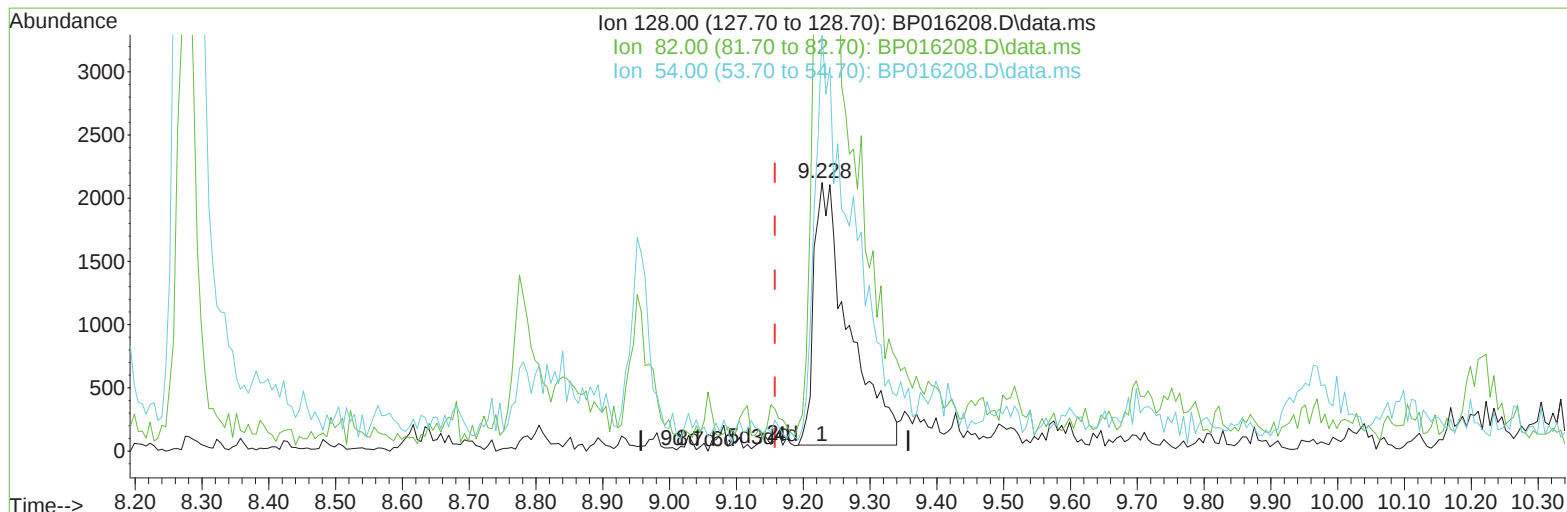

TIC: BP016208.D\data.ms

(21) Nitrobenzene-d5 (S)

9.228min (+ 0.071) 1.97 ng/u1 m

response 7489

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	290.58
54.00	136.80	156.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 19:18:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

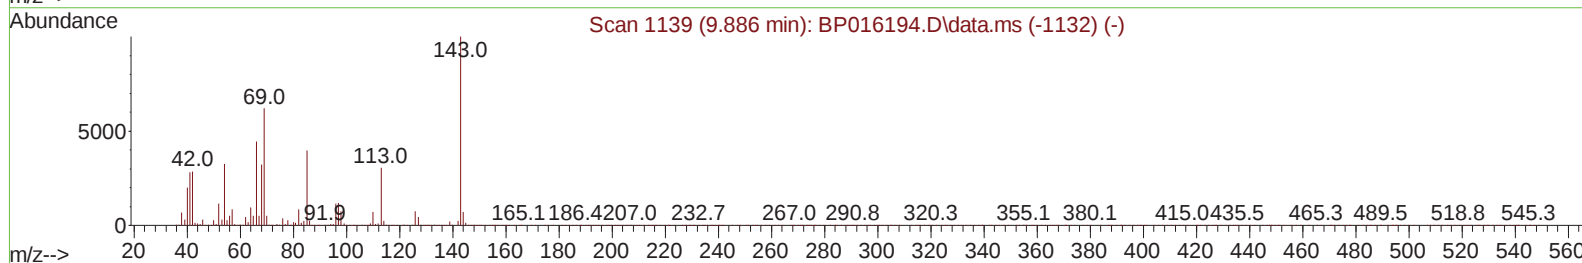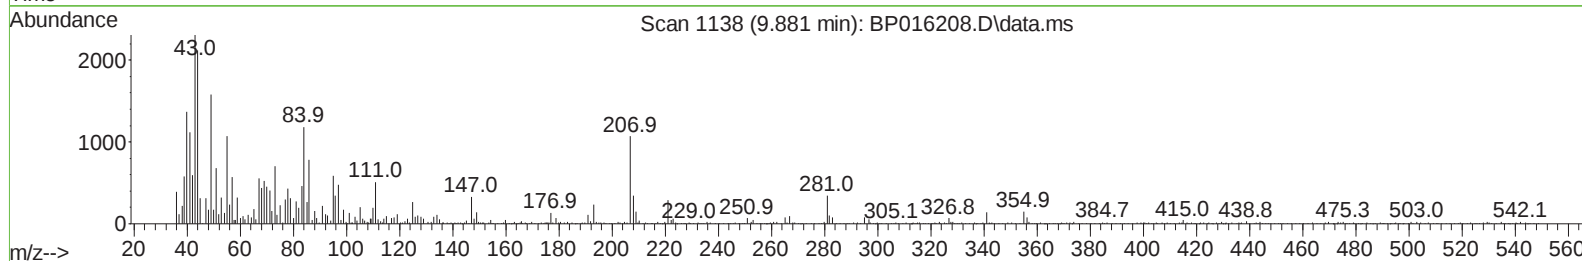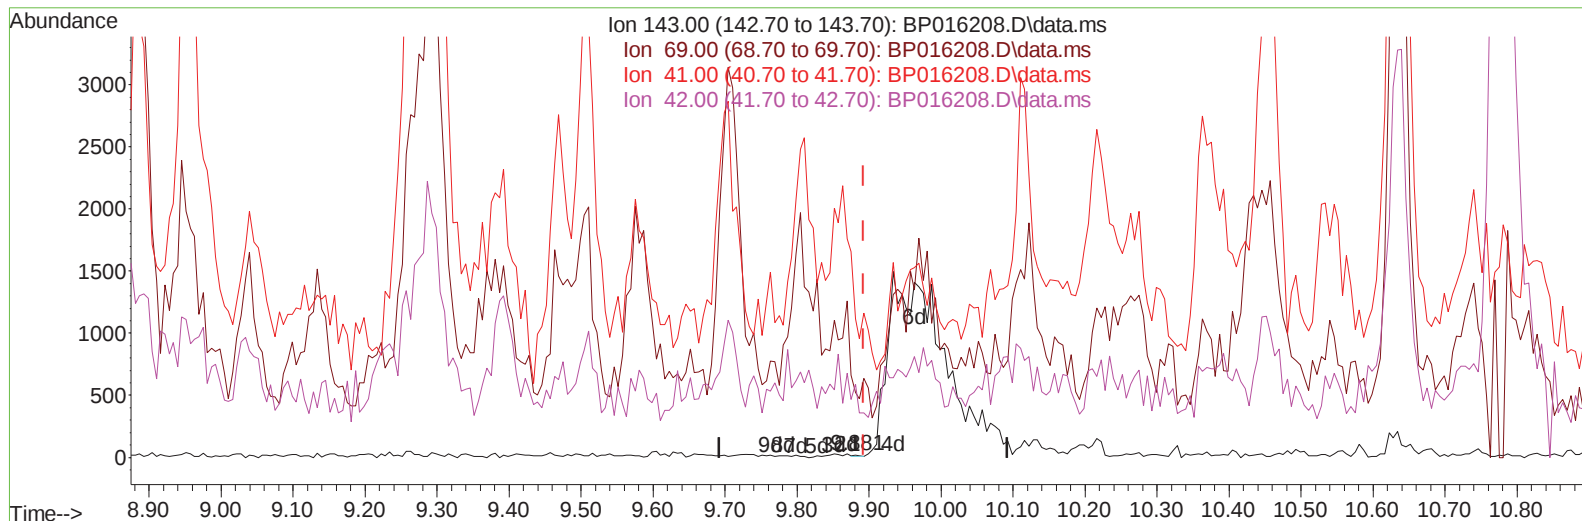

TIC: BP016208.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.881min (-0.012) 0.00 ng/u1

response 4

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	2747.37#
41.00	28.60	5878.95#
42.00	29.20	3110.53#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:21:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

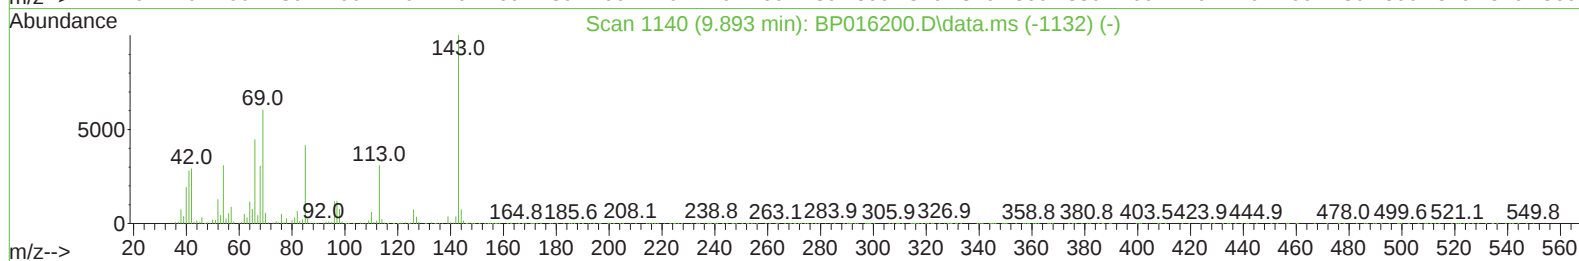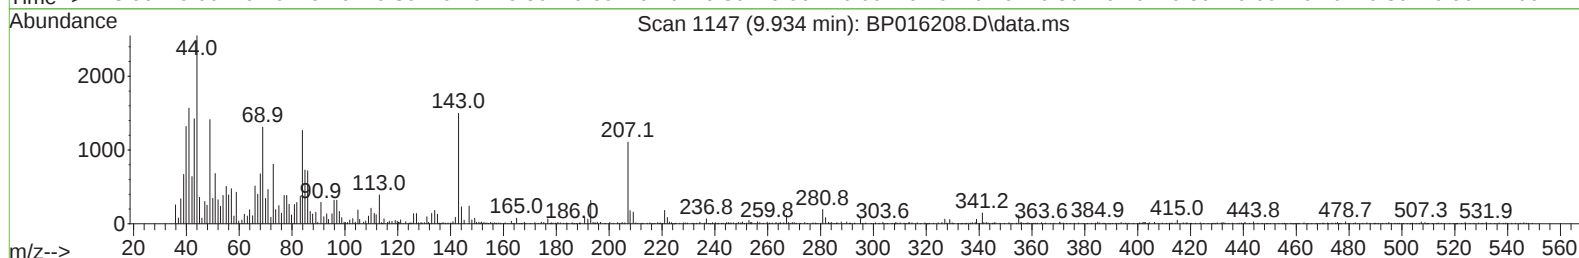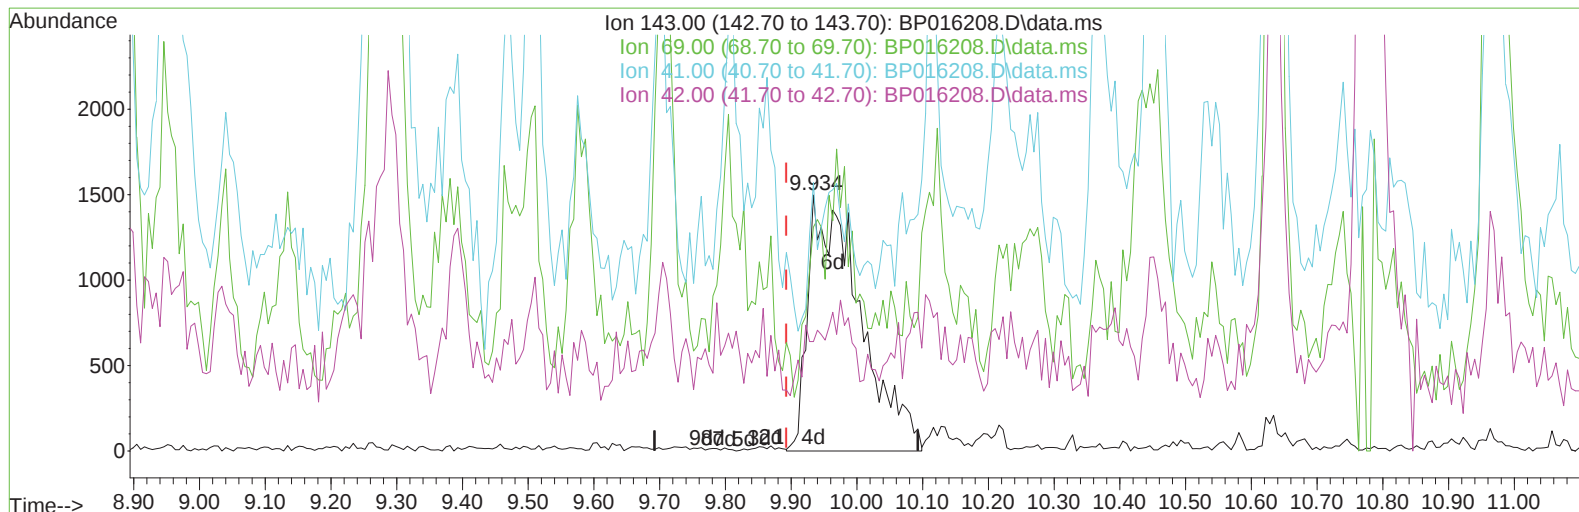

TIC: BP016208.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.934min (+ 0.041) 1.88 ng/ul m

response 8169

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	87.52#
41.00	28.60	104.81#
42.00	29.20	42.79#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:20:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

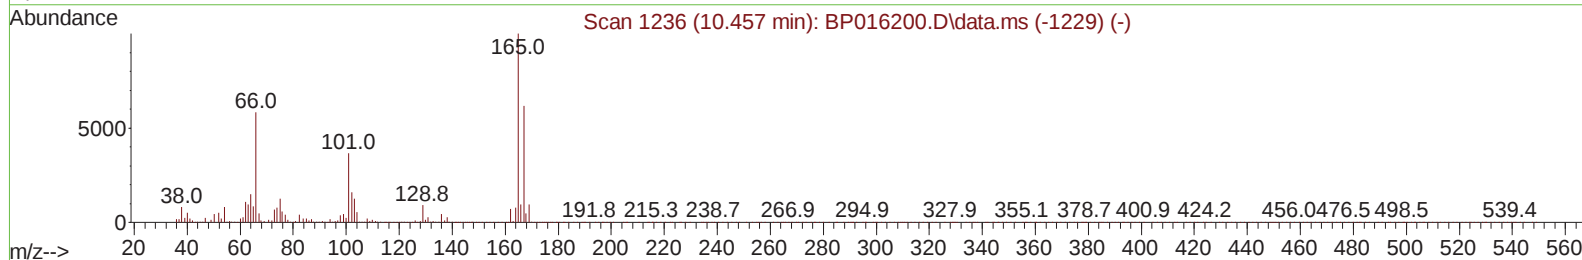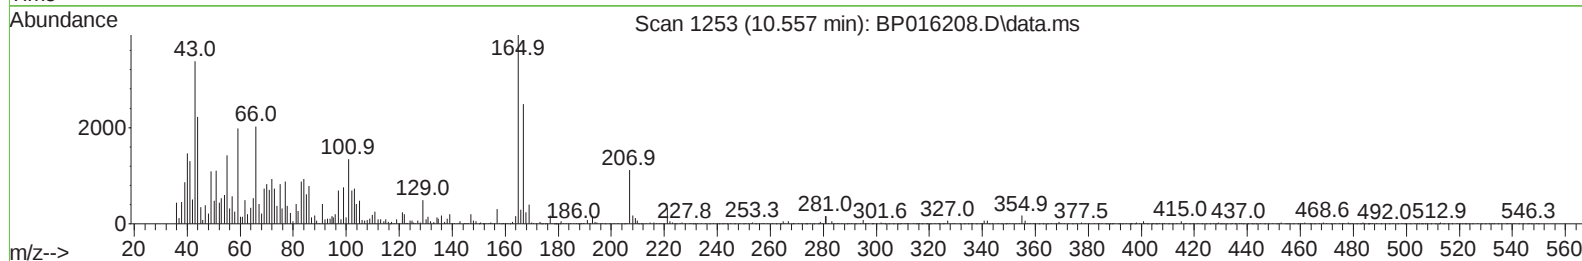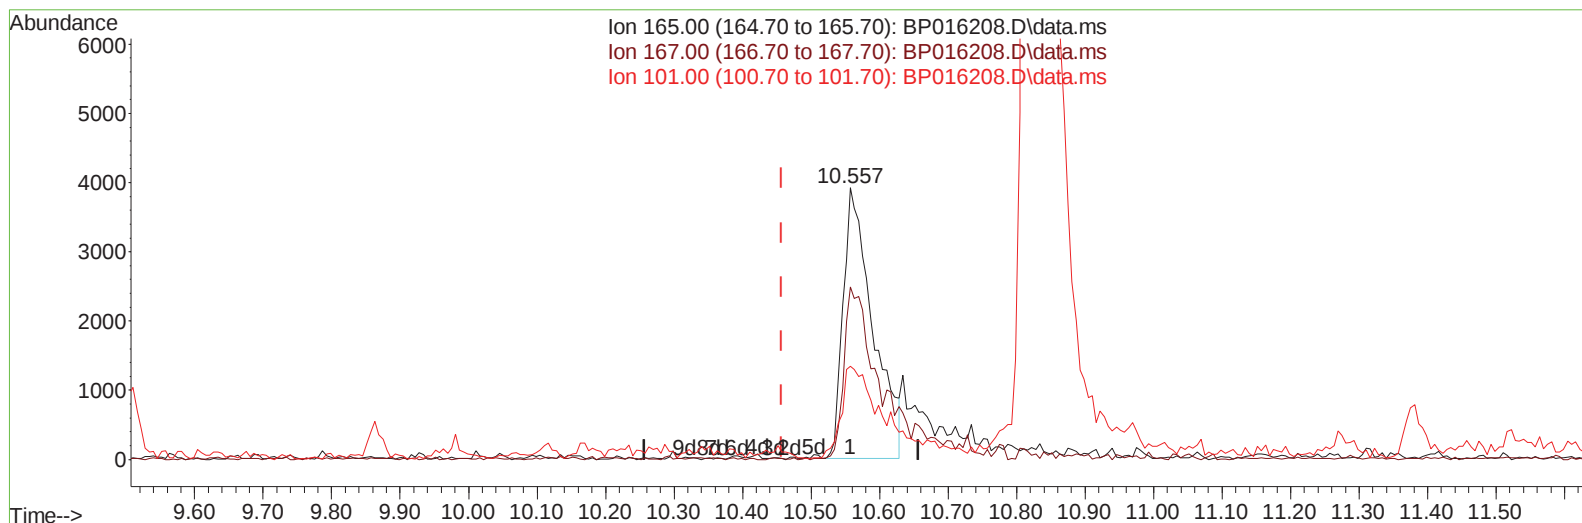

TIC: BP016208.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.557min (+ 0.100) 1.57 ng/ul

response 11834

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	63.55
101.00	38.50	34.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:20:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

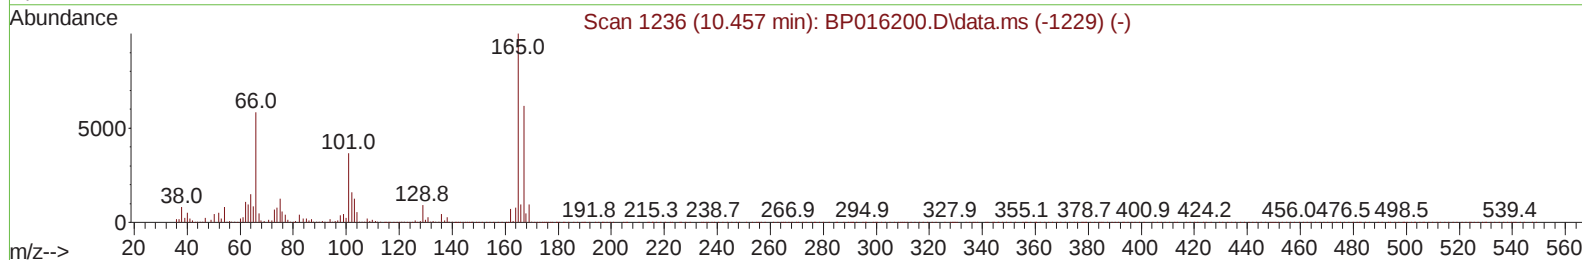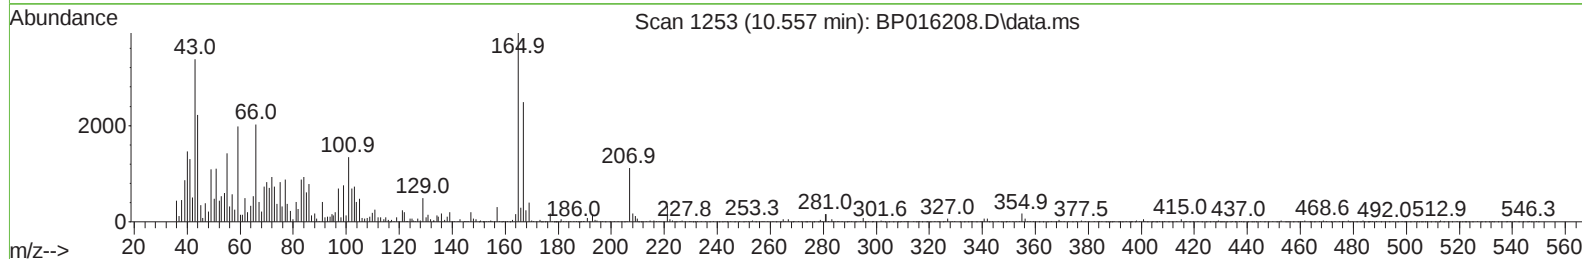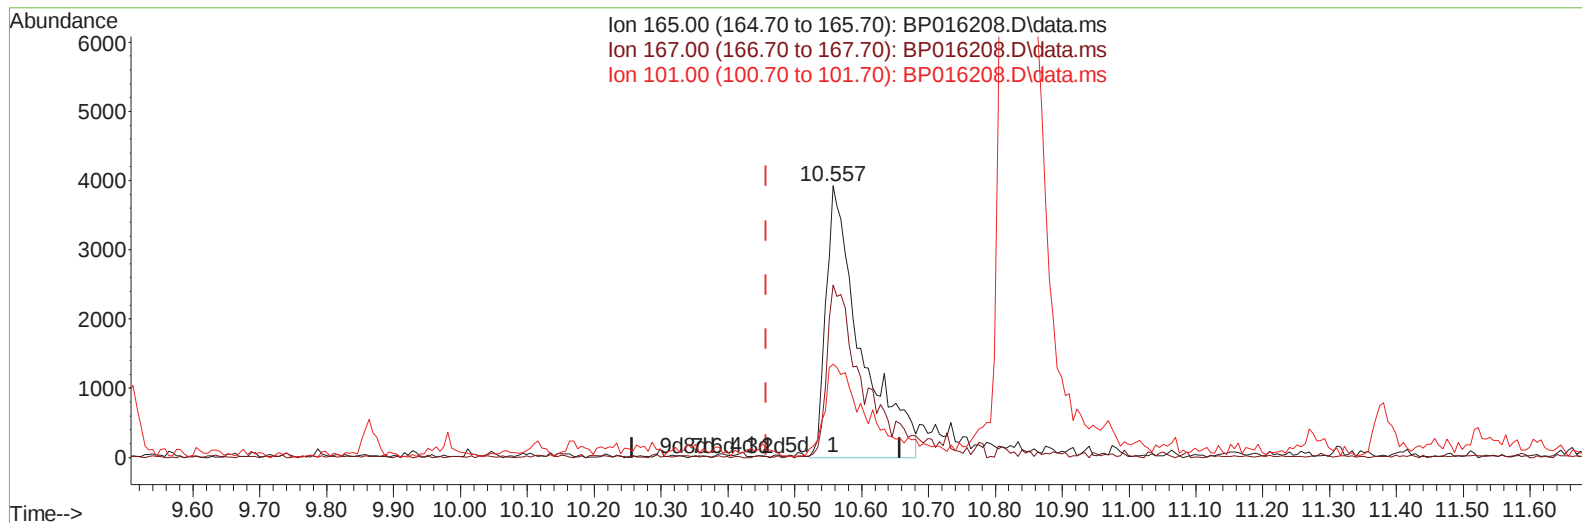

TIC: BP016208.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.557min (+ 0.100) 1.88 ng/ul m

response 14133

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	63.55
101.00	38.50	34.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:21:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

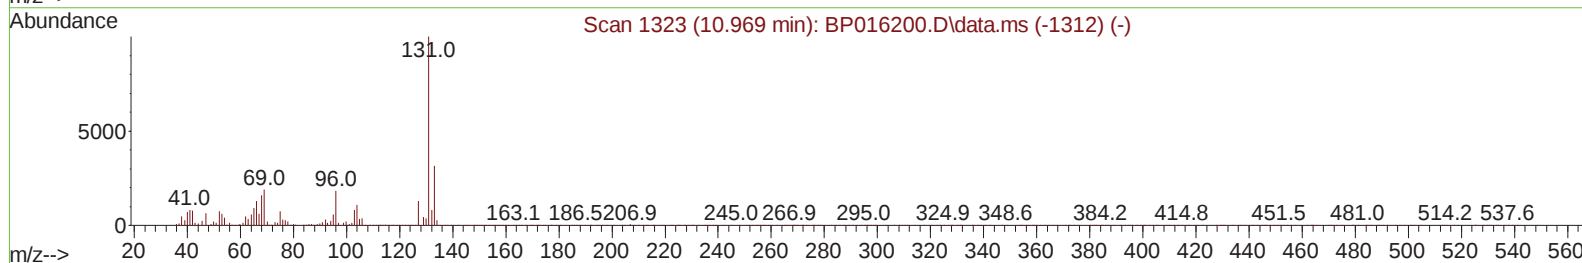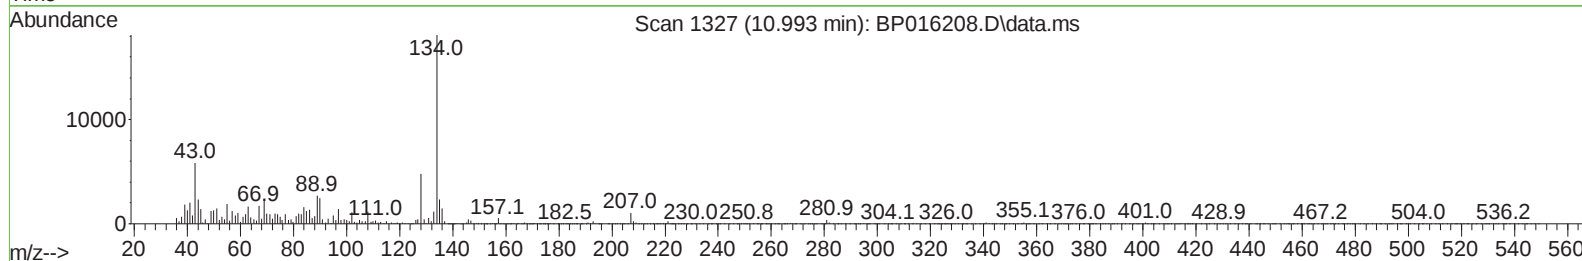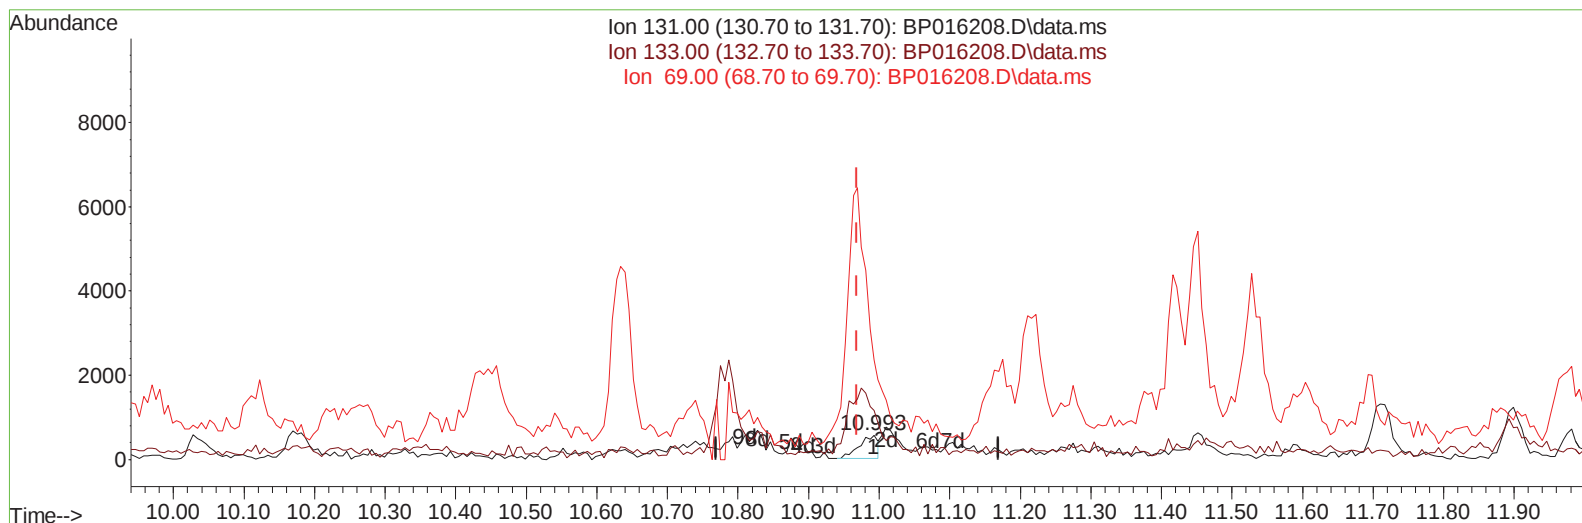

TIC: BP016208.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.993min (+ 0.024) 0.09 ng/u1

response 1036

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.50	200.52#
69.00	21.00	411.09#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016208.D
Acq On : 13 Jul 2023 14:57
Operator : MA/JU
Sample : 03385-01ME 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:21:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :Sohil Jodhani 07/14/2023

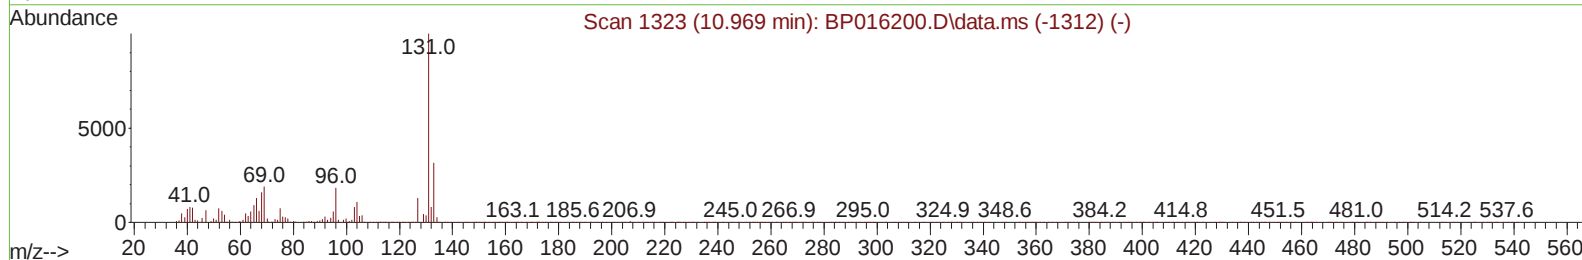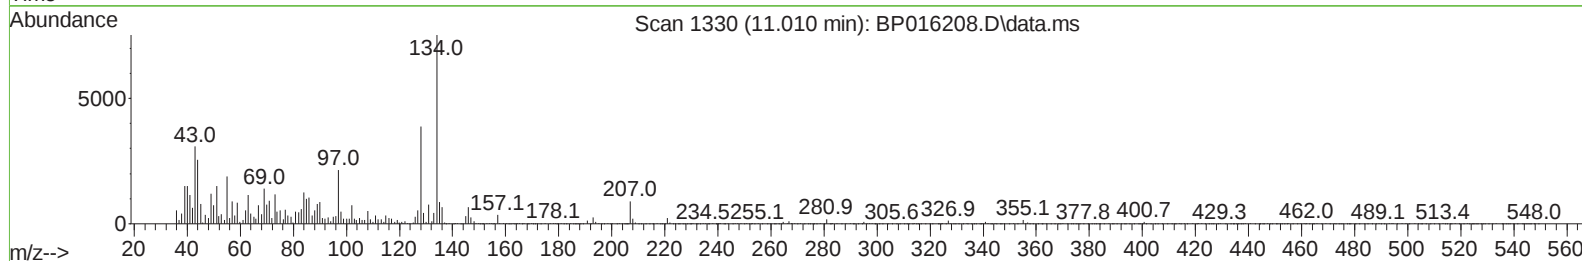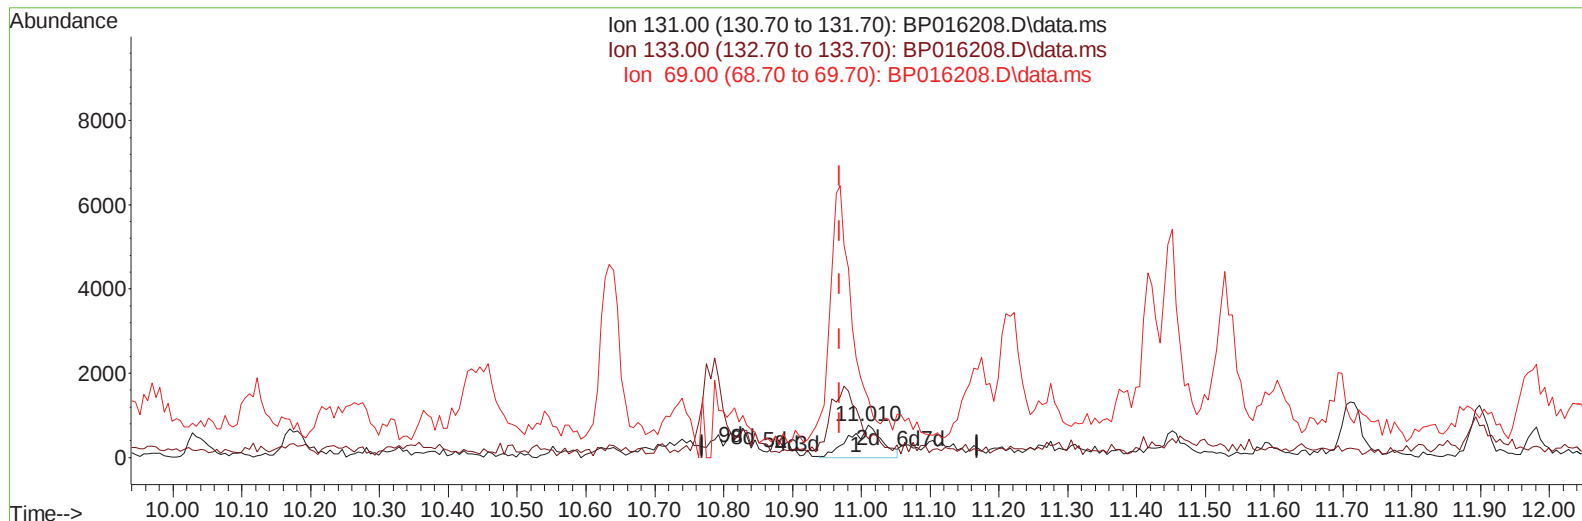

TIC: BP016208.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.010min (+ 0.041) 0.21 ng/ul m

response 2497

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.50	57.83#
69.00	21.00	183.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Quant Time: Jul 13 22:21:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	111448	20.000	ng/ul	0.00
20) Naphthalene-d8	10.781	136	552171	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.616	164	374260	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.381	188	909726	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240	980201	20.000	ng/ul	0.00
88) Perylene-d12	23.968	264	1129231	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	1488	0.472	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.234	99	16729m	1.662	ng/ul	0.08
9) Bis-(2-Chloroethyl)eth...	7.340	67	15604m	2.292	ng/ul	0.04
11) 2-Chlorophenol-d4	7.563	132	13990m	1.925	ng/ul	0.06
15) 4-Methylphenol-d8	8.828	113	12661m	1.561	ng/ul	0.12
21) Nitrobenzene-d5	9.228	128	7489m	1.966	ng/ul	0.07
24) 2-Nitrophenol-d4	9.934	143	8169m	1.882	ng/ul	0.04
28) 2,4-Dichlorophenol-d3	10.557	165	14133m	1.880	ng/ul	0.10
31) 4-Chloroaniline-d4	11.010	131	2497m	0.207	ng/ul	0.04
46) Dimethylphthalate-d6	14.045	166	76993	2.697	ng/ul	0.01
49) Acenaphthylene-d8	14.322	160	68210	2.180	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	42	0.007	ng/ul	0.01
60) Fluorene-d10	15.616	176	68815	2.880	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	69	0.013	ng/ul	0.00
73) Anthracene-d10	17.486	188	98901	2.485	ng/ul	0.00
81) Pyrene-d10	19.710	212	147082	2.892	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.810	264	123267	2.273	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.263	94	25647m	2.377	ng/ul	
16) Acetophenone	8.858	105	131565	9.839	ng/ul	97
30) Naphthalene	10.828	128	3588176	123.827	ng/ul	100
36) 2-Methylnaphthalene	12.446	142	1140083	58.679	ng/ul	99
37) 1-Methylnaphthalene	12.663	142	530373	26.543	ng/ul	99
43) 1,1'-Biphenyl	13.463	154	382523	14.011	ng/ul	99
50) Acenaphthylene	14.351	152	41739	1.162	ng/ul#	89
52) Acenaphthene	14.681	153	1538609	63.307	ng/ul	99
56) Dibenzofuran	15.028	168	1720260	51.965	ng/ul	100
61) Fluorene	15.675	166	1652768	59.764	ng/ul	98
72) Phenanthrene	17.428	178	8317315	175.468	ng/ul	99
74) Anthracene	17.528	178	2050489	43.051	ng/ul	97
77) Carbazole	17.810	167	825432	19.007	ng/ul	98
80) Fluoranthene	19.392	202	7113928	119.608	ng/ul	98
82) Pyrene	19.745	202	5011586	78.921	ng/ul	98
85) Benzo(a)anthracene	21.457	228	2518942	39.463	ng/ul	96
86) Bis(2-ethylhexyl)phtha...	21.339	149	67991	1.662	ng/ul	97
87) Chrysene	21.516	228	2071371	32.034	ng/ul	98
90) Benzo(b)fluoranthene	23.204	252	2812857	43.608	ng/ul	99
91) Benzo(k)fluoranthene	23.251	252	879582	13.400	ng/ul	100
93) Benzo(a)pyrene	23.863	252	1138668	17.820	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	26.615	276	1044492	13.201	ng/ul	97
95) Dibenzo(a,h)anthracene	26.615	278	310846	4.816	ng/ul#	80

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016208.D
 Acq On : 13 Jul 2023 14:57
 Operator : MA/JU
 Sample : 03385-01ME 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EX7X7ME

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :Sohil Jodhani 07/14/2023

Quant Time: Jul 13 22:21:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
96) Benzo(g,h,i)perylene	27.462	276	92548	1.465	ng/ul#	86
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed