

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016201.D
 Acq On : 13 Jul 2023 09:58
 Operator : MA/JU
 Sample : PB153962BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK962

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	13	17	27	rVB	44227	71023	1.40%	0.152%
2	3.740	92	94	123	rBV	332701	862827	17.01%	1.843%
3	4.058	145	148	157	rVB2	12430	21838	0.43%	0.047%
4	7.175	671	678	695	rBV	280833	982365	19.36%	2.098%
5	7.305	695	700	729	rVV	300120	940453	18.54%	2.009%
6	7.511	729	735	760	rVB	371315	1058678	20.87%	2.261%
7	7.981	807	815	839	rBV	236787	820670	16.18%	1.753%
8	8.516	901	906	911	rBV8	4348	10597	0.21%	0.023%
9	8.728	934	942	981	rBV	362359	1455915	28.70%	3.110%
10	9.028	991	993	1001	rVB9	4557	9543	0.19%	0.020%
11	9.175	1011	1018	1044	rBV	350849	1136582	22.40%	2.428%
12	9.916	1136	1144	1172	rBV	221348	941216	18.55%	2.010%
13	10.505	1237	1244	1258	rBV2	211836	863187	17.01%	1.844%
14	10.799	1287	1294	1314	rVB	488350	1330773	26.23%	2.843%
15	11.010	1323	1330	1352	rBV2	246911	1253427	24.71%	2.677%
16	12.499	1577	1583	1585	rBV6	6809	12908	0.25%	0.028%
17	12.757	1617	1627	1628	rBV7	6919	12468	0.25%	0.027%
18	12.922	1649	1655	1658	rBV7	5839	9382	0.18%	0.020%
19	13.493	1747	1752	1756	rBV7	8172	17986	0.35%	0.038%
20	14.046	1839	1846	1874	rBV	1049987	2547869	50.22%	5.442%
21	14.322	1886	1893	1922	rBV	1559467	2795276	55.10%	5.971%
22	14.622	1938	1944	1968	rBV	1104942	1937505	38.19%	4.139%
23	14.987	1996	2006	2020	rBV7	111166	607180	11.97%	1.297%
24	15.340	2062	2066	2071	rVB9	9583	17394	0.34%	0.037%
25	15.469	2085	2088	2095	rVB	16013	23671	0.47%	0.051%
26	15.634	2109	2116	2137	rBV	1539919	3609755	71.15%	7.710%
27	15.828	2143	2149	2177	rBV2	219527	1019065	20.09%	2.177%
28	16.422	2246	2250	2255	rBV8	3779	6263	0.12%	0.013%
29	16.592	2273	2279	2286	rBV7	14239	29326	0.58%	0.063%
30	16.698	2292	2297	2302	rVB4	16629	24666	0.49%	0.053%
31	16.963	2336	2342	2345	rBV8	5262	11382	0.22%	0.024%
32	17.198	2378	2382	2385	rBV6	4857	7581	0.15%	0.016%
33	17.392	2408	2415	2427	rBV	1462556	2441594	48.12%	5.215%
34	17.498	2427	2433	2463	rVV2	1390860	3925011	77.36%	8.384%
35	17.934	2503	2507	2509	rBV4	4552	7047	0.14%	0.015%
36	19.316	2738	2742	2746	rBV3	32432	43867	0.86%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016201.D
Acq On : 13 Jul 2023 09:58
Operator : MA/JU
Sample : PB153962BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK962

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION

37	19.398	2753	2756	2757	rBV2	14018	16875	0.33%	0.036%
38	19.728	2806	2812	2842	rBV2	2027295	5073508	100.00%	10.837%
39	21.504	3109	3114	3131	rBV	1125425	2792373	55.04%	5.965%
40	23.816	3501	3507	3528	rVB2	2046670	5046853	99.47%	10.780%
41	23.992	3530	3537	3564	rVB	852517	3020544	59.54%	6.452%




Sum of corrected areas: 46816443

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016201.D
Acq On : 13 Jul 2023 09:58
Operator : MA/JU
Sample : PB153962BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK962

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

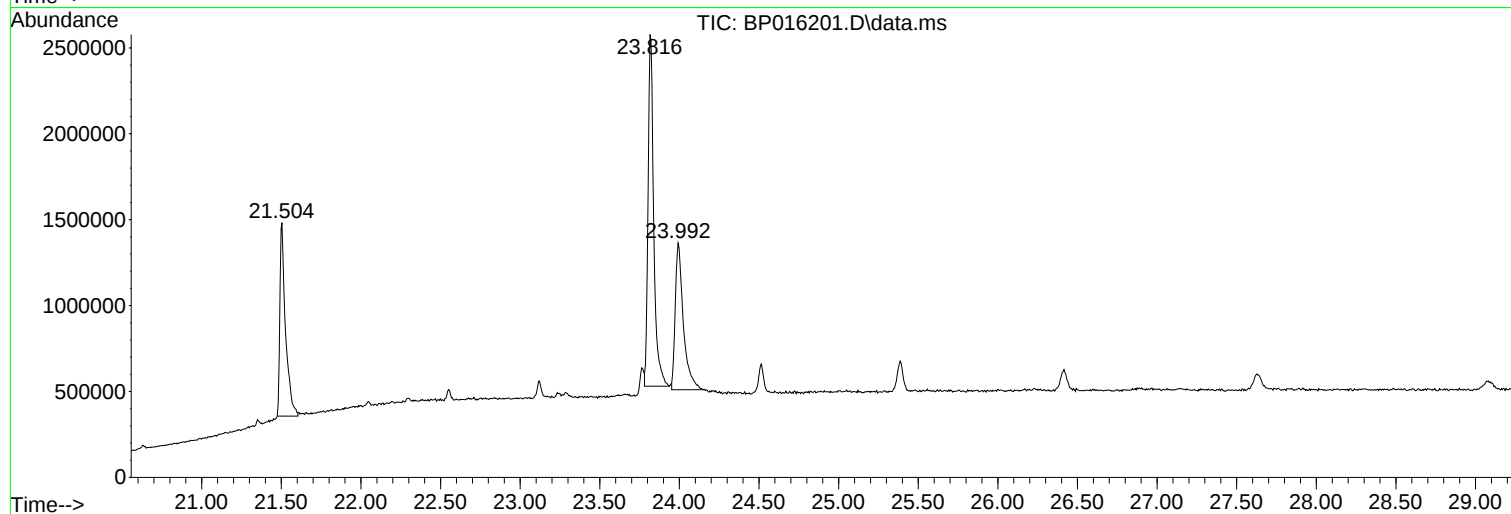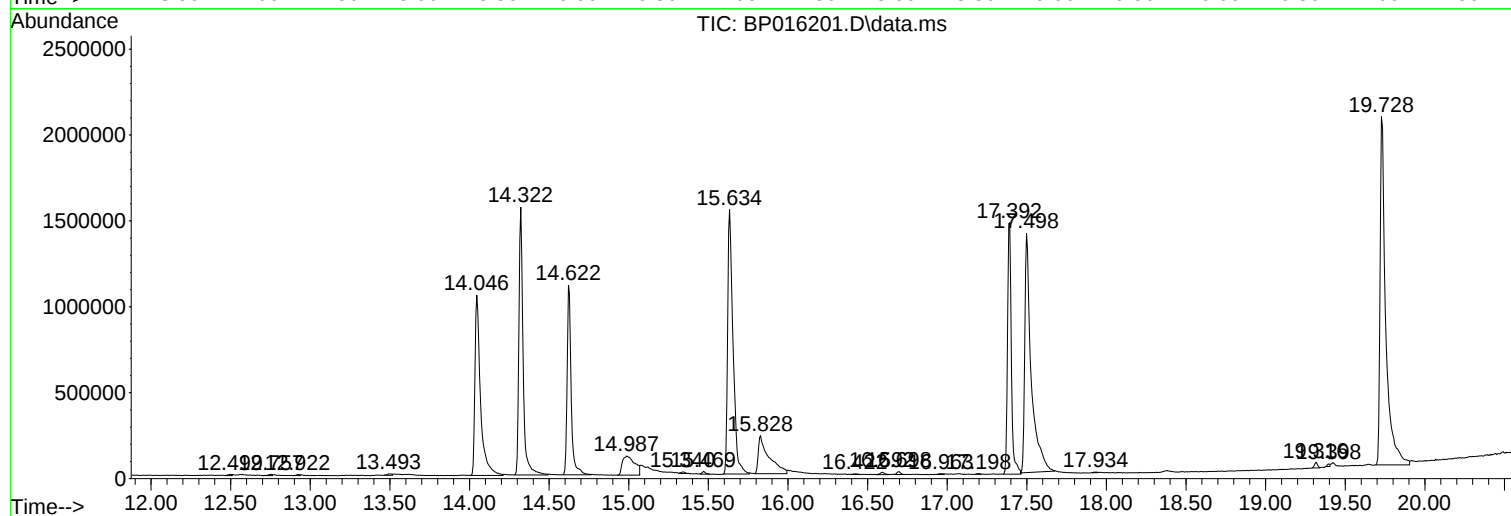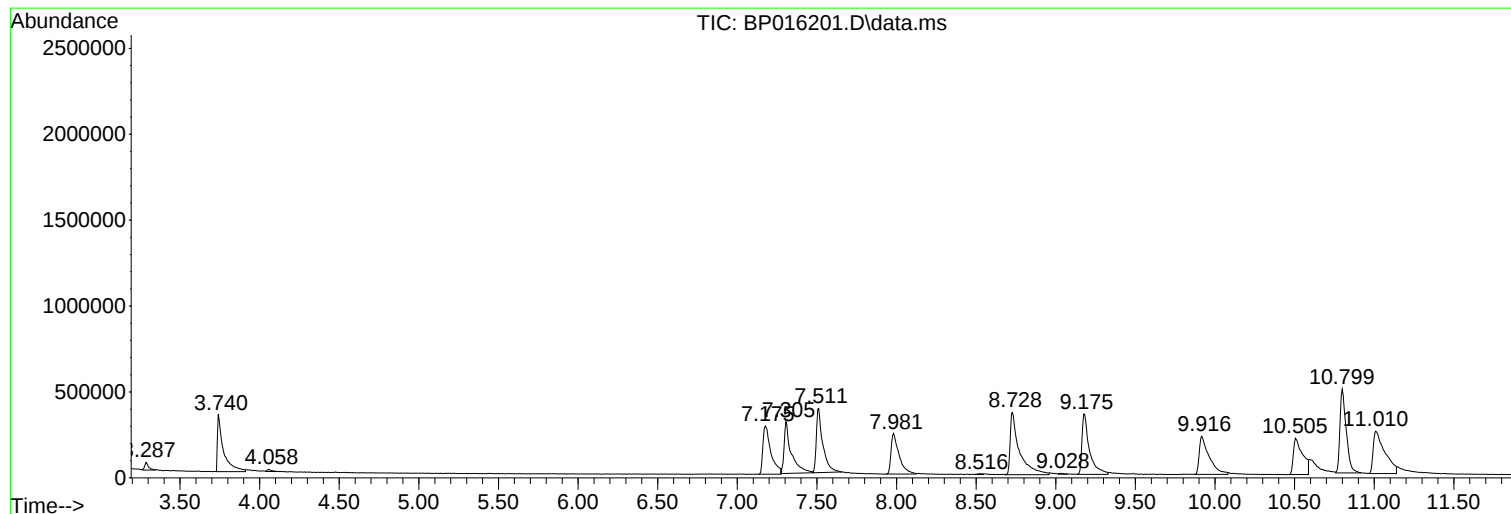

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016201.D
Acq On : 13 Jul 2023 09:58
Operator : MA/JU
Sample : PB153962BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK962

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016201.D
Acq On : 13 Jul 2023 09:58
Operator : MA/JU
Sample : PB153962BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK962

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------