

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016207.D
 Acq On : 13 Jul 2023 14:22
 Operator : MA/JU
 Sample : PB154150BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	14	17	32	rVB	47185	90222	1.50%	0.161%
2	3.740	92	94	121	rBV	398801	961233	15.94%	1.716%
3	4.052	144	147	153	rBV2	12531	19056	0.32%	0.034%
4	7.169	669	677	694	rBV2	312697	1130329	18.74%	2.018%
5	7.298	694	699	728	rVV	391273	1083852	17.97%	1.935%
6	7.504	728	734	761	rVB	435845	1210031	20.07%	2.160%
7	7.969	805	813	839	rBV	329572	1053408	17.47%	1.881%
8	8.134	839	841	850	rVB9	4193	7927	0.13%	0.014%
9	8.504	898	904	905	rBV4	9623	14454	0.24%	0.026%
10	8.722	934	941	977	rBV	454605	1617533	26.82%	2.888%
11	9.175	1011	1018	1046	rBV	419845	1265370	20.98%	2.259%
12	9.775	1115	1120	1122	rBV4	5113	8691	0.14%	0.016%
13	9.904	1135	1142	1164	rBV	289274	1049979	17.41%	1.875%
14	10.492	1235	1242	1257	rBV2	253851	1071582	17.77%	1.913%
15	10.792	1286	1293	1319	rVB	707544	1738500	28.83%	3.104%
16	10.998	1321	1328	1355	rBV	300992	1490439	24.71%	2.661%
17	12.475	1574	1579	1585	rBV7	8398	21813	0.36%	0.039%
18	12.545	1585	1591	1599	rVV6	10476	26332	0.44%	0.047%
19	12.733	1617	1623	1627	rBV2	14665	28302	0.47%	0.051%
20	12.904	1645	1652	1665	rBV7	13006	37546	0.62%	0.067%
21	13.204	1699	1703	1704	rBV3	4519	6473	0.11%	0.012%
22	13.481	1744	1750	1751	rBV2	18019	25471	0.42%	0.045%
23	13.569	1763	1765	1769	rVB6	7539	9089	0.15%	0.016%
24	14.039	1838	1845	1875	rBV	1232274	2851649	47.29%	5.091%
25	14.316	1886	1892	1916	rBV	1739174	3139133	52.05%	5.604%
26	14.622	1937	1944	1953	rBV	1447756	2412993	40.01%	4.308%
27	14.980	1995	2005	2016	rBV4	177533	800559	13.28%	1.429%
28	15.327	2059	2064	2070	rVB9	18139	30744	0.51%	0.055%
29	15.463	2082	2087	2092	rVB	28636	41970	0.70%	0.075%
30	15.627	2108	2115	2125	rBV	1836887	3925041	65.09%	7.008%
31	15.816	2141	2147	2161	rBV2	293055	984856	16.33%	1.758%
32	16.580	2272	2277	2282	rBV3	24638	39773	0.66%	0.071%
33	16.692	2291	2296	2302	rVB2	31543	47907	0.79%	0.086%
34	16.939	2334	2338	2344	rBV9	5209	11364	0.19%	0.020%
35	17.186	2378	2380	2389	rBV7	5100	10427	0.17%	0.019%
36	17.386	2407	2414	2426	rBV	2010006	3158639	52.38%	5.639%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
 Data File : BP016207.D
 Acq On : 13 Jul 2023 14:22
 Operator : MA/JU
 Sample : PB154150BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK150

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

37	17.498	2426	2433	2464	rVB2	1675463	4466974	74.07%	7.975%
38	17.910	2498	2503	2511	rBV4	12760	33599	0.56%	0.060%
39	18.345	2572	2577	2585	rBV2	20705	51272	0.85%	0.092%
40	18.621	2620	2624	2626	rBV5	5162	8414	0.14%	0.015%
41	19.310	2737	2741	2746	rBV3	37817	60780	1.01%	0.109%
42	19.392	2751	2755	2756	rBV	24219	30669	0.51%	0.055%
43	19.415	2757	2759	2764	rVB	36574	50033	0.83%	0.089%
44	19.727	2806	2812	2843	rBV	2586359	5698601	94.50%	10.174%
45	20.615	2960	2963	2969	rBV4	40882	78988	1.31%	0.141%
46	21.345	3085	3087	3093	rBV3	57271	72121	1.20%	0.129%
47	21.498	3107	3113	3131	rBV2	1630815	3774452	62.59%	6.739%
48	23.815	3500	3507	3527	rVB2	2505201	6030518	100.00%	10.767%
49	23.986	3529	3536	3563	rVB	1259680	4232452	70.18%	7.556%




Sum of corrected areas: 56011560

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016207.D
Acq On : 13 Jul 2023 14:22
Operator : MA/JU
Sample : PB154150BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

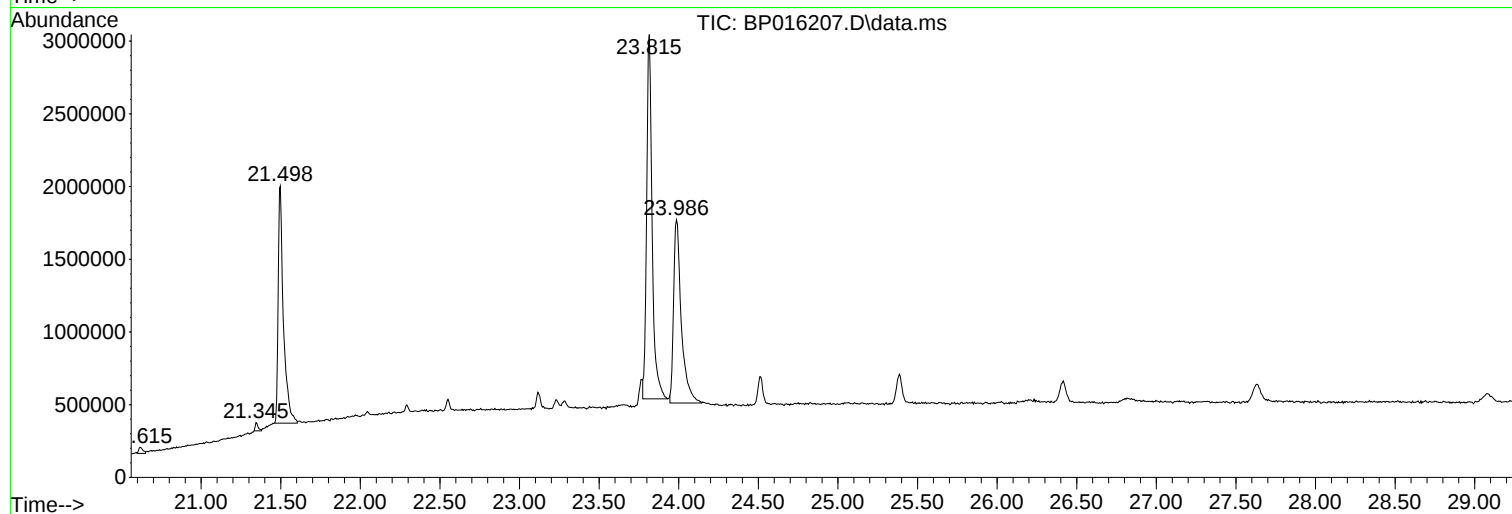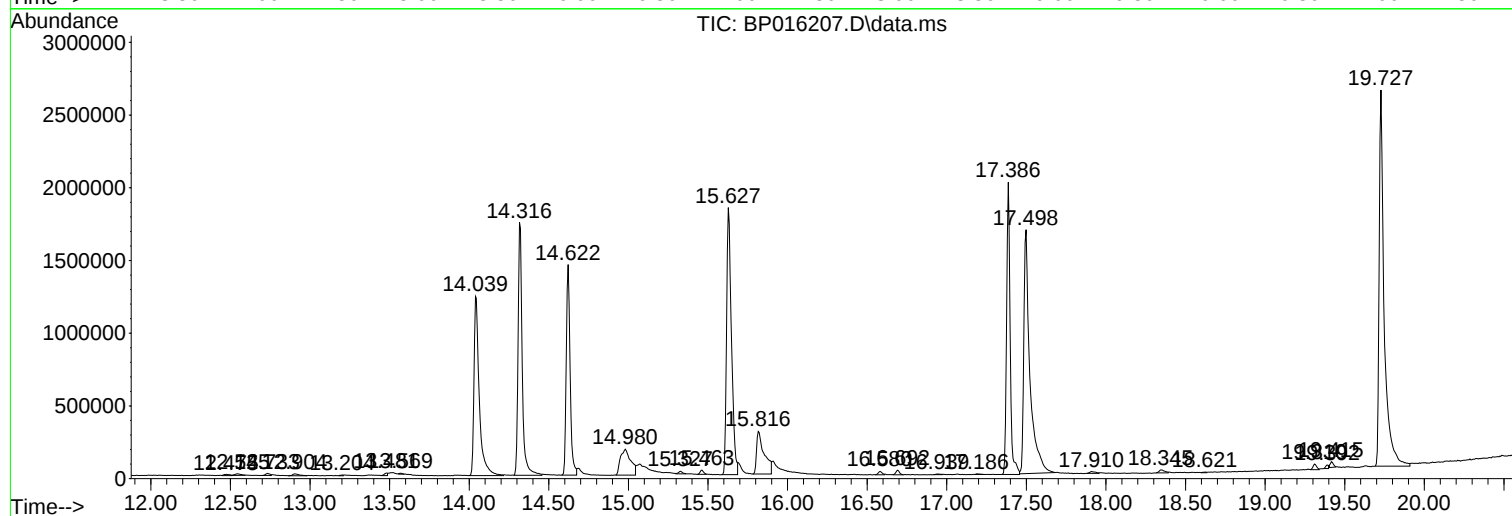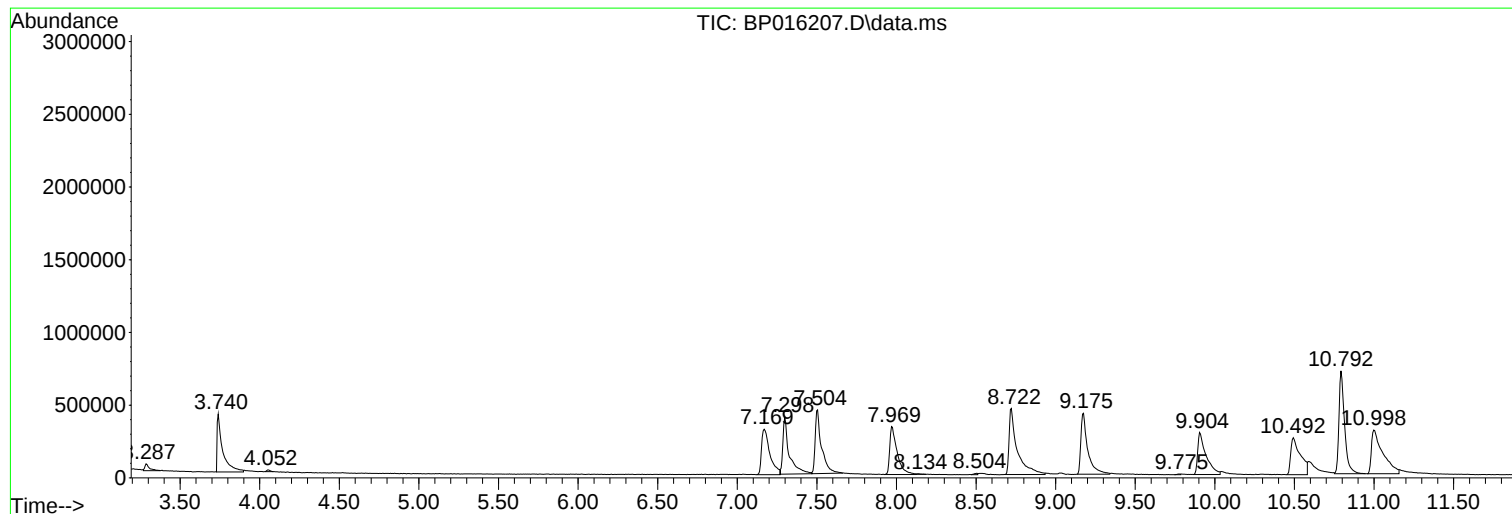

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016207.D
Acq On : 13 Jul 2023 14:22
Operator : MA/JU
Sample : PB154150BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071323\
Data File : BP016207.D
Acq On : 13 Jul 2023 14:22
Operator : MA/JU
Sample : PB154150BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK150

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------