

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
 Data File : BP016219.D
 Acq On : 14 Jul 2023 11:06
 Operator : MA/JU
 Sample : 03414-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4634

Quant Time: Jul 14 22:19:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	190682	20.000	ng/ul	0.00
20) Naphthalene-d8	10.793	136	917130	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.622	164	624491	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.387	188	1424518	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1454229	20.000	ng/ul	0.00
88) Perylene-d12	23.974	264	1598867	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	1856	0.344	ng/uL	0.00
4) Pyridine-d5	3.723	84	594	0.044	ng/ul	-0.02
7) Phenol-d5	7.187	99	129251	7.504	ng/ul	0.03
9) Bis-(2-Chloroethyl)eth...	7.305	67	92775	7.966	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	96532	7.764	ng/ul	0.02
15) 4-Methylphenol-d8	8.763	113	67098	4.836	ng/ul	0.05
21) Nitrobenzene-d5	9.205	128	48059	7.596	ng/ul	0.05
24) 2-Nitrophenol-d4	9.940	143	21474	2.978	ng/ul	0.05
28) 2,4-Dichlorophenol-d3	10.557	165	31376	2.513	ng/ul	0.10
31) 4-Chloroaniline-d4	10.987	131	67	0.003	ng/ul	0.02
46) Dimethylphthalate-d6	14.051	166	439500	9.226	ng/ul	0.02
49) Acenaphthylene-d8	14.322	160	450824	8.636	ng/ul	0.00
54) 4-Nitrophenol-d4	14.940	143	99	0.010	ng/ul	0.00
60) Fluorene-d10	15.634	176	379428	9.517	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.863	200	17706	2.153	ng/ul	0.07
73) Anthracene-d10	17.498	188	533773	8.566	ng/ul	0.01
81) Pyrene-d10	19.728	212	766195	10.154	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.810	264	648428	8.445	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.869	105	61479	2.687	ng/ul	Qvalue 100
17) N-Nitroso-di-n-propyla...	8.781	70	19494	1.589	ng/ul#	71
86) Bis(2-ethylhexyl)phtha...	21.333	149	87378	1.440	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016219.D
Acq On : 14 Jul 2023 11:06
Operator : MA/JU
Sample : 03414-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4634

Quant Time: Jul 14 22:19:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration




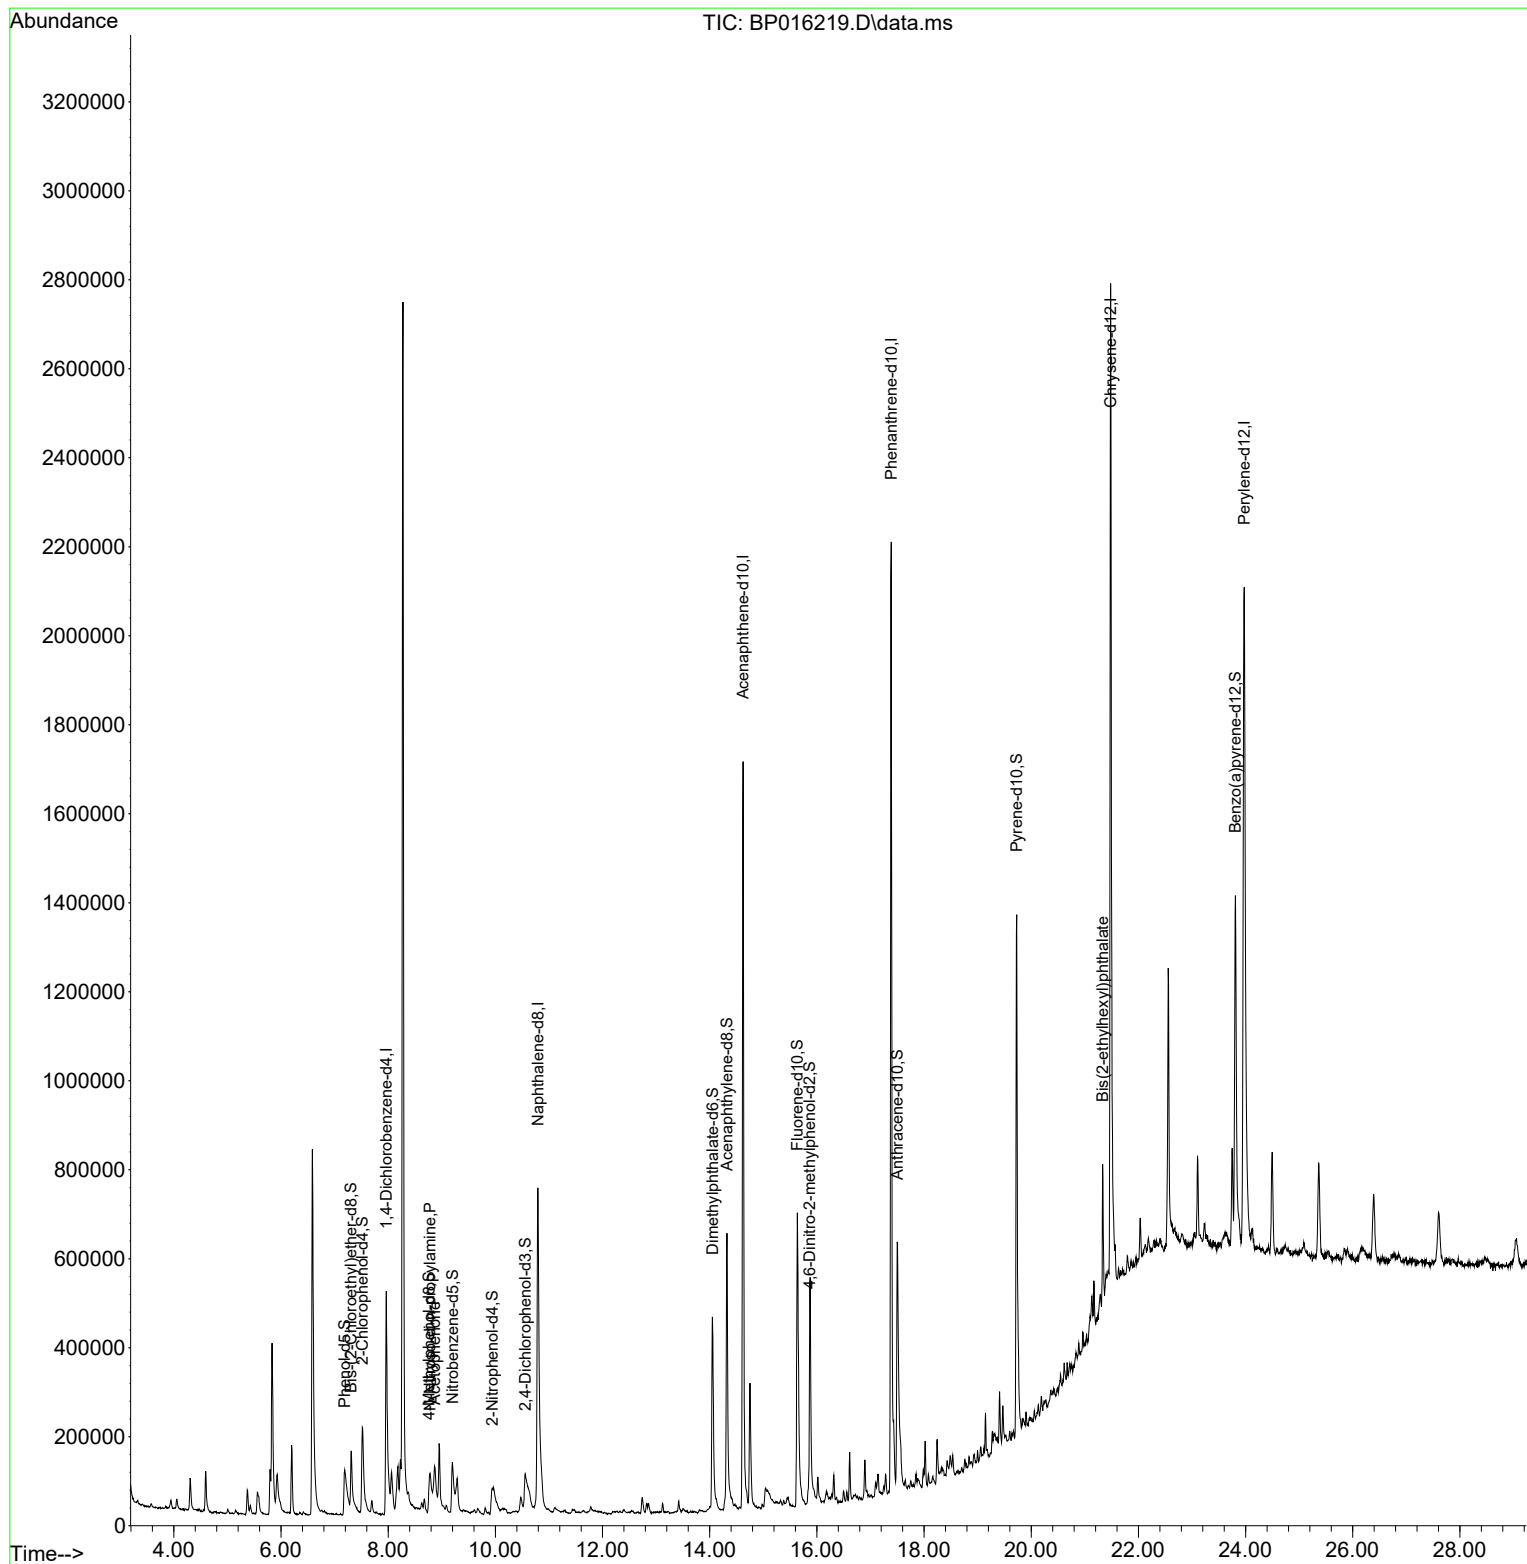


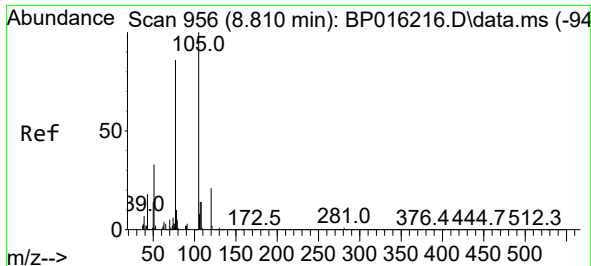

#16
Acetophenone
Concen: 2.687 ng/ul
RT: 8.869 min Scan# 90
Delta R.T. 0.047 min
Lab File: BP016219.D
Acq: 14 Jul 2023 11:06




Instrument :
BNA_P
ClientSampleId :
A4634


Tgt Ion:105 Resp: 61479
Ion Ratio Lower Upper
105 100
77 87.4 70.2 105.2
51 33.3 26.3 39.5

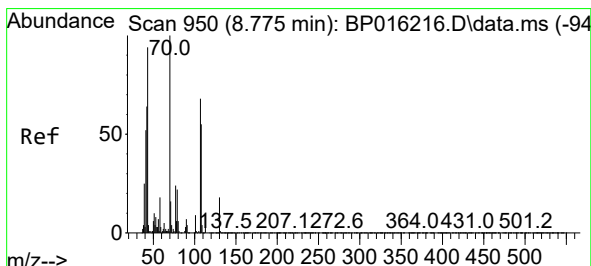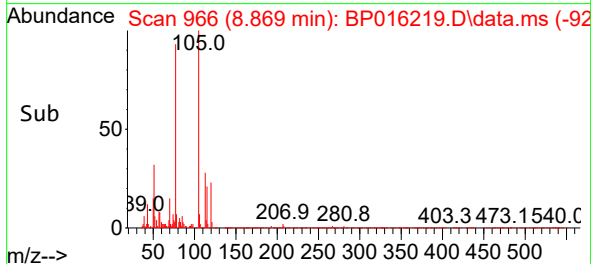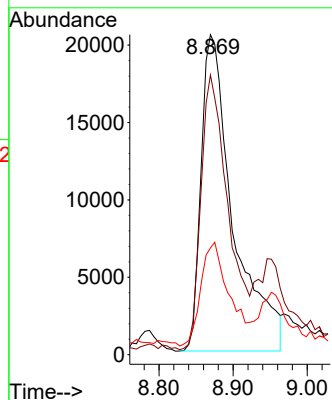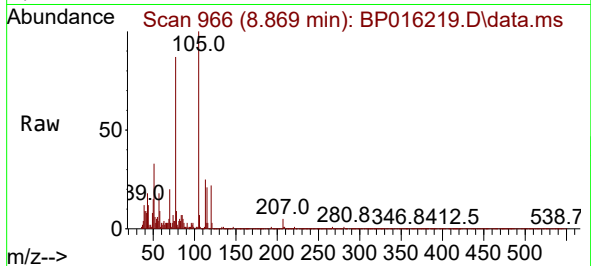

#17
N-Nitroso-di-n-propylamine
Concen: 1.589 ng/ul
RT: 8.781 min Scan# 951
Delta R.T. 0.000 min
Lab File: BP016219.D
Acq: 14 Jul 2023 11:06

Tgt Ion: 70 Resp: 19494
Ion Ratio Lower Upper
70 100
42 42.2 50.8 76.2#
101 0.3 7.0 10.6#
130 0.2 13.3 19.9#

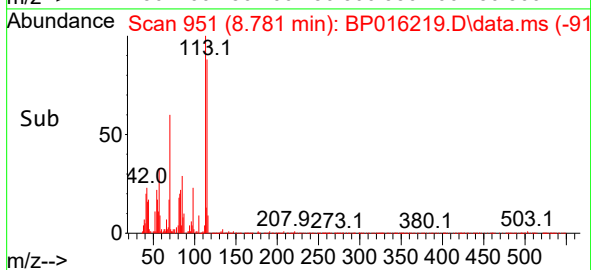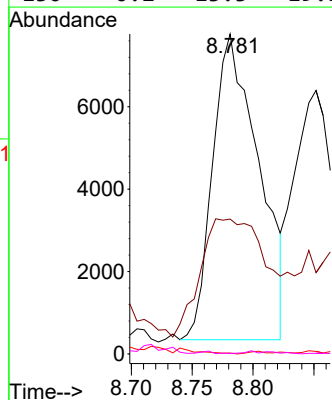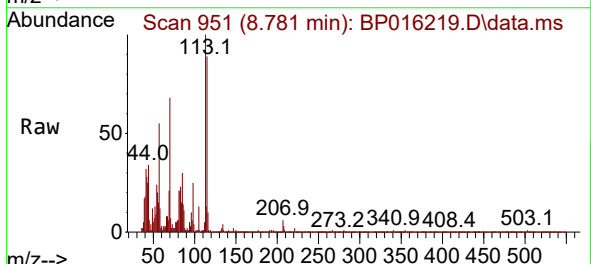

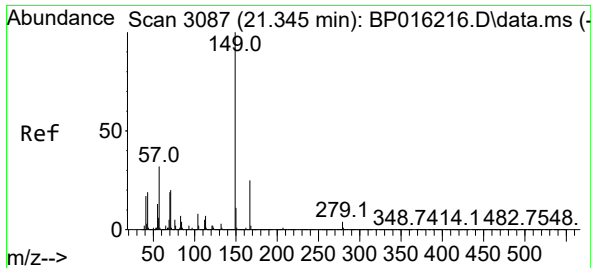

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.440 ng/ul
 RT: 21.333 min Scan# 3085
 Delta R.T. -0.006 min
 Lab File: BP016219.D
 Acq: 14 Jul 2023 11:06

Instrument :
 BNA_P
 ClientSampleId :
 A4634

Tgt Ion:	149	Resp:	87378
Ion Ratio	Lower	Upper	
149	100		
167	23.2	21.0	31.4
279	3.7	3.0	4.6

