

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
 Data File : BP016227.D
 Acq On : 14 Jul 2023 15:40
 Operator : MA/JU
 Sample : 03437-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46K9

Quant Time: Jul 14 22:22:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 13 18:57:06 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	136231	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.786	136	666124	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.616	164	438556	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.380	188	1009433	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	1051877	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	1182652	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	20243	5.258	ng/uL	0.00
4) Pyridine-d5	3.740	84	247407	25.768	ng/ul	0.00
7) Phenol-d5	7.151	99	394440	32.055	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	259749	31.218	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	298309	33.583	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	138979	14.021	ng/ul	0.02
21) Nitrobenzene-d5	9.163	128	147194	32.030	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	162550	31.034	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.492	165	263365	29.036	ng/ul	0.04
31) 4-Chloroaniline-d4	11.063	131	18200	1.252	ng/ul	0.09
46) Dimethylphthalate-d6	14.033	166	1013125	30.285	ng/ul	0.00
49) Acenaphthylene-d8	14.316	160	1088009	29.677	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	102877	15.069	ng/ul	0.01
60) Fluorene-d10	15.621	176	890366	31.802	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	112946	19.382	ng/ul	0.02
73) Anthracene-d10	17.492	188	966466	21.888	ng/ul	0.00
81) Pyrene-d10	19.715	212	1781316	32.636	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.809	264	1190084	20.954	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.845	105	44342	2.713	ng/ul	95
17) N-Nitroso-di-n-propyla...	8.769	70	21704	2.477	ng/ul#	81
86) Bis(2-ethylhexyl)phtha...	21.333	149	126180	2.874	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016227.D
Acq On : 14 Jul 2023 15:40
Operator : MA/JU
Sample : 03437-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46K9

Quant Time: Jul 14 22:22:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 13 18:57:06 2023
Response via : Initial Calibration




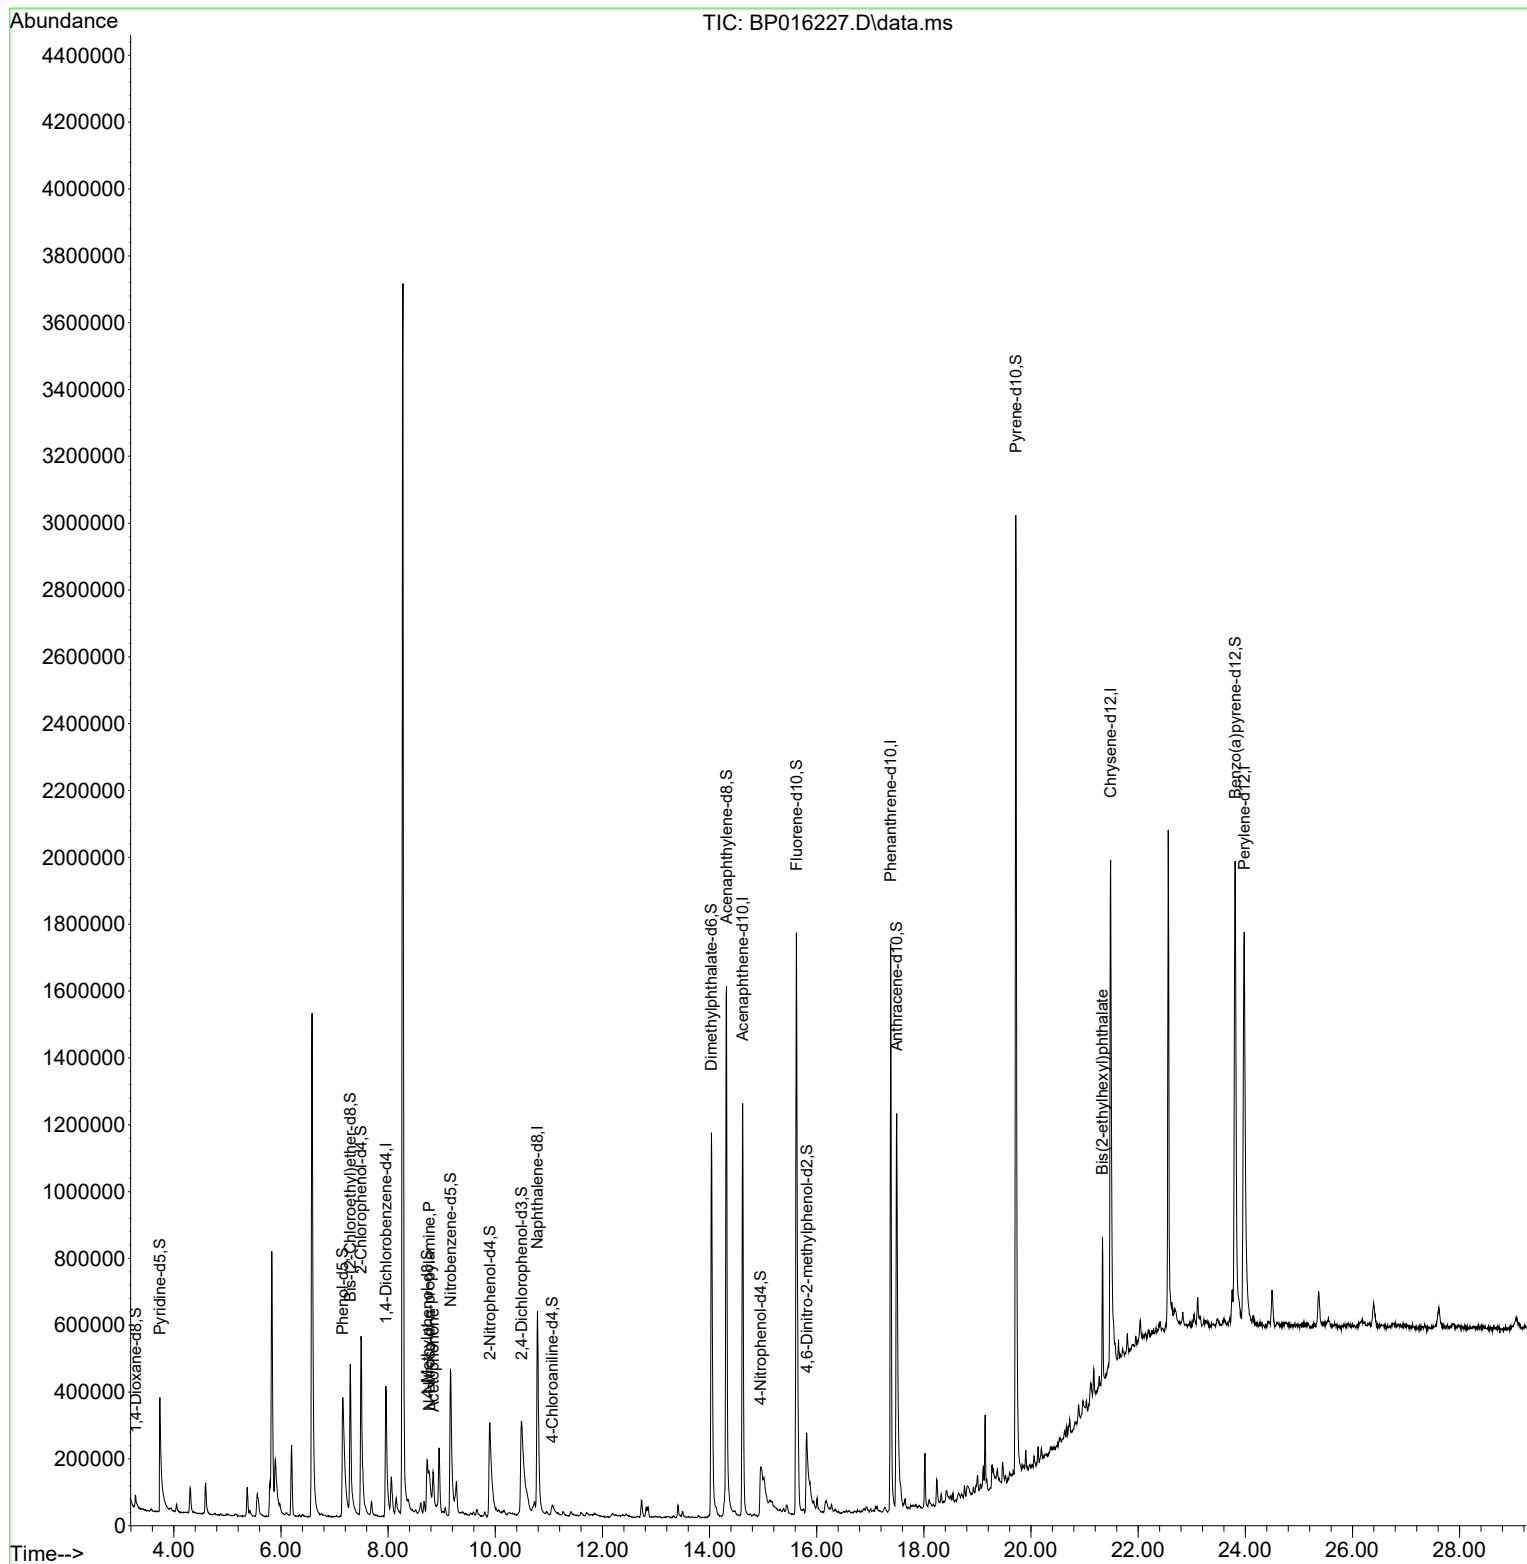


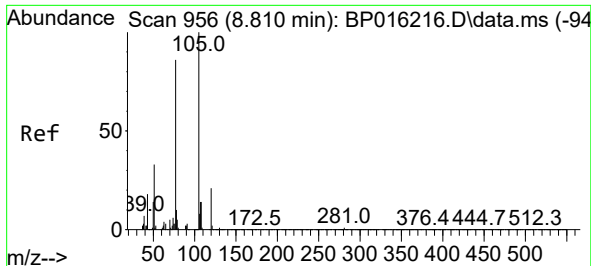

#16
Acetophenone
Concen: 2.713 ng/ul
RT: 8.845 min Scan# 949
Delta R.T. 0.023 min
Lab File: BP016227.D
Acq: 14 Jul 2023 15:40




Instrument :
BNA_P
ClientSampleId :
A46K9


Tgt Ion:105 Resp: 44342
Ion Ratio Lower Upper
105 100
77 83.7 70.2 105.2
51 36.0 26.3 39.5

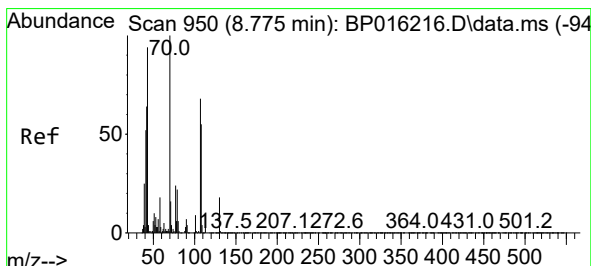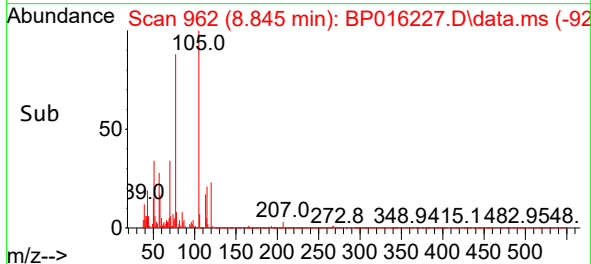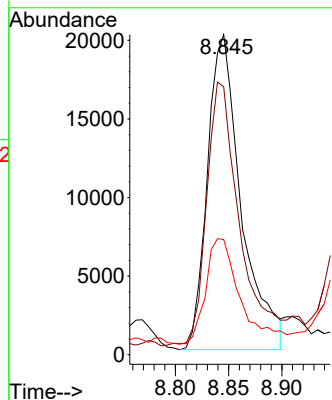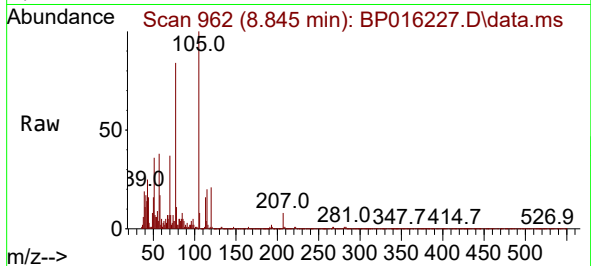

#17
N-Nitroso-di-n-propylamine
Concen: 2.477 ng/ul
RT: 8.769 min Scan# 949
Delta R.T. -0.012 min
Lab File: BP016227.D
Acq: 14 Jul 2023 15:40

Tgt Ion: 70 Resp: 21704
Ion Ratio Lower Upper
70 100
42 52.7 50.8 76.2
101 0.1 7.0 10.6#
130 0.1 13.3 19.9#

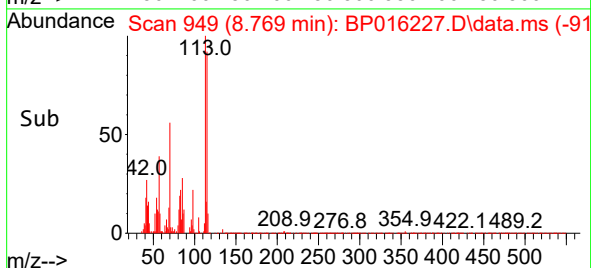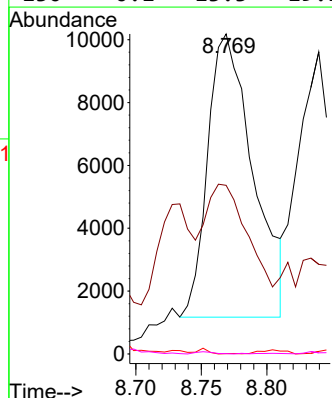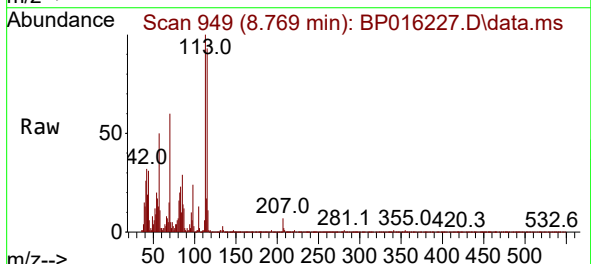

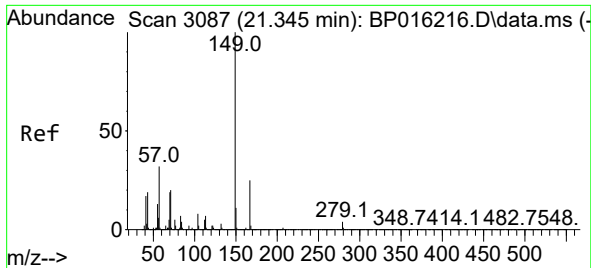

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.874 ng/ul
 RT: 21.333 min Scan# 3085
 Delta R.T. -0.006 min
 Lab File: BP016227.D
 Acq: 14 Jul 2023 15:40

Instrument :
 BNA_P
 ClientSampleId :
 A46K9

Tgt Ion:	149	Resp:	126180
Ion Ratio	Lower	Upper	
149	100		
167	26.7	21.0	31.4
279	3.8	3.0	4.6

