

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
 Data File : BP016236.D
 Acq On : 14 Jul 2023 20:48
 Operator : MA/JU
 Sample : 03457-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.793	99	103	108	rBV2	26004	56409	2.30%	0.272%
2	4.052	145	147	153	rVB6	7228	8664	0.35%	0.042%
3	5.710	427	429	433	rVB5	2866	2787	0.11%	0.013%
4	5.963	470	472	477	rVB6	2054	3090	0.13%	0.015%
5	7.257	687	692	693	rBV4	2137	2846	0.12%	0.014%
6	7.334	699	705	709	rBV2	52310	122622	5.00%	0.592%
7	7.646	749	758	760	rBV9	7555	18127	0.74%	0.088%
8	7.881	796	798	803	rVB6	2586	4199	0.17%	0.020%
9	7.999	809	818	819	rBV3	120641	253740	10.34%	1.225%
10	8.257	860	862	865	rVB4	2662	2970	0.12%	0.014%
11	8.287	865	867	870	rVB4	3139	3724	0.15%	0.018%
12	8.334	870	875	876	rBV5	2171	3368	0.14%	0.016%
13	8.857	954	964	965	rBV5	16887	33003	1.34%	0.159%
14	8.922	973	975	980	rVB6	4993	5376	0.22%	0.026%
15	9.040	994	995	999	rVB4	2796	2867	0.12%	0.014%
16	9.240	1020	1029	1050	rBV2	65406	375738	15.31%	1.814%
17	9.675	1098	1103	1105	rBV6	2039	3166	0.13%	0.015%
18	10.657	1266	1270	1271	rBV4	3627	4811	0.20%	0.023%
19	10.804	1287	1295	1318	rBV	306058	1126089	45.88%	5.436%
20	11.081	1334	1342	1359	rBV2	58433	273459	11.14%	1.320%
21	12.134	1520	1521	1526	rVB5	2929	3441	0.14%	0.017%
22	12.328	1550	1554	1555	rBV4	2458	2456	0.10%	0.012%
23	12.463	1571	1577	1580	rBV7	4186	9188	0.37%	0.044%
24	12.840	1637	1641	1644	rBV6	2136	2648	0.11%	0.013%
25	12.963	1659	1662	1664	rBV4	2278	2943	0.12%	0.014%
26	13.051	1674	1677	1680	rBV5	1908	2753	0.11%	0.013%
27	13.504	1747	1754	1765	rBV3	25531	66430	2.71%	0.321%
28	14.057	1840	1848	1867	rBV	255450	704671	28.71%	3.402%
29	14.322	1886	1893	1910	rBV	585319	1218393	49.64%	5.882%
30	14.622	1937	1944	1962	rBV	868962	1646900	67.09%	7.950%
31	14.998	2004	2008	2010	rBV5	2489	3740	0.15%	0.018%
32	15.310	2059	2061	2066	rVB6	2831	3541	0.14%	0.017%
33	15.369	2066	2071	2072	rBV5	2504	3988	0.16%	0.019%
34	15.392	2072	2075	2077	rBV4	2165	2632	0.11%	0.013%
35	15.469	2085	2088	2091	rBV5	1895	2576	0.10%	0.012%
36	15.522	2095	2097	2101	rVB5	3225	4334	0.18%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
 Data File : BP016236.D
 Acq On : 14 Jul 2023 20:48
 Operator : MA/JU
 Sample : 03457-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

37	15.634	2109	2116	2143	rBV	600907	1650753	67.25%	7.969%
38	15.875	2155	2157	2160	rBV4	2591	4037	0.16%	0.019%
39	16.033	2179	2184	2197	rBV	32955	97079	3.95%	0.469%
40	16.263	2219	2223	2224	rBV4	2826	3204	0.13%	0.015%
41	16.433	2248	2252	2256	rBV7	3903	6977	0.28%	0.034%
42	16.569	2271	2275	2280	rVB5	8900	13072	0.53%	0.063%
43	16.769	2307	2309	2310	rBV2	3362	3119	0.13%	0.015%
44	17.063	2354	2359	2361	rBV5	4251	6181	0.25%	0.030%
45	17.198	2379	2382	2383	rBV3	3794	3518	0.14%	0.017%
46	17.392	2408	2415	2428	rBV	1024804	1971417	80.31%	9.517%
47	17.504	2428	2434	2457	rVB	587015	1704923	69.46%	8.230%
48	18.257	2559	2562	2566	rBV6	12733	24060	0.98%	0.116%
49	18.327	2571	2574	2578	rVB2	10552	16049	0.65%	0.077%
50	19.722	2806	2811	2832	rBV	1094570	2298962	93.66%	11.098%
51	21.486	3106	3111	3129	rBV	1140854	2454674	100.00%	11.849%
52	23.810	3500	3506	3525	rVB2	868273	2152411	87.69%	10.390%
53	23.974	3528	3534	3553	rVB	811126	2317407	94.41%	11.187%




Sum of corrected areas: 20715532

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016236.D
Acq On : 14 Jul 2023 20:48
Operator : MA/JU
Sample : 03457-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C50

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

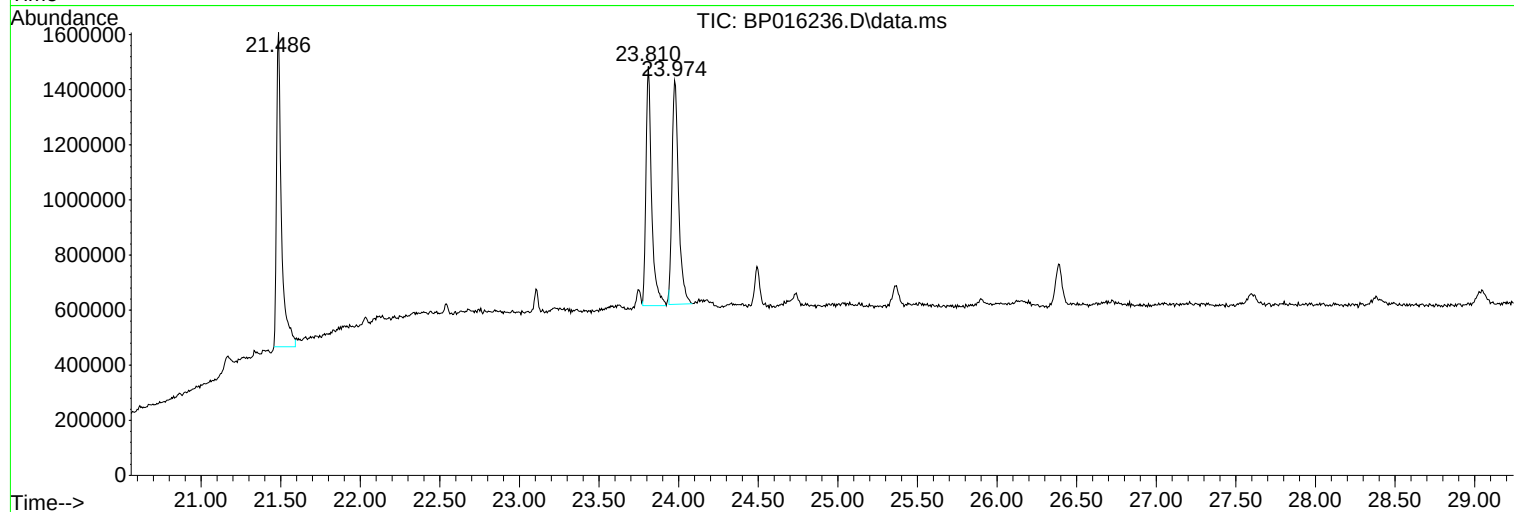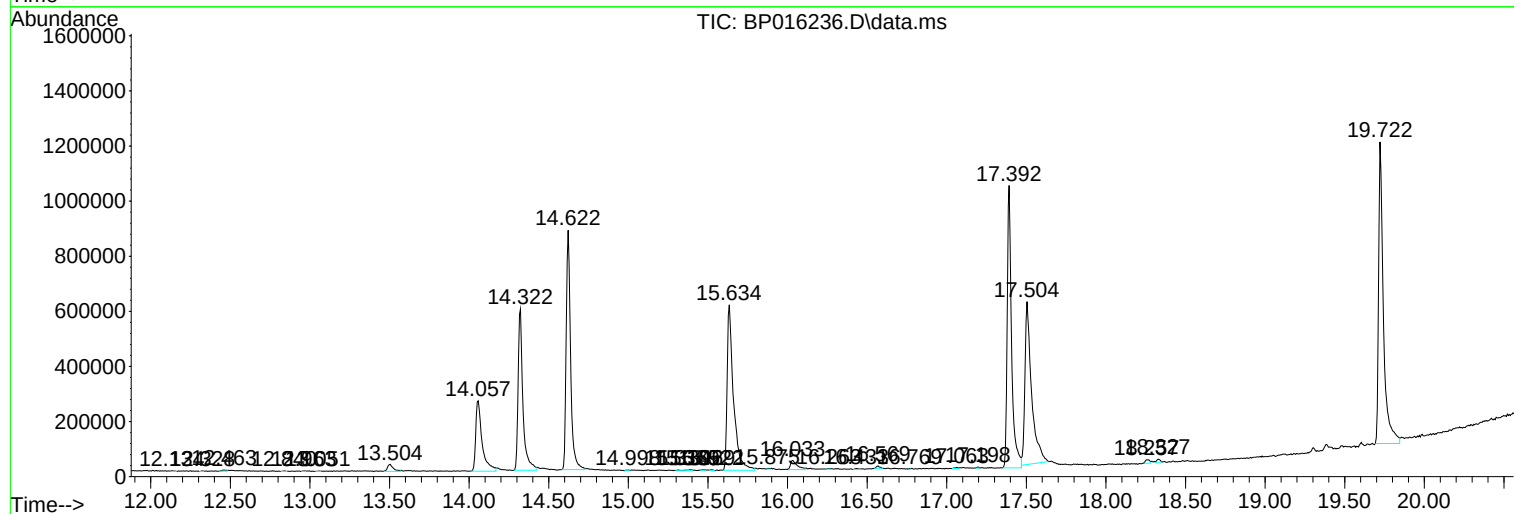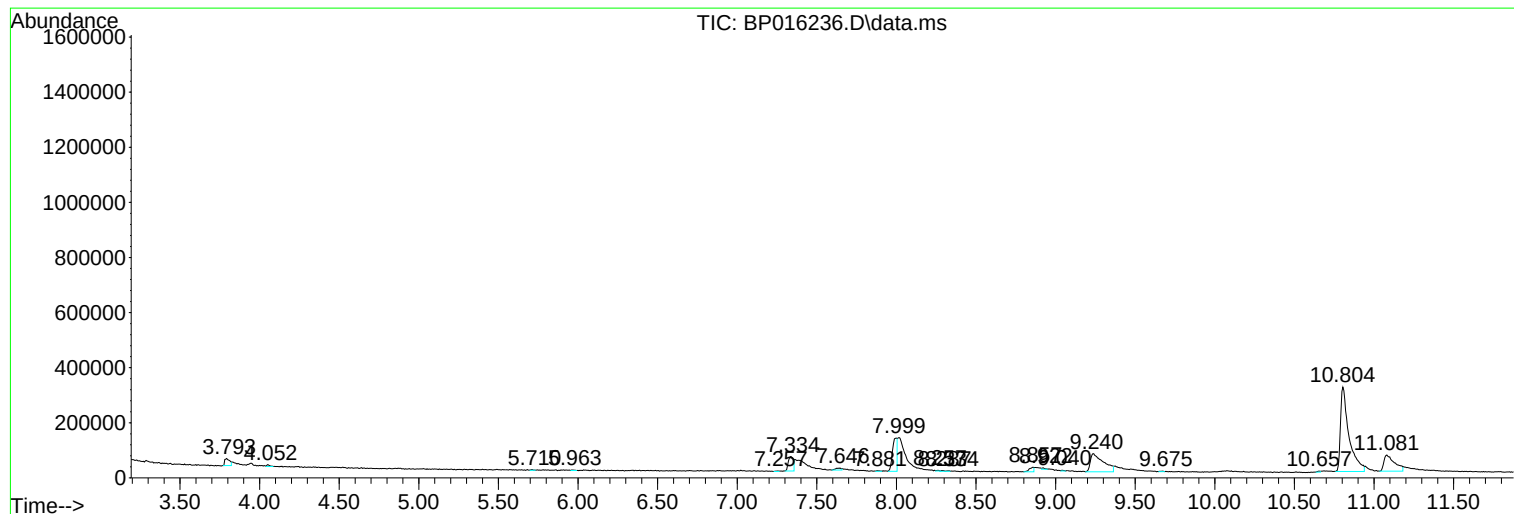

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016236.D
Acq On : 14 Jul 2023 20:48
Operator : MA/JU
Sample : 03457-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C50

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016236.D
Acq On : 14 Jul 2023 20:48
Operator : MA/JU
Sample : 03457-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C50

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc