

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
 Data File : BP016242.D
 Acq On : 15 Jul 2023 00:13
 Operator : MA/JU
 Sample : PB153903BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	13	16	25	rVB	44444	66265	1.22%	0.124%
2	3.734	91	93	113	rBV	430484	966621	17.73%	1.804%
3	4.046	144	146	152	rVB5	9293	13372	0.25%	0.025%
4	7.158	668	675	693	rBV2	350297	1184390	21.73%	2.210%
5	7.293	693	698	725	rVV	393719	1005732	18.45%	1.877%
6	7.493	726	732	754	rVV	492256	1176643	21.58%	2.195%
7	7.963	803	812	836	rBV	411927	1132555	20.78%	2.113%
8	8.710	932	939	971	rBV	462334	1562750	28.67%	2.916%
9	9.163	1009	1016	1047	rBV	433327	1228042	22.53%	2.291%
10	9.899	1133	1141	1171	rBV	290017	1041498	19.11%	1.943%
11	10.475	1232	1239	1275	rBV	270594	1400968	25.70%	2.614%
12	10.781	1284	1291	1309	rVB	799526	1765432	32.39%	3.294%
13	10.987	1319	1326	1361	rBV	301958	1416551	25.99%	2.643%
14	12.457	1571	1576	1580	rBV6	4859	10274	0.19%	0.019%
15	13.498	1745	1753	1760	rBV4	17391	36448	0.67%	0.068%
16	14.034	1837	1844	1872	rBV	1139827	2483332	45.56%	4.633%
17	14.310	1884	1891	1923	rBV2	1676741	2867071	52.59%	5.349%
18	14.616	1936	1943	1957	rBV	1485678	2482942	45.55%	4.633%
19	14.969	1995	2003	2029	rBV4	122803	816676	14.98%	1.524%
20	15.622	2106	2114	2141	rBV	1674444	3741302	68.63%	6.981%
21	15.816	2141	2147	2178	rBV	197129	854633	15.68%	1.595%
22	17.051	2354	2357	2361	rBV6	4614	6414	0.12%	0.012%
23	17.181	2376	2379	2384	rVB6	5341	8145	0.15%	0.015%
24	17.375	2406	2412	2424	rBV	2050182	3211728	58.92%	5.992%
25	17.486	2424	2431	2459	rVB2	1799964	4218207	77.38%	7.870%
26	19.298	2735	2739	2745	rBV3	35025	49897	0.92%	0.093%
27	19.380	2749	2753	2757	rBV	28618	47178	0.87%	0.088%
28	19.716	2804	2810	2834	rBV	2686679	5379746	98.69%	10.038%
29	21.480	3105	3110	3130	rBV	1865980	4002624	73.43%	7.468%
30	23.804	3498	3505	3518	rVB2	2444939	5451255	100.00%	10.171%
31	23.974	3526	3534	3551	rBV	1310202	3967460	72.78%	7.403%




Sum of corrected areas: 53596151

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016242.D
Acq On : 15 Jul 2023 00:13
Operator : MA/JU
Sample : PB153903BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

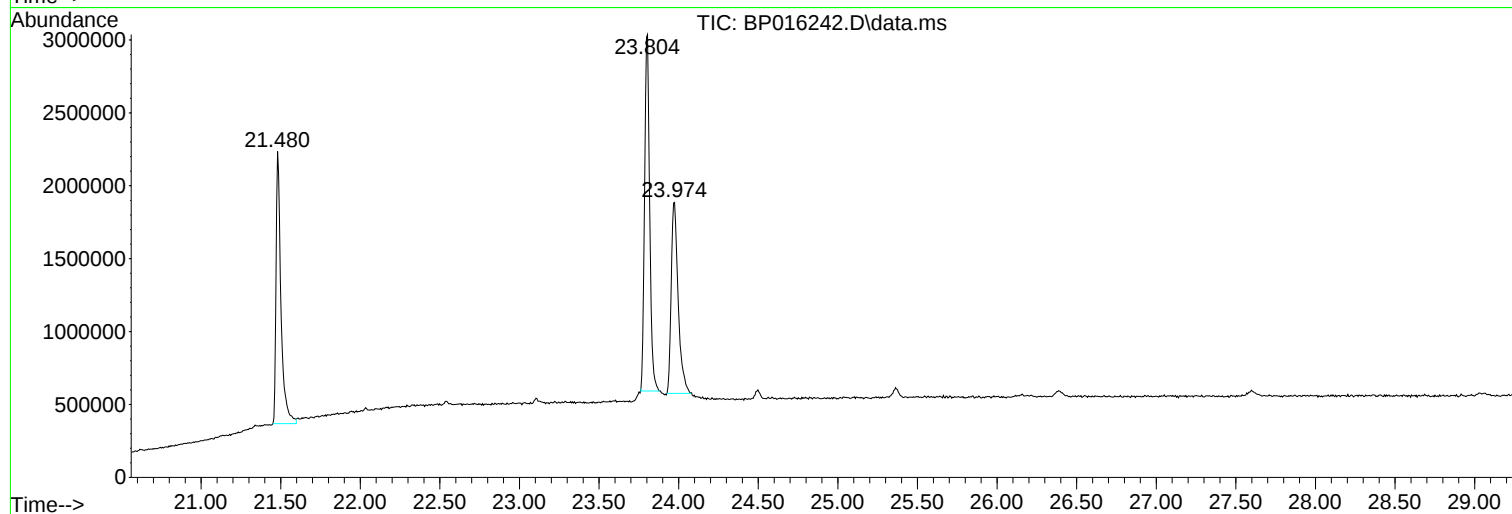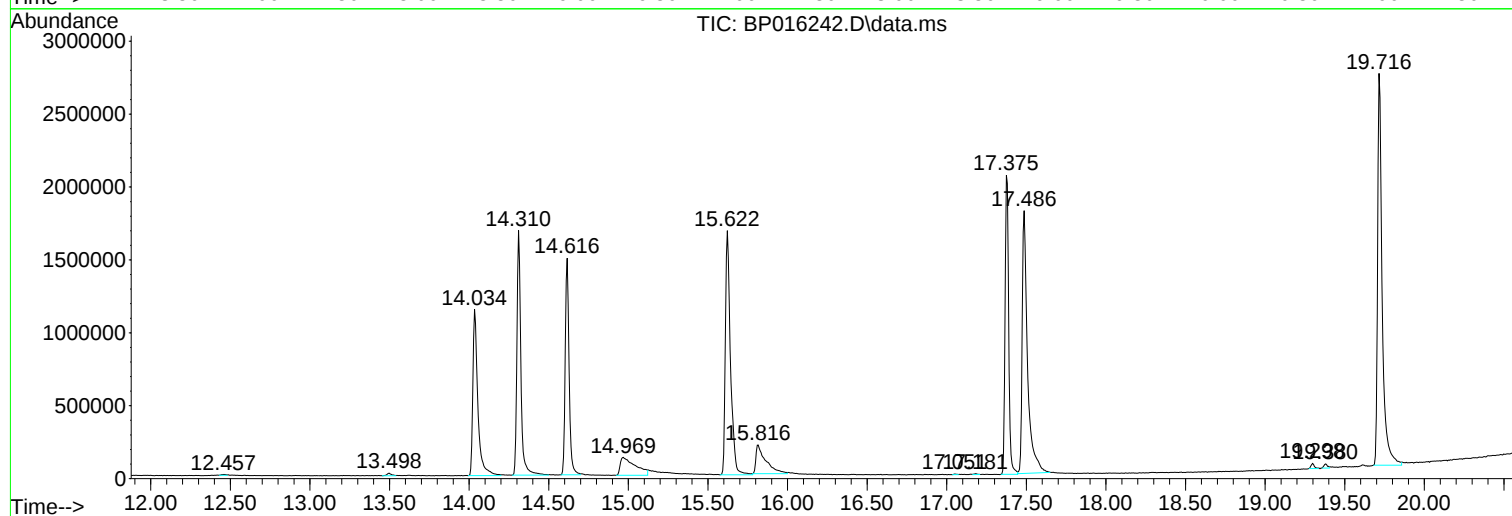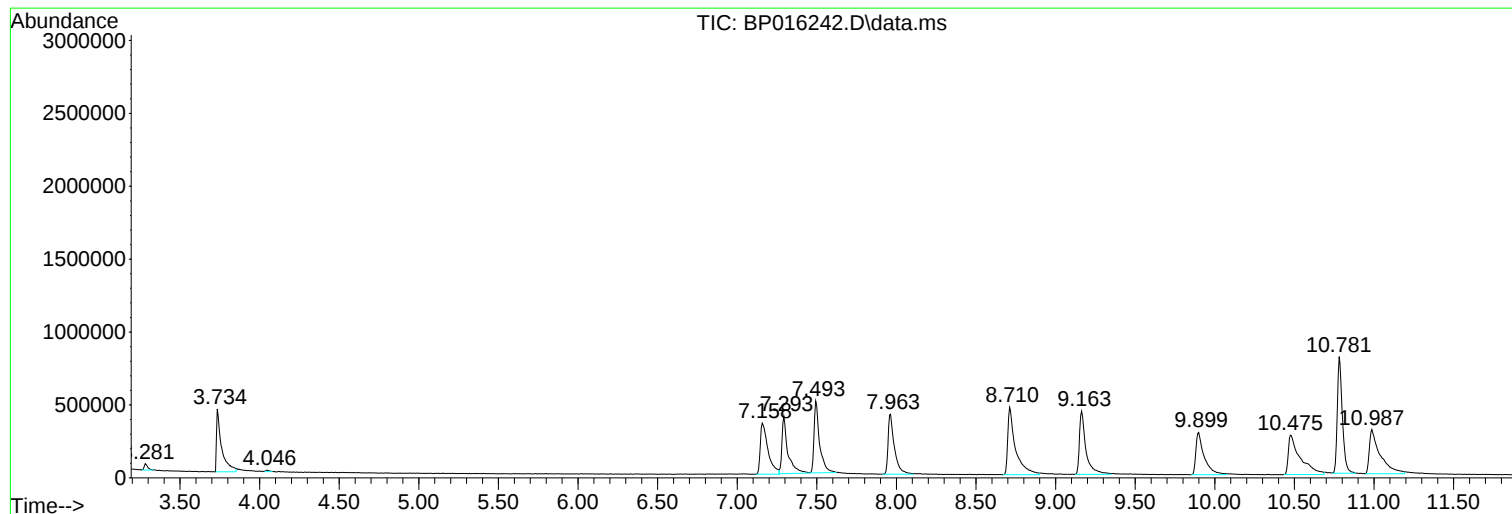

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016242.D
Acq On : 15 Jul 2023 00:13
Operator : MA/JU
Sample : PB153903BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071423\
Data File : BP016242.D
Acq On : 15 Jul 2023 00:13
Operator : MA/JU
Sample : PB153903BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------