
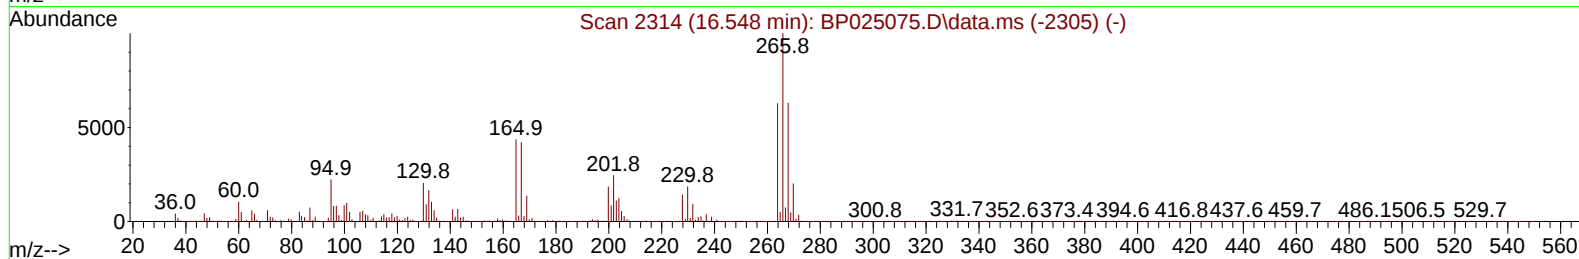
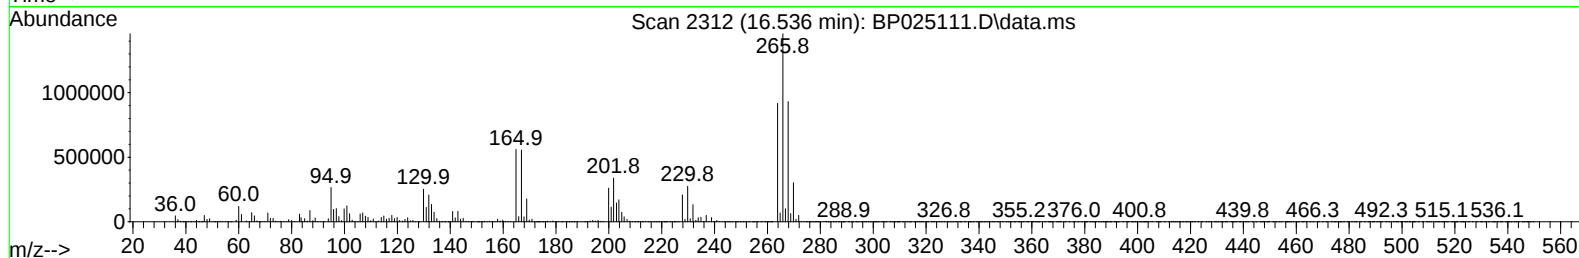


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025111.D
Acq On : 14 Jul 2025 08:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 11:12:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

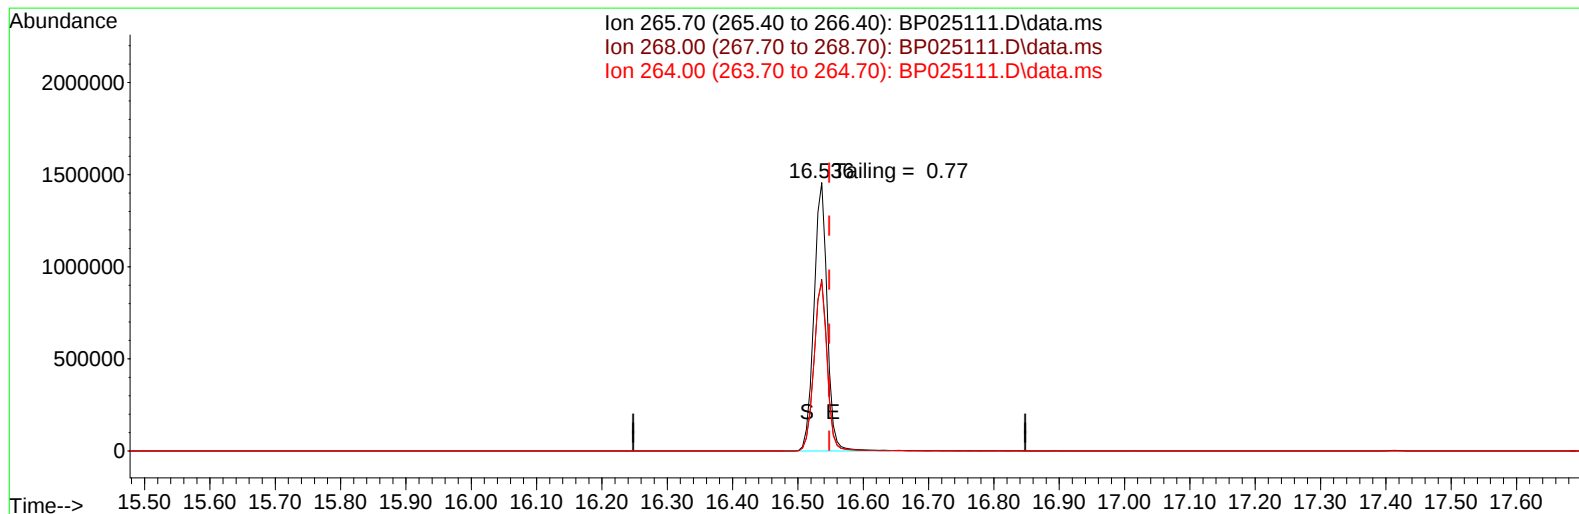

TIC: BP025111.D\data.ms

(70) Pentachlorophenol (C)




16.536min (-0.012) 861221.03 ng

response 2052664

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.89
264.00	62.70	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025111.D
Acq On : 14 Jul 2025 08:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 11:12:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

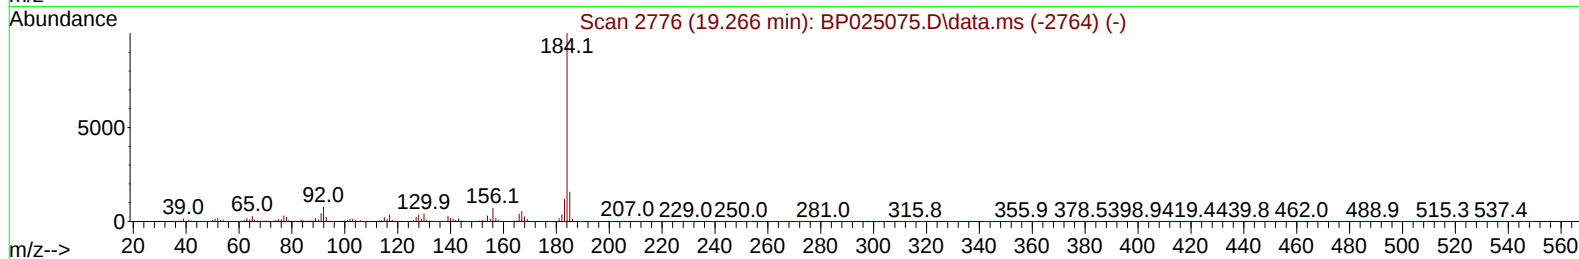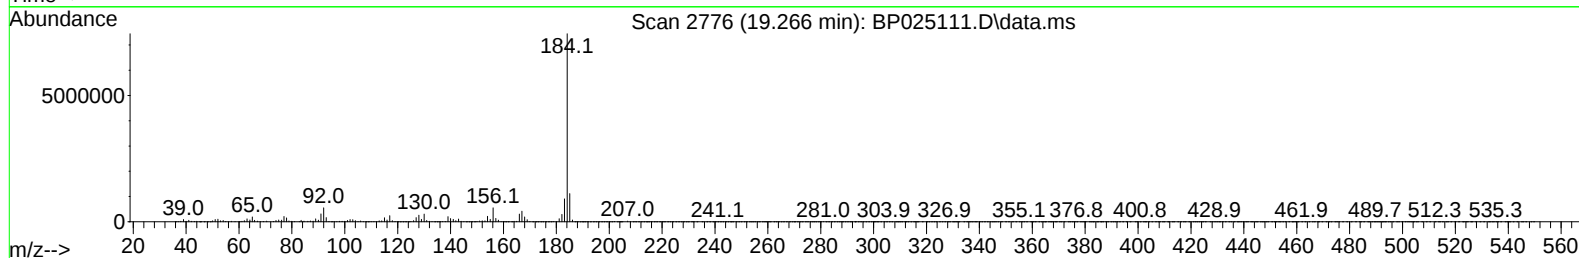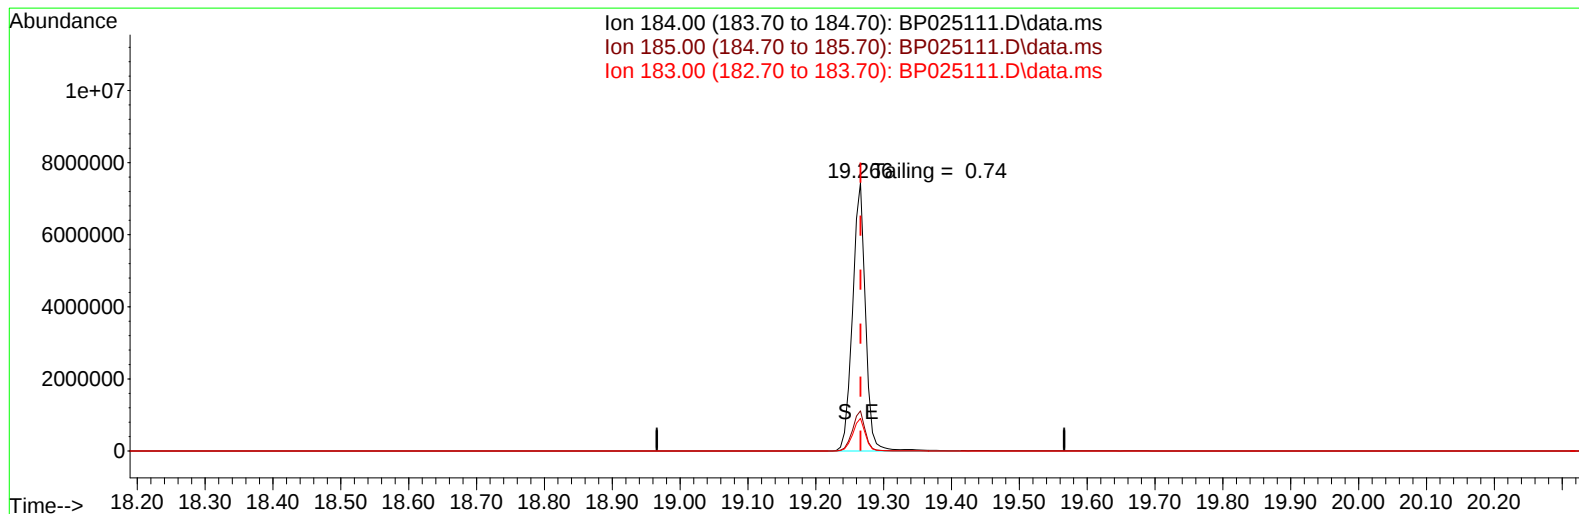

TIC: BP025111.D\data.ms

(77) Benzidine**19.266min (-0.000) 3130.07 ng****response 9756838**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.97
183.00	11.80	12.18
0.00	0.00	0.00