
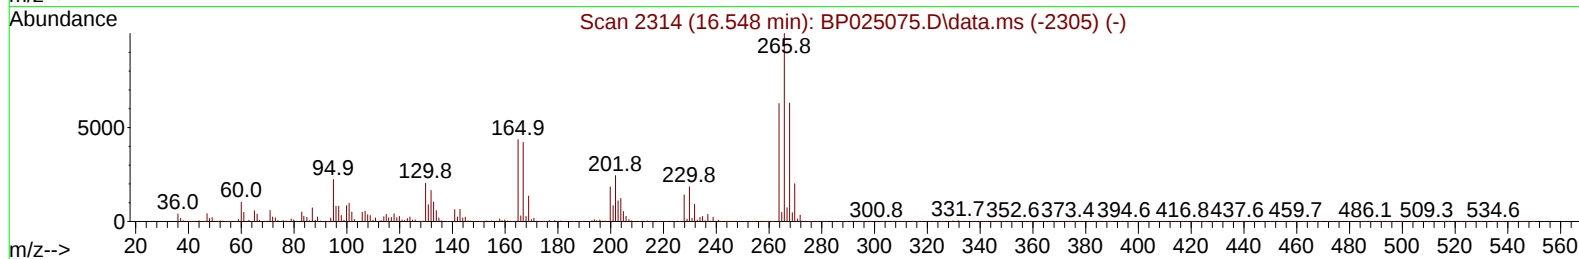
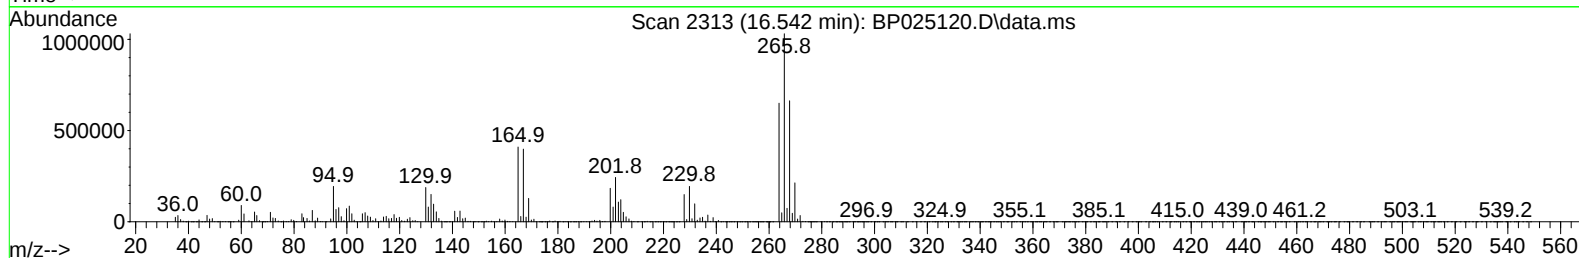


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025120.D
Acq On : 14 Jul 2025 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 15:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

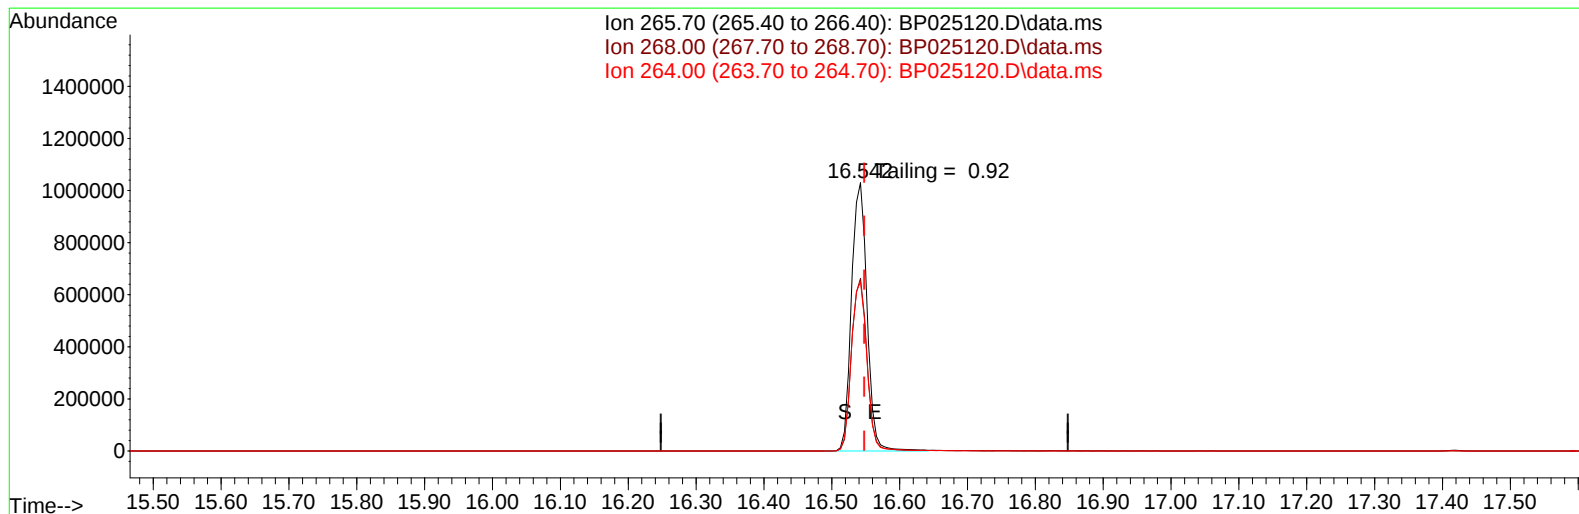

TIC: BP025120.D\data.ms

(70) Pentachlorophenol (C)




16.542min (-0.006) 5398504.81 ng

response 1596966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.31
264.00	62.70	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025120.D
Acq On : 14 Jul 2025 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 15:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

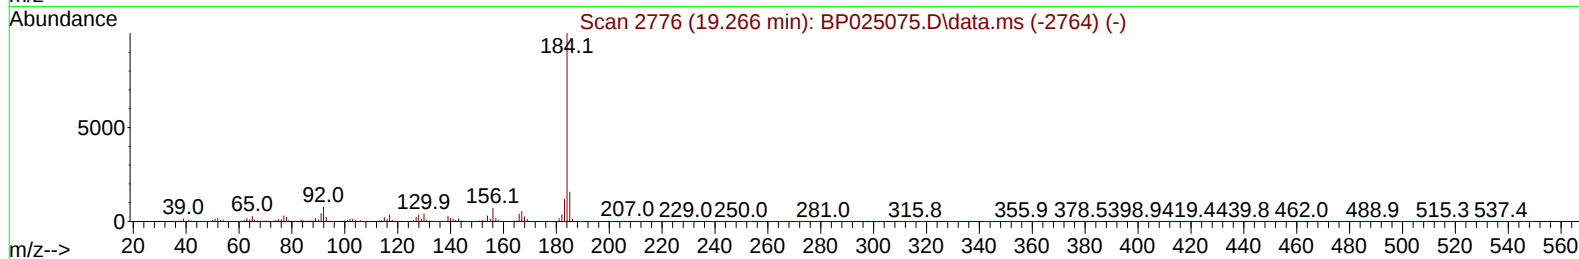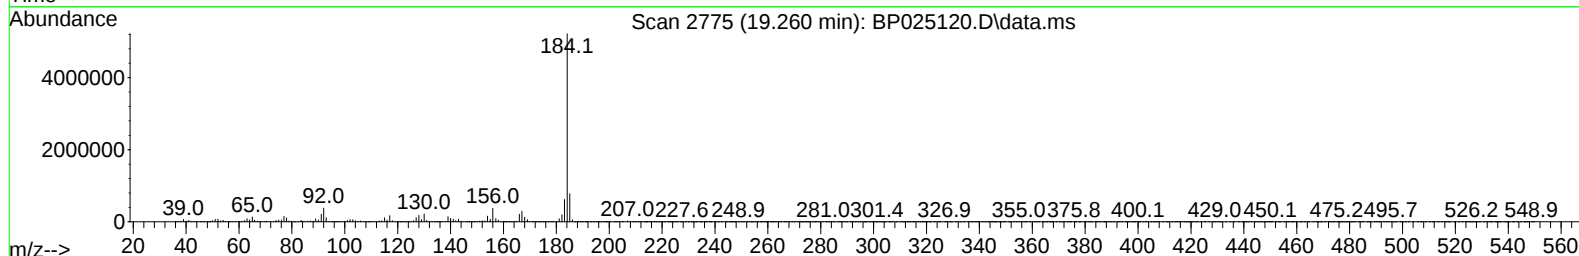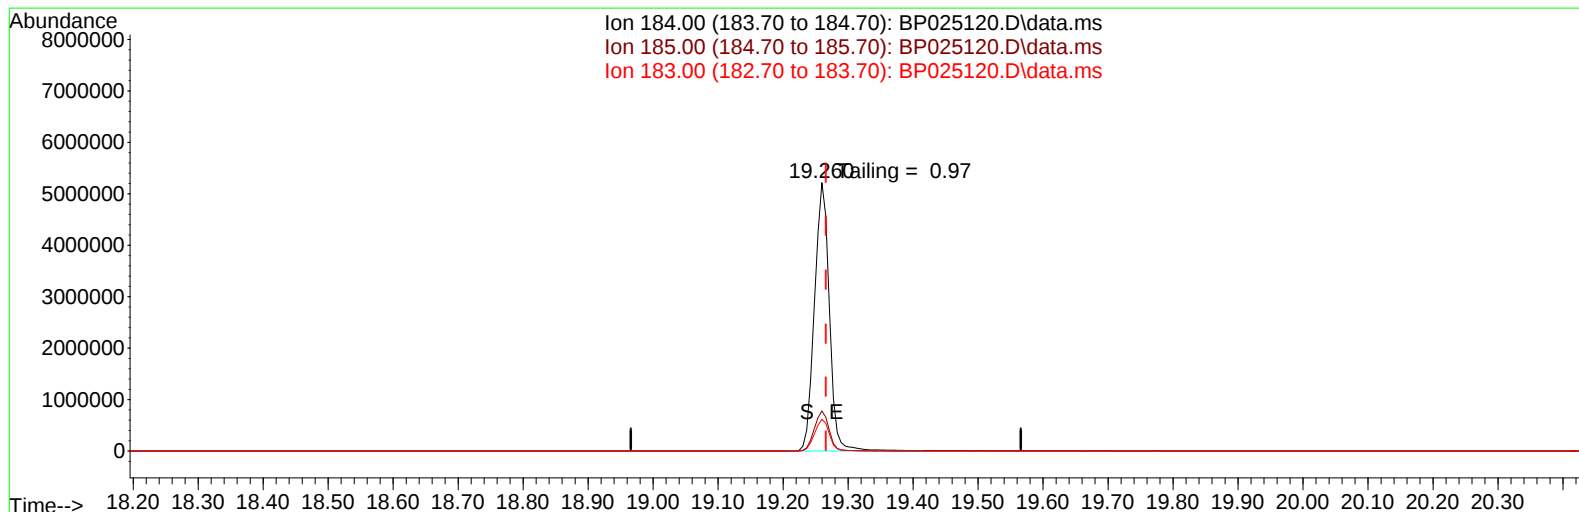

TIC: BP025120.D\data.ms

(77) Benzidine

19.260min (-0.006) 5818741.59 ng m

response 8324135

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.90
183.00	11.80	11.82
0.00	0.00	0.00