


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025111.D
Acq On : 14 Jul 2025 08:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 29 08:52:24 2022

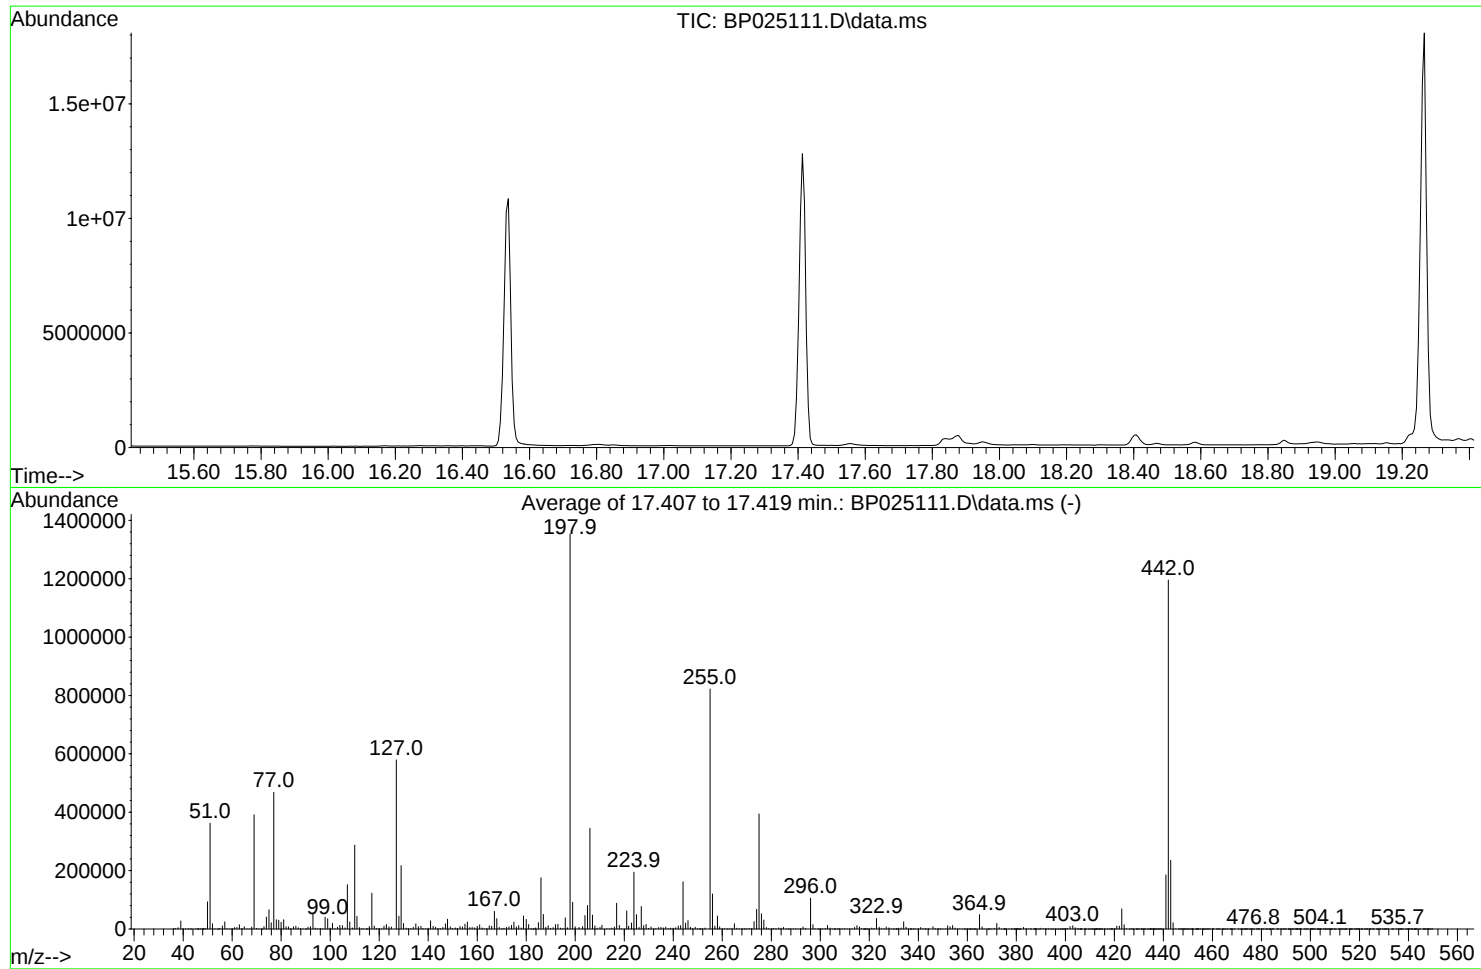




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	6618	PASS
69	69	100	100	100.0	391570	PASS
70	69	0.00	2	0.5	2085	PASS
197	198	0.00	2	0.3	4237	PASS
198	198	100	100	100.0	1352669	PASS
199	198	5	9	6.8	91451	PASS
365	198	1	100	3.6	49349	PASS
441	443	0.01	150	78.6	185024	PASS
442	442	100	100	100.0	1195776	PASS
443	442	15	24	19.7	235369	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025111.D
Acq On : 14 Jul 2025 08:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 14 11:12:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

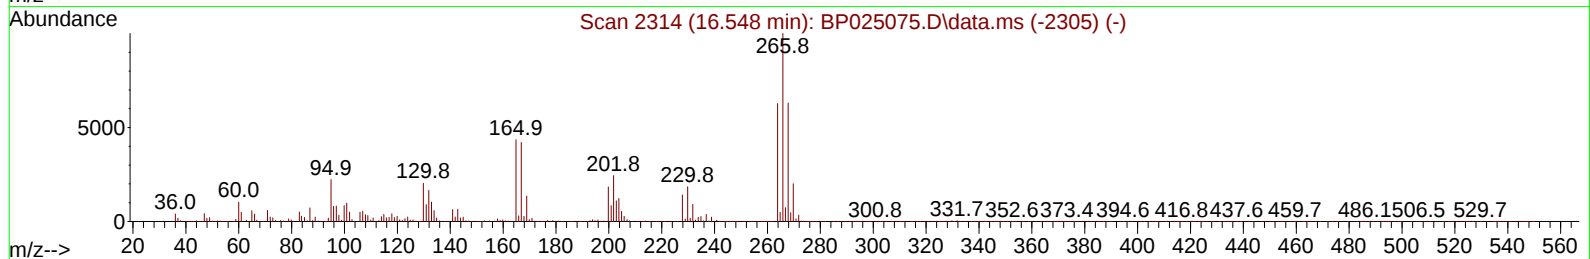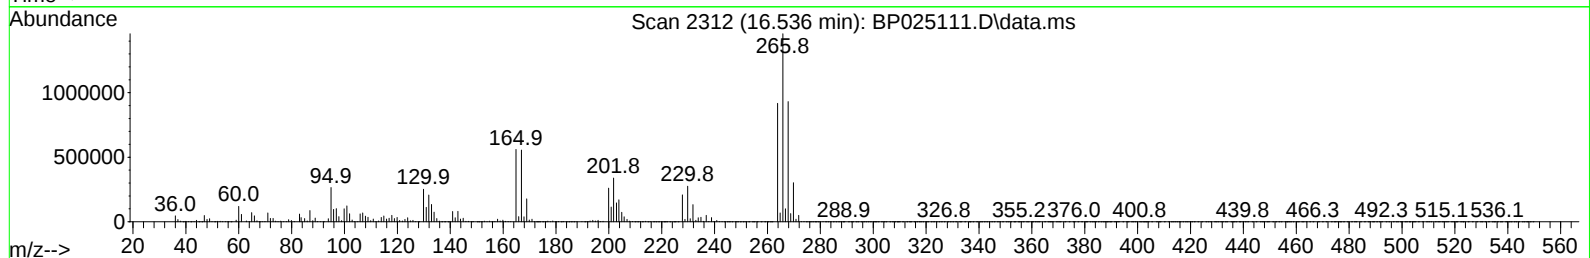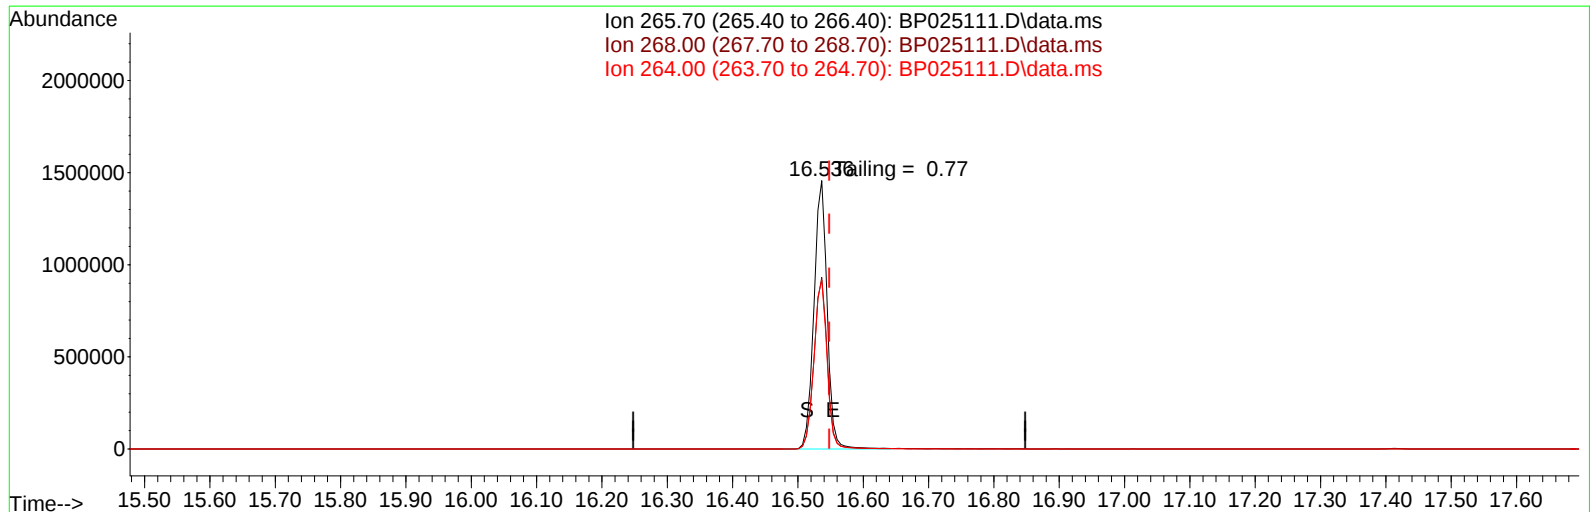

TIC: BP025111.D\data.ms

(70) Pentachlorophenol (C)

16.536min (-0.012) 861221.03 ng




response 2052664

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.89
264.00	62.70	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025111.D
Acq On : 14 Jul 2025 08:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 14 11:12:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

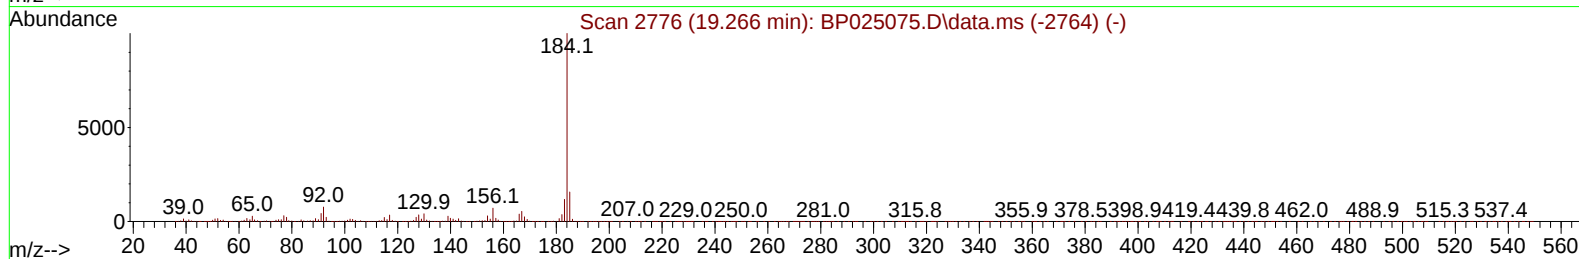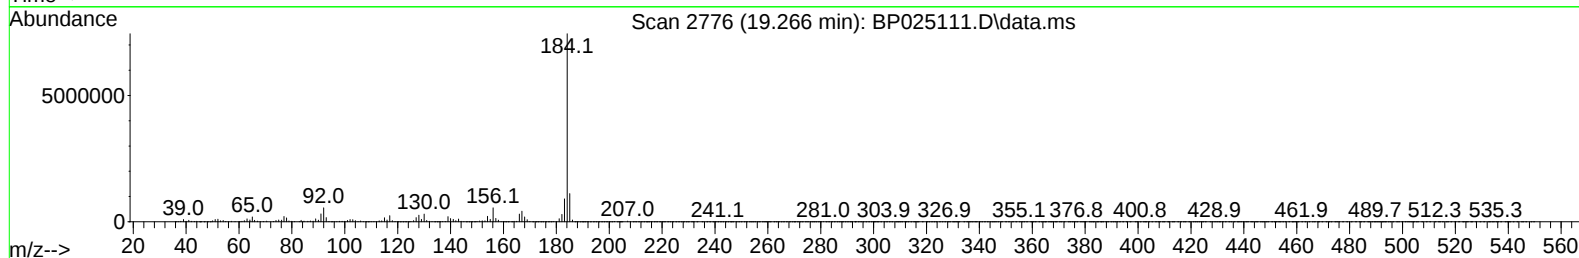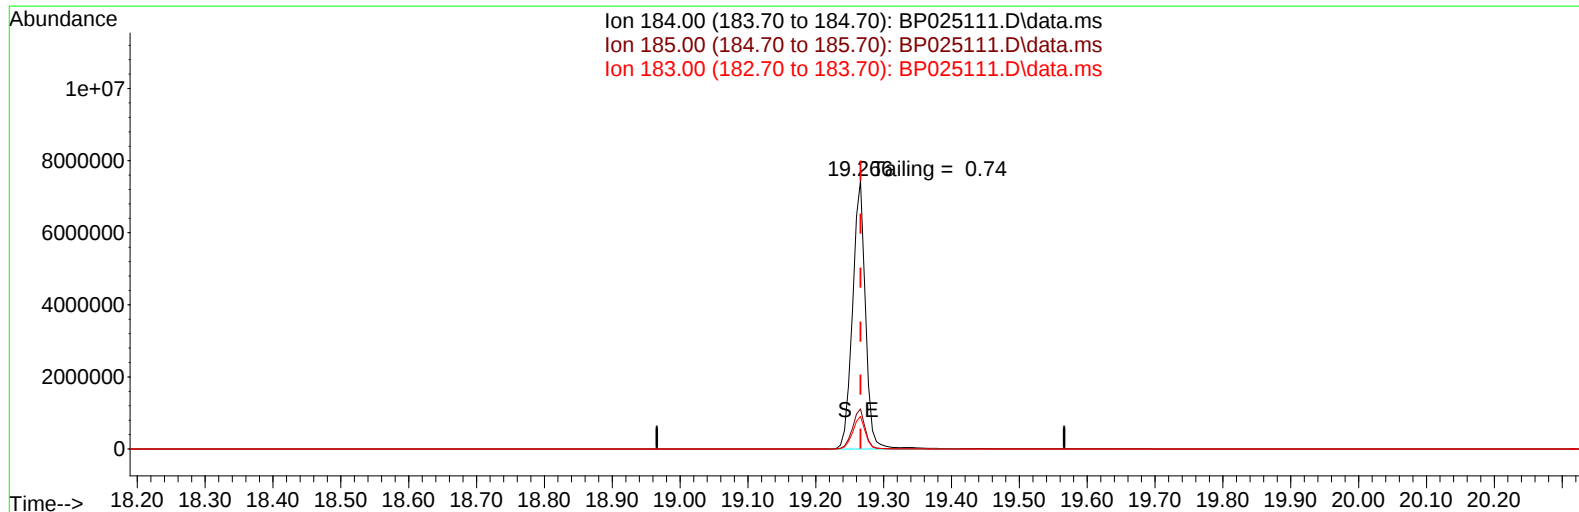

TIC: BP025111.D\data.ms

(77) Benzidine

19.266min (-0.000) 3130.07 ng

response 9756838

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.97
183.00	11.80	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2025	BNA_P	<u>BP025111.D</u>
Compound Name	Response	Retention Time
DDT	5001733	20.577
DDD	82513	20.101
DDE	1069	19.219
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
83582	5085315	1.64

Instrument :
BNA_P
ClientSampleId :
DFTPP