


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025120.D
Acq On : 14 Jul 2025 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 29 08:52:24 2022

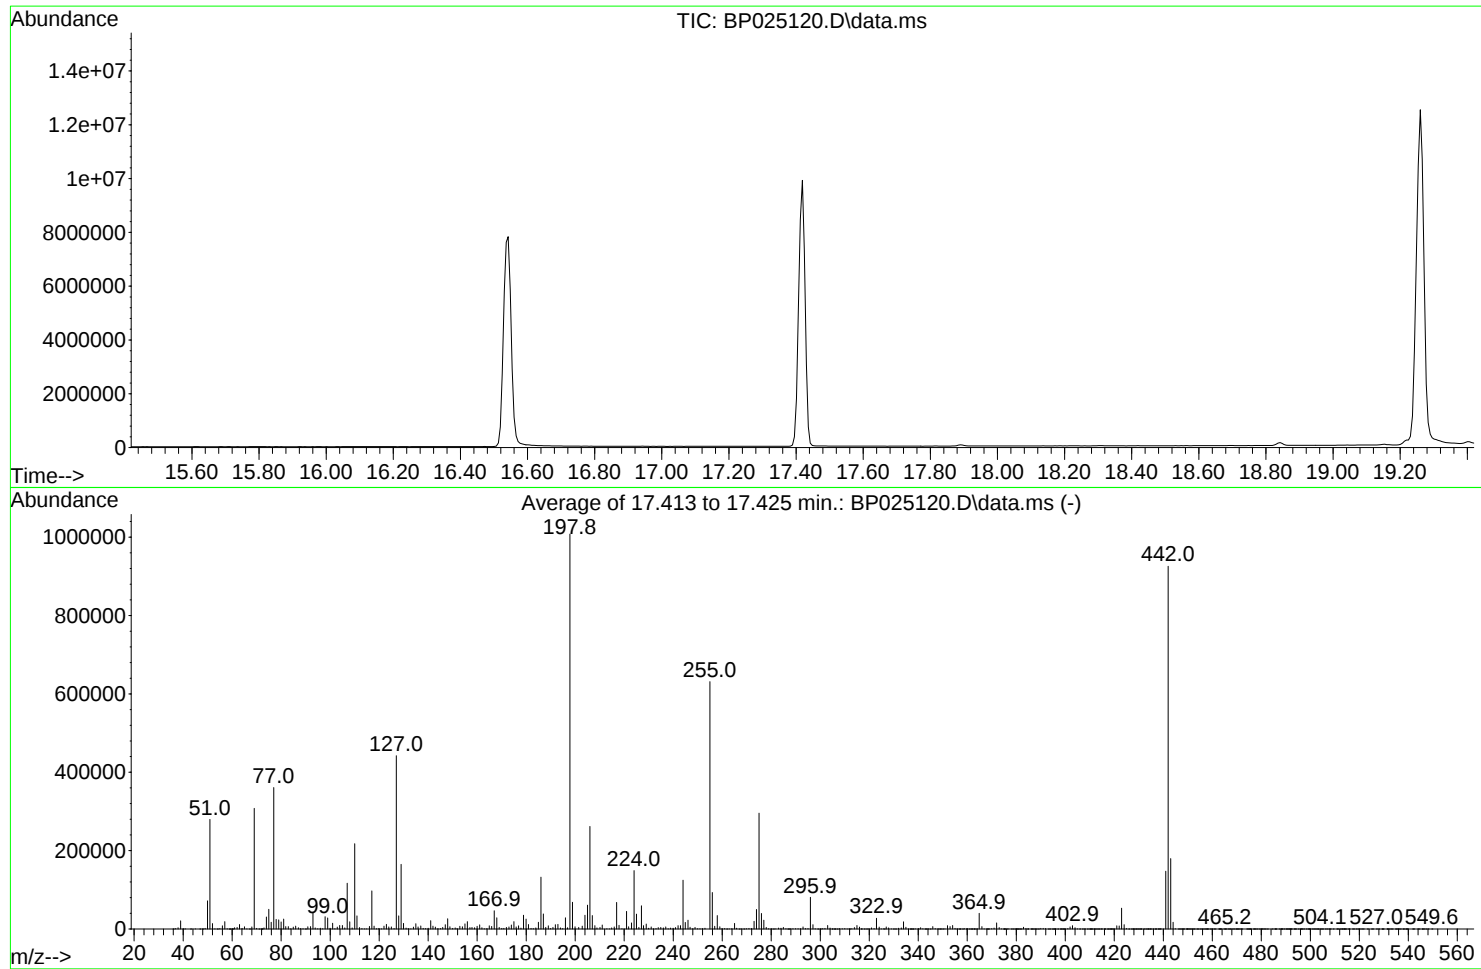




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2453

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	5156	PASS
69	69	100	100	100.0	307764	PASS
70	69	0.00	2	0.5	1628	PASS
197	198	0.00	2	0.3	3222	PASS
198	198	100	100	100.0	1007639	PASS
199	198	5	9	6.8	68264	PASS
365	198	1	100	4.0	39878	PASS
441	443	0.01	150	82.1	147567	PASS
442	442	100	100	100.0	925653	PASS
443	442	15	24	19.4	179733	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025120.D
Acq On : 14 Jul 2025 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 14 15:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

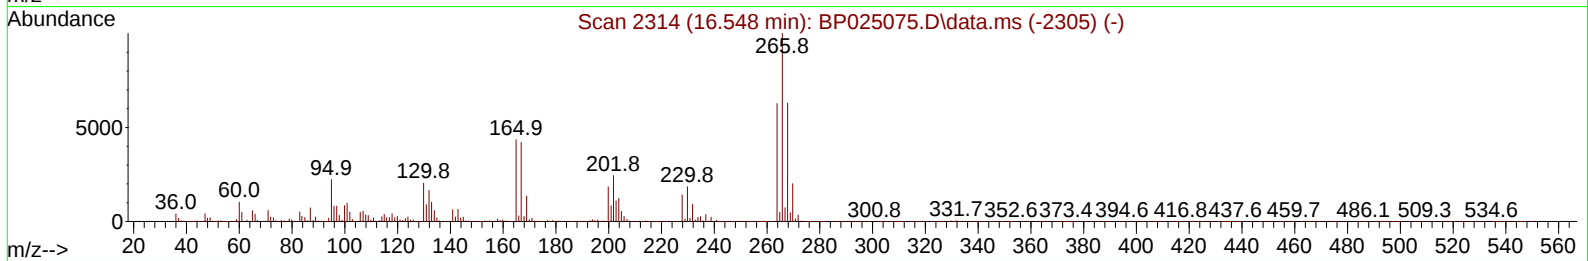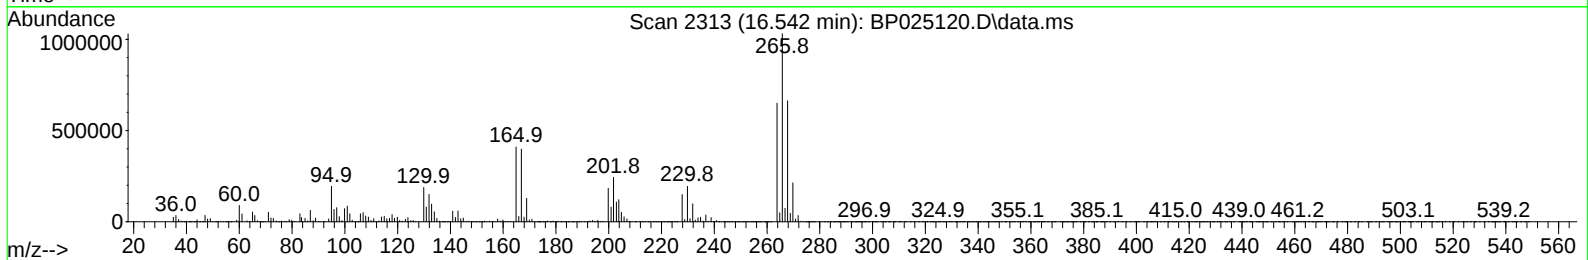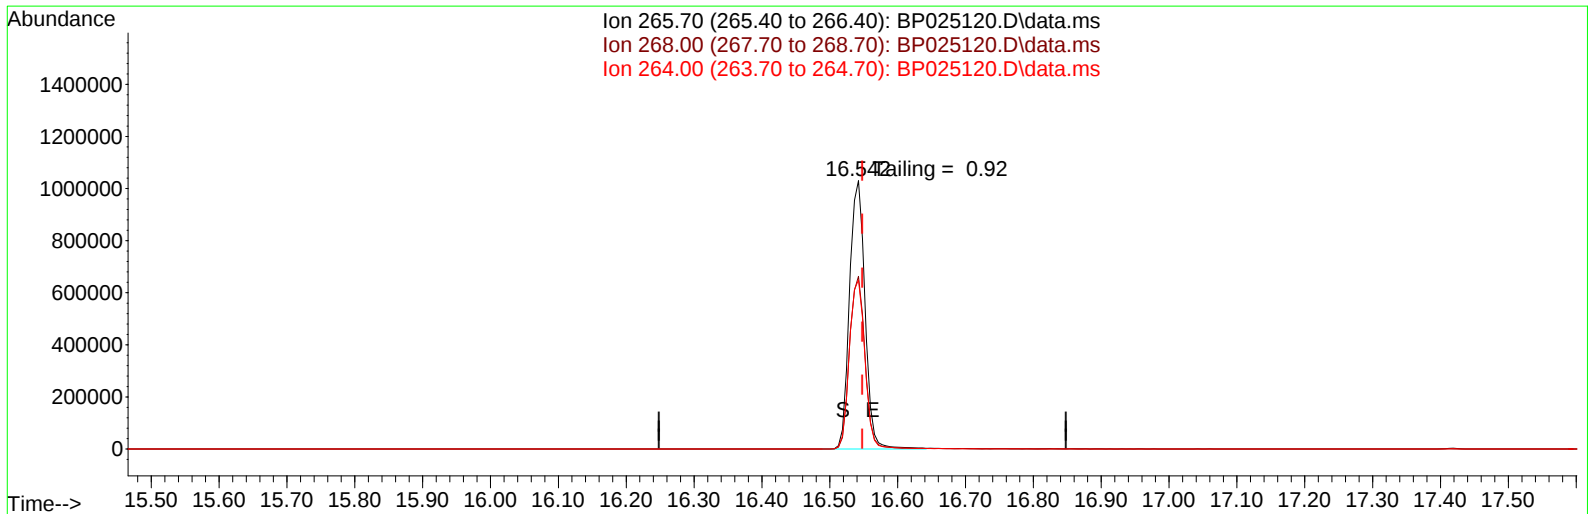

TIC: BP025120.D\data.ms

(70) Pentachlorophenol (C)

16.542min (-0.006) 5398504.81 ng




response 1596966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.31
264.00	62.70	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071425\
Data File : BP025120.D
Acq On : 14 Jul 2025 14:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 14 15:23:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

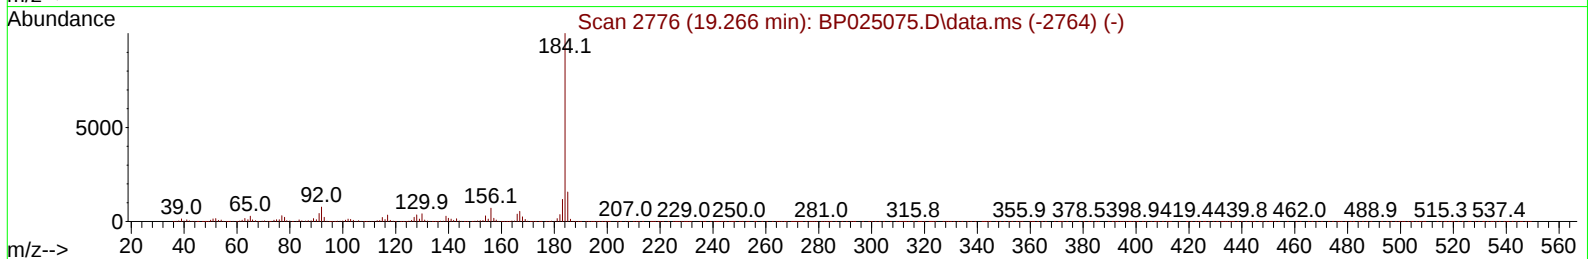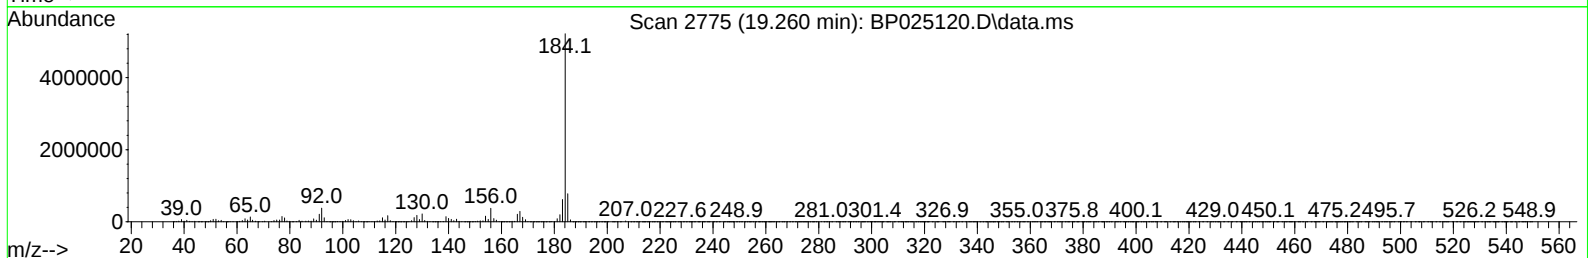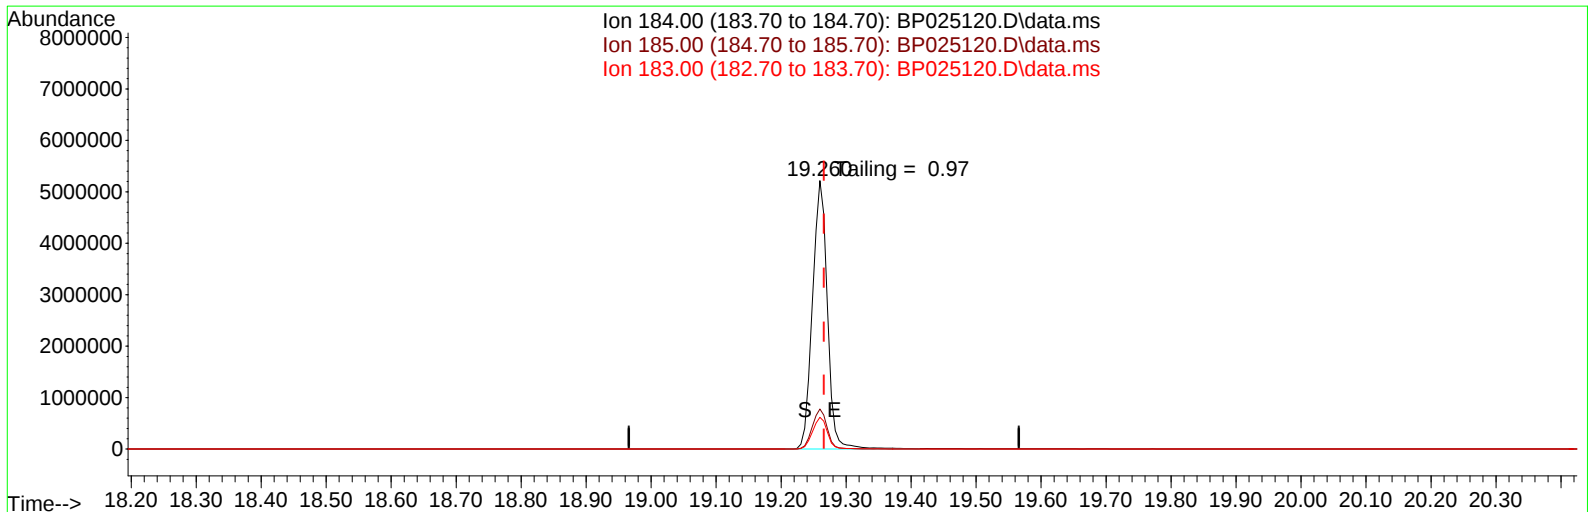

TIC: BP025120.D\data.ms

(77) Benzidine

19.260min (-0.006) 5818741.59 ng m

response 8324135

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.90
183.00	11.80	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2025	BNA_P	<u>BP025120.D</u>
Compound Name	Response	Retention Time
DDT	3857757	20.571
DDD	70556	20.107
DDE	3094	19.577
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
73650	3931407	1.87

Instrument :
BNA_P
ClientSampleId :
DFTPP