
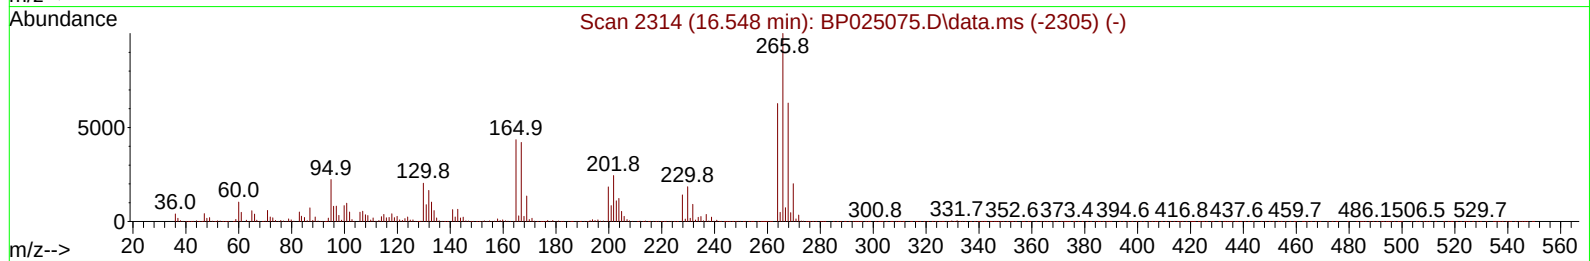
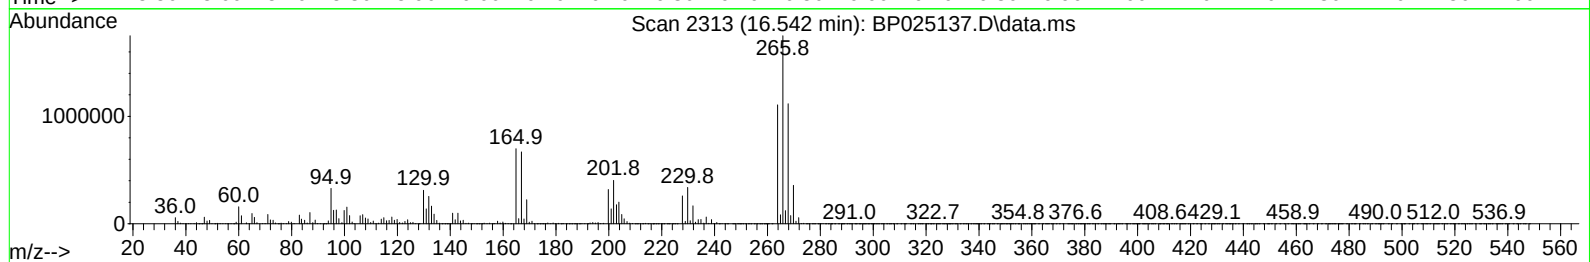


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071525\
Data File : BP025137.D
Acq On : 15 Jul 2025 08:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 11:52:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

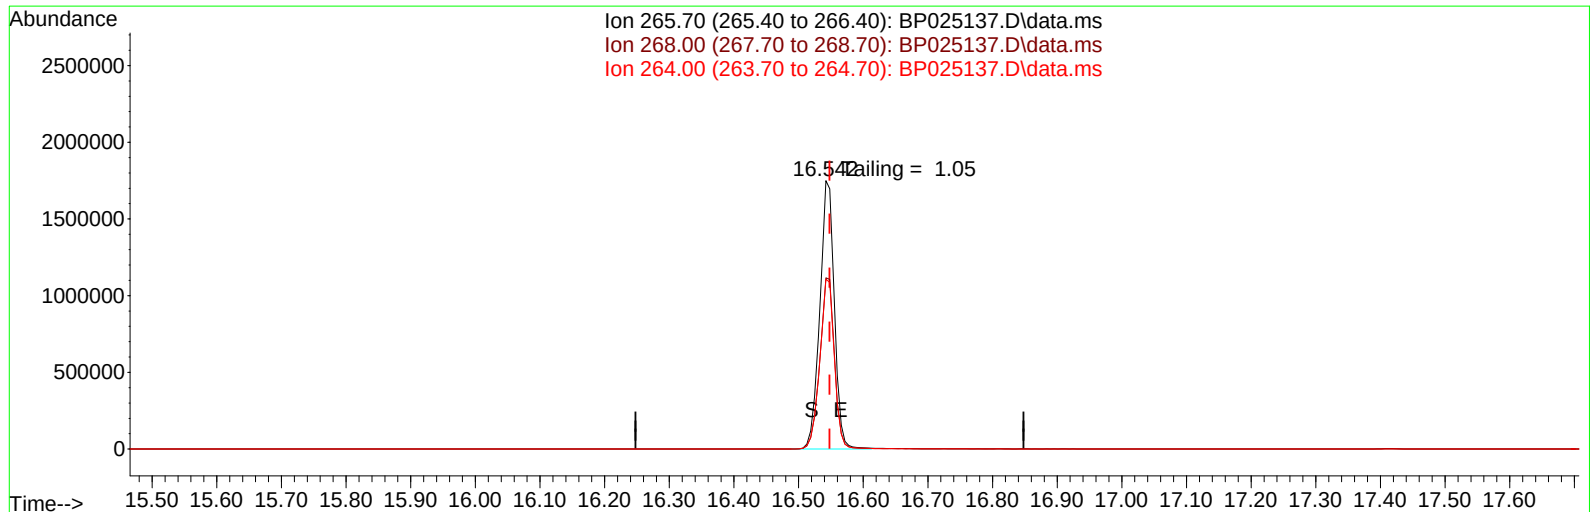

TIC: BP025137.D\data.ms

(70) Pentachlorophenol (C)




16.542min (-0.006) 102240.67 ng

response 2751382

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.81
264.00	62.70	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071525\
Data File : BP025137.D
Acq On : 15 Jul 2025 08:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 11:52:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

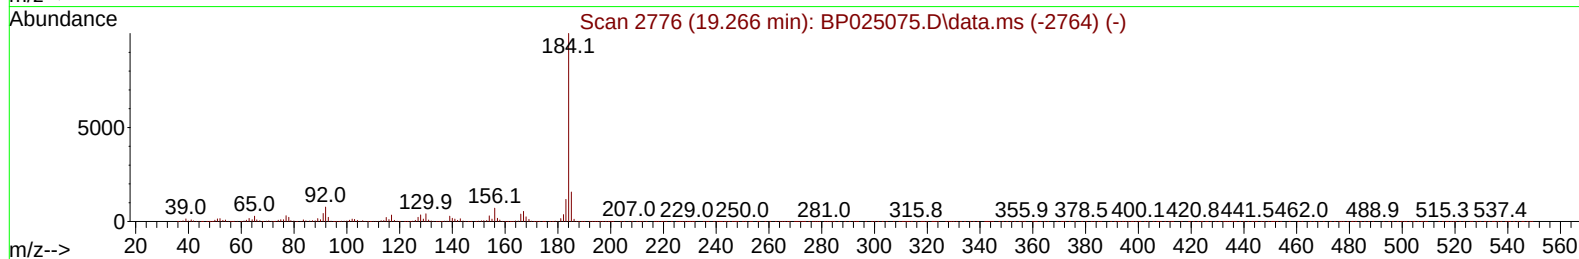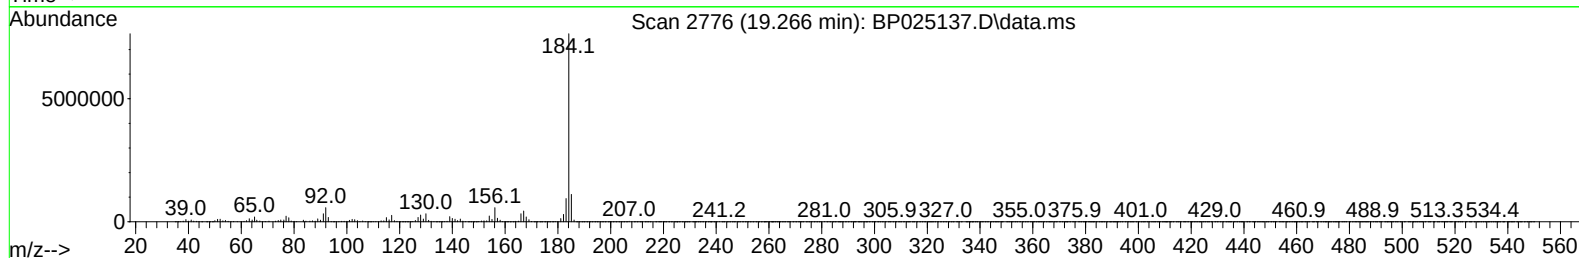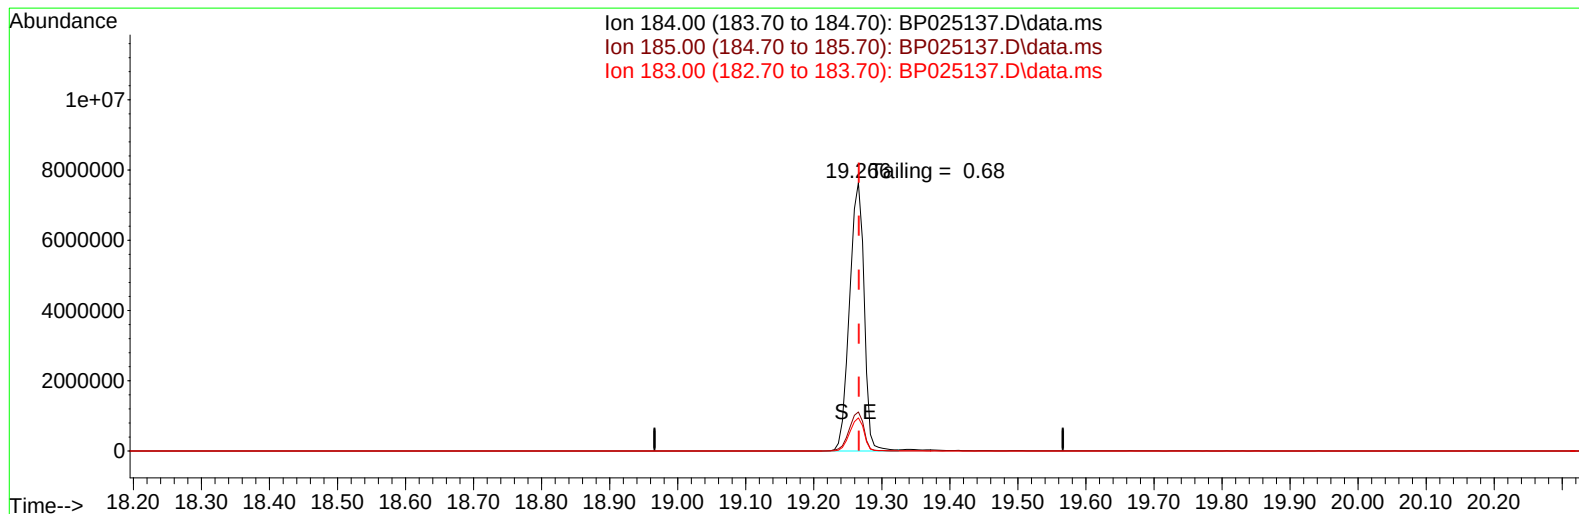

TIC: BP025137.D\data.ms

(77) Benzidine**19.266min (-0.000) 24087.44 ng****response 11322496**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.57
183.00	11.80	12.35
0.00	0.00	0.00