

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
 Data File : BM040919.D
 Acq On : 17 Jul 2023 12:47
 Operator : MA/JU
 Sample : 03457-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jul 18 02:46:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 03:58:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.853	152	4046	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.653	136	12749	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.504	164	5802	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.253	188	10868	0.400	ng/ul	0.00
17) Chrysene-d12	21.451	240	7945	0.400	ng/ul	0.00
23) Perylene-d12	23.825	264	10289	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	28208	4.438	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.253	152	4334	0.242	ng/ul	0.00
18) Fluoranthene-d10	19.287	212	6975	0.274	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.650	202	1627	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.670	252	3065	0.085	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
Data File : BM040919.D
Acq On : 17 Jul 2023 12:47
Operator : MA/JU
Sample : 03457-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Jul 18 02:46:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 03:58:02 2023
Response via : Initial Calibration




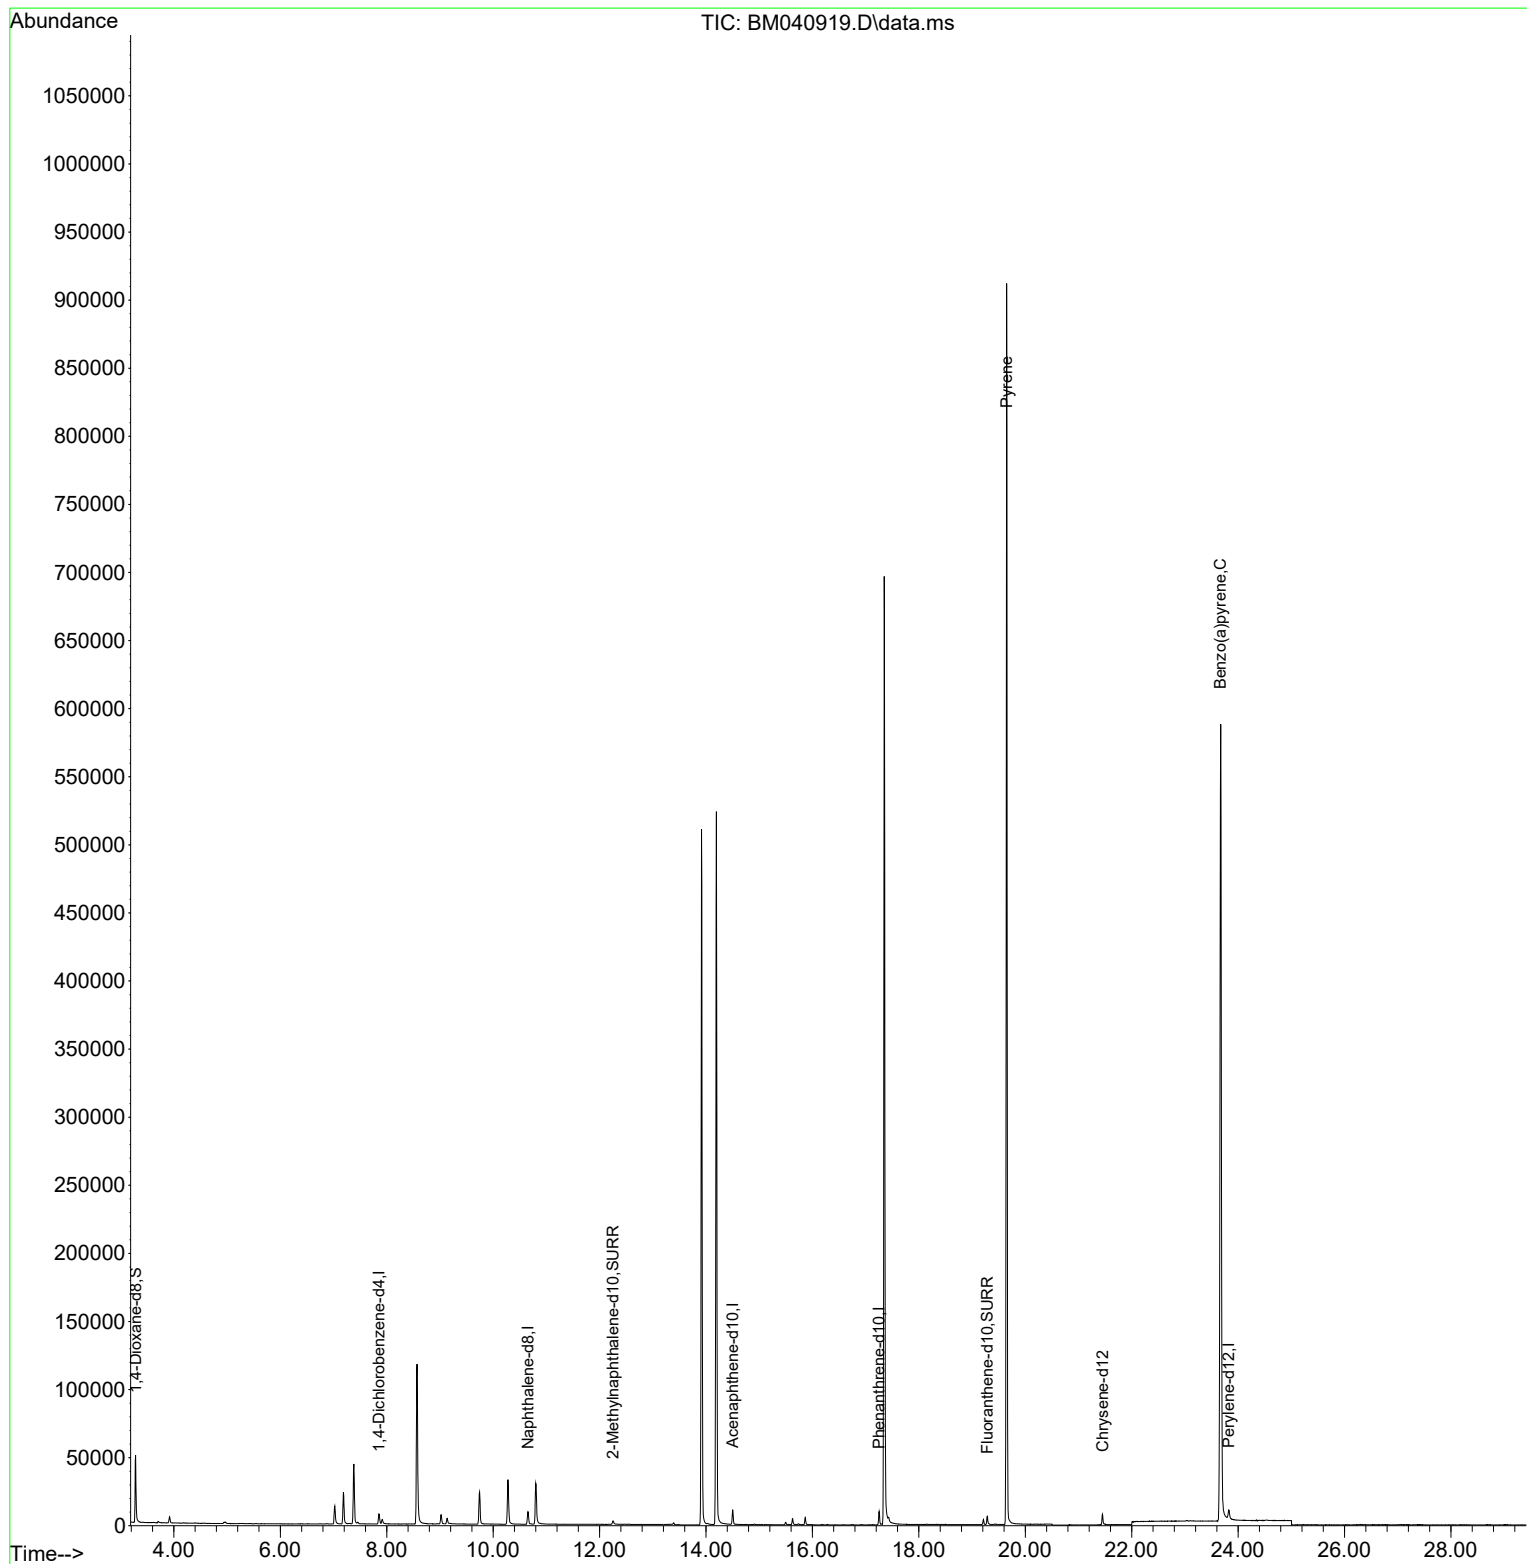


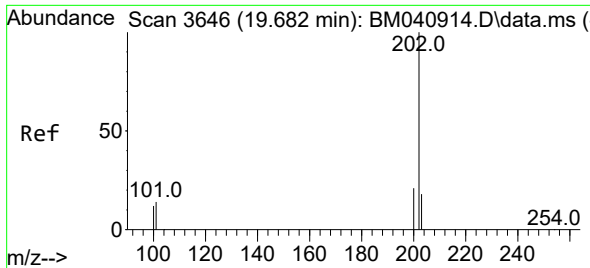

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.650 min Scan# 3639
Delta R.T. -0.037 min
Lab File: BM040919.D
Acq: 17 Jul 2023 12:47

Instrument :
BNA_P
ClientSampleId :

Tgt Ion:202 Resp: 1627
Ion Ratio Lower Upper
202 100
101 189.1 12.6 18.8#
100 1419.6 9.8 14.6#

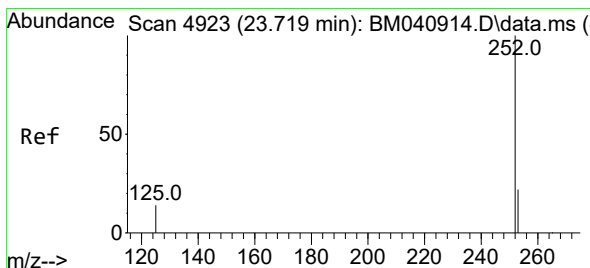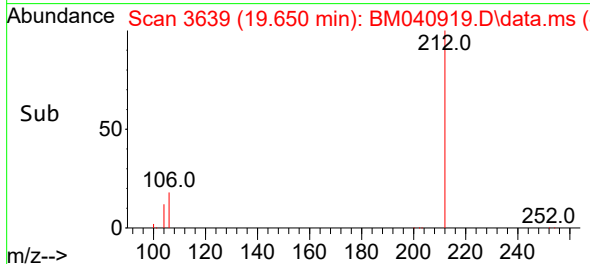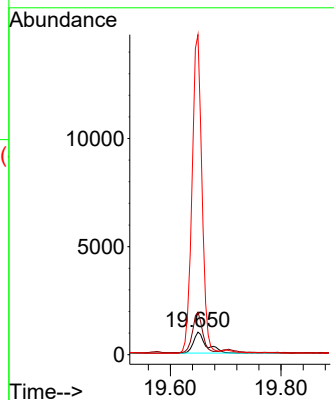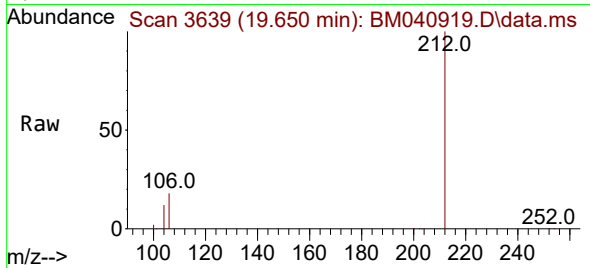

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.670 min Scan# 4906
Delta R.T. -0.053 min
Lab File: BM040919.D
Acq: 17 Jul 2023 12:47

Tgt Ion:252 Resp: 3065
Ion Ratio Lower Upper
252 100
253 52.3 22.9 34.3#
125 57.5 21.0 31.4#

