




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:26:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

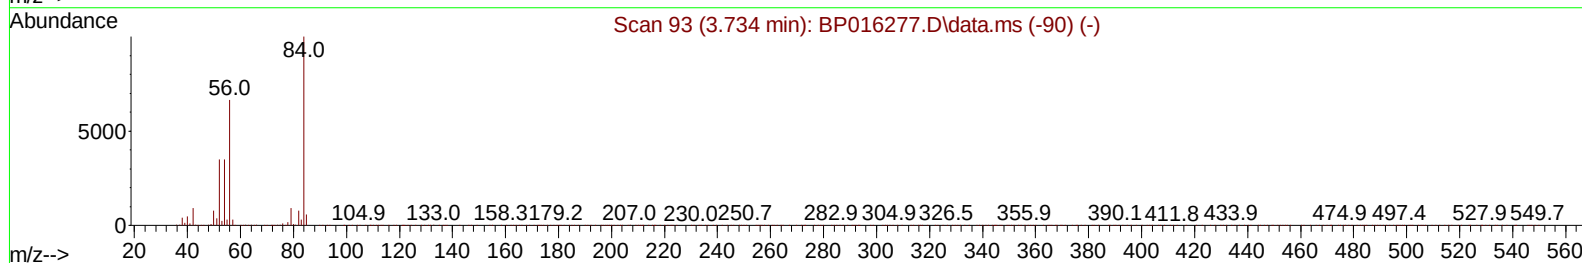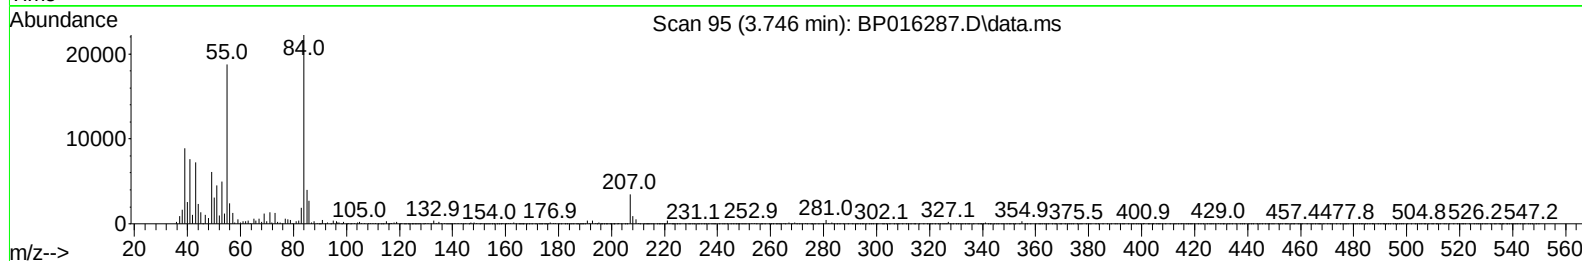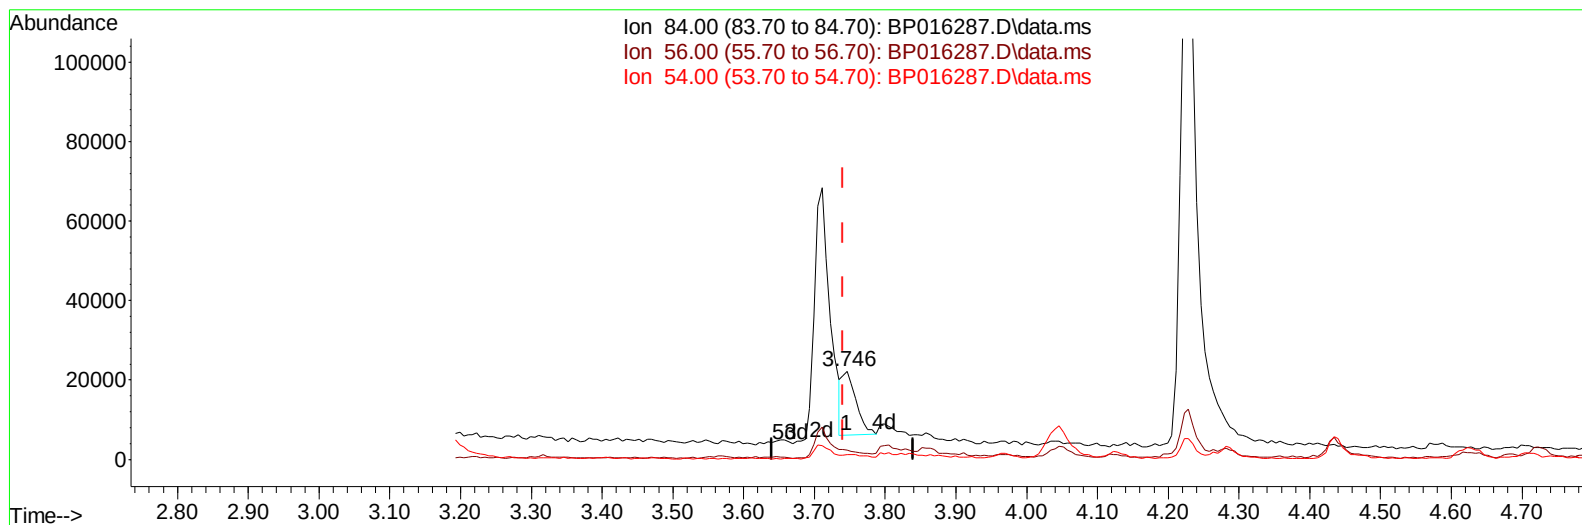

TIC: BP016287.D\data.ms

(4) Pyridine-d5 (S)

3.746min (+ 0.006) 1.63 ng/uL

response 22668

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.90	10.83#
54.00	32.50	5.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:26:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

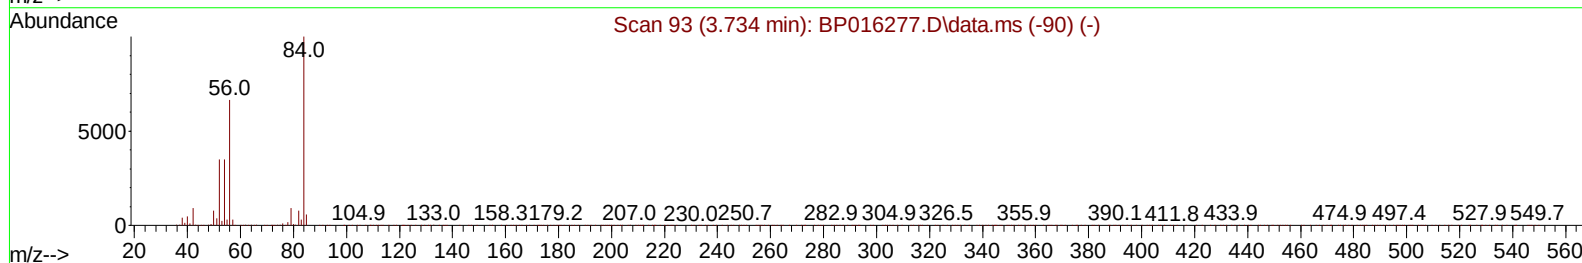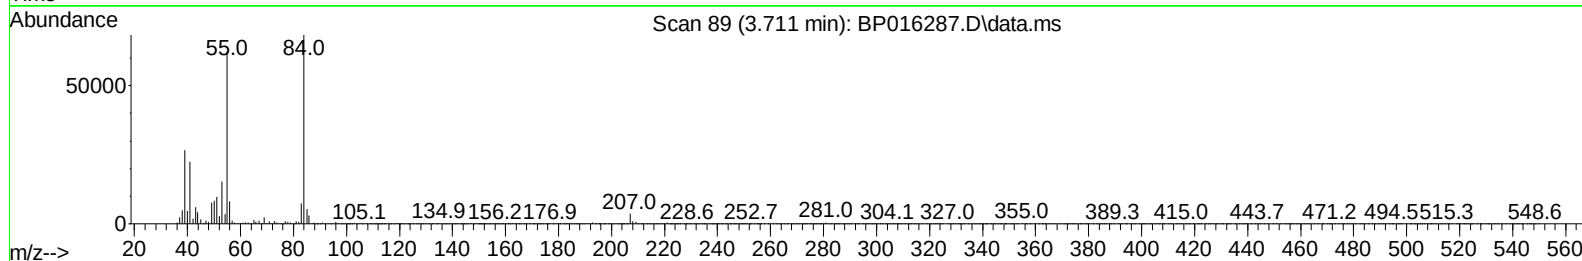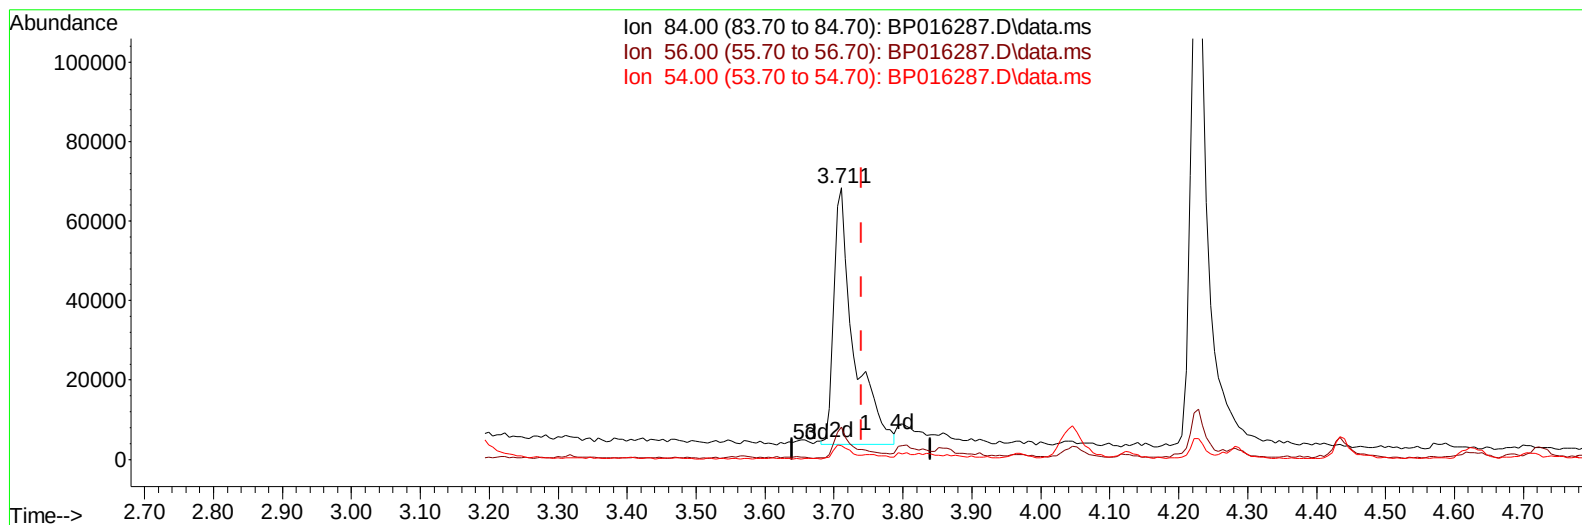

TIC: BP016287.D\data.ms

(4) Pyridine-d5 (S)

3.711min (-0.029) 9.35 ng/ul m

response 130233

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.90	11.92#
54.00	32.50	5.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

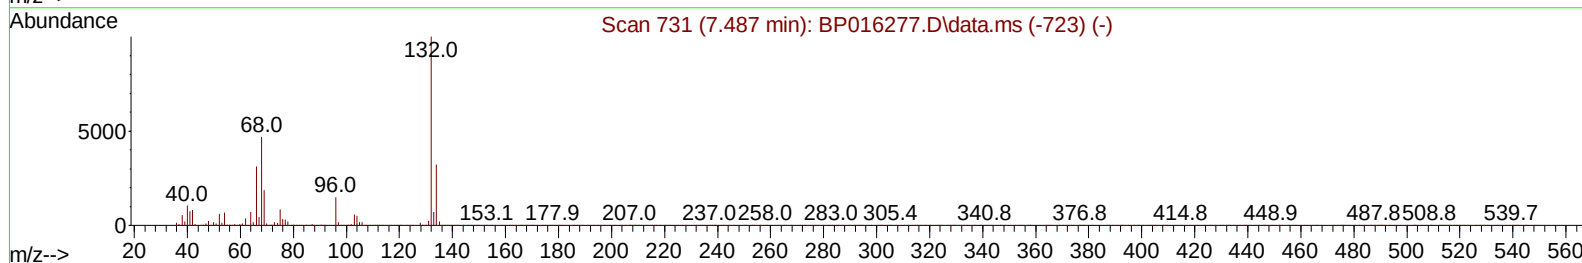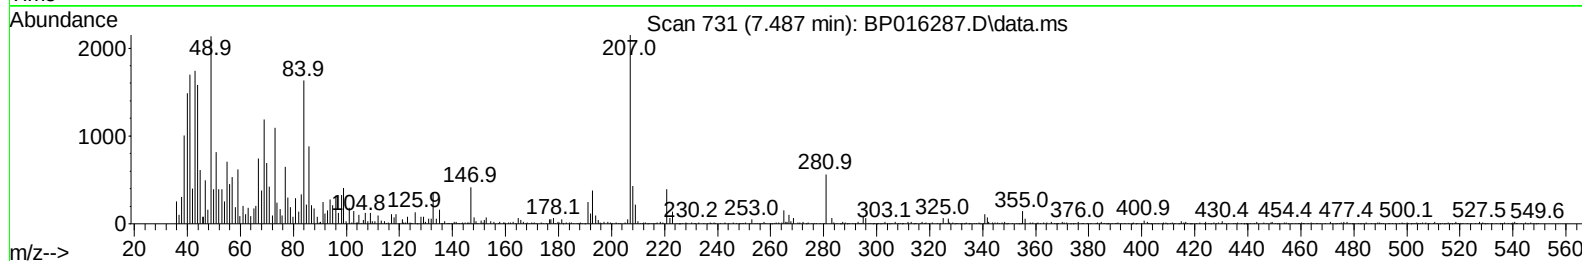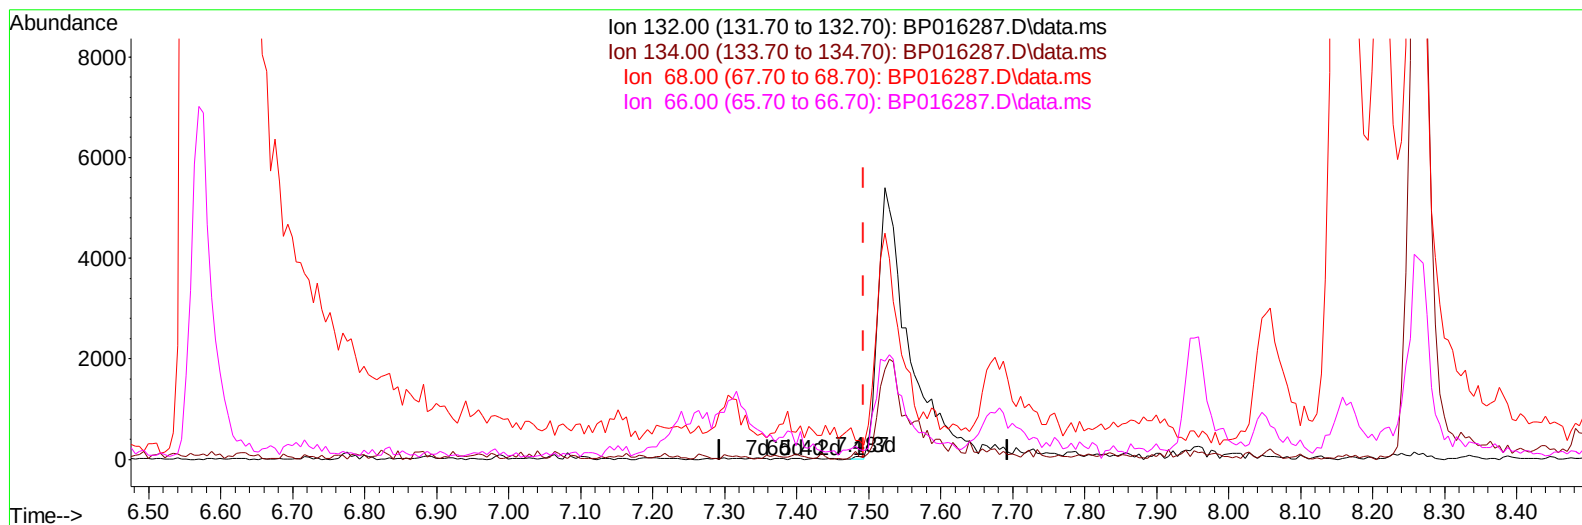

TIC: BP016287.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.487min (-0.006) 0.00 ng/u1

response 50

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	31.50	105.26#
68.00	47.30	666.67#
66.00	33.60	356.14#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

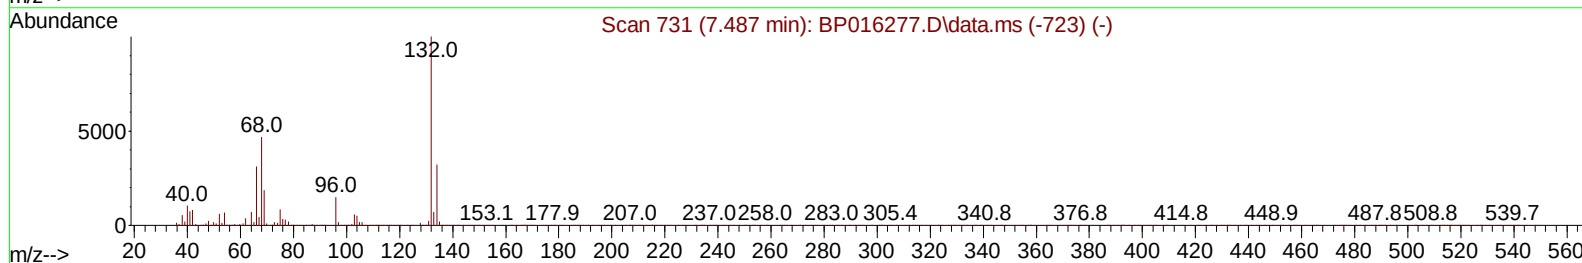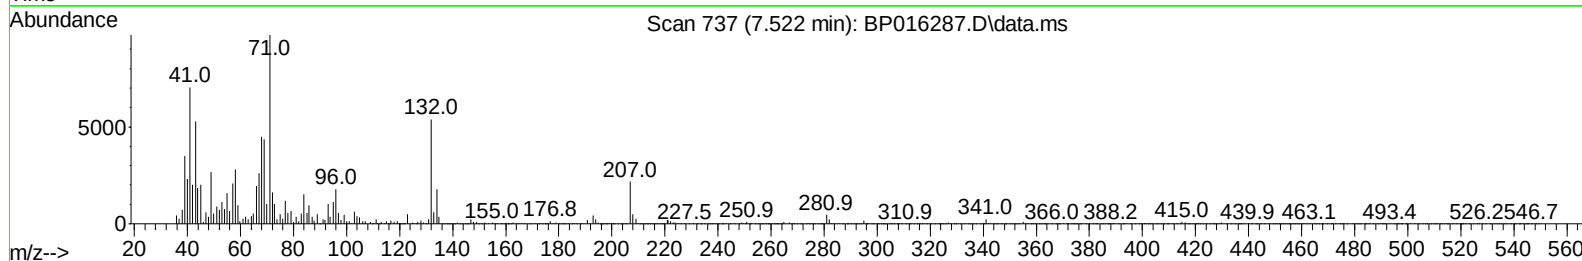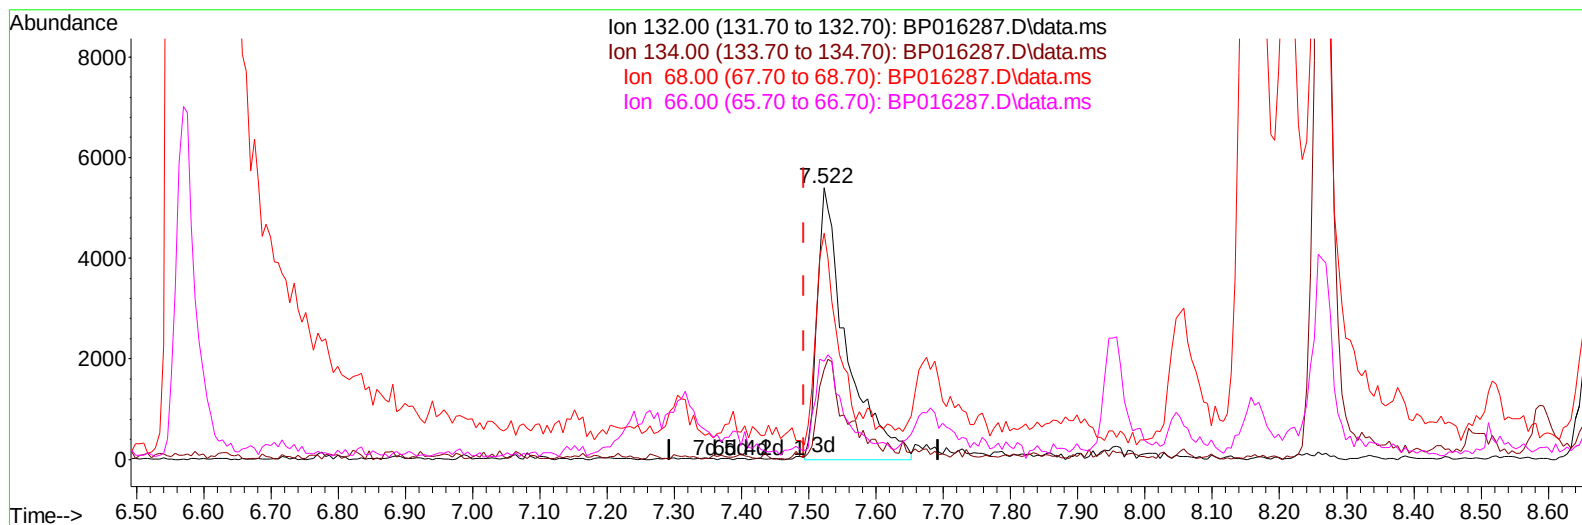

TIC: BP016287.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.522min (+ 0.030) 1.26 ng/ul m

response 16226

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	31.50	33.12
68.00	47.30	83.41#
66.00	33.60	36.27




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

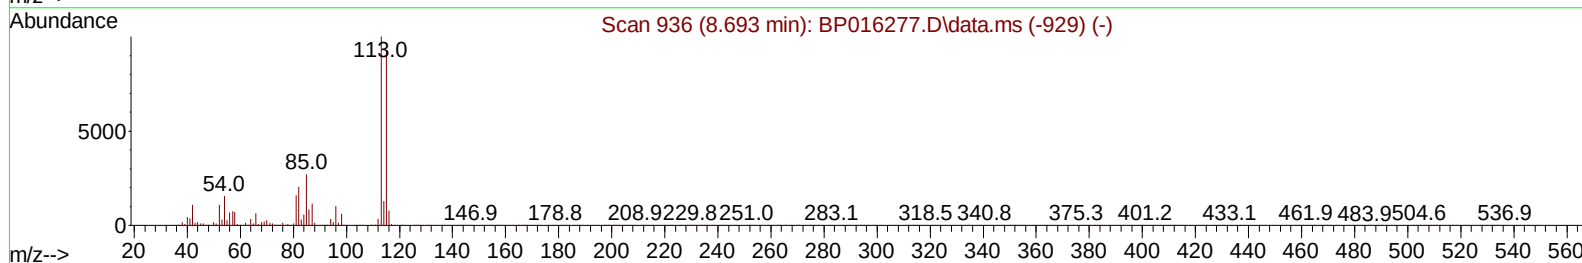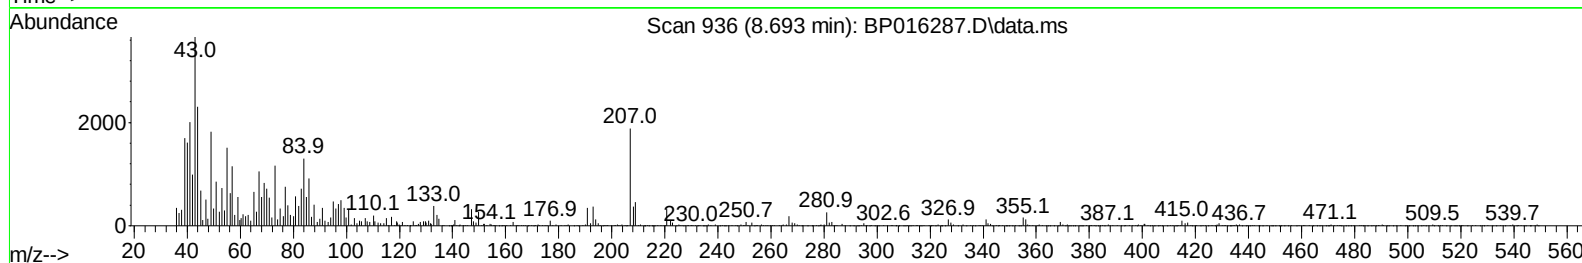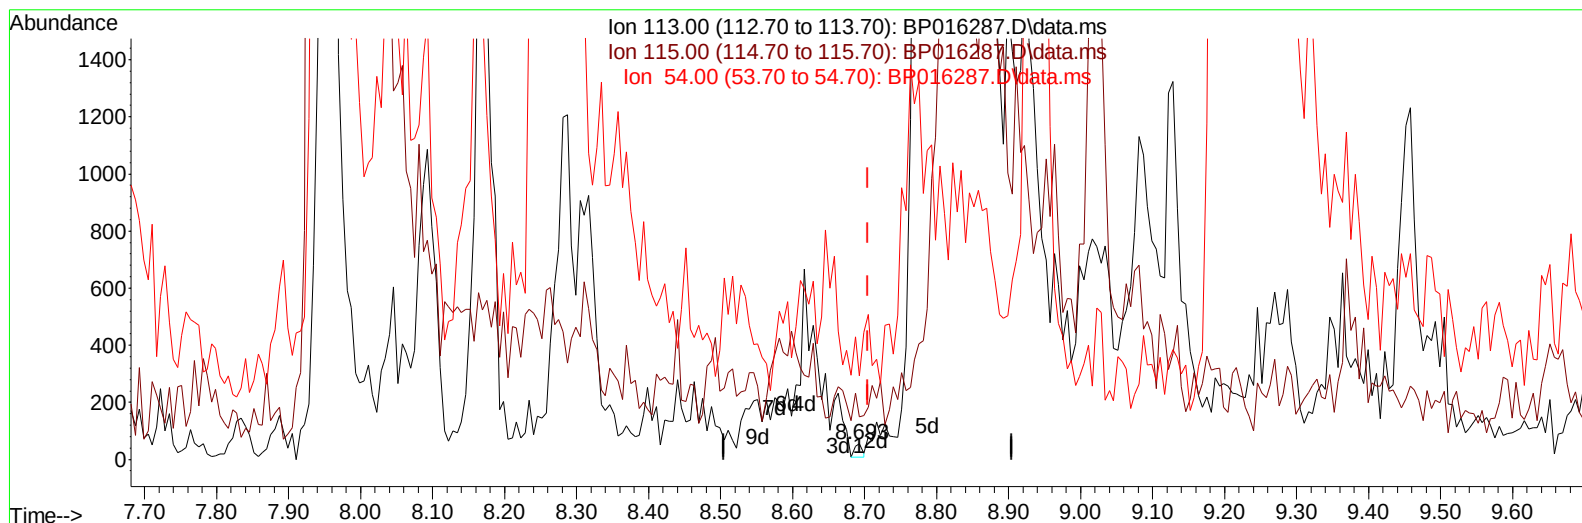

TIC: BP016287.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.693min (-0.012) 0.00 ng/u1

response 35

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	270.91#
54.00	16.30	532.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

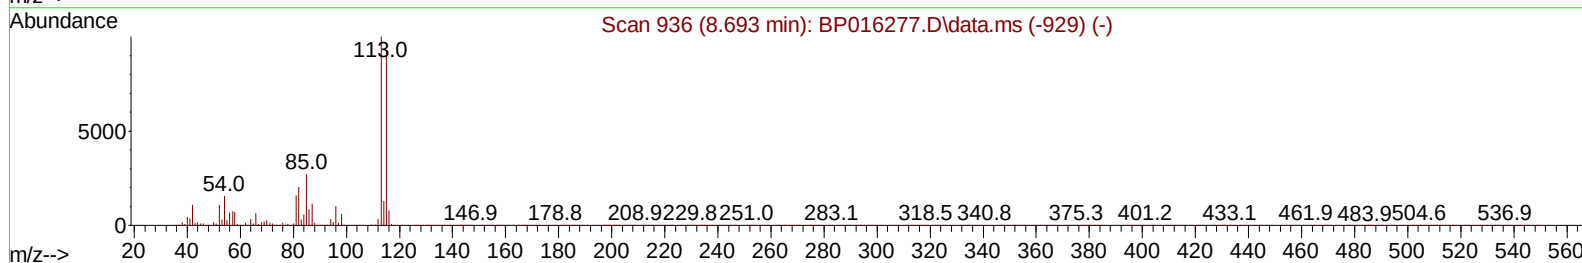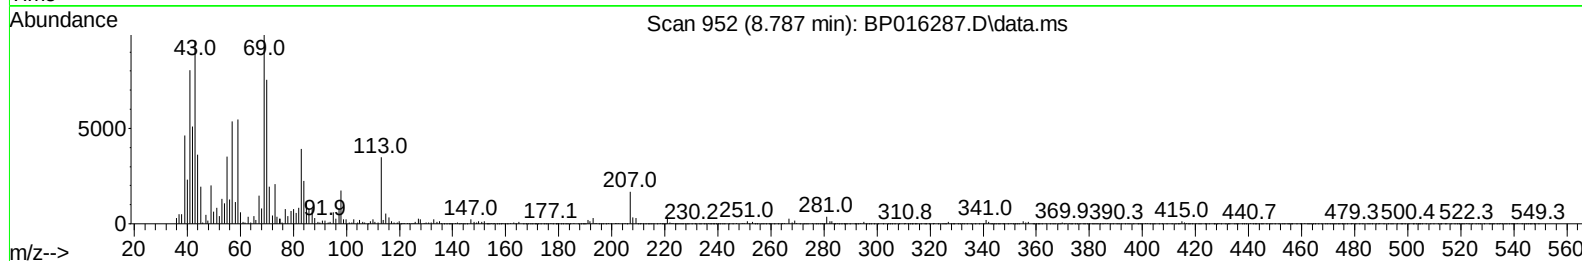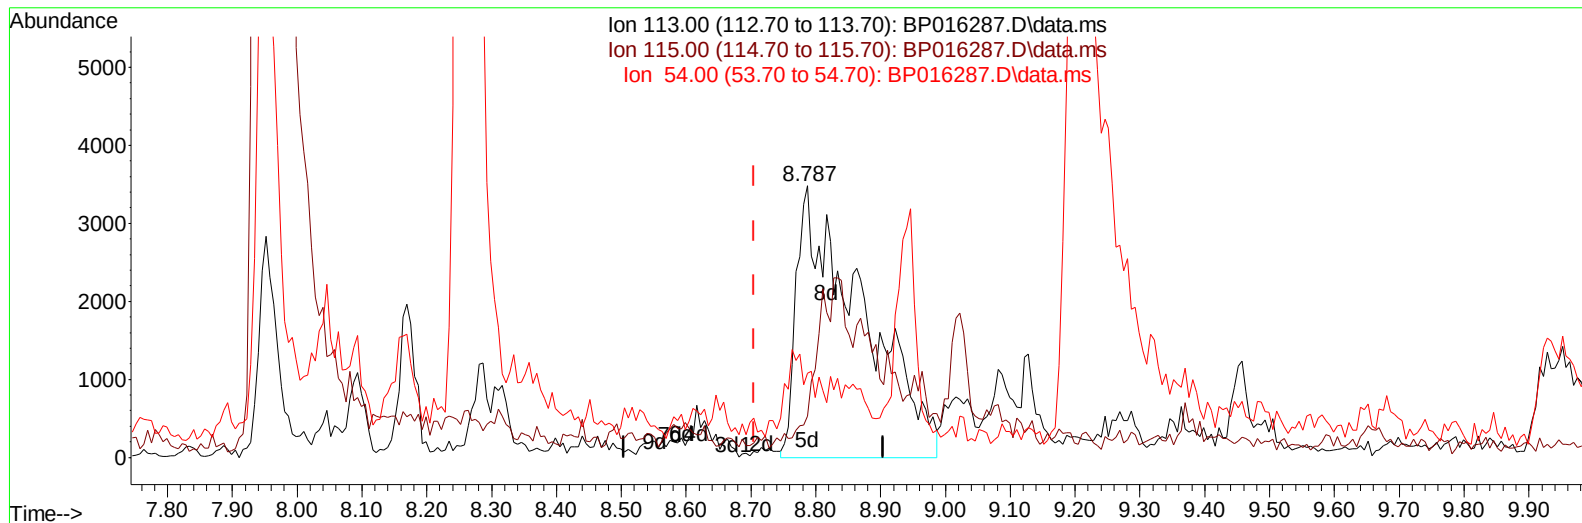

TIC: BP016287.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.787min (+ 0.083) 1.68 ng/ul m

response 24205

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	15.20#
54.00	16.30	31.06#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

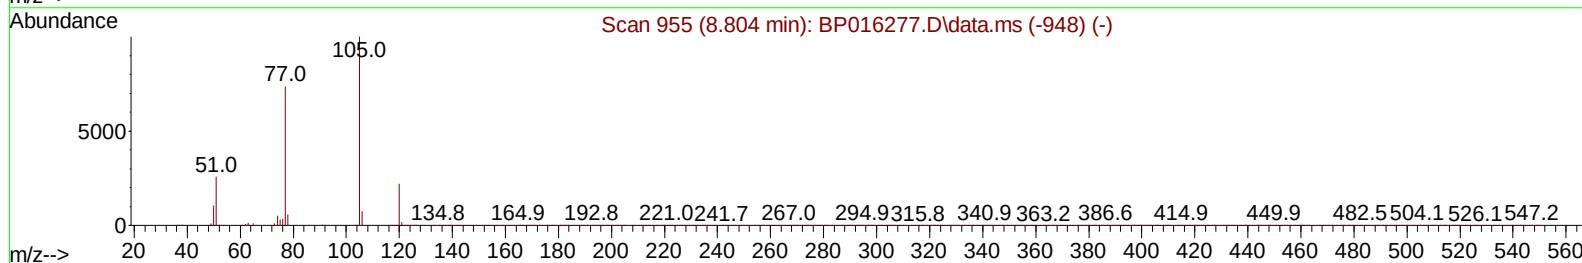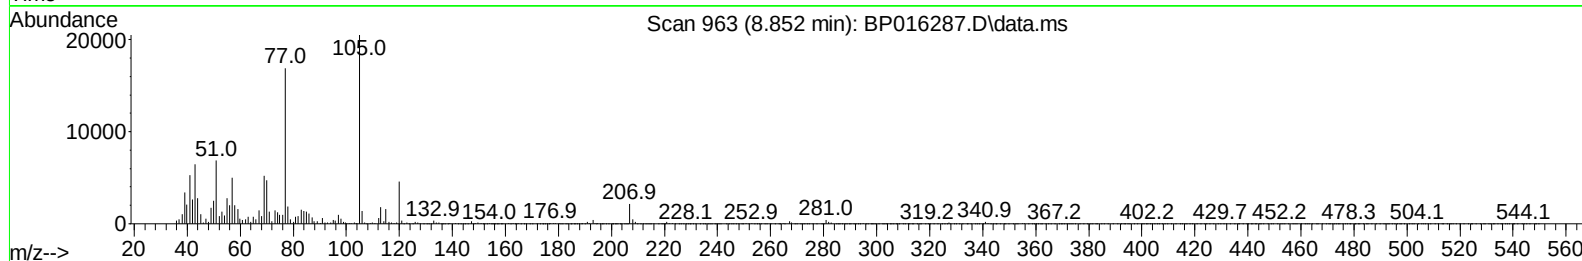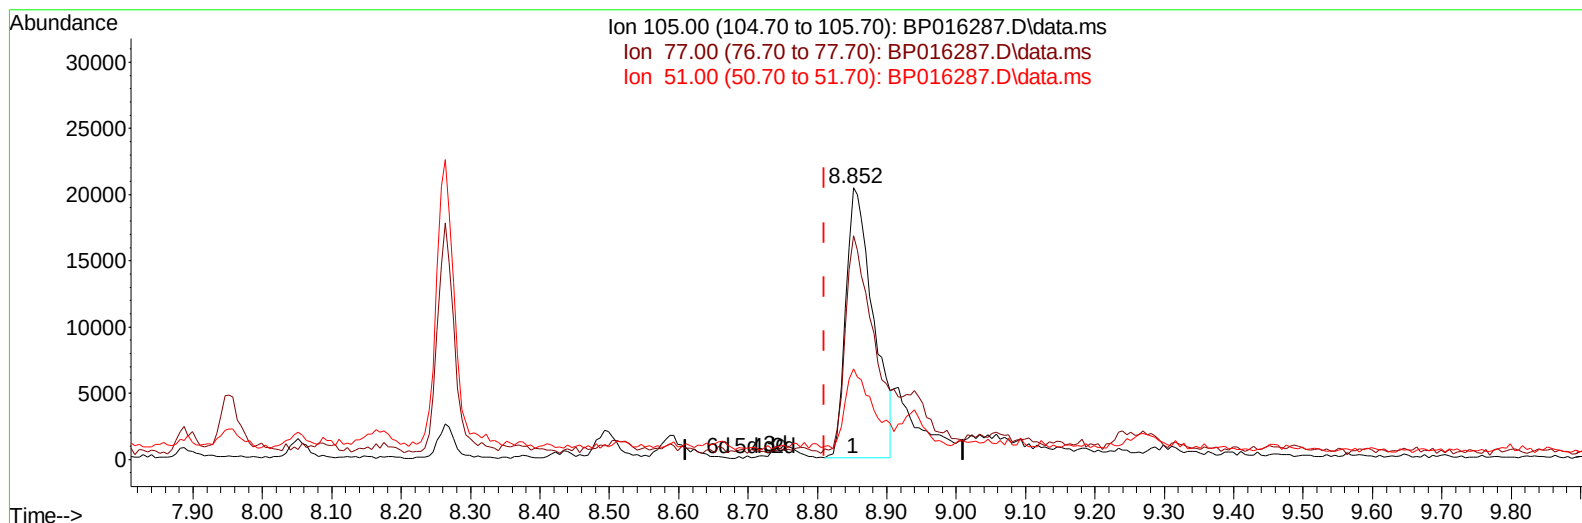

TIC: BP016287.D\data.ms

(16) Acetophenone

8.852min (+ 0.041) 2.35 ng/ul

response 55662

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	87.70	82.52
51.00	32.90	33.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

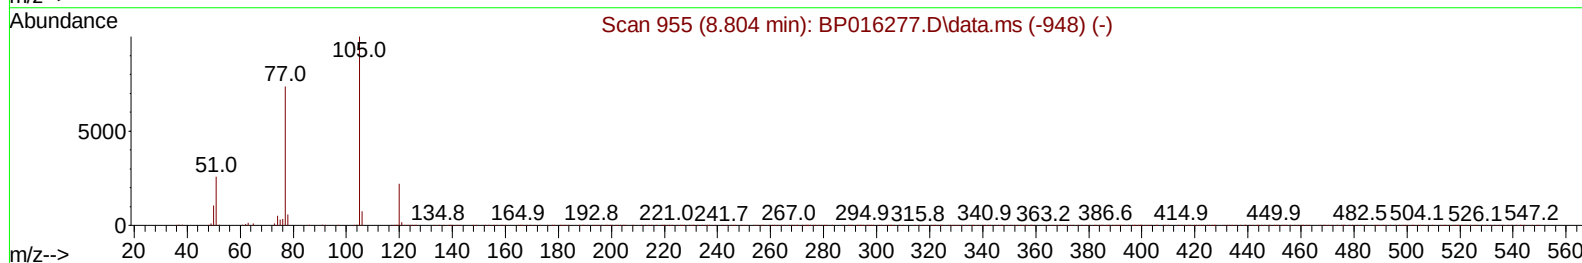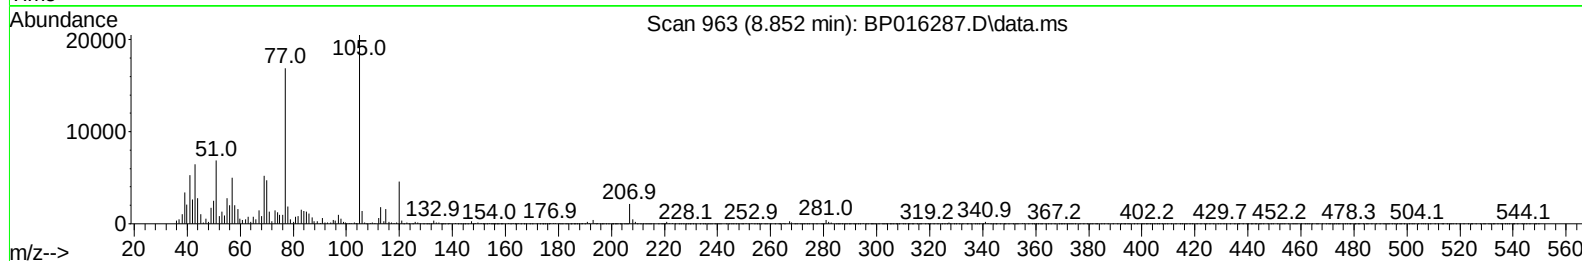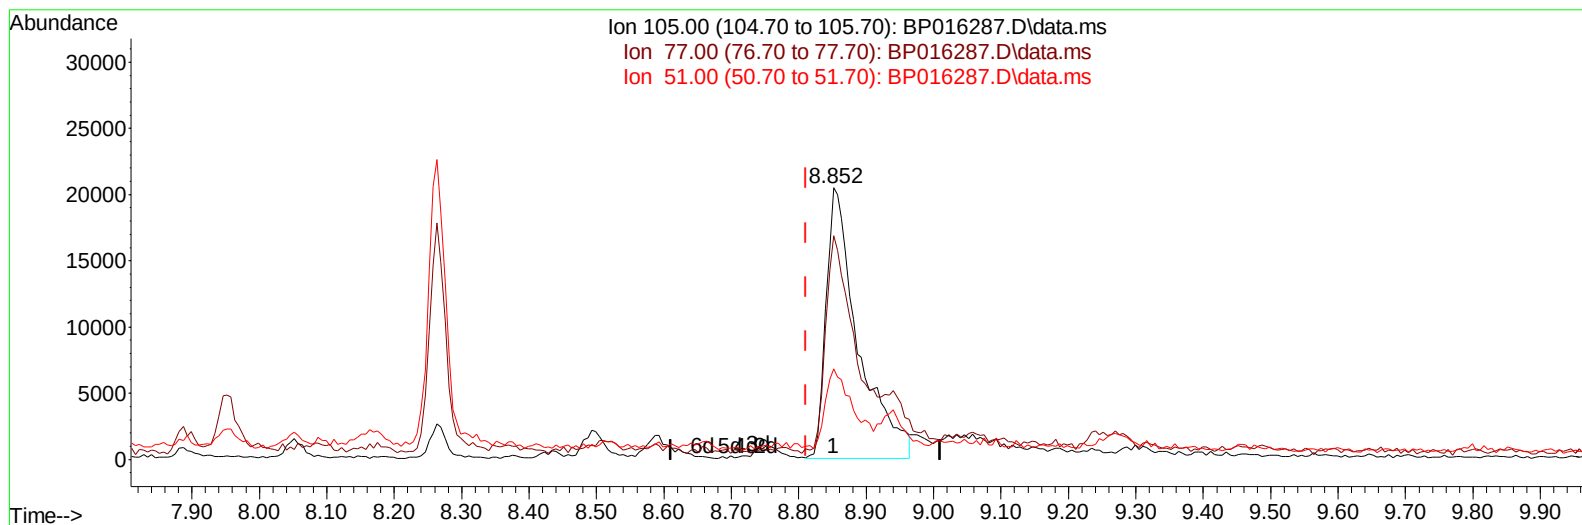

TIC: BP016287.D\data.ms

(16) Acetophenone

8.852min (+ 0.041) 2.85 ng/ul m

response 67464

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	87.70	82.52
51.00	32.90	33.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

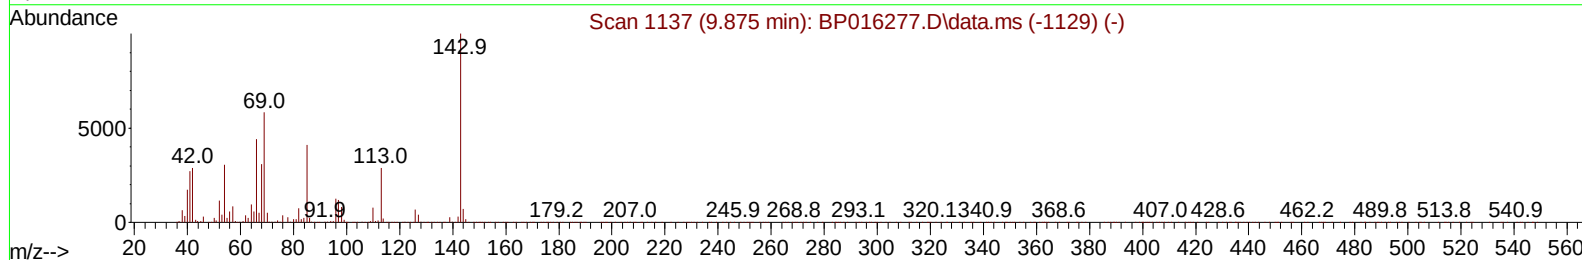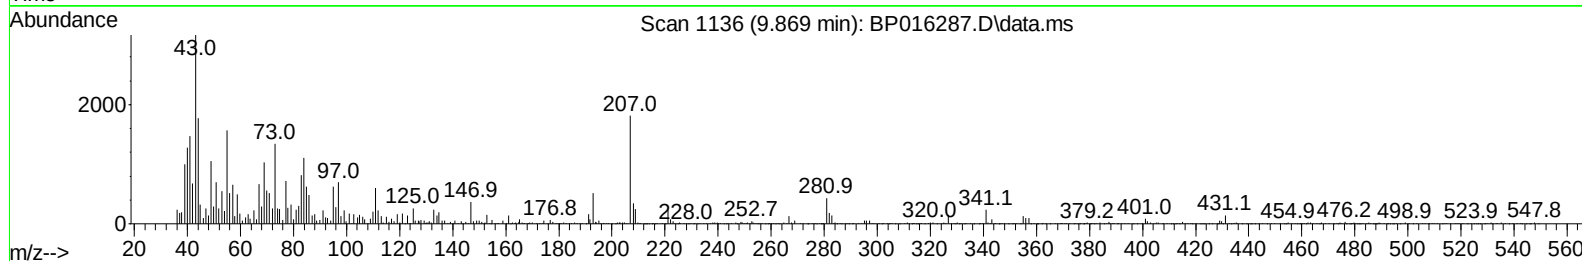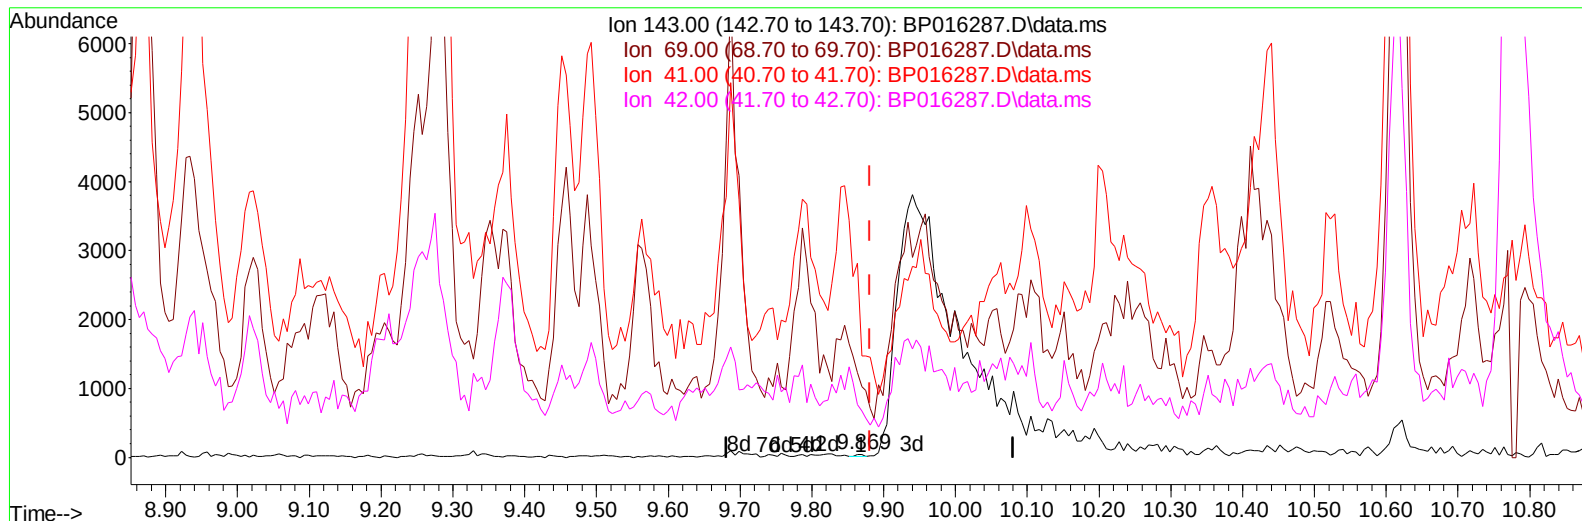

TIC: BP016287.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.869min (-0.012) 0.00 ng/u1

response 24

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	2282.22#
41.00	28.60	3275.56#
42.00	29.20	1500.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

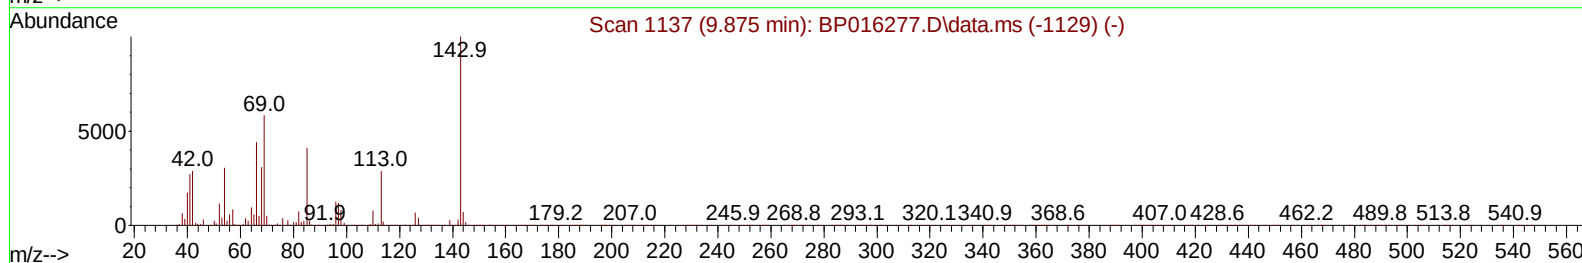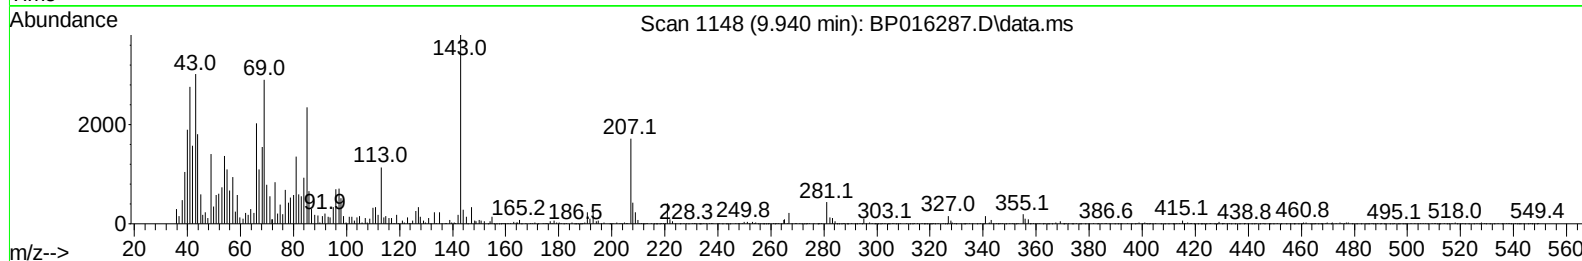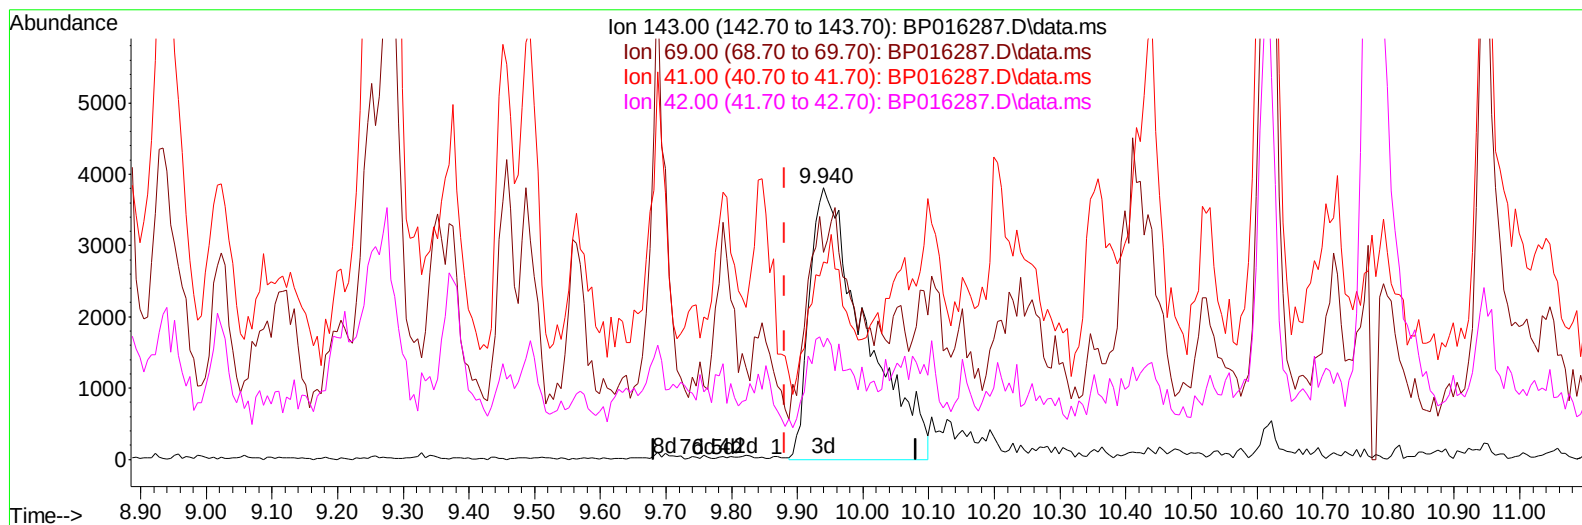

TIC: BP016287.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.940min (+ 0.059) 3.03 ng/ul m

response 22208

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	76.23#
41.00	28.60	72.69#
42.00	29.20	41.36#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

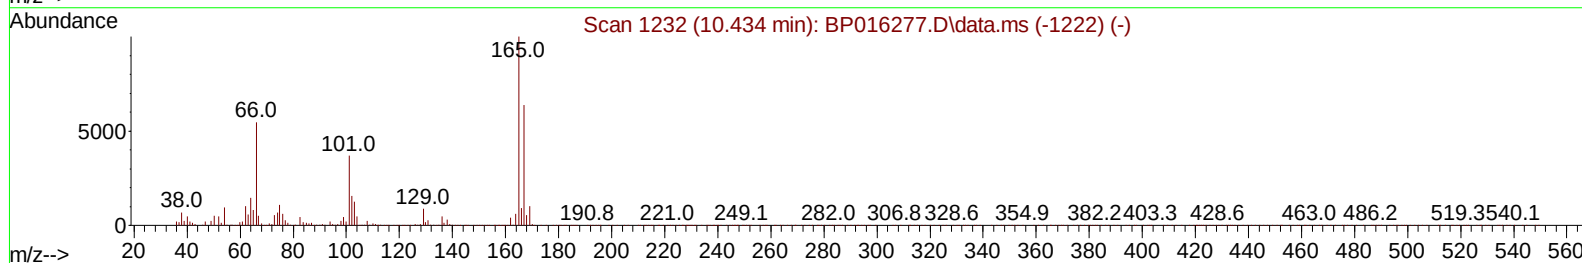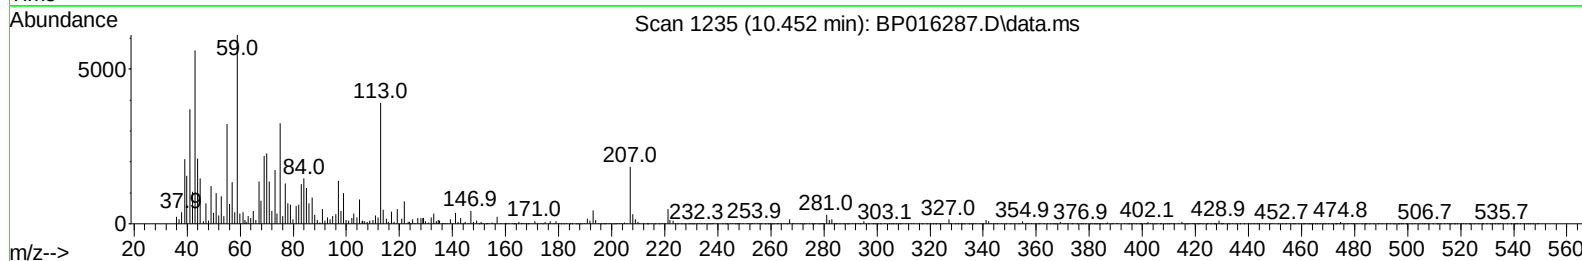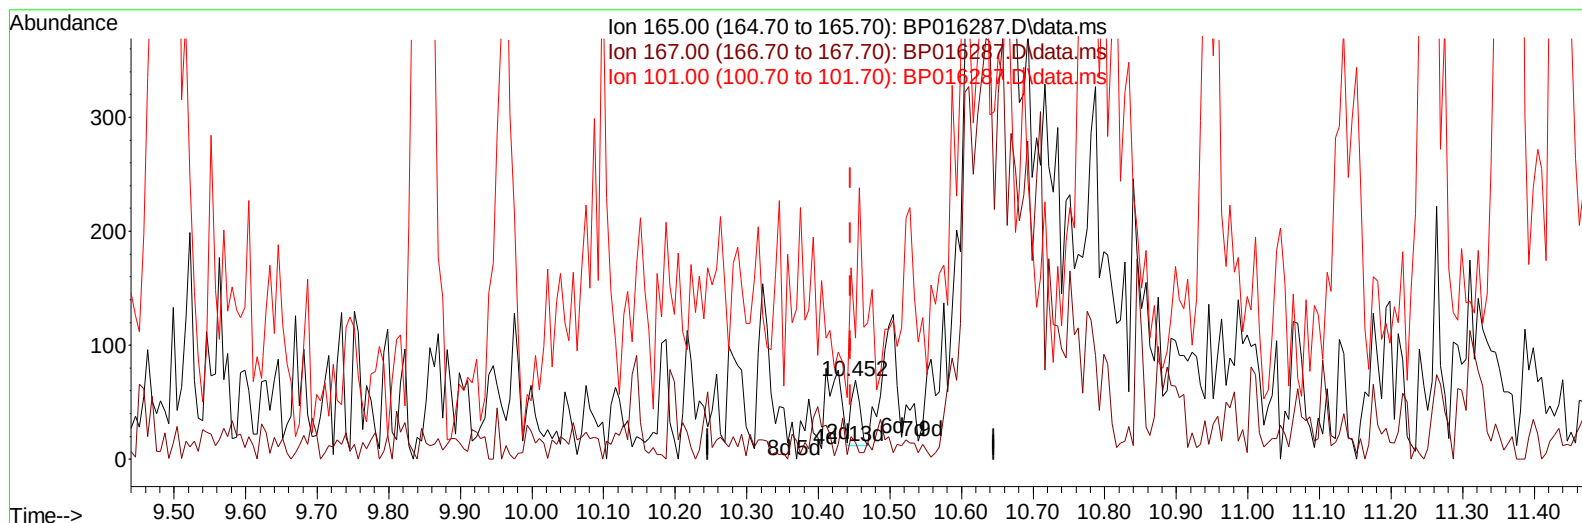

TIC: BP016287.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.452min (+ 0.006) 0.00 ng/ul

response 49

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	31.88#
101.00	38.50	153.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016287.D
Acq On : 18 Jul 2023 10:48
Operator : MA/JU
Sample : 03458-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:55:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

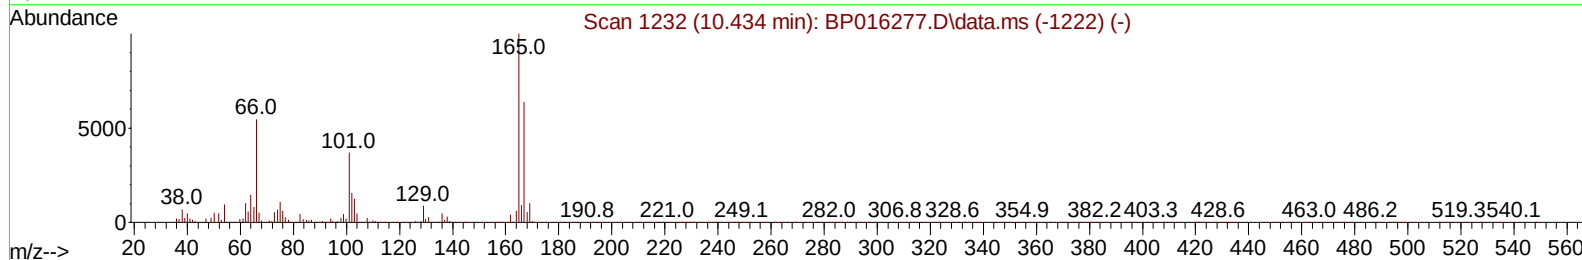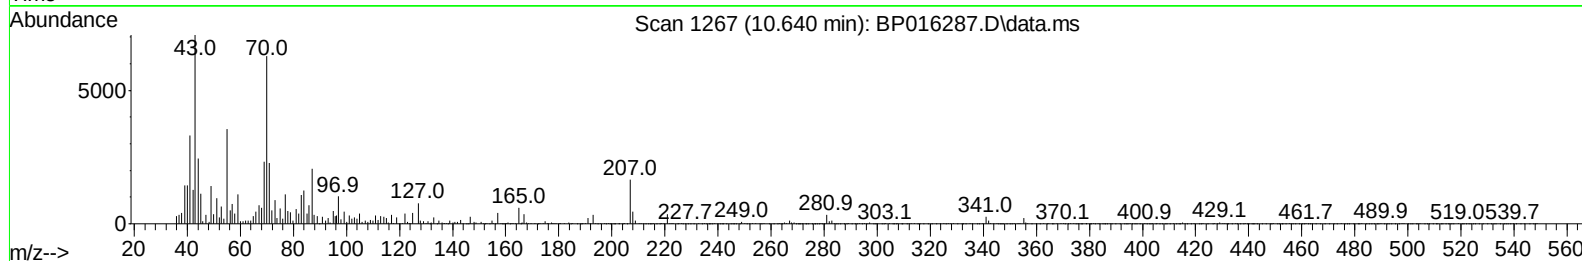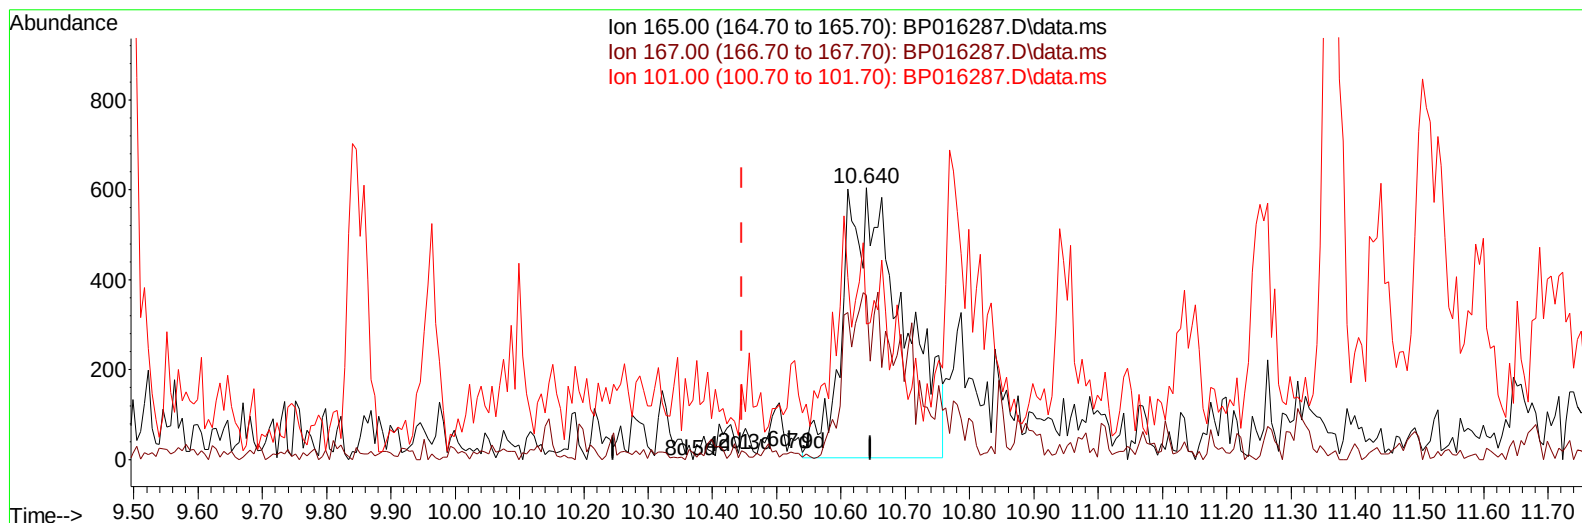

TIC: BP016287.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.640min (+ 0.194) 0.31 ng/ul m

response 3885

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	60.60
101.00	38.50	50.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016287.D
Acq On : 18 Jul 2023 10:48
Operator : MA/JU
Sample : 03458-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:57:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

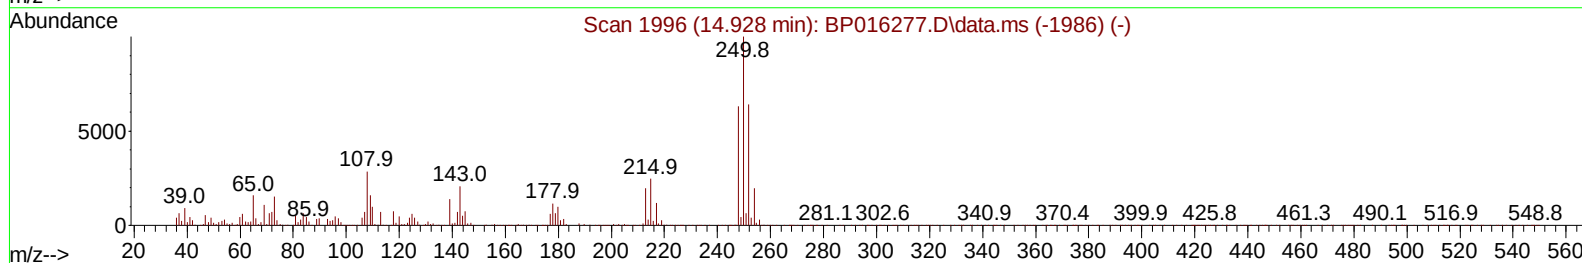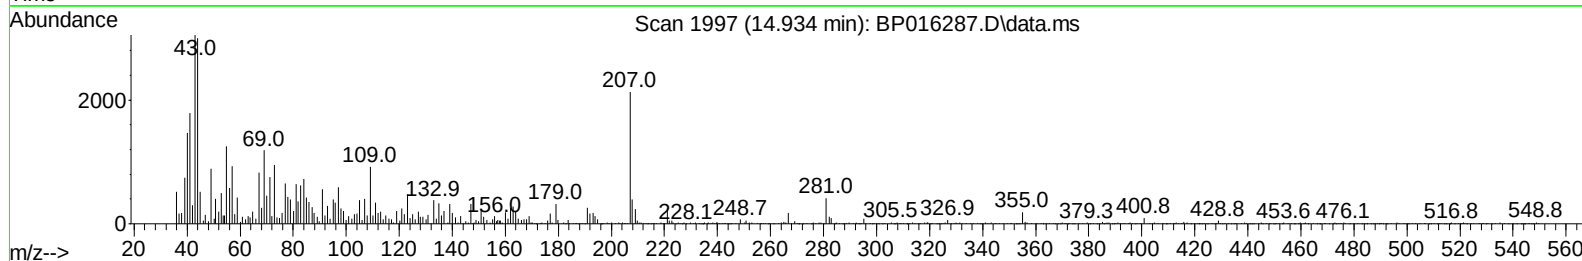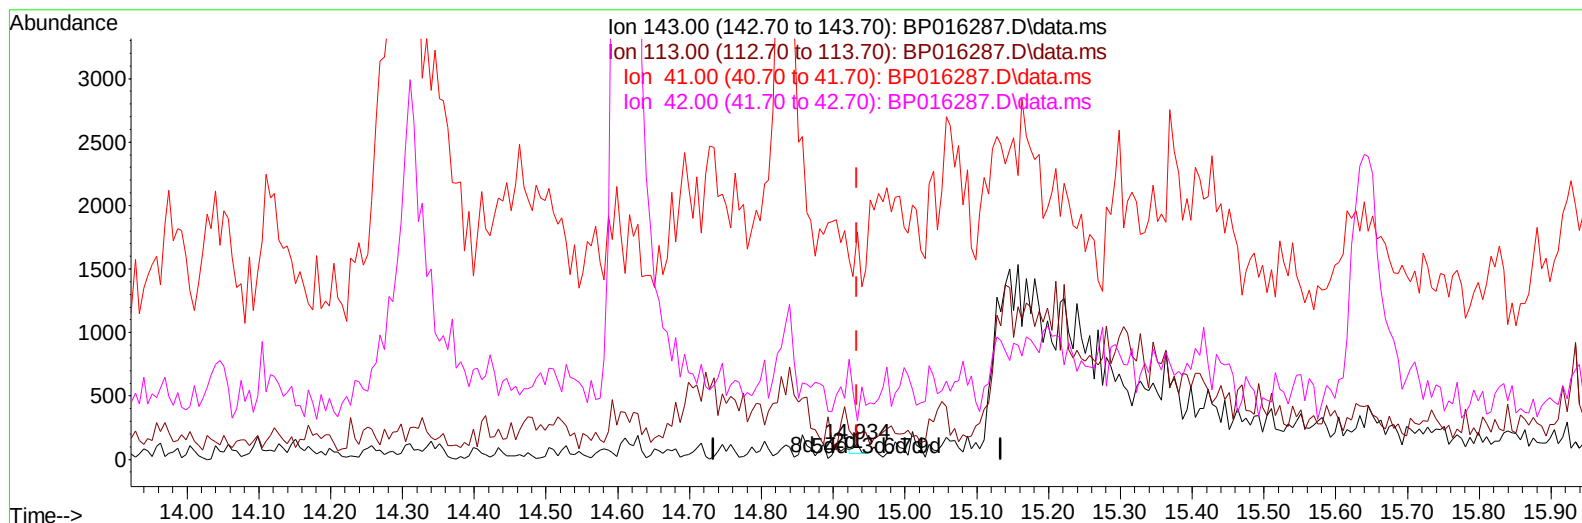

TIC: BP016287.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (+ 0.000) 0.00 ng/u1

response 40

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	157.26#
41.00	49.30	1445.97#
42.00	32.70	245.97#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016287.D
Acq On : 18 Jul 2023 10:48
Operator : MA/JU
Sample : 03458-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:57:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

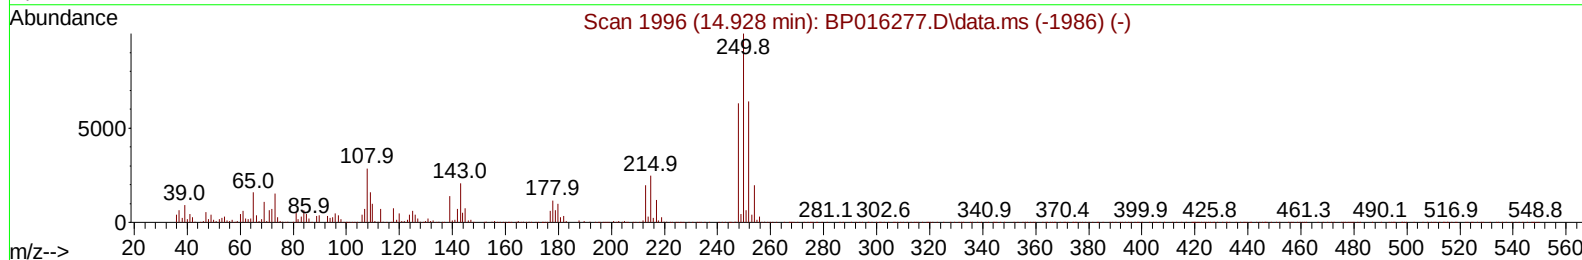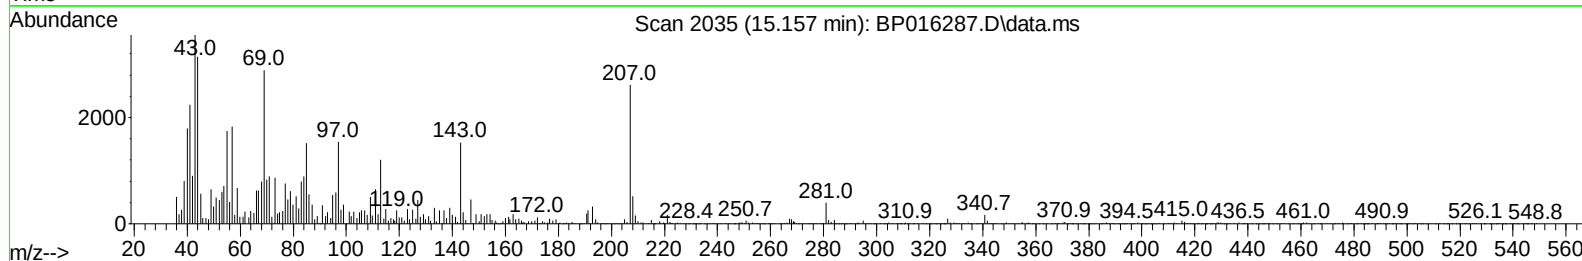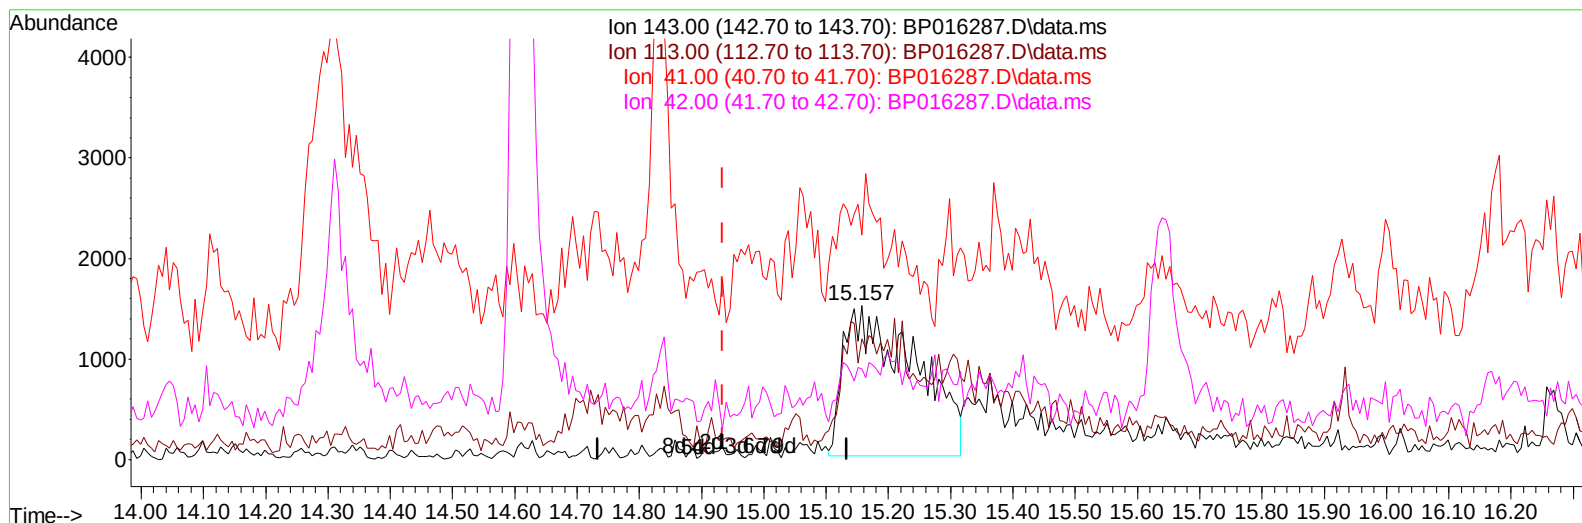

TIC: BP016287.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.157min (+ 0.224) 1.23 ng/ul m

response 11718

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	78.44
41.00	49.30	145.60#
42.00	32.70	58.70#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016287.D
Acq On : 18 Jul 2023 10:48
Operator : MA/JU
Sample : 03458-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:57:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

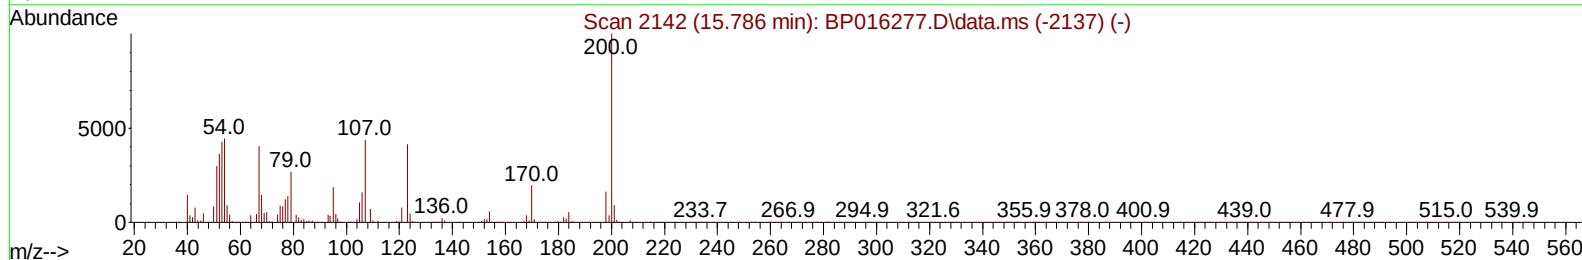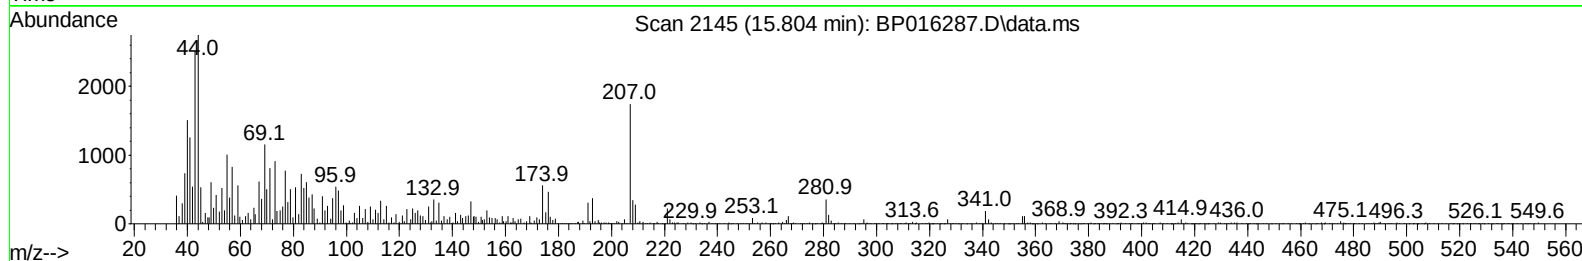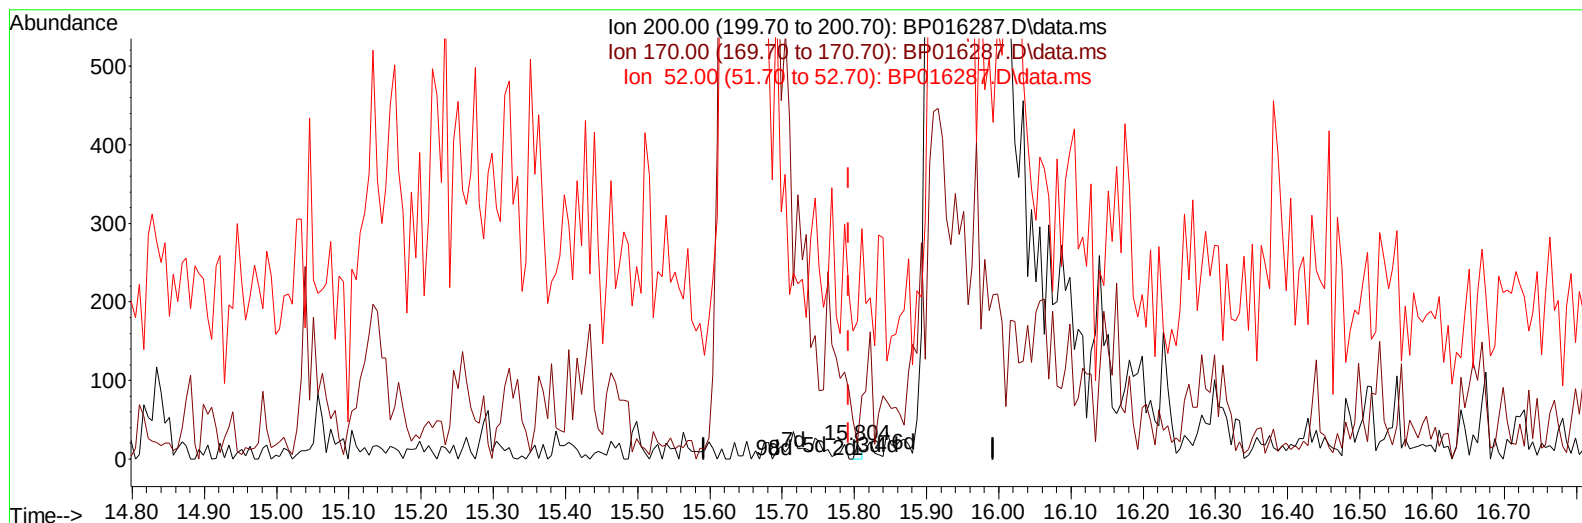

TIC: BP016287.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.804min (+ 0.012) 0.00 ng/ul

response 10

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	116.67#
52.00	58.00	972.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:57:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

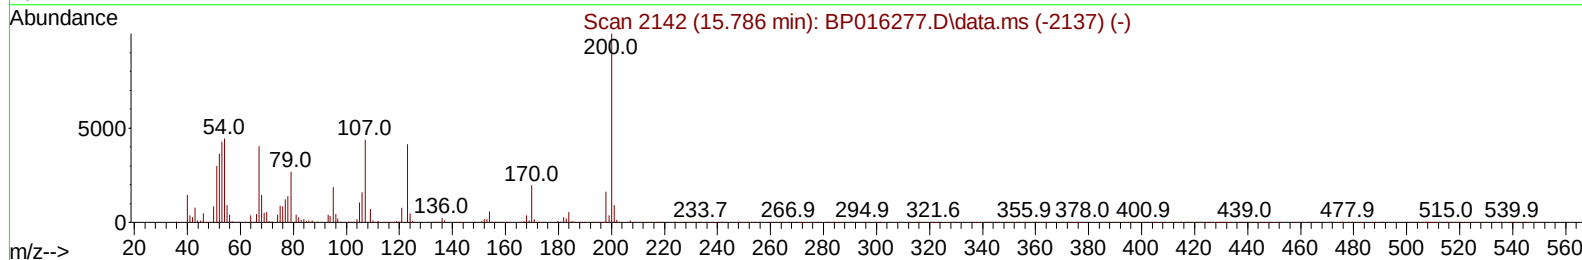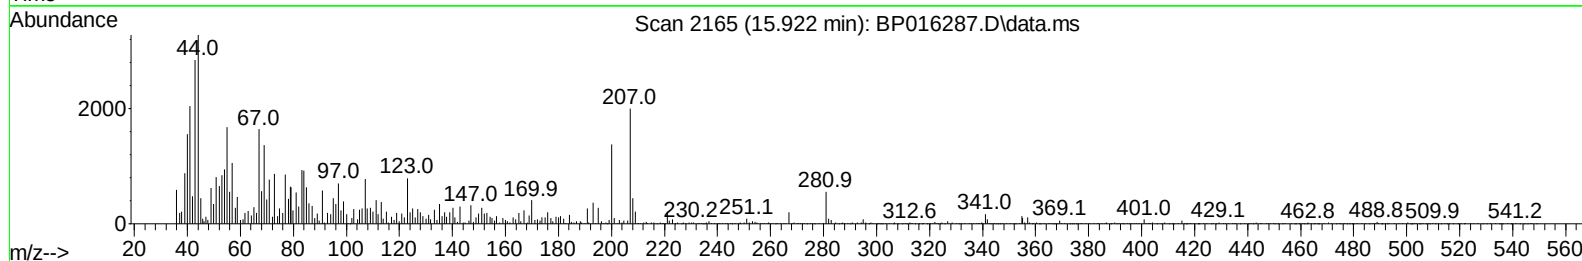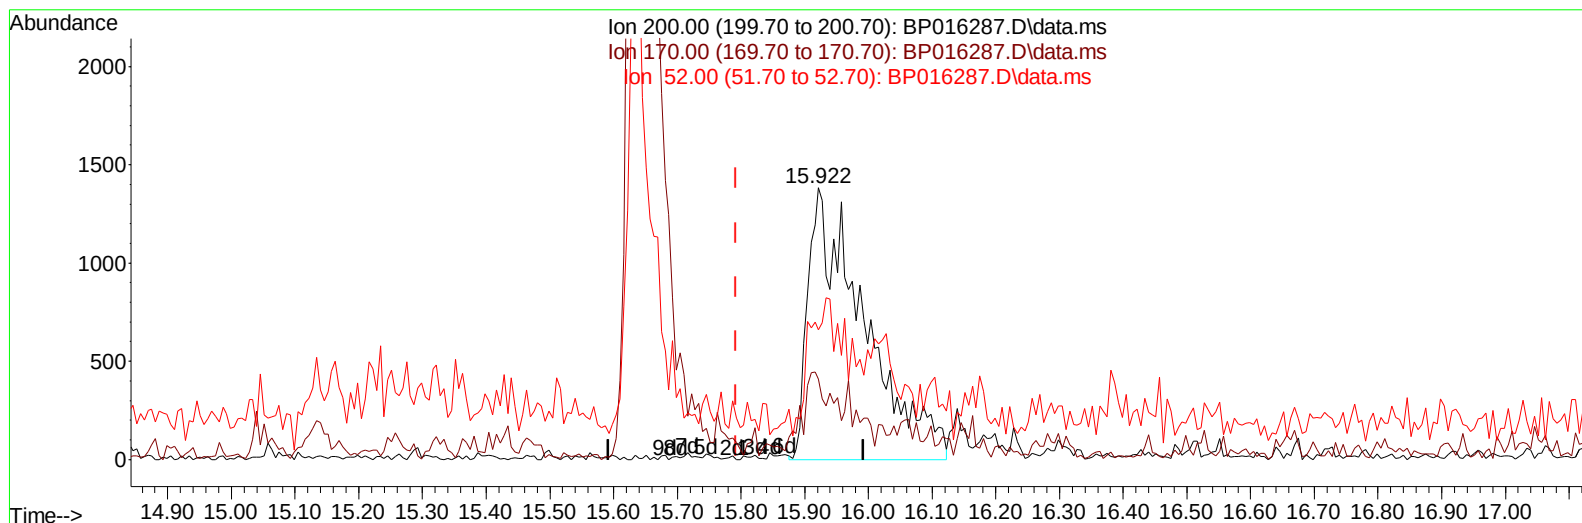

TIC: BP016287.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.922min (+ 0.130) 1.03 ng/ul m

response 8347

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	29.52#
52.00	58.00	47.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016287.D
Acq On : 18 Jul 2023 10:48
Operator : MA/JU
Sample : 03458-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:57:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

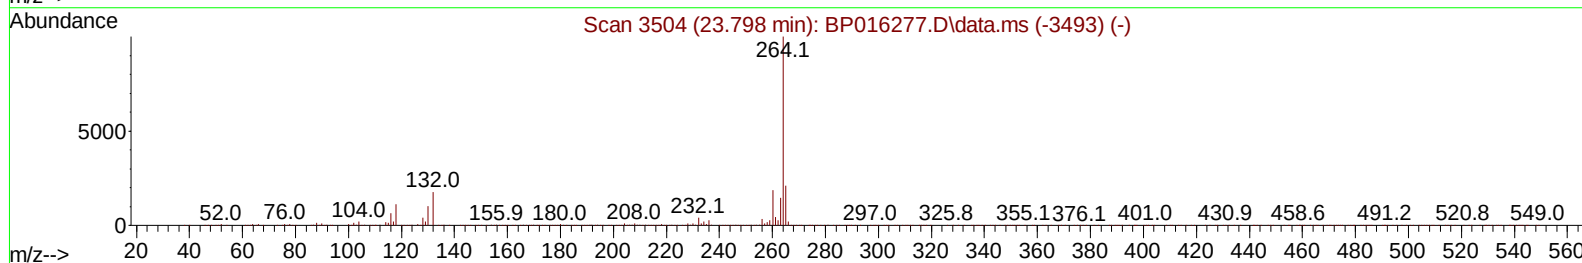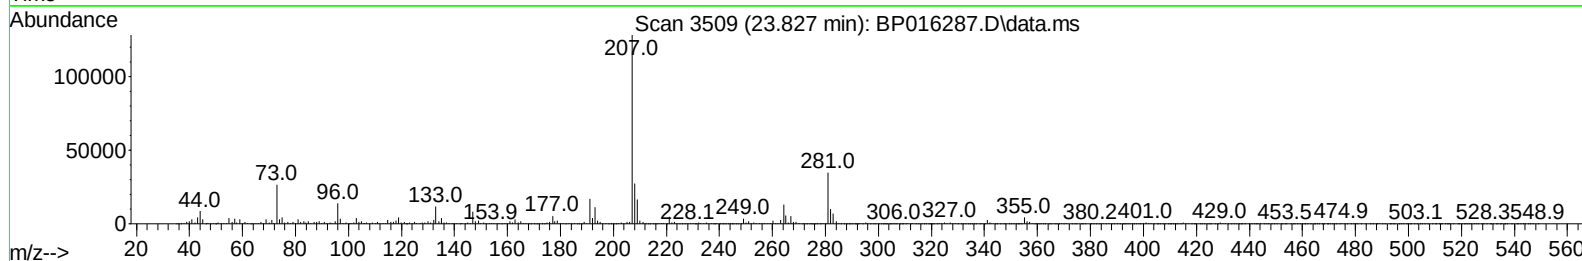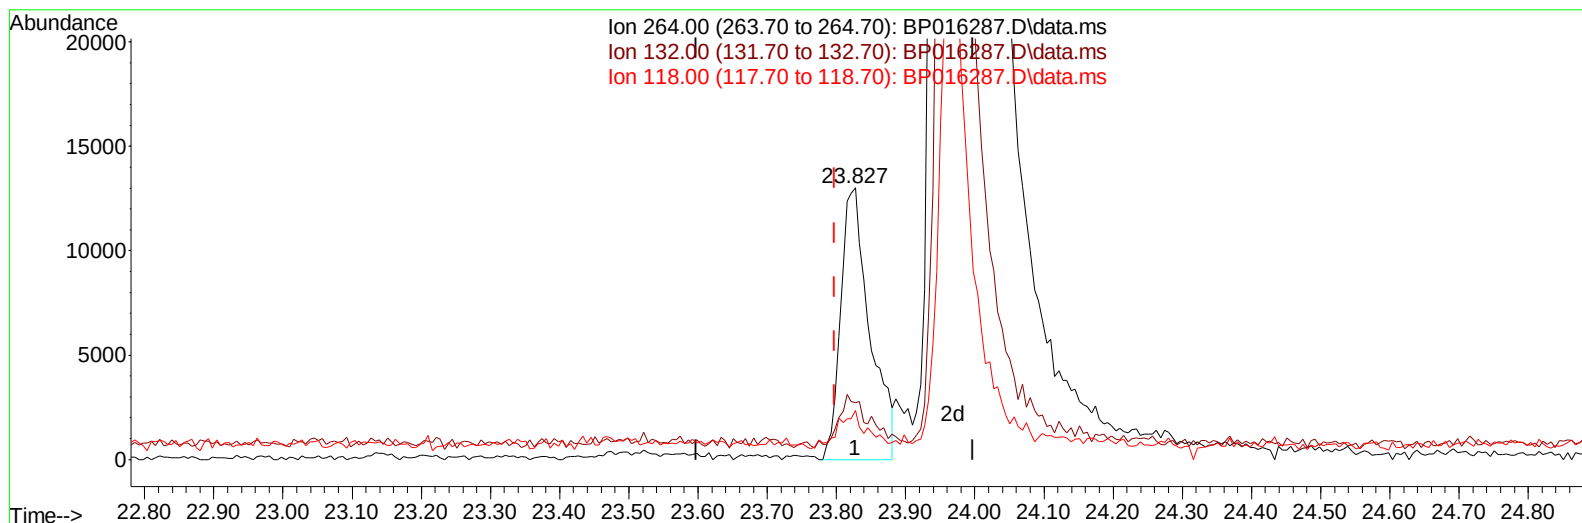

TIC: BP016287.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

23.827min (+ 0.030) 0.71 ng/u1

response 37910

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	17.90	20.98
118.00	11.20	18.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016287.D
Acq On : 18 Jul 2023 10:48
Operator : MA/JU
Sample : 03458-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:57:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

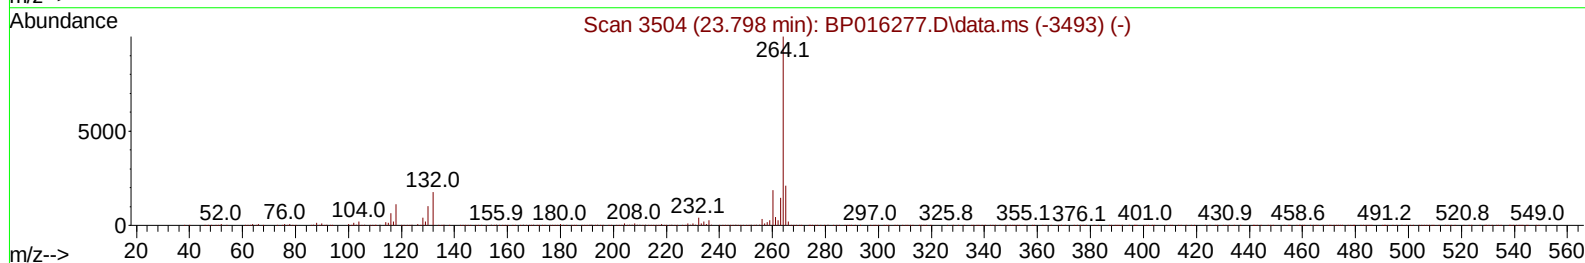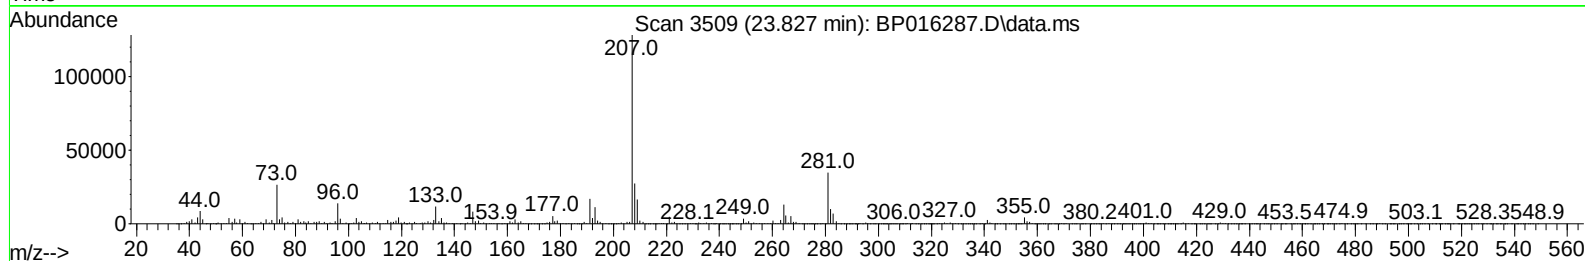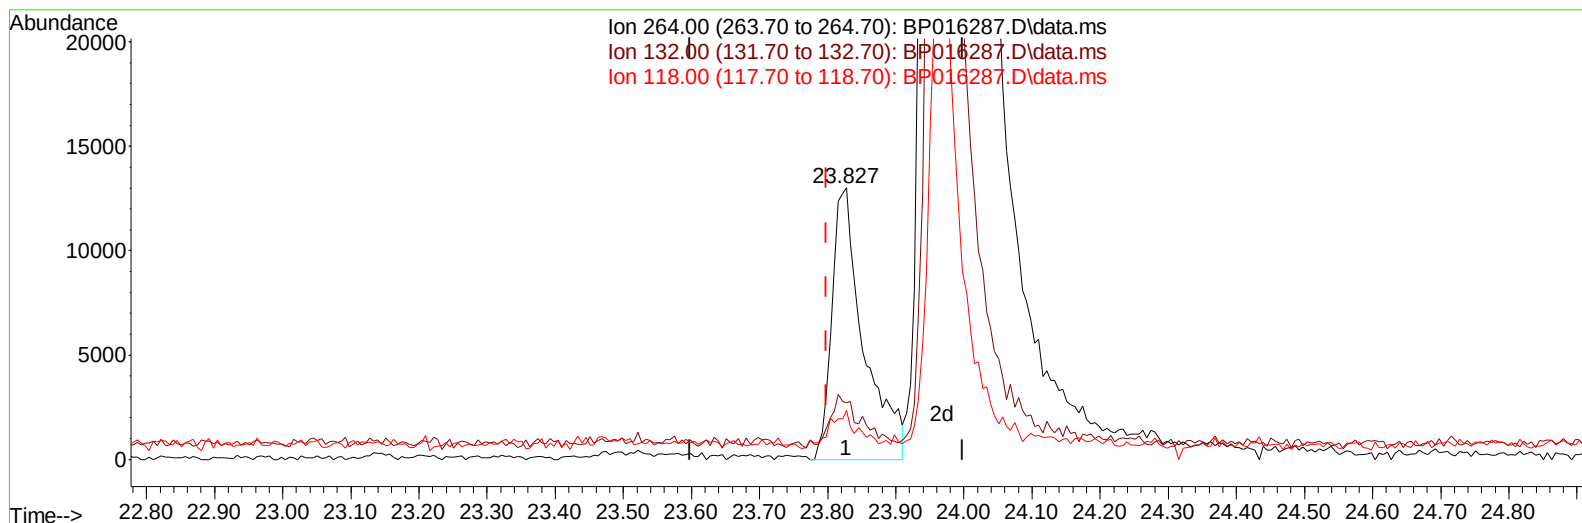

TIC: BP016287.D\data.ms

(92) Benzo(a)pyrene-d12 (S)

23.827min (+ 0.030) 0.79 ng/ul m

response 42022

Ion	Exp%	Act%
264.00	100.00	100.00
132.00	17.90	20.98
118.00	11.20	18.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016287.D
 Acq On : 18 Jul 2023 10:48
 Operator : MA/JU
 Sample : 03458-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

Quant Time: Jul 18 23:58:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.952	152		197614	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.775	136		930827	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164		612239	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.381	188		1407332	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240		1422386	20.000	ng/ul	0.00
88) Perylene-d12	23.969	264		1108185	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.281	96		7078	1.267	ng/uL	0.00
4) Pyridine-d5	3.711	84		130233m	9.351	ng/ul	-0.03
7) Phenol-d5	7.146	99		1865	0.104	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.305	67		42770	3.544	ng/ul	0.01
11) 2-Chlorophenol-d4	7.522	132		16226m	1.259	ng/ul	0.03
15) 4-Methylphenol-d8	8.787	113		24205m	1.683	ng/ul	0.08
21) Nitrobenzene-d5	9.205	128		20530	3.197	ng/ul	0.05
24) 2-Nitrophenol-d4	9.940	143		22208m	3.034	ng/ul	0.06
28) 2,4-Dichlorophenol-d3	10.640	165		3885m	0.307	ng/ul	0.19
31) 4-Chloroaniline-d4	10.946	131		128	0.006	ng/ul	-0.01
46) Dimethylphthalate-d6	14.051	166		195646	4.189	ng/ul	0.02
49) Acenaphthylene-d8	14.316	160		163259	3.190	ng/ul	0.01
54) 4-Nitrophenol-d4	15.157	143		11718m	1.229	ng/ul	0.22
60) Fluorene-d10	15.634	176		154013	3.940	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.922	200		8347m	1.027	ng/ul	0.13
73) Anthracene-d10	17.522	188		88412	1.436	ng/ul	0.04
81) Pyrene-d10	19.728	212		345663	4.683	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.827	264		42022m	0.790	ng/ul	0.03
Target Compounds							
16) Acetophenone	8.852	105		67464m	2.845	ng/ul	
86) Bis(2-ethylhexyl)phtha...	21.328	149		124807	2.102	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016287.D
Acq On : 18 Jul 2023 10:48
Operator : MA/JU
Sample : 03458-11
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:58:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

