




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016295.D
 Acq On : 18 Jul 2023 15:21
 Operator : MA/JU
 Sample : 03458-26
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46L6

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:28:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

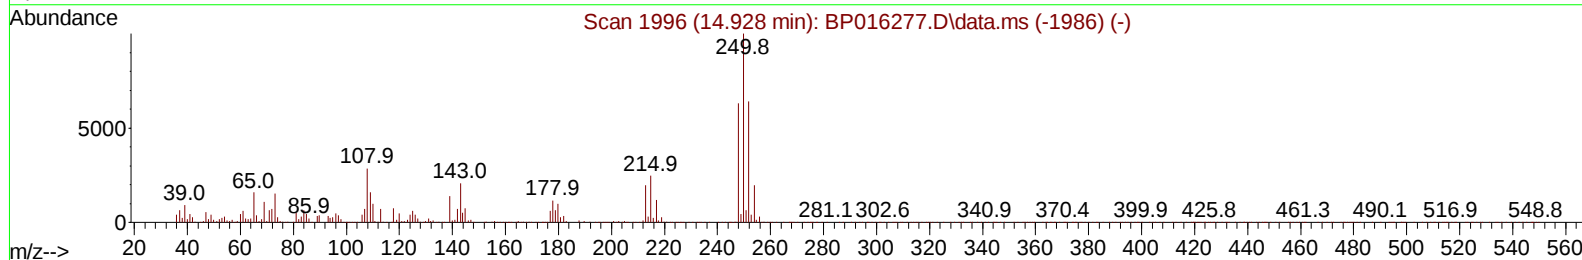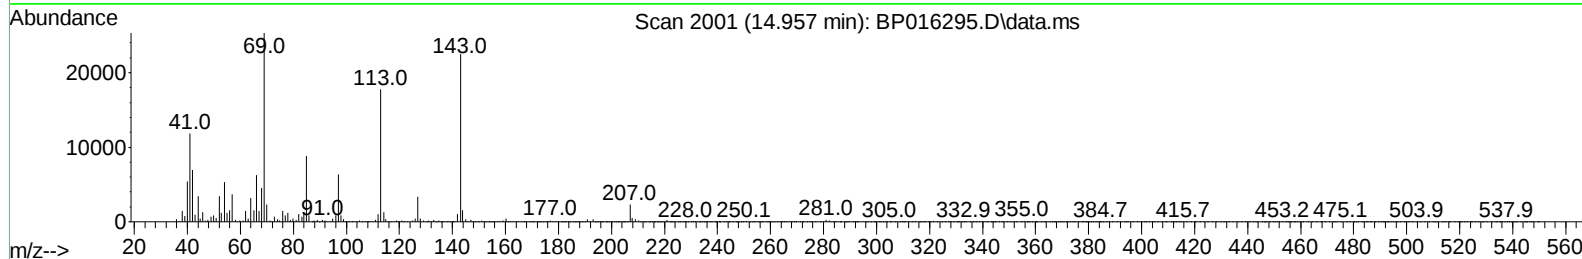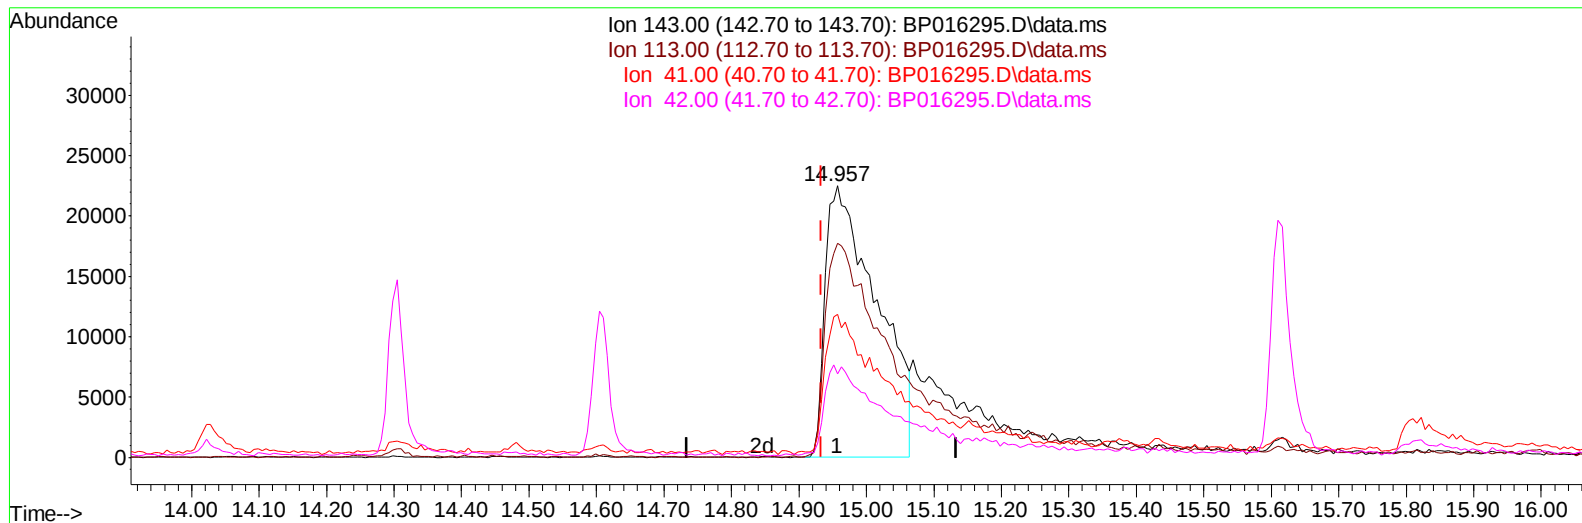

TIC: BP016295.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.957min (+ 0.024) 15.07 ng/u1

response 119209

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	78.90
41.00	49.30	52.69
42.00	32.70	30.82




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016295.D
Acq On : 18 Jul 2023 15:21
Operator : MA/JU
Sample : 03458-26
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46L6

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:28:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

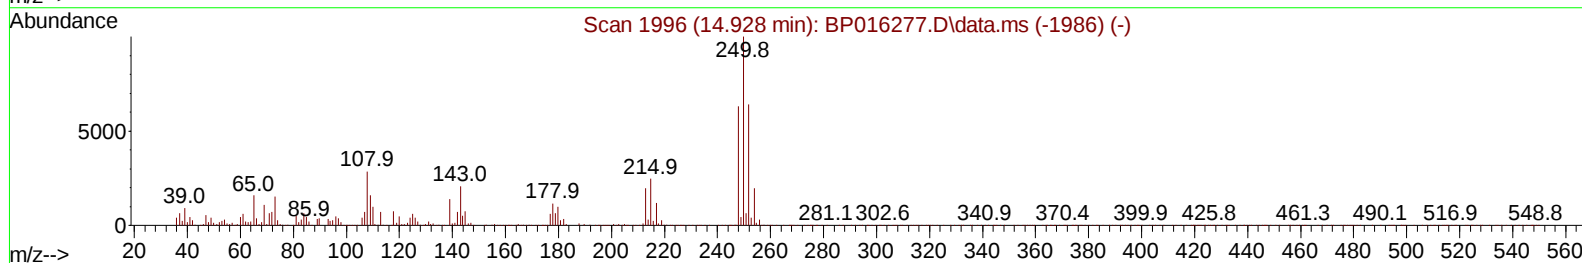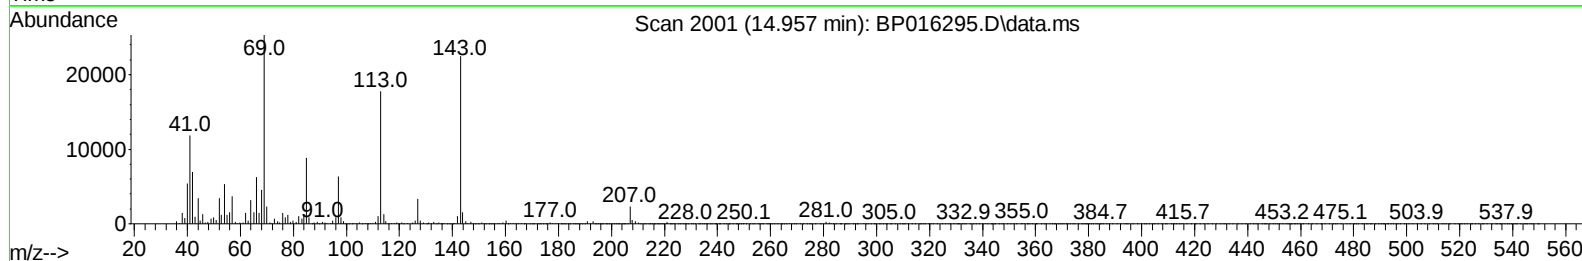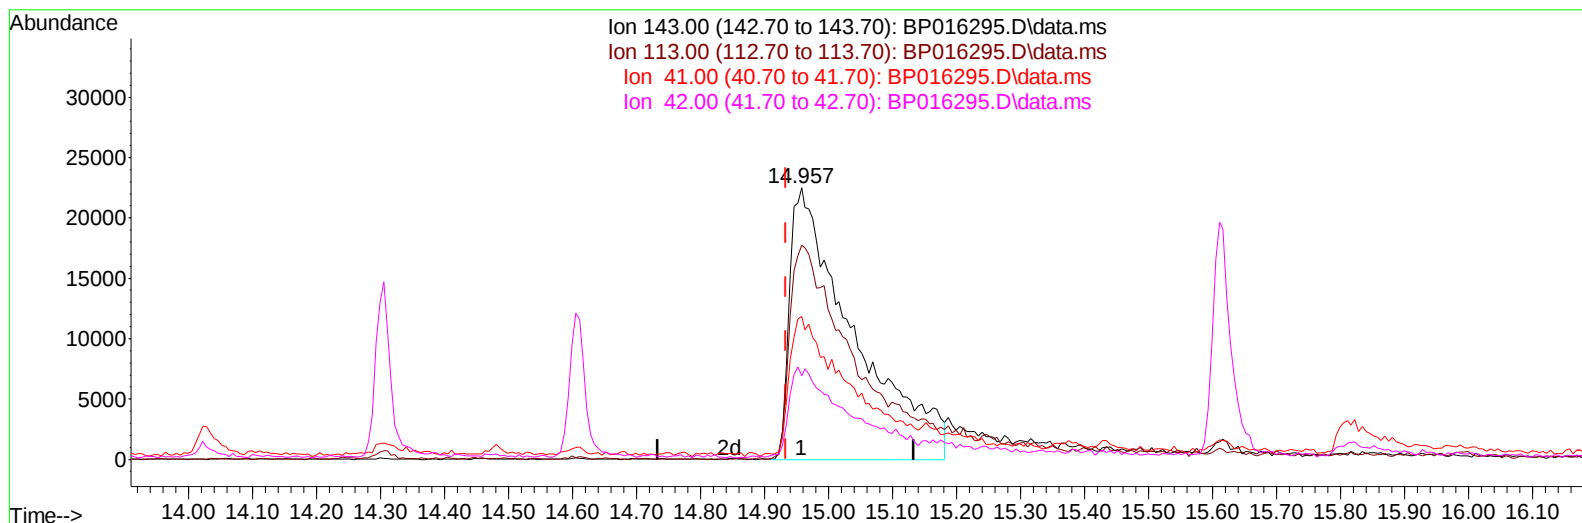

TIC: BP016295.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.957min (+ 0.024) 19.69 ng/ul m

response 155771

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	78.90
41.00	49.30	52.69
42.00	32.70	30.82

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016295.D
 Acq On : 18 Jul 2023 15:21
 Operator : MA/JU
 Sample : 03458-26
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46L6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

Quant Time: Jul 19 00:52:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 14 23:53:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	143990	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	798333	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	508292	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.369	188	1159300	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1156143	20.000	ng/ul	0.01
88) Perylene-d12	23.963	264	1323012	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	20574	5.056	ng/uL	0.00
4) Pyridine-d5	3.740	84	121215	11.944	ng/ul	0.00
7) Phenol-d5	7.152	99	401888	30.900	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	269052	30.593	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	308512	32.860	ng/ul	0.00
15) 4-Methylphenol-d8	8.705	113	419657	40.055	ng/ul	0.00
21) Nitrobenzene-d5	9.152	128	188262	34.182	ng/ul	0.00
24) 2-Nitrophenol-d4	9.881	143	174093	27.734	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	310578	28.571	ng/ul	0.01
31) 4-Chloroaniline-d4	10.969	131	507495	29.127	ng/ul	0.01
46) Dimethylphthalate-d6	14.028	166	1322937	34.120	ng/ul	0.00
49) Acenaphthylene-d8	14.304	160	1491168	35.093	ng/ul	0.00
54) 4-Nitrophenol-d4	14.957	143	155771m	19.686	ng/ul	0.02
60) Fluorene-d10	15.610	176	1157855	35.682	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	97657	14.592	ng/ul	0.02
73) Anthracene-d10	17.475	188	1883340	37.139	ng/ul	0.00
81) Pyrene-d10	19.710	212	2341143	39.024	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.792	264	2356142	37.084	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016295.D
Acq On : 18 Jul 2023 15:21
Operator : MA/JU
Sample : 03458-26
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46L6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

Quant Time: Jul 19 00:52:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 14 23:53:26 2023
Response via : Initial Calibration

