

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016246.D
 Acq On : 17 Jul 2023 09:10
 Operator : MA/JU
 Sample : PB154013BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	13	16	22	rVB	23731	36346	0.72%	0.091%
2	3.740	93	94	125	rBV	223251	602926	12.01%	1.508%
3	7.175	671	678	694	rBV2	208468	752639	15.00%	1.883%
4	7.299	694	699	726	rVV	206405	681897	13.59%	1.706%
5	7.505	728	734	757	rVB	284674	773845	15.42%	1.936%
6	7.969	805	813	838	rBV	196694	636635	12.69%	1.592%
7	8.722	934	941	977	rBV2	267679	1093914	21.80%	2.736%
8	9.175	1010	1018	1046	rBV	255070	833344	16.60%	2.084%
9	9.911	1133	1143	1170	rBV	169617	713339	14.21%	1.784%
10	10.499	1235	1243	1257	rBV2	173100	755648	15.06%	1.890%
11	10.787	1285	1292	1307	rBV	421637	1063282	21.19%	2.660%
12	10.993	1321	1327	1358	rBV2	182935	994524	19.82%	2.488%
13	12.457	1572	1576	1577	rBV4	5074	5562	0.11%	0.014%
14	13.493	1747	1752	1760	rBV7	7268	15091	0.30%	0.038%
15	14.040	1838	1845	1875	rBV	766201	1850544	36.87%	4.629%
16	14.310	1885	1891	1910	rBV2	1132498	2121052	42.26%	5.305%
17	14.616	1936	1943	1958	rBV	943803	1639860	32.68%	4.102%
18	14.981	1998	2005	2006	rBV2	79987	125338	2.50%	0.314%
19	15.622	2108	2114	2140	rBV	1221998	2878479	57.36%	7.200%
20	15.822	2142	2148	2182	rBV	148893	695397	13.86%	1.739%
21	17.051	2354	2357	2365	rBV10	3929	8375	0.17%	0.021%
22	17.181	2376	2379	2384	rVB6	3778	6118	0.12%	0.015%
23	17.381	2406	2413	2424	rBV	1450624	2237089	44.58%	5.596%
24	17.487	2425	2431	2458	rVB2	1426587	3333014	66.41%	8.337%
25	18.269	2561	2564	2573	rBV10	6320	16177	0.32%	0.040%
26	19.298	2736	2739	2746	rBV4	28943	42587	0.85%	0.107%
27	19.381	2750	2753	2762	rVB2	19497	35435	0.71%	0.089%
28	19.716	2805	2810	2835	rBV	2279041	4491777	89.50%	11.235%
29	21.486	3105	3111	3126	rBV	1431882	3008571	59.95%	7.525%
30	23.751	3492	3496	3498	rBV2	168342	264760	5.28%	0.662%
31	23.804	3498	3505	3525	rVV2	2136911	5018649	100.00%	12.553%
32	23.974	3527	3534	3556	rVB	1057565	3246253	64.68%	8.120%




Sum of corrected areas: 39978467

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016246.D
Acq On : 17 Jul 2023 09:10
Operator : MA/JU
Sample : PB154013BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

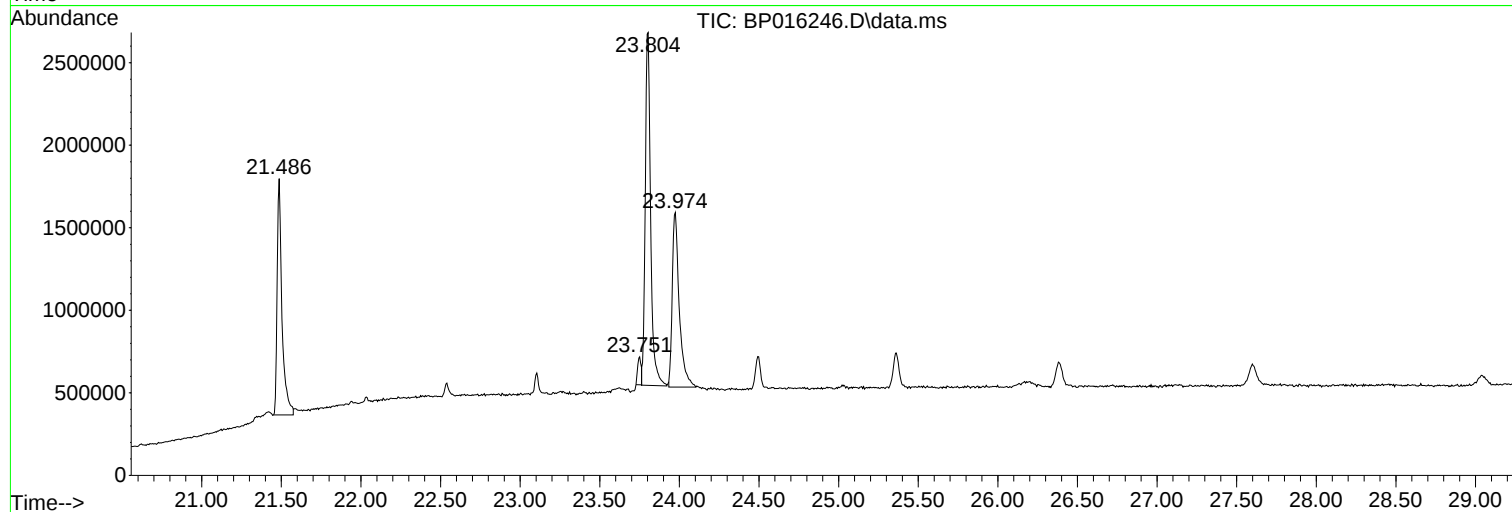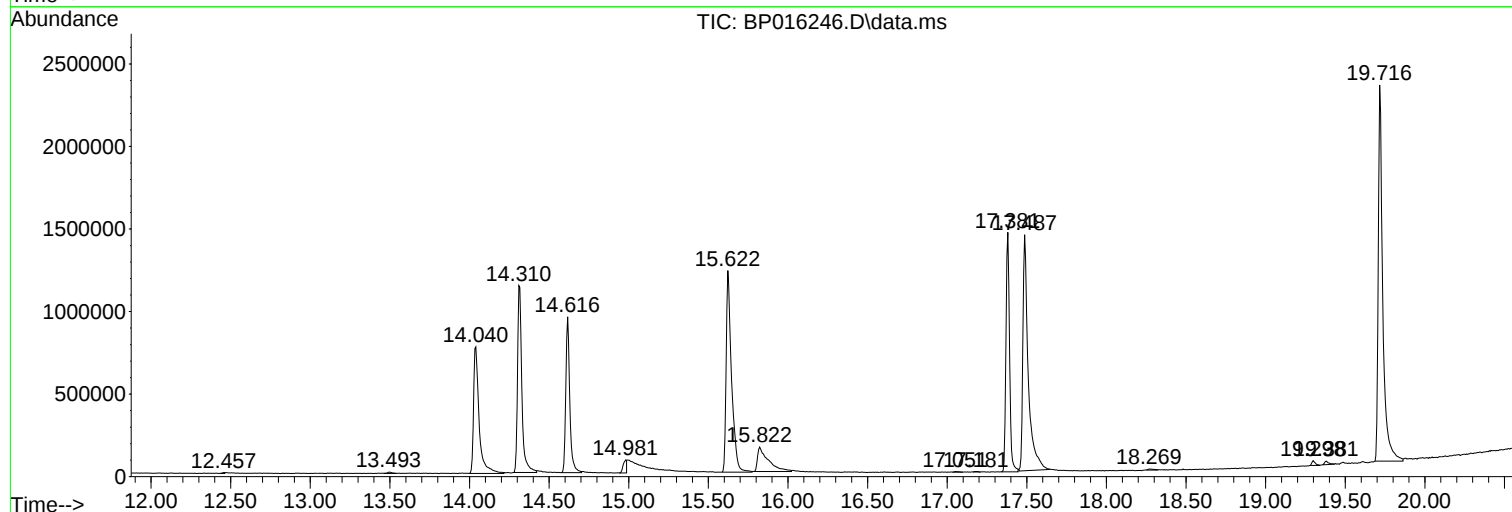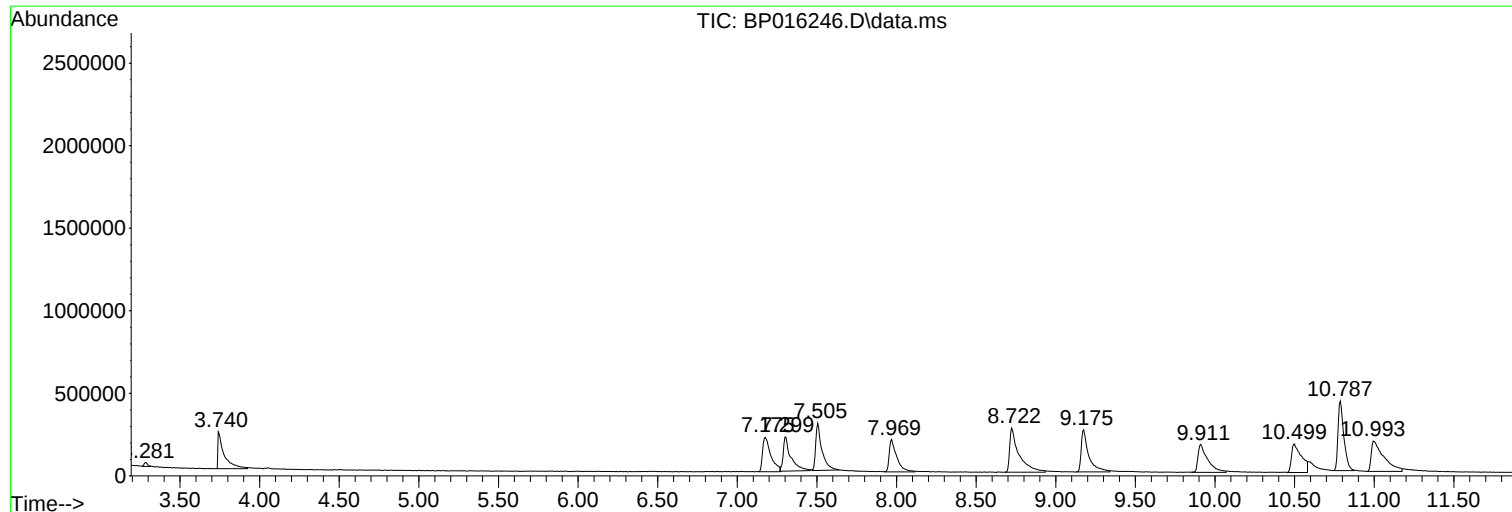

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016246.D
Acq On : 17 Jul 2023 09:10
Operator : MA/JU
Sample : PB154013BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016246.D
Acq On : 17 Jul 2023 09:10
Operator : MA/JU
Sample : PB154013BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------