

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016256.D
 Acq On : 17 Jul 2023 16:40
 Operator : MA/JU
 Sample : 03477-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	4	9	18	rBV	1048575	1749071	8.11%	2.466%
2	3.311	18	21	39	rVB	567579	957963	4.44%	1.351%
3	3.763	97	98	113	rBV	62130	184627	0.86%	0.260%
4	3.940	125	128	134	rVB2	14382	22058	0.10%	0.031%
5	4.587	231	238	267	rBV	11802734	21564106	100.00%	30.408%
6	5.199	337	342	352	rBV	21177	46278	0.21%	0.065%
7	7.216	678	685	694	rBV3	42163	138874	0.64%	0.196%
8	7.304	694	700	722	rVV	235478	788114	3.65%	1.111%
9	7.487	726	731	732	rVV2	41350	61316	0.28%	0.086%
10	7.528	732	738	765	rVB2	210453	723627	3.36%	1.020%
11	7.863	788	795	804	rBV9	11097	29126	0.14%	0.041%
12	7.969	804	813	843	rVV	302759	949275	4.40%	1.339%
13	8.340	870	876	889	rVB3	30935	90701	0.42%	0.128%
14	8.757	938	947	971	rBV4	84293	475413	2.20%	0.670%
15	9.175	1011	1018	1038	rBV	337102	970853	4.50%	1.369%
16	9.910	1136	1143	1171	rBV	184617	836204	3.88%	1.179%
17	10.504	1236	1244	1273	rBV	228486	1115197	5.17%	1.573%
18	10.787	1285	1292	1311	rBV	612990	1564890	7.26%	2.207%
19	11.022	1325	1332	1360	rBV2	84980	445669	2.07%	0.628%
20	11.728	1444	1452	1475	rBV4	38016	193417	0.90%	0.273%
21	13.492	1746	1752	1760	rBV3	22887	45864	0.21%	0.065%
22	14.033	1837	1844	1866	rBV	1083245	2323842	10.78%	3.277%
23	14.310	1885	1891	1910	rBV	1408543	2436470	11.30%	3.436%
24	14.616	1936	1943	1961	rBV	1381259	2316206	10.74%	3.266%
25	15.063	2015	2019	2022	rBV6	17133	29281	0.14%	0.041%
26	15.380	2068	2073	2081	rVV	41194	73346	0.34%	0.103%
27	15.622	2107	2114	2128	rBV	1703381	3532972	16.38%	4.982%
28	15.733	2128	2133	2142	rVV2	123878	353756	1.64%	0.499%
29	15.816	2142	2147	2172	rVV	312622	1178497	5.47%	1.662%
30	16.004	2174	2179	2189	rVB	85704	154865	0.72%	0.218%
31	17.263	2388	2393	2398	rBV5	19466	34971	0.16%	0.049%
32	17.380	2406	2413	2425	rBV	1902857	2964877	13.75%	4.181%
33	17.486	2425	2431	2456	rVB	1809006	3937544	18.26%	5.552%
34	18.239	2554	2559	2568	rBV	135578	247270	1.15%	0.349%
35	18.316	2569	2572	2578	rVV	37495	51353	0.24%	0.072%
36	18.374	2578	2582	2594	rVV	115756	236038	1.09%	0.333%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016256.D
Acq On : 17 Jul 2023 16:40
Operator : MA/JU
Sample : 03477-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA48

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION

37	19.292	2735	2738	2744	rVB3	38701	54918	0.25%	0.077%
38	19.374	2748	2752	2760	rBV	42981	72636	0.34%	0.102%
39	19.468	2764	2768	2772	rBV2	59035	80649	0.37%	0.114%
40	19.598	2788	2790	2793	rVB2	23014	22232	0.10%	0.031%
41	19.716	2804	2810	2830	rBV	3072061	5483870	25.43%	7.733%
42	21.480	3105	3110	3127	rBV2	1872468	3727701	17.29%	5.256%
43	23.804	3498	3505	3525	rVB2	2156821	4986639	23.12%	7.032%
44	23.968	3527	3533	3555	rVB	1234595	3664088	16.99%	5.167%




Sum of corrected areas: 70916664

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016256.D
Acq On : 17 Jul 2023 16:40
Operator : MA/JU
Sample : 03477-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

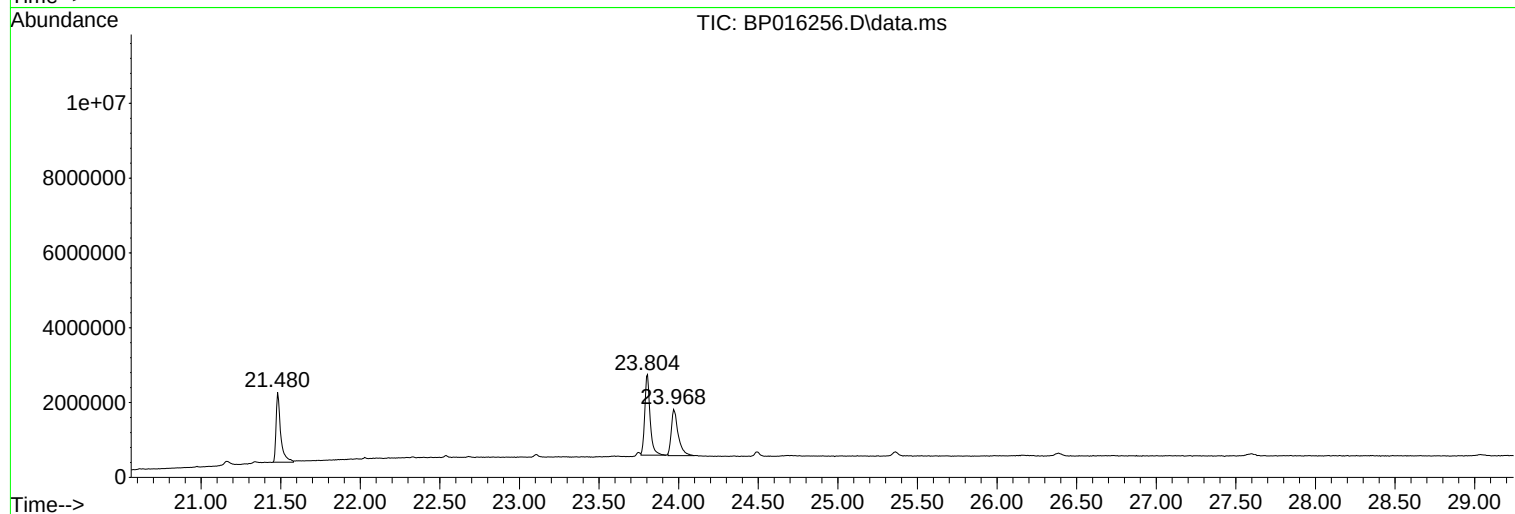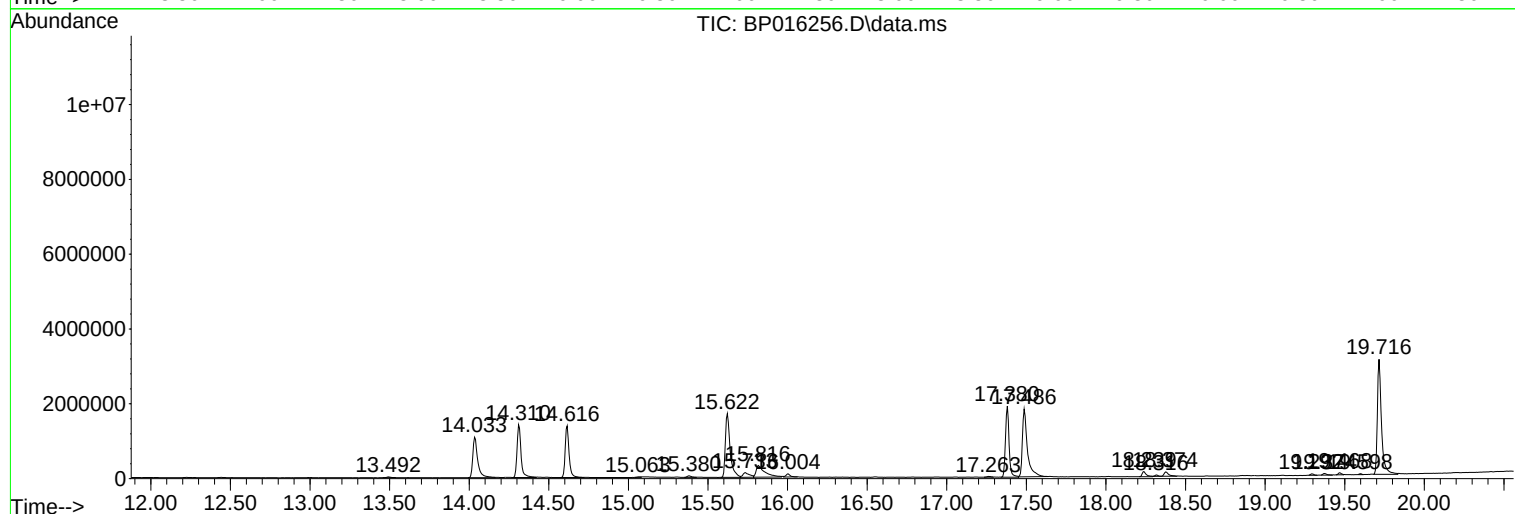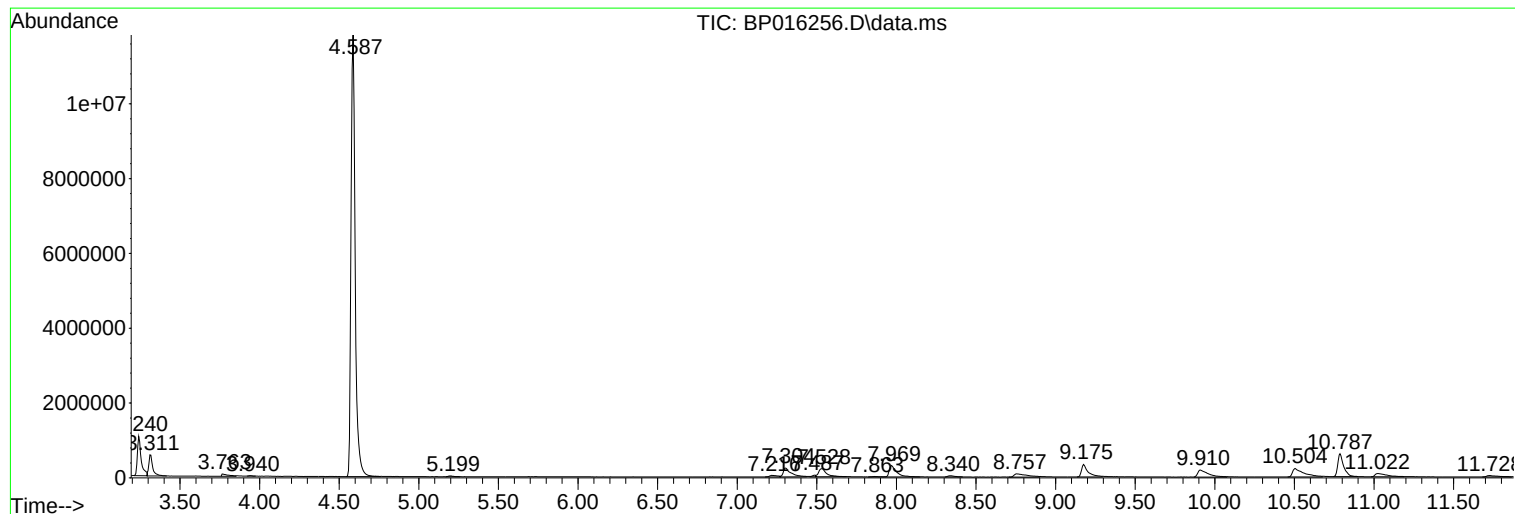

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016256.D
Acq On : 17 Jul 2023 16:40
Operator : MA/JU
Sample : 03477-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA48










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.728	2.47 ng/ul	193417	Naphthalene-d8	10.787

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			benzo[b]thiophene-3-carbonitrile	159	C9H5NS	1000404-37-8	38
2			2,4-Difluoronitrobenzene	159	C6H3F2NO2	000446-35-5	35
3			2,6-Difluorobenzoic acid, octyl ...	270	C15H20F2O2	1000292-39-2	35
4			2,5-Difluorobenzoic acid, nonyl ...	284	C16H22F2O2	1000338-80-8	35
5			2,3,4-Trifluorobenzoic acid, 2-i...	310	C16H13F3O3	1000293-72-8	27

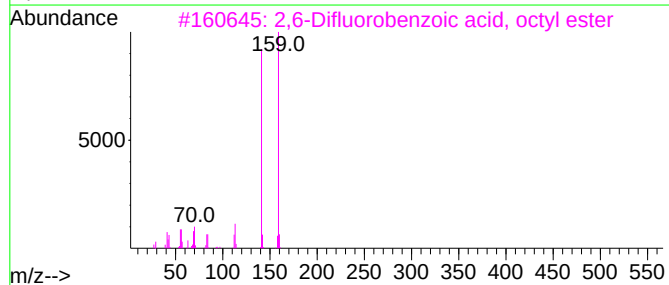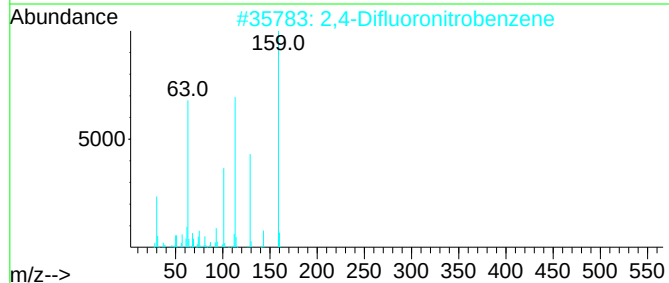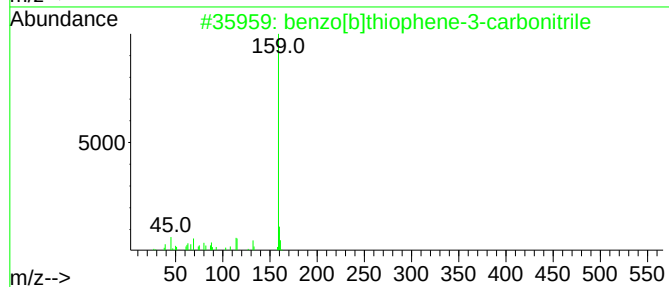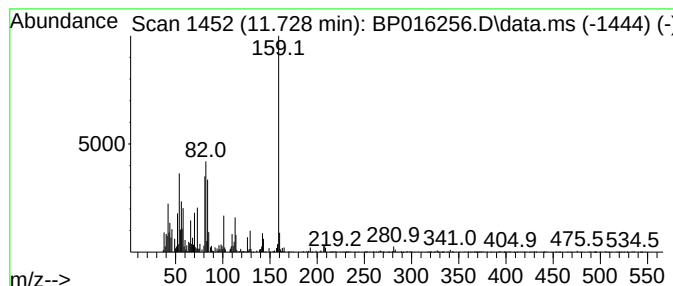

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016256.D
Acq On : 17 Jul 2023 16:40
Operator : MA/JU
Sample : 03477-10
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
HOA48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown-02 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD			R.T.
15.733	3.05 ng/ul	353756	Acenaphthene-d10			14.616
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	6-Chloropyridazin-3-amine		129	C4H4ClN3	005469-69-2	46
2	3-Chloro-4-fluoronitrobenzene		175	C6H3ClFN02	000350-30-1	43
3	3-Chloro-4-fluoronitrobenzene		175	C6H3ClFN02	000350-30-1	43
4	3-Chloro-4-fluoronitrobenzene		175	C6H3ClFN02	000350-30-1	38
5	3-Chloro-4-fluoronitrobenzene		175	C6H3ClFN02	000350-30-1	38

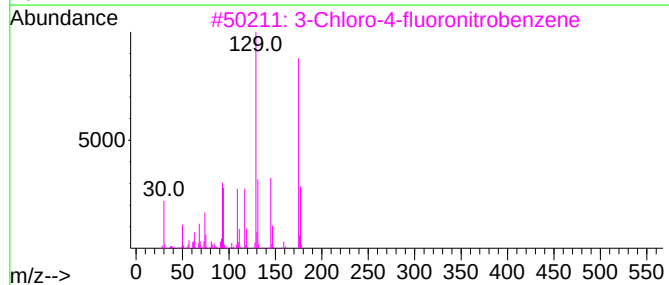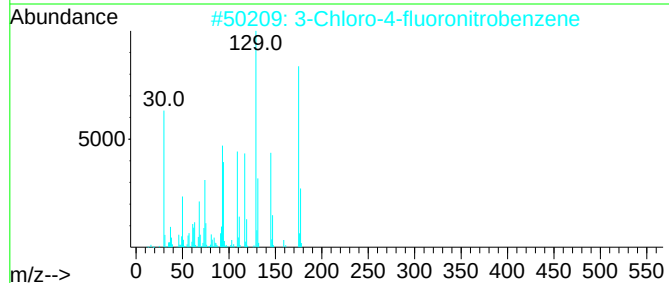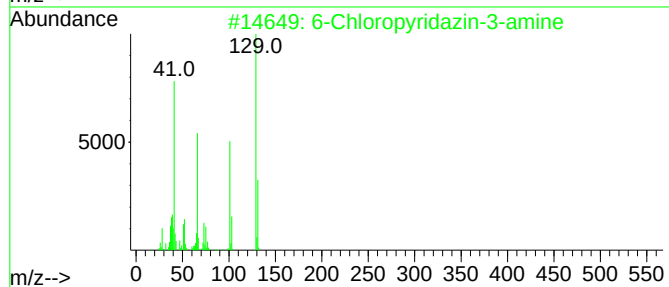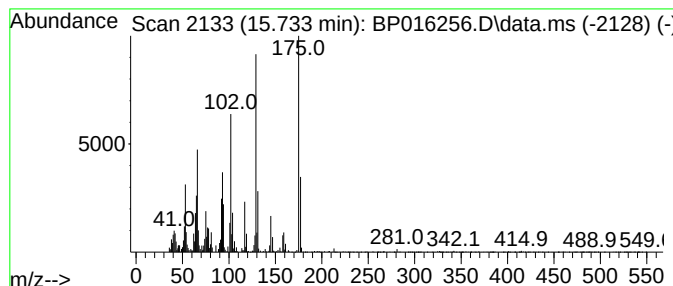

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016256.D
Acq On : 17 Jul 2023 16:40
Operator : MA/JU
Sample : 03477-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	11.728	2.5	ng/u1	193417	2	10.787	1564890	20.0
unknown-02	15.733	3.0	ng/u1	353756	3	14.616	2316210	20.0