

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016259.D
 Acq On : 17 Jul 2023 18:23
 Operator : MA/JU
 Sample : PB153940BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK940

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	13	16	24	rVB	40217	58421	1.15%	0.119%
2	3.734	91	93	116	rBV	363916	831757	16.32%	1.700%
3	4.052	143	147	152	rVB6	8628	12783	0.25%	0.026%
4	7.163	669	676	694	rBV	328678	1108353	21.75%	2.265%
5	7.299	694	699	718	rVB	314880	819022	16.07%	1.674%
6	7.499	727	733	754	rBV	445337	1059875	20.80%	2.166%
7	7.963	805	812	839	rBV	320701	961978	18.88%	1.966%
8	8.716	933	940	970	rBV	413084	1476967	28.99%	3.018%
9	9.169	1010	1017	1042	rBV	378422	1147179	22.51%	2.344%
10	9.904	1135	1142	1171	rBV	248080	979869	19.23%	2.003%
11	10.487	1232	1241	1257	rBV	251741	1080125	21.20%	2.207%
12	10.787	1284	1292	1312	rVB	651881	1616539	31.72%	3.304%
13	10.993	1320	1327	1369	rBV2	254180	1366367	26.82%	2.792%
14	12.469	1573	1578	1582	rBV8	5742	12782	0.25%	0.026%
15	13.498	1748	1753	1755	rBV6	3154	5514	0.11%	0.011%
16	14.039	1838	1845	1875	rBV	975094	2368960	46.49%	4.841%
17	14.310	1885	1891	1912	rBV2	1507421	2743904	53.85%	5.608%
18	14.616	1936	1943	1968	rBV	1337473	2331497	45.76%	4.765%
19	14.981	1998	2005	2046	rBV2	106023	889750	17.46%	1.818%
20	15.628	2108	2115	2136	rBV	1525862	3599569	70.64%	7.356%
21	15.816	2141	2147	2183	rVV	206029	912066	17.90%	1.864%
22	17.380	2406	2413	2425	rBV	1887855	2963233	58.15%	6.056%
23	17.486	2425	2431	2462	rVB2	1544840	4006132	78.62%	8.187%
24	19.304	2736	2740	2744	rBV3	32352	43864	0.86%	0.090%
25	19.380	2750	2753	2760	rBV2	23493	44659	0.88%	0.091%
26	19.722	2805	2811	2836	rBV	2368096	5095521	100.00%	10.413%
27	21.486	3106	3111	3128	rBV	1569106	3536190	69.40%	7.227%
28	23.804	3498	3505	3526	rVV2	1915352	4551395	89.32%	9.301%
29	23.974	3528	3534	3557	rVB	1006927	3307768	64.92%	6.760%




Sum of corrected areas: 48932039

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016259.D
Acq On : 17 Jul 2023 18:23
Operator : MA/JU
Sample : PB153940BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

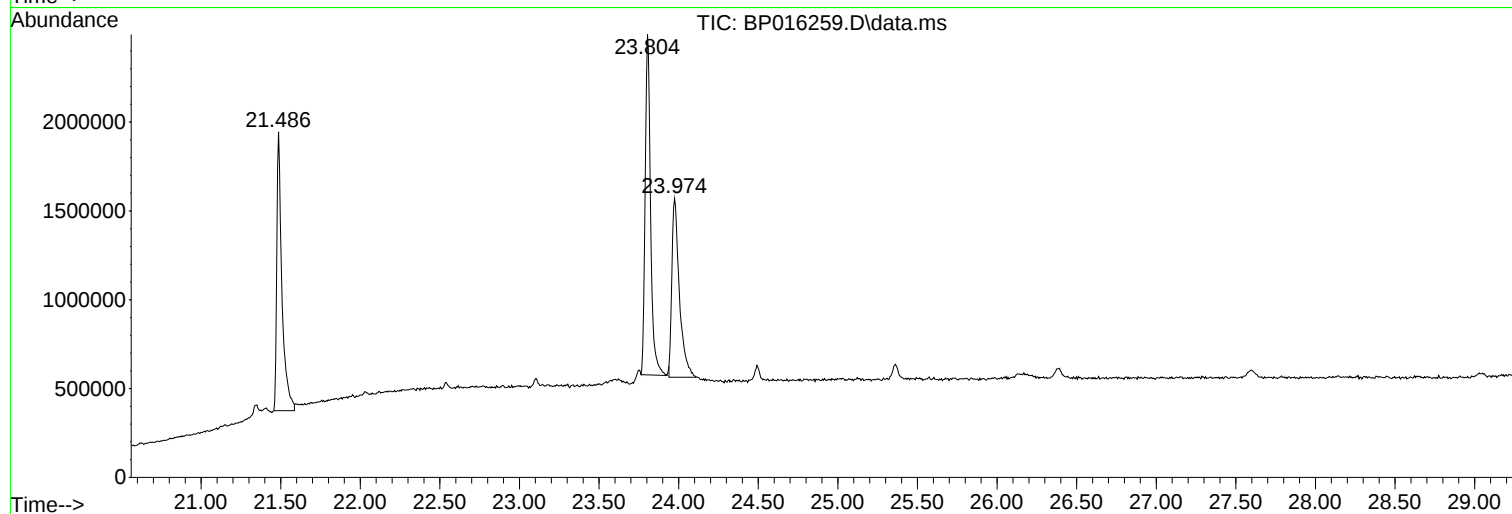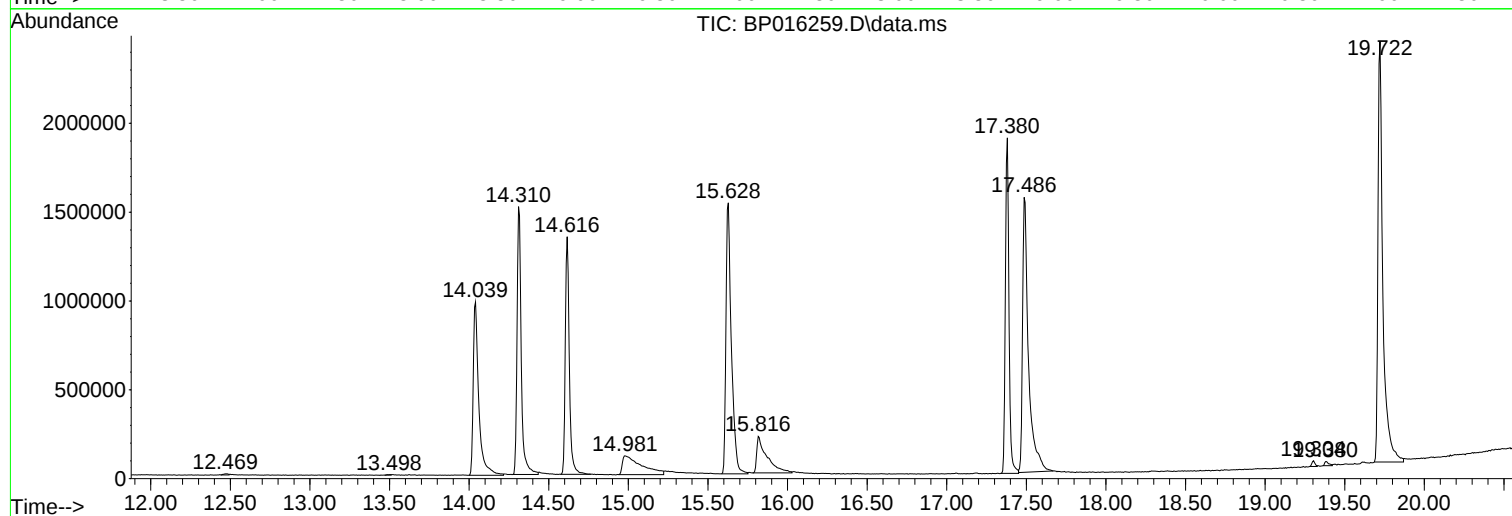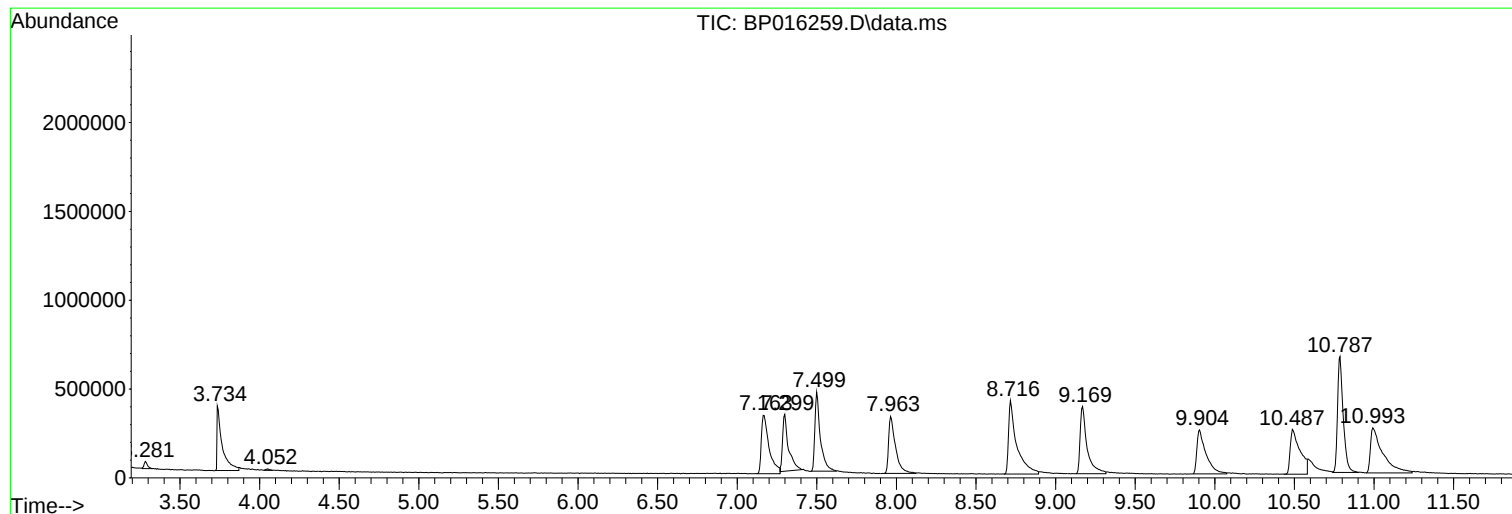

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016259.D
Acq On : 17 Jul 2023 18:23
Operator : MA/JU
Sample : PB153940BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016259.D
Acq On : 17 Jul 2023 18:23
Operator : MA/JU
Sample : PB153940BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------