

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016260.D
 Acq On : 17 Jul 2023 18:57
 Operator : MA/JU
 Sample : PB153975BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK975

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	13	16	30	rVB	51029	90256	1.69%	0.186%
2	3.734	91	93	127	rBV	431229	1023571	19.19%	2.105%
3	7.163	669	676	692	rBV	371760	1189365	22.30%	2.445%
4	7.293	693	698	726	rVV	373032	1026802	19.25%	2.111%
5	7.499	726	733	756	rVV	495082	1211913	22.72%	2.492%
6	7.963	805	812	834	rBV	288931	853148	15.99%	1.754%
7	8.710	932	939	971	rBV2	470029	1615936	30.29%	3.323%
8	9.163	1009	1016	1045	rBV	428472	1266374	23.74%	2.604%
9	9.899	1133	1141	1168	rBV	291500	1094183	20.51%	2.250%
10	10.481	1232	1240	1256	rBV2	283045	1191739	22.34%	2.450%
11	10.787	1285	1292	1312	rVB	611184	1445225	27.09%	2.972%
12	10.987	1319	1326	1348	rBV	293768	1338282	25.09%	2.752%
13	12.416	1562	1569	1572	rBV9	3384	8084	0.15%	0.017%
14	12.475	1572	1579	1587	rVV8	7054	22662	0.42%	0.047%
15	13.498	1745	1753	1757	rBV3	14587	27938	0.52%	0.057%
16	14.034	1835	1844	1874	rBV	1088153	2541272	47.64%	5.225%
17	14.310	1884	1891	1915	rBV2	1623066	2971320	55.70%	6.109%
18	14.616	1936	1943	1965	rVB	1203992	2063853	38.69%	4.243%
19	14.981	1997	2005	2029	rBV4	120893	787502	14.76%	1.619%
20	15.622	2107	2114	2139	rBV	1615887	3883825	72.81%	7.986%
21	15.816	2141	2147	2181	rBV2	223002	983430	18.44%	2.022%
22	17.381	2406	2413	2425	rBV	1687673	2602386	48.79%	5.351%
23	17.486	2425	2431	2468	rVB2	1713284	4334131	81.25%	8.911%
24	19.304	2736	2740	2747	rBV5	32319	46159	0.87%	0.095%
25	19.380	2750	2753	2759	rBV2	23437	39503	0.74%	0.081%
26	19.722	2805	2811	2832	rBV2	2457498	5334032	100.00%	10.967%
27	21.492	3107	3112	3127	rBV2	1247918	2858956	53.60%	5.878%
28	23.804	3499	3505	3526	rVB2	1767094	4410050	82.68%	9.067%
29	23.980	3528	3535	3552	rVB	775039	2374011	44.51%	4.881%




Sum of corrected areas: 48635908

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016260.D
Acq On : 17 Jul 2023 18:57
Operator : MA/JU
Sample : PB153975BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

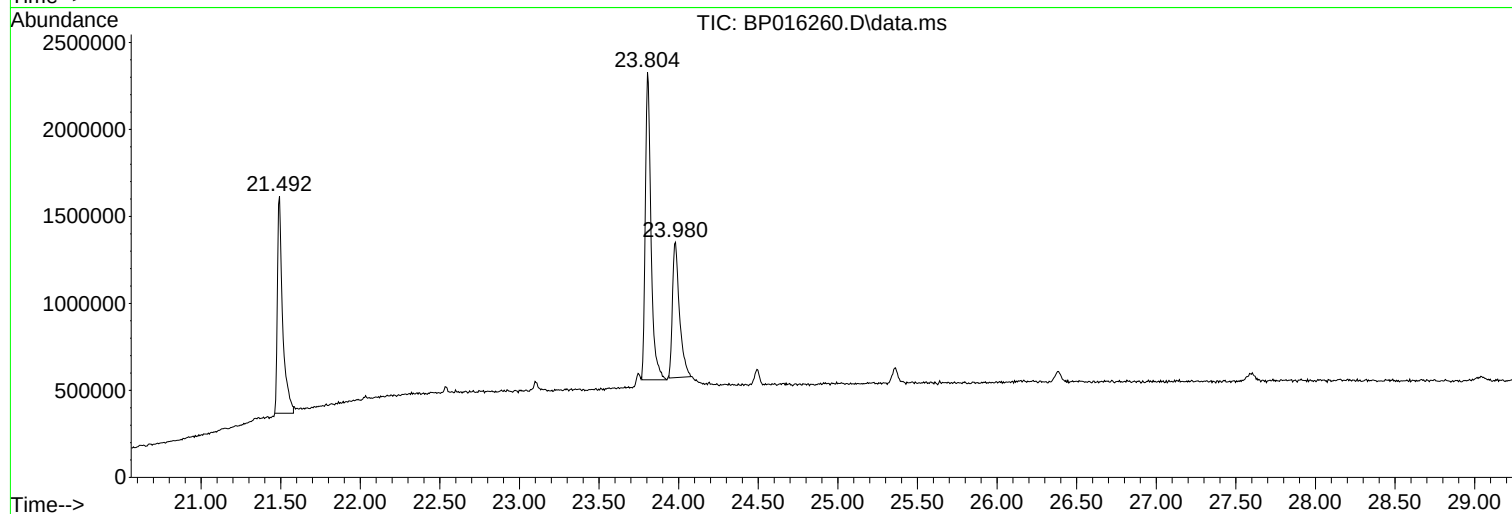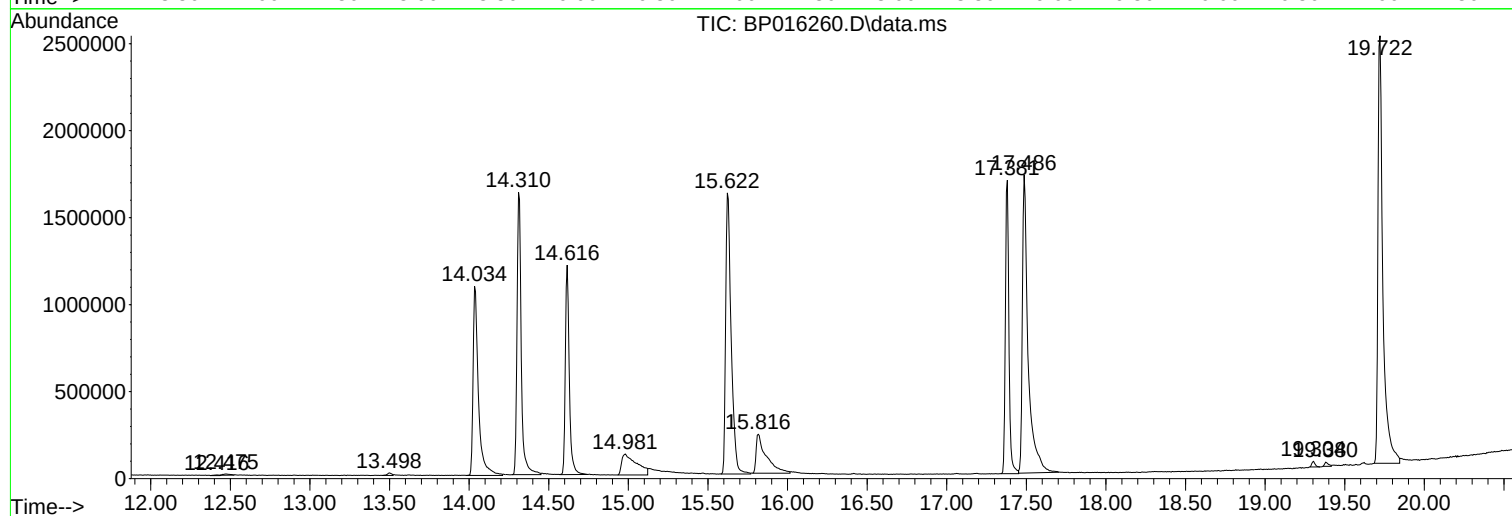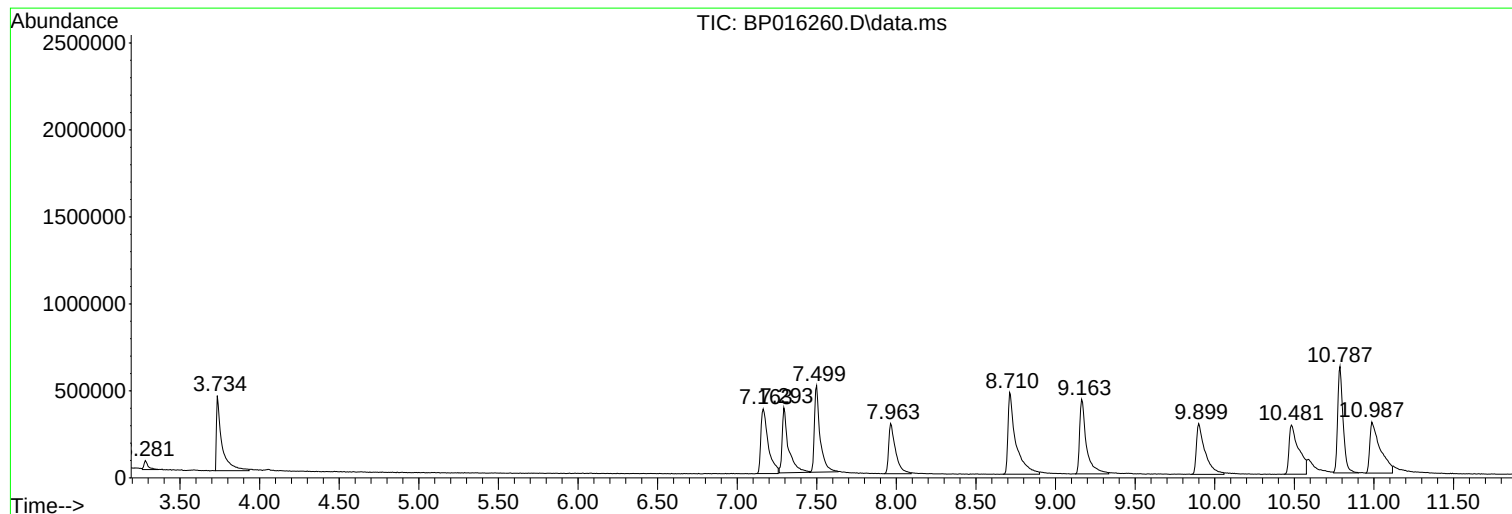

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016260.D
Acq On : 17 Jul 2023 18:57
Operator : MA/JU
Sample : PB153975BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016260.D
Acq On : 17 Jul 2023 18:57
Operator : MA/JU
Sample : PB153975BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------