

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016262.D
 Acq On : 17 Jul 2023 20:06
 Operator : MA/JU
 Sample : 03477-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	5	9	14	rBV	161766	252196	2.06%	0.398%
2	3.317	19	22	34	rVB	73827	127806	1.04%	0.202%
3	3.758	95	97	120	rBV	91666	278926	2.28%	0.440%
4	3.940	126	128	137	rVB2	16426	25913	0.21%	0.041%
5	4.581	231	237	265	rBV	6683223	12240176	100.00%	19.303%
6	7.211	675	684	694	rBV	53352	188129	1.54%	0.297%
7	7.299	694	699	724	rVB	294712	909769	7.43%	1.435%
8	7.522	730	737	763	rVB2	275684	847947	6.93%	1.337%
9	7.969	805	813	838	rBV	330494	1041720	8.51%	1.643%
10	8.734	937	943	970	rBV2	165173	728668	5.95%	1.149%
11	9.169	1010	1017	1047	rBV	420629	1239387	10.13%	1.955%
12	9.905	1133	1142	1175	rBV2	241589	1017977	8.32%	1.605%
13	10.493	1234	1242	1256	rBV	242180	1028034	8.40%	1.621%
14	10.781	1284	1291	1312	rVB	712636	1765845	14.43%	2.785%
15	10.999	1321	1328	1359	rBV2	211403	1113934	9.10%	1.757%
16	12.469	1571	1578	1583	rBV9	7096	17727	0.14%	0.028%
17	13.498	1747	1753	1759	rBV5	9858	22699	0.19%	0.036%
18	14.034	1838	1844	1874	rBV	1093354	2512595	20.53%	3.962%
19	14.310	1884	1891	1920	rBV	1721834	3004354	24.55%	4.738%
20	14.616	1936	1943	1959	rBV	1447595	2487023	20.32%	3.922%
21	15.116	2023	2028	2032	rBV8	12070	28590	0.23%	0.045%
22	15.387	2069	2074	2081	rBV	27523	54942	0.45%	0.087%
23	15.622	2107	2114	2141	rBV	1732323	3961561	32.37%	6.247%
24	15.828	2142	2149	2175	rVV3	221286	1010706	8.26%	1.594%
25	16.010	2175	2180	2191	rVB	88365	178939	1.46%	0.282%
26	16.557	2268	2273	2279	rVB3	12860	20351	0.17%	0.032%
27	17.381	2406	2413	2425	rBV	1920372	3102162	25.34%	4.892%
28	17.486	2425	2431	2458	rVB	1839073	4250744	34.73%	6.703%
29	18.022	2519	2522	2530	rVB10	10434	15936	0.13%	0.025%
30	18.239	2554	2559	2569	rBV2	77759	163637	1.34%	0.258%
31	18.322	2569	2573	2576	rVV	26348	39675	0.32%	0.063%
32	18.369	2576	2581	2600	rVV	305249	634677	5.19%	1.001%
33	19.292	2735	2738	2742	rBV	37826	51992	0.42%	0.082%
34	19.375	2748	2752	2761	rBV2	44118	74149	0.61%	0.117%
35	19.469	2764	2768	2771	rBV2	49834	74680	0.61%	0.118%
36	19.716	2804	2810	2826	rBV	2963159	5497777	44.92%	8.670%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016262.D
Acq On : 17 Jul 2023 20:06
Operator : MA/JU
Sample : 03477-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA45

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION

37	20.192	2888	2891	2897	rVB5	47313	63047	0.52%	0.099%
38	20.463	2935	2937	2941	rBV5	36559	42550	0.35%	0.067%
39	21.480	3105	3110	3128	rBV	1726466	3701852	30.24%	5.838%
40	23.798	3498	3504	3524	rVB2	2479710	5679080	46.40%	8.956%
41	23.969	3526	3533	3554	rVB	1359739	3913617	31.97%	6.172%




Sum of corrected areas: 63411489

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016262.D
Acq On : 17 Jul 2023 20:06
Operator : MA/JU
Sample : 03477-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

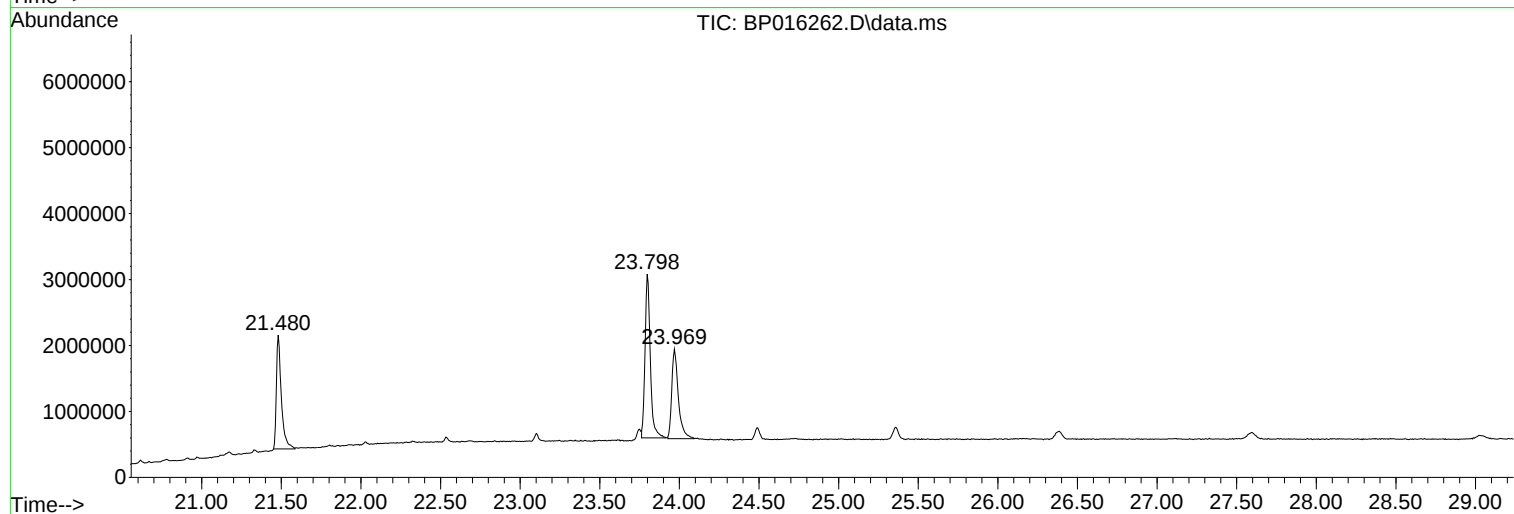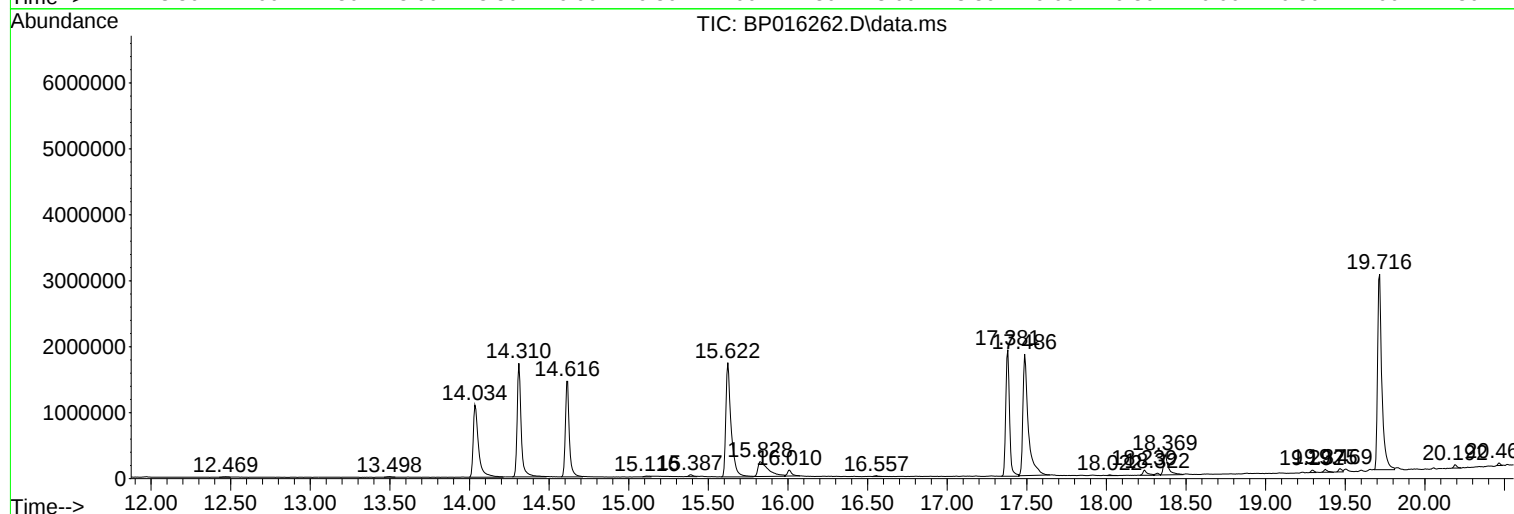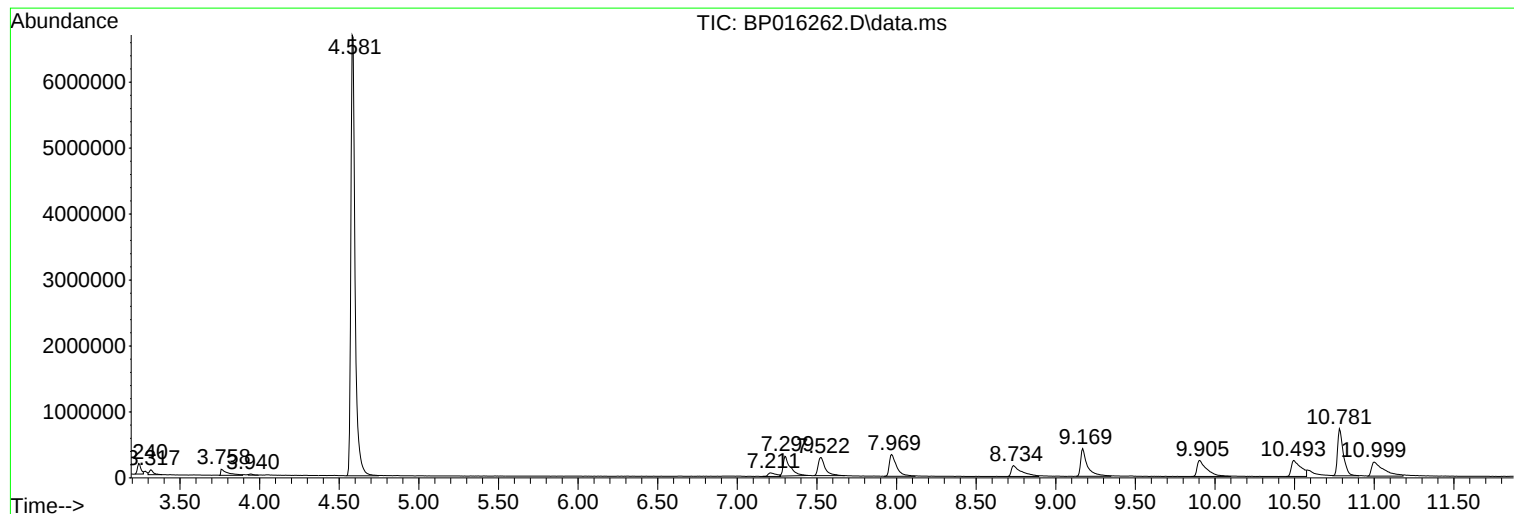

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016262.D
Acq On : 17 Jul 2023 20:06
Operator : MA/JU
Sample : 03477-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA45










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Bromacil Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.369	4.09 ng/ul	634677	Phenanthrene-d10	17.381

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bromacil	260	C9H13BrN2O2	000314-40-9	94
2			Bromacil	260	C9H13BrN2O2	000314-40-9	87
3			Bromacil	260	C9H13BrN2O2	000314-40-9	64
4			2,4,6-Trichlorobenzonitrile	205	C7H2Cl3N	006575-05-9	47
5			5-Acetamido-2,4-dichlorobenzoic ...	247	C9H7Cl2NO3	050602-49-8	47

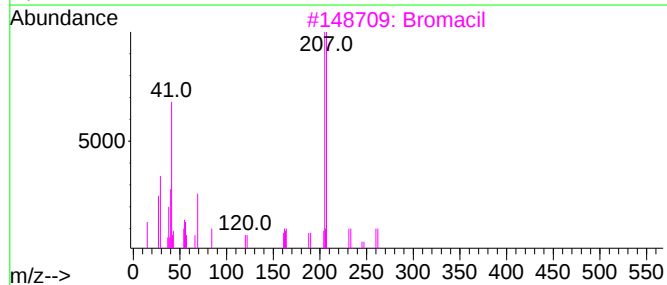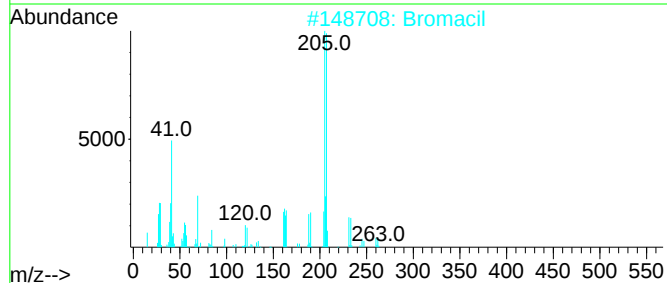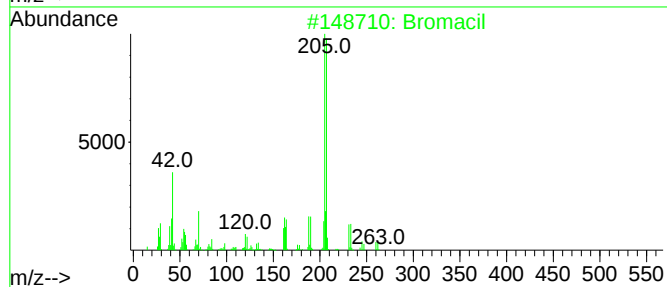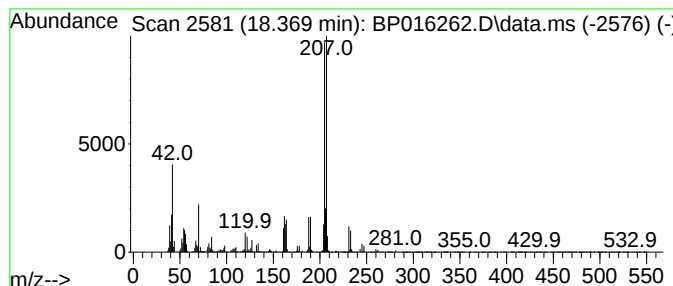

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016262.D
Acq On : 17 Jul 2023 20:06
Operator : MA/JU
Sample : 03477-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Bromacil	18.369	4.1	ng/u1	634677	4	17.381	3102160	20.0