

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016266.D
 Acq On : 17 Jul 2023 22:22
 Operator : MA/JU
 Sample : 03477-10DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA48DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016266.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	4	9	18	rBV	247679	422306	6.48%	1.578%
2	3.317	18	22	32	rVB	138676	218908	3.36%	0.818%
3	4.058	143	148	150	rBV6	6866	11398	0.17%	0.043%
4	4.581	231	237	259	rBV	3682183	6519527	100.00%	24.361%
5	7.381	702	713	730	rBV4	23753	138714	2.13%	0.518%
6	7.628	749	755	772	rBV4	22310	87873	1.35%	0.328%
7	8.005	810	819	855	rBV3	155814	895821	13.74%	3.347%
8	8.916	968	974	975	rBV5	9032	15741	0.24%	0.059%
9	9.299	1029	1039	1061	rBV4	28269	171206	2.63%	0.640%
10	10.028	1155	1163	1164	rBV6	15995	32453	0.50%	0.121%
11	10.663	1263	1271	1274	rBV3	31319	75813	1.16%	0.283%
12	10.804	1288	1295	1330	rBV	386439	1516568	23.26%	5.667%
13	11.157	1348	1355	1356	rBV5	9904	15061	0.23%	0.056%
14	11.846	1465	1472	1474	rBV8	4640	10953	0.17%	0.041%
15	13.516	1749	1756	1764	rBV4	13611	36431	0.56%	0.136%
16	14.075	1844	1851	1866	rBV	147700	492424	7.55%	1.840%
17	14.328	1887	1894	1916	rBV	216801	516056	7.92%	1.928%
18	14.622	1937	1944	1971	rBV	1043000	2359350	36.19%	8.816%
19	15.410	2076	2078	2082	rBV5	5945	7738	0.12%	0.029%
20	15.657	2113	2120	2144	rBV2	261806	842231	12.92%	3.147%
21	15.845	2148	2152	2153	rBV4	8812	10482	0.16%	0.039%
22	15.916	2159	2164	2179	rBV4	20551	80885	1.24%	0.302%
23	16.051	2183	2187	2189	rBV4	6255	7748	0.12%	0.029%
24	16.863	2321	2325	2330	rVB8	4067	7913	0.12%	0.030%
25	17.392	2408	2415	2431	rBV	1383900	2842456	43.60%	10.621%
26	17.522	2431	2437	2459	rVB2	222262	824845	12.65%	3.082%
27	18.257	2557	2562	2569	rBV8	20854	48682	0.75%	0.182%
28	18.404	2585	2587	2597	rBV10	9186	20607	0.32%	0.077%
29	19.486	2767	2771	2776	rBV7	15901	33036	0.51%	0.123%
30	19.739	2808	2814	2832	rBV2	472754	1259413	19.32%	4.706%
31	21.480	3105	3110	3128	rBV2	1377286	3436524	52.71%	12.841%
32	23.816	3502	3507	3525	rVB	299973	745930	11.44%	2.787%
33	23.974	3527	3534	3556	rVB	986411	3056798	46.89%	11.422%




Sum of corrected areas: 26761891

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016266.D
Acq On : 17 Jul 2023 22:22
Operator : MA/JU
Sample : 03477-10DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA48DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

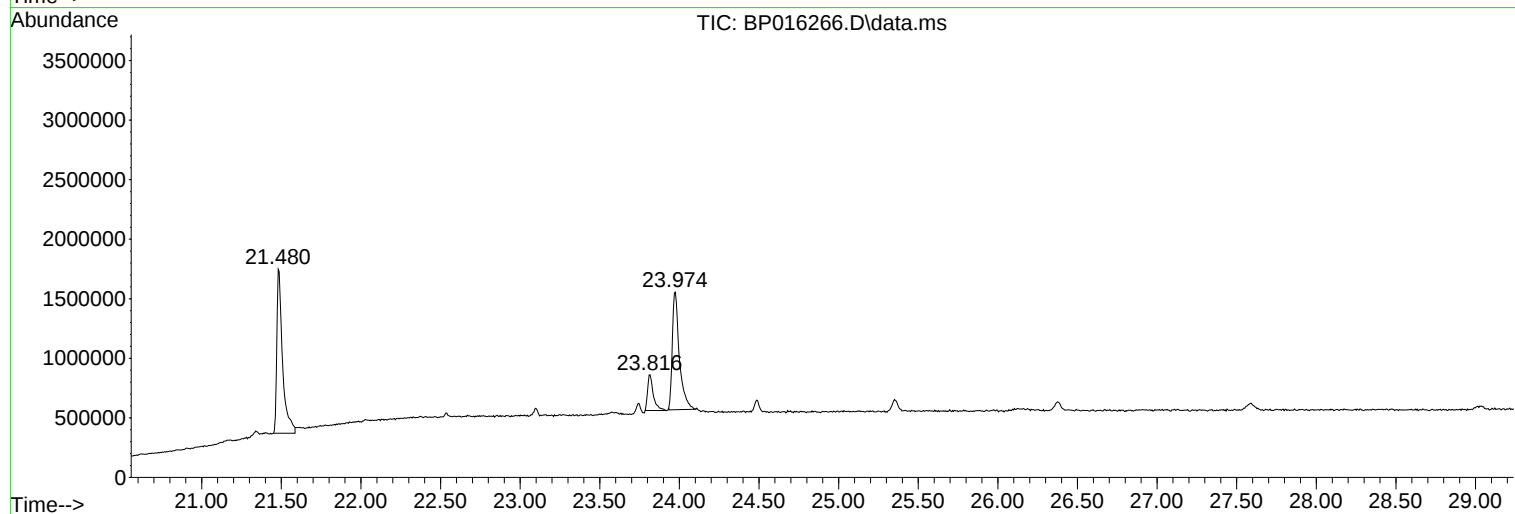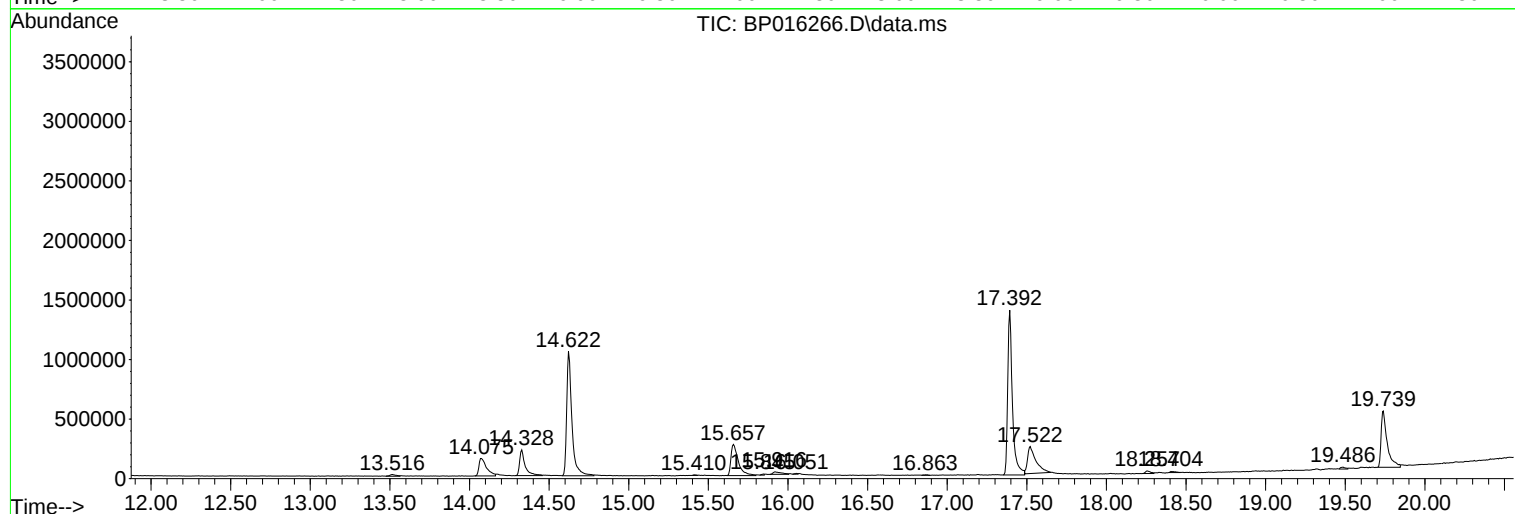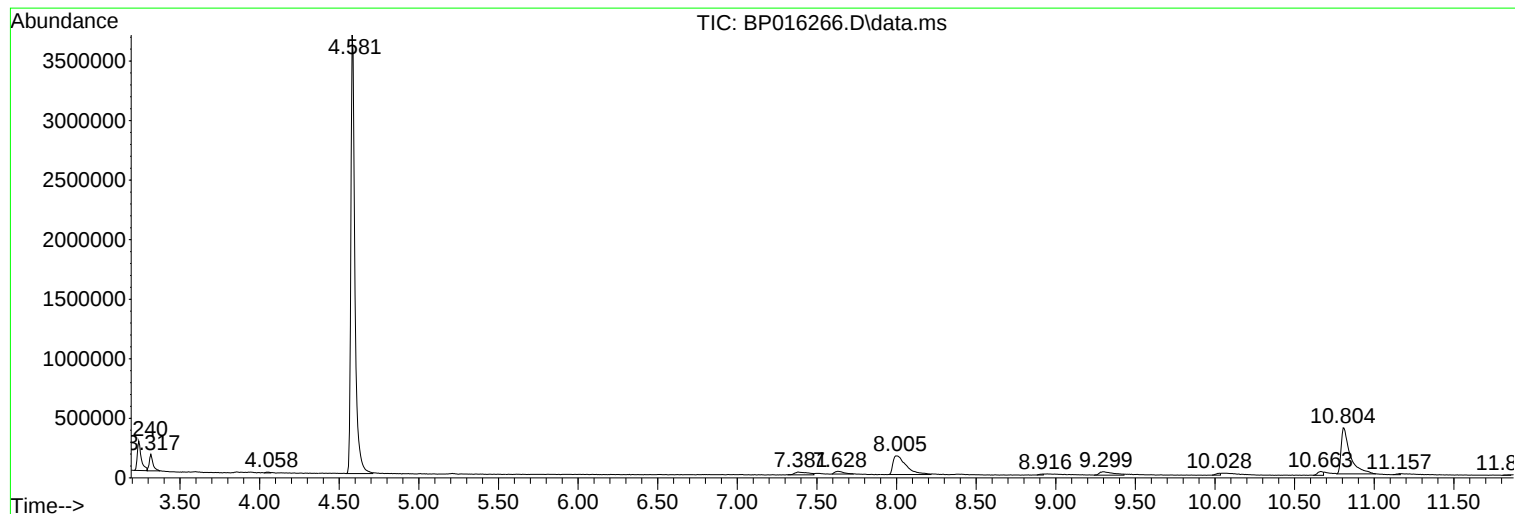

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016266.D
Acq On : 17 Jul 2023 22:22
Operator : MA/JU
Sample : 03477-10DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA48DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016266.D
Acq On : 17 Jul 2023 22:22
Operator : MA/JU
Sample : 03477-10DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA48DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------